

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY072523\
 Data File : VY014826.D
 Acq On : 26 Jul 2023 01:35
 Operator : SY/MD
 Sample : 03741-07
 Misc : 5.05g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 B-P25B

Quant Time: Jul 26 03:35:15 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y071323S.M
 Quant Title : SW846 8260
 QLast Update : Fri Jul 14 02:09:50 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.801	168	165593	50.000	ug/l	0.01
34) 1,4-Difluorobenzene	8.697	114	296716	50.000	ug/l	0.01
63) Chlorobenzene-d5	11.495	117	282442	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.428	152	131388	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.148	65	107901	57.181	ug/l	0.01
Spiked Amount	50.000	Range	50 - 163	Recovery	=	114.360%
35) Dibromofluoromethane	7.728	113	94357	49.955	ug/l	0.01
Spiked Amount	50.000	Range	54 - 147	Recovery	=	99.920%
50) Toluene-d8	10.184	98	353465	50.758	ug/l	0.00
Spiked Amount	50.000	Range	58 - 134	Recovery	=	101.520%
62) 4-Bromofluorobenzene	12.483	95	129655	48.557	ug/l	0.00
Spiked Amount	50.000	Range	30 - 143	Recovery	=	97.120%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY072523\
Data File : VY014826.D
Acq On : 26 Jul 2023 01:35
Operator : SY/MD
Sample : 03741-07
Misc : 5.05g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 43 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
B-P25B

Quant Time: Jul 26 03:35:15 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y071323S.M
Quant Title : SW846 8260
QLast Update : Fri Jul 14 02:09:50 2023
Response via : Initial Calibration




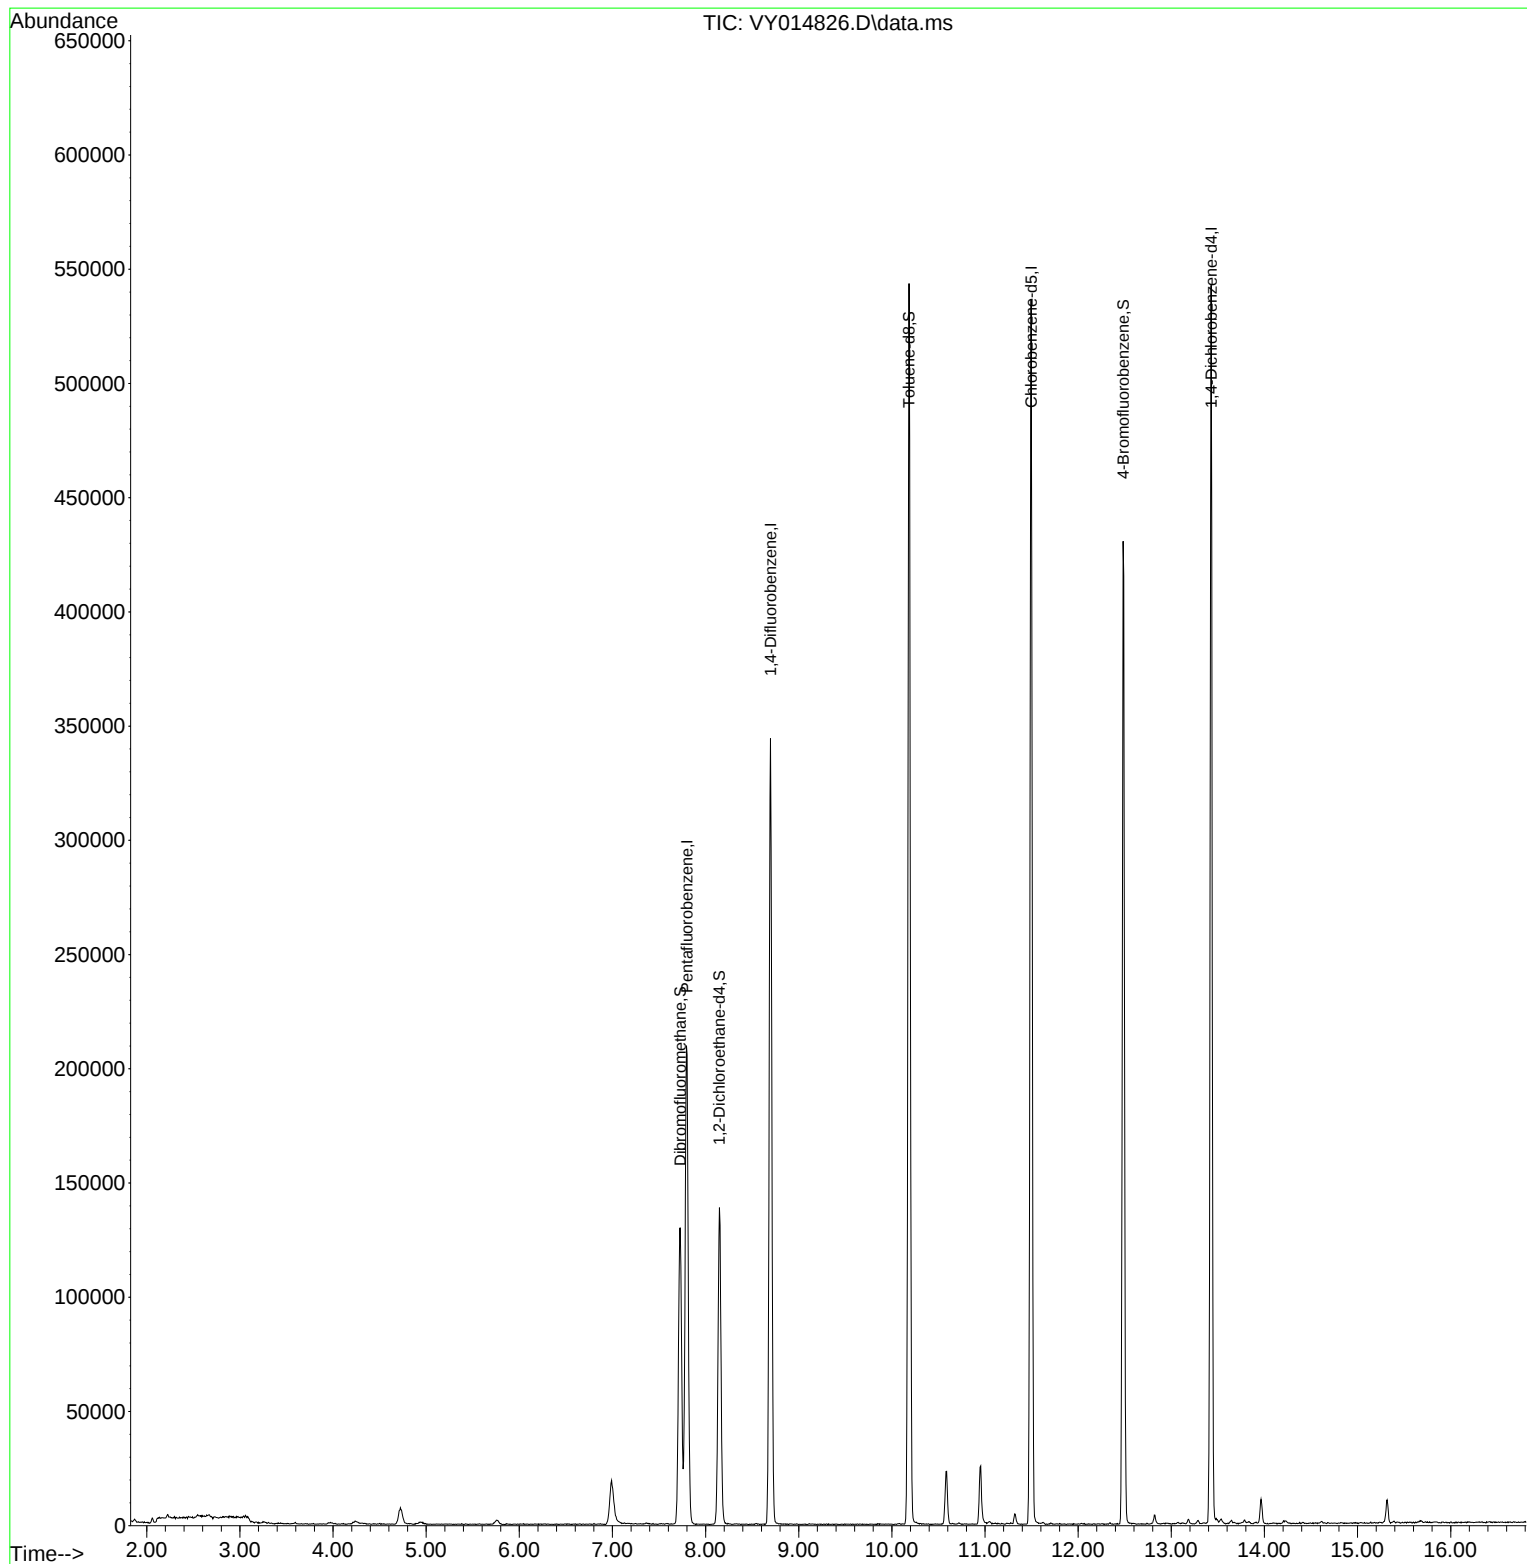


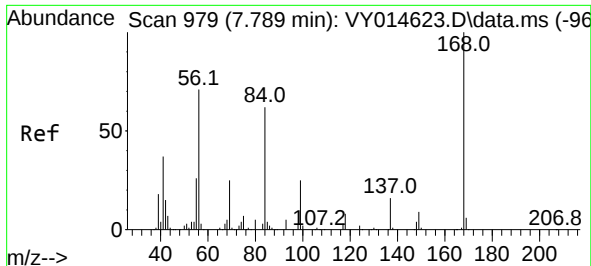

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.801 min Scan# 91
Delta R.T. 0.012 min
Lab File: VY014826.D
Acq: 26 Jul 2023 01:35




Instrument :
MSVOA_Y
ClientSampleId :
B-P25B


Tgt Ion:168 Resp: 165593
Ion Ratio Lower Upper
168 100
99 54.3 43.4 65.0

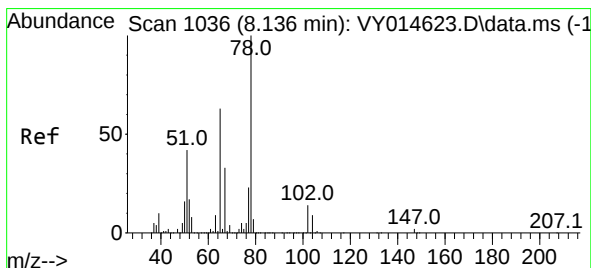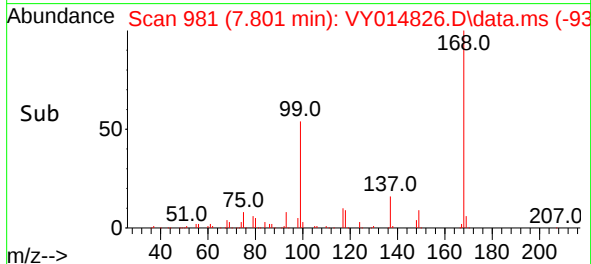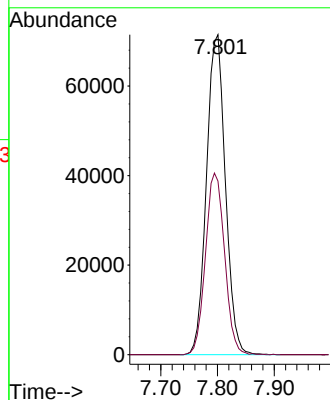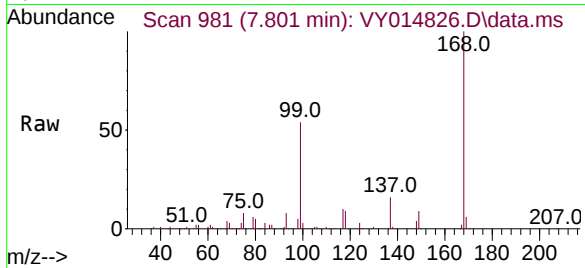

#33
1,2-Dichloroethane-d4
Concen: 57.181 ug/l
RT: 8.148 min Scan# 1038
Delta R.T. 0.012 min
Lab File: VY014826.D
Acq: 26 Jul 2023 01:35

Tgt Ion: 65 Resp: 107901
Ion Ratio Lower Upper
65 100
67 52.7 0.0 101.8


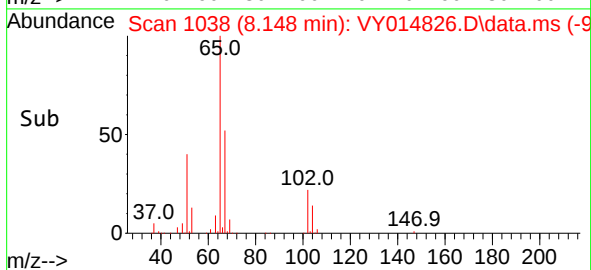
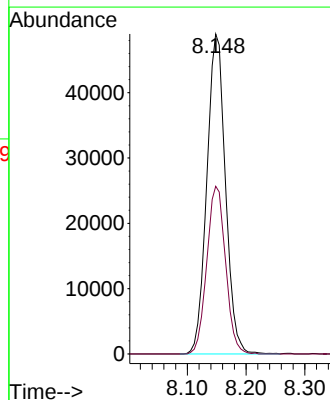
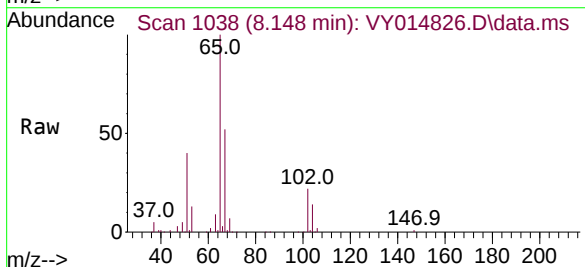


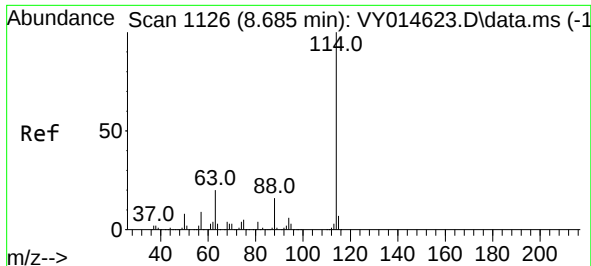

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.697 min Scan# 1126
Delta R.T. 0.012 min
Lab File: VY014826.D
Acq: 26 Jul 2023 01:35




Instrument :
MSVOA_Y
ClientSampleId :
B-P25B


Tgt Ion:114 Resp: 296716
Ion Ratio Lower Upper
114 100
63 19.4 0.0 42.4
88 15.9 0.0 30.6

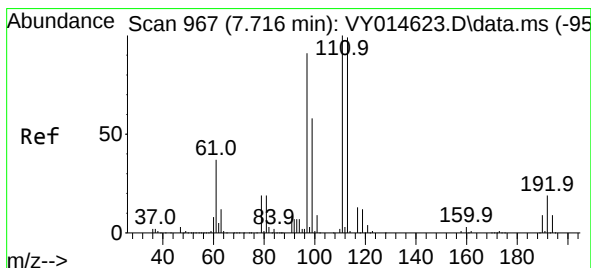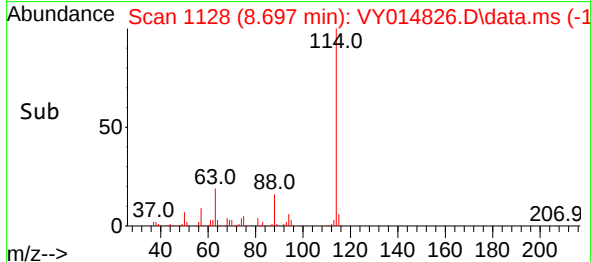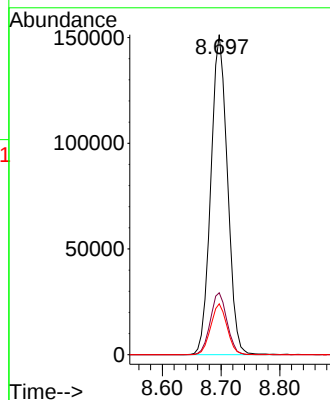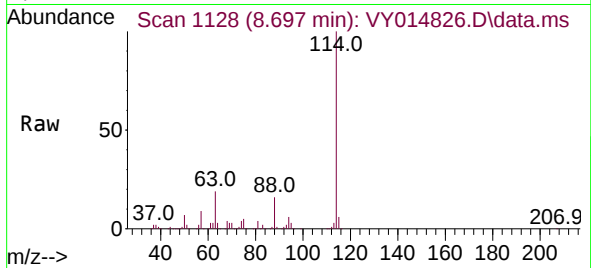

#35
Dibromofluoromethane
Concen: 49.955 ug/l
RT: 7.728 min Scan# 969
Delta R.T. 0.012 min
Lab File: VY014826.D
Acq: 26 Jul 2023 01:35

Tgt Ion:113 Resp: 94357
Ion Ratio Lower Upper
113 100
111 102.4 81.3 121.9
192 18.8 16.9 25.3


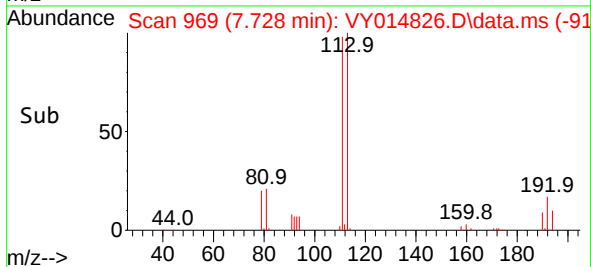
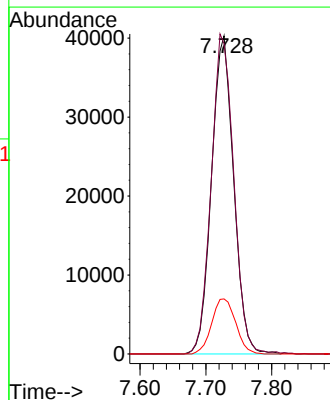
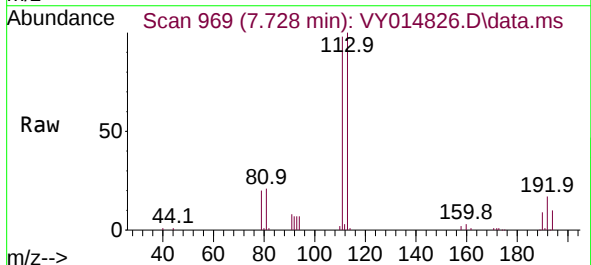


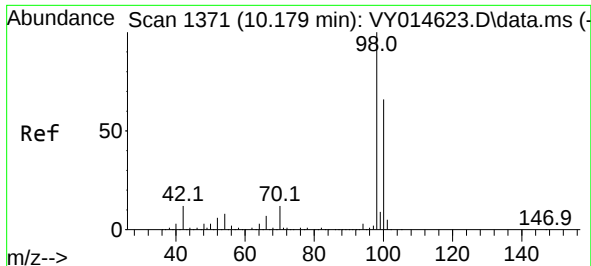

#50
Toluene-d8
Concen: 50.758 ug/l
RT: 10.184 min Scan# 1371
Delta R.T. 0.005 min
Lab File: VY014826.D
Acq: 26 Jul 2023 01:35




Instrument :
MSVOA_Y
ClientSampleId :
B-P25B


Tgt Ion: 98 Resp: 353465
Ion Ratio Lower Upper
98 100
100 65.1 50.1 75.1

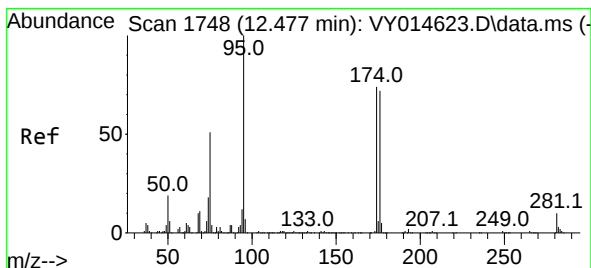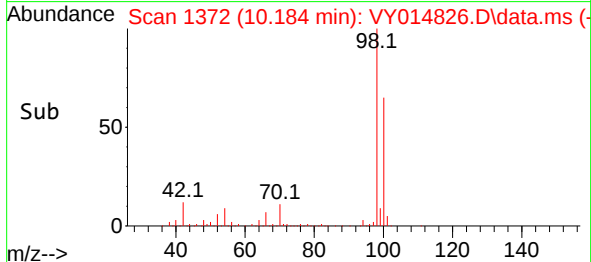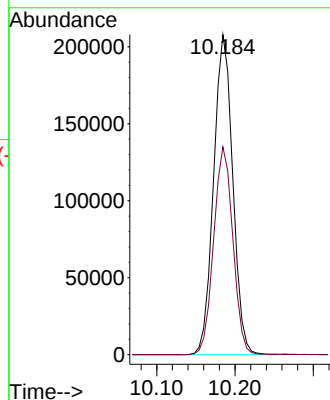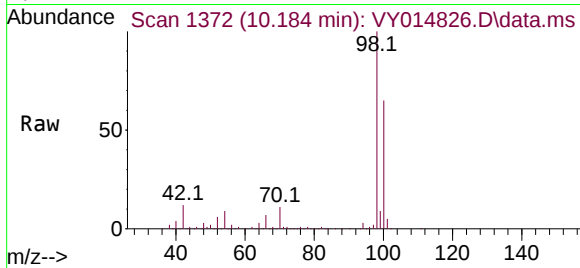

#62
4-Bromofluorobenzene
Concen: 48.557 ug/l
RT: 12.483 min Scan# 1749
Delta R.T. 0.006 min
Lab File: VY014826.D
Acq: 26 Jul 2023 01:35

Tgt Ion: 95 Resp: 129655
Ion Ratio Lower Upper
95 100
174 82.2 0.0 178.2
176 79.3 0.0 173.8

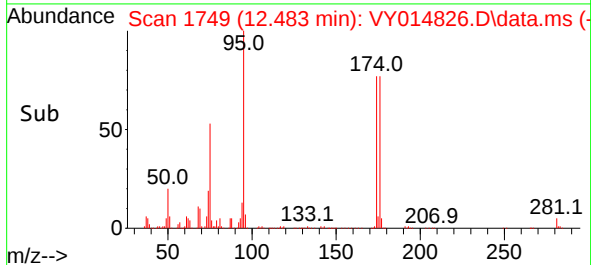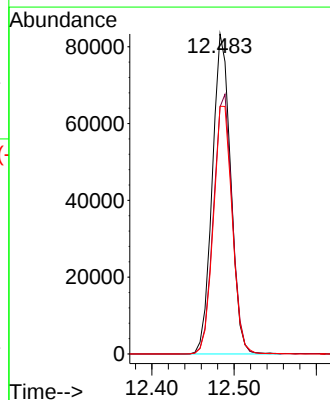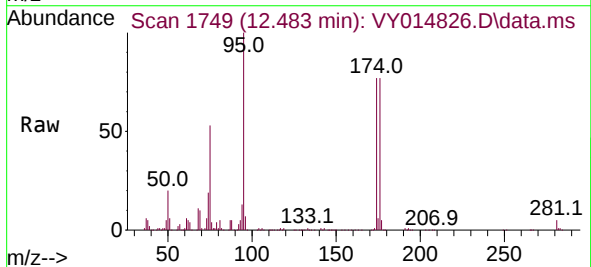

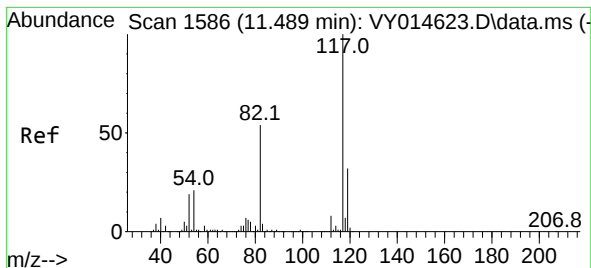

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.495 min Scan# 11

Delta R.T. 0.006 min

Lab File: VY014826.D

Acq: 26 Jul 2023 01:35

Instrument :

MSVOA_Y

ClientSampleId :

B-P25B





Tgt Ion:117 Resp: 282442

Ion Ratio Lower Upper

117 100

82 54.8 43.4 65.0

119 32.9 26.3 39.5

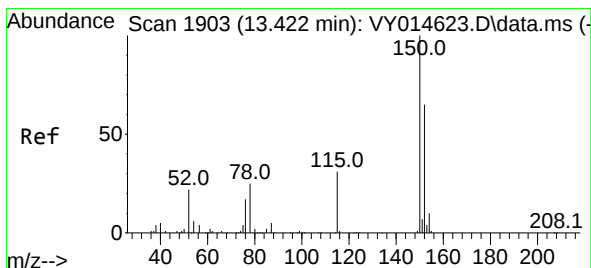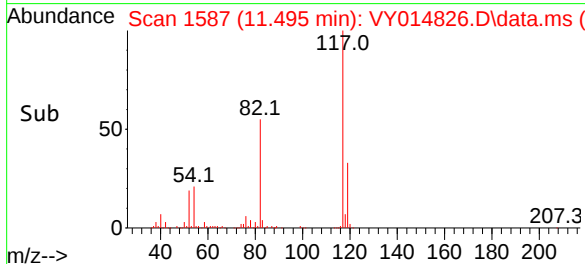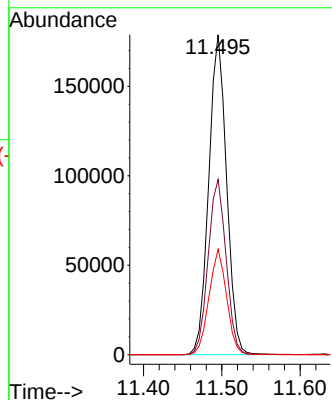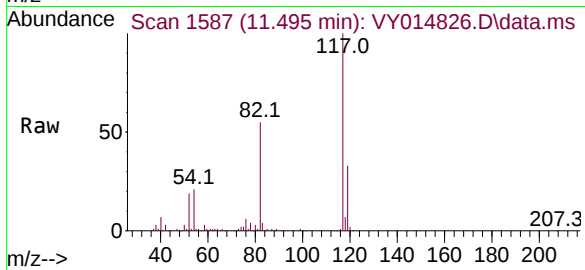

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.428 min Scan# 1904

Delta R.T. 0.006 min

Lab File: VY014826.D

Acq: 26 Jul 2023 01:35

Tgt Ion:152 Resp: 131388

Ion Ratio Lower Upper

152 100

115 60.2 28.8 86.5

150 158.5 0.0 348.8

