
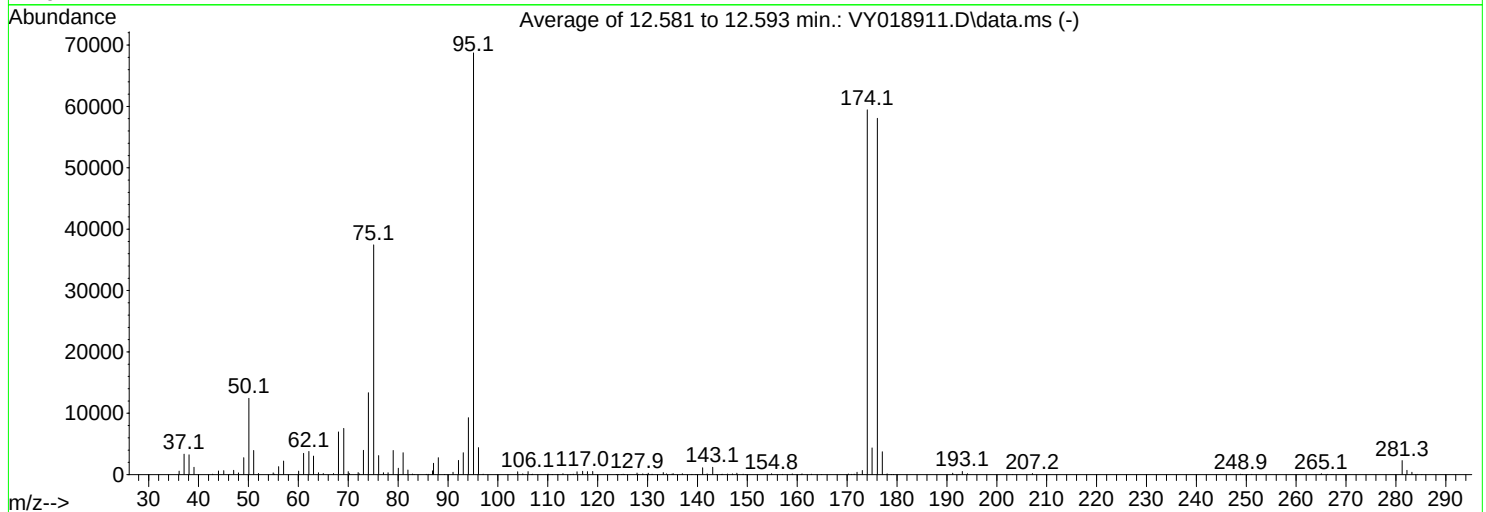


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY072524\
Data File : VY018911.D
Acq On : 25 Jul 2024 07:56
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y070924S.M
Title : SW846 8260
Last Update : Tue Jul 09 14:28:51 2024

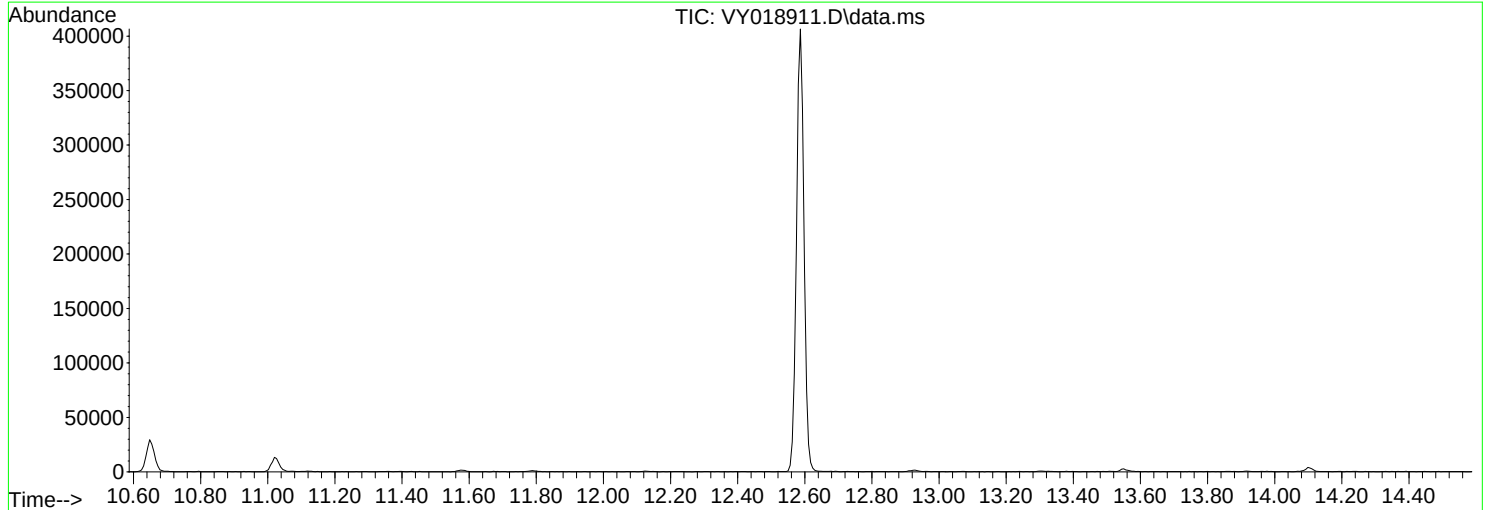

AutoFind: Scans 1765, 1766, 1767; Background Corrected with Scan 1757

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.1	12443	PASS
75	95	30	60	54.5	37443	PASS
95	95	100	100	100.0	68733	PASS
96	95	5	9	6.4	4400	PASS
173	174	0.00	2	1.1	675	PASS
174	95	50	100	86.5	59440	PASS
175	174	5	9	7.3	4365	PASS
176	174	95	101	97.7	58059	PASS
177	176	5	9	6.4	3734	PASS