

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY072621\
 Data File : VY005450.D
 Acq On : 26 Jul 2021 17:21
 Operator : SY/MD
 Sample : M3151-03
 Misc : 5.60G/5ML/MSVOA_Y/SOIL
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 COMP-3

Quant Time: Jul 27 03:11:36 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y072221S.M
 Quant Title : SW846 8260
 QLast Update : Fri Jul 23 06:20:14 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	7.801	168	230716	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.697	114	351305	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.496	117	351967	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.428	152	179543	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.149	65	128905	52.298	ug/l	0.00
Spiked Amount	50.000	Range 50 - 163	Recovery	=	104.600%	
35) Dibromofluoromethane	7.728	113	119769	59.044	ug/l	0.00
Spiked Amount	50.000	Range 54 - 147	Recovery	=	118.080%	
50) Toluene-d8	10.185	98	444730	51.728	ug/l	0.00
Spiked Amount	50.000	Range 49 - 140	Recovery	=	103.460%	
62) 4-Bromofluorobenzene	12.483	95	156103	55.014	ug/l	0.00
Spiked Amount	50.000	Range 25 - 144	Recovery	=	110.020%	
Target Compounds						
16) Acetone	3.966	43	13623	24.202	ug/l	Qvalue 98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY072621\
Data File : VY005450.D
Acq On : 26 Jul 2021 17:21
Operator : SY/MD
Sample : M3151-03
Misc : 5.60G/5ML/MSVOA_Y/SOIL
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
COMP-3

Quant Time: Jul 27 03:11:36 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y072221S.M
Quant Title : SW846 8260
QLast Update : Fri Jul 23 06:20:14 2021
Response via : Initial Calibration




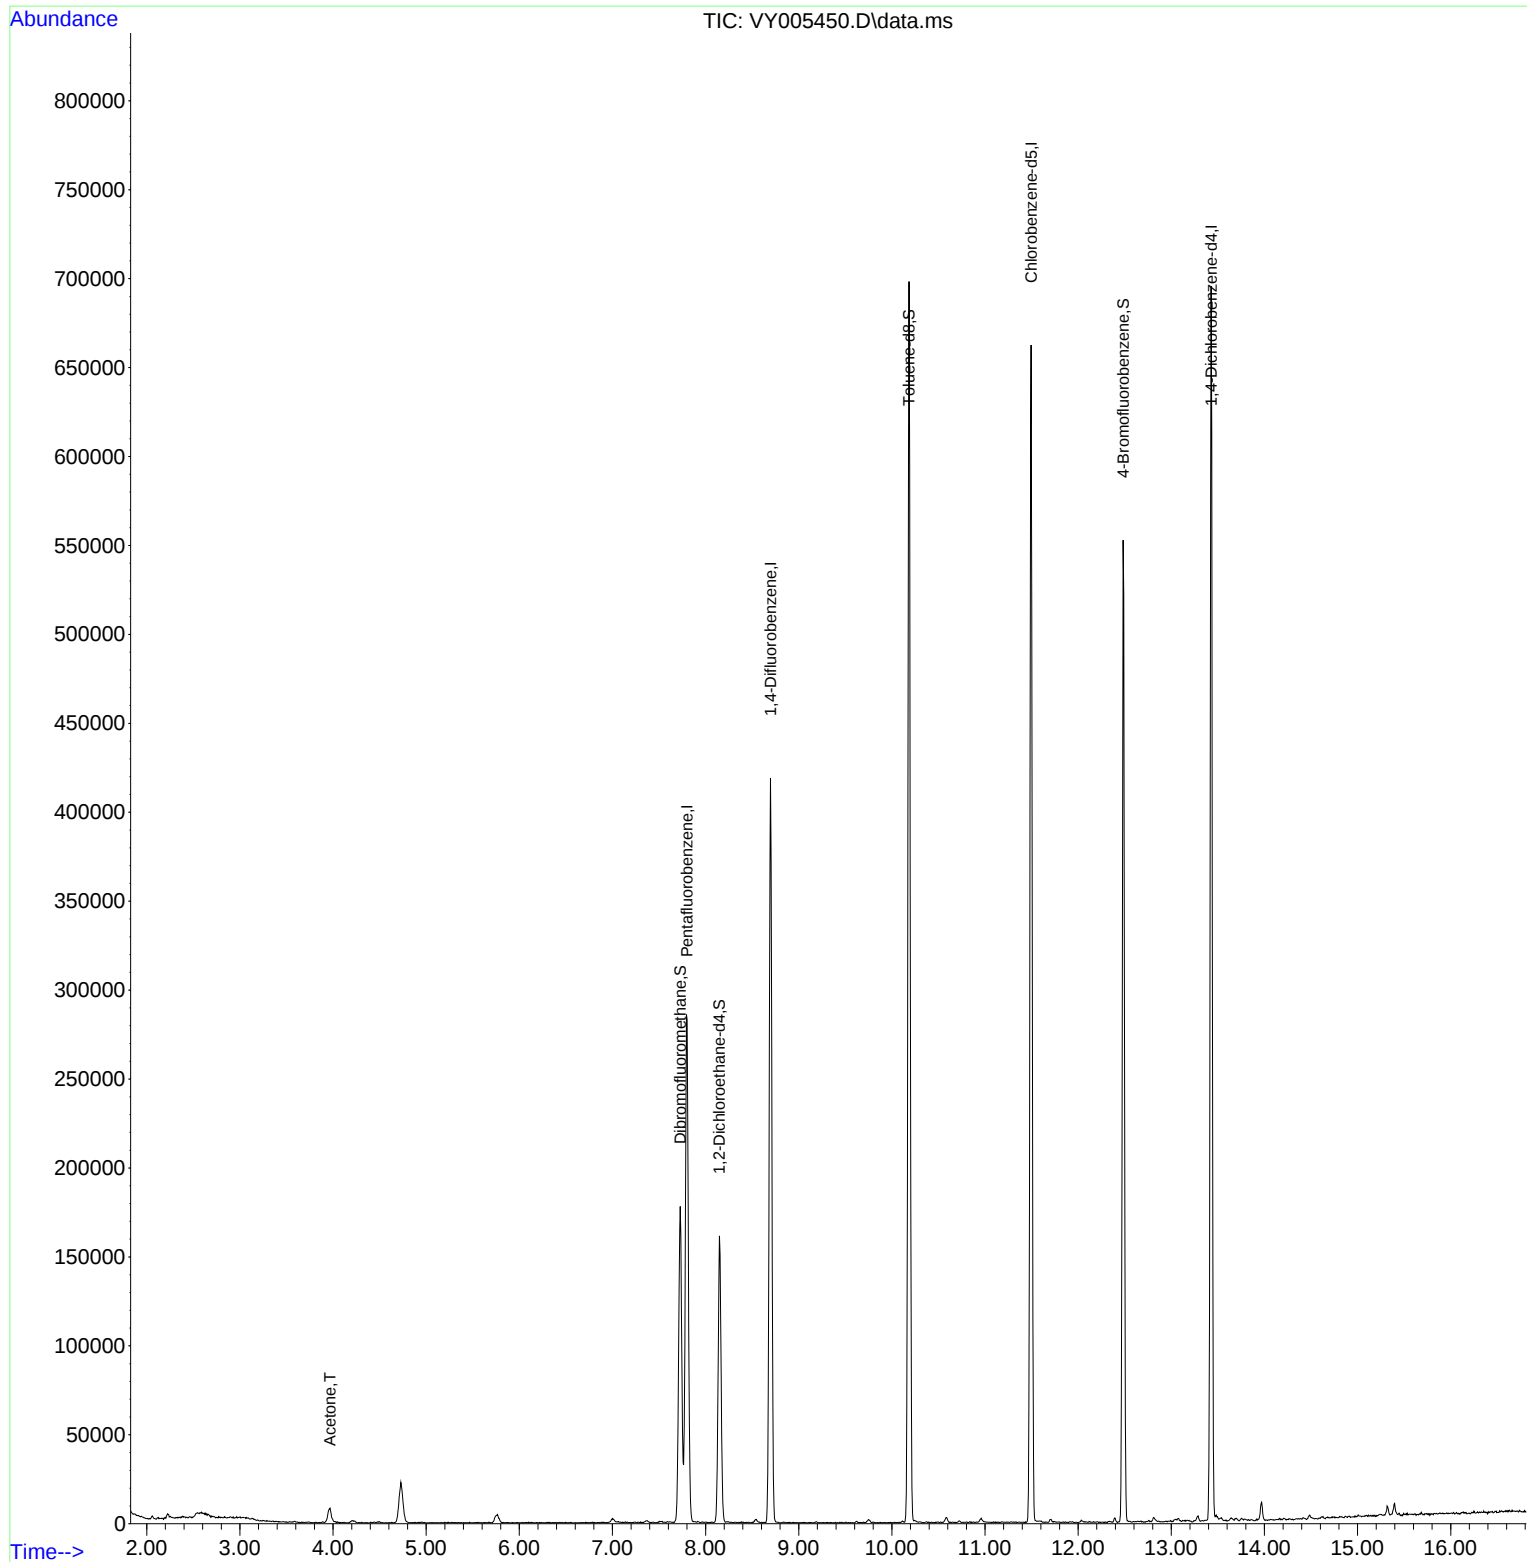


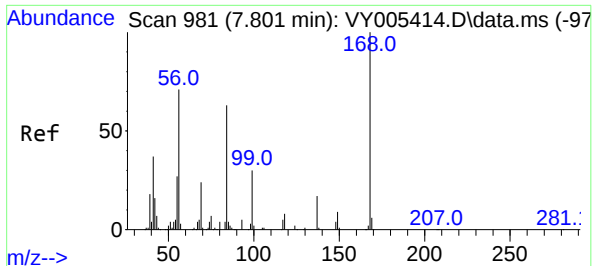

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.801 min Scan# 981
Delta R.T. 0.000 min
Lab File: VY005450.D
Acq: 26 Jul 2021 17:21




Instrument :
MSVOA_Y
ClientSampleId :
COMP-3


Tgt Ion:168 Resp: 230716
Ion Ratio Lower Upper
168 100
99 48.1 39.8 59.6

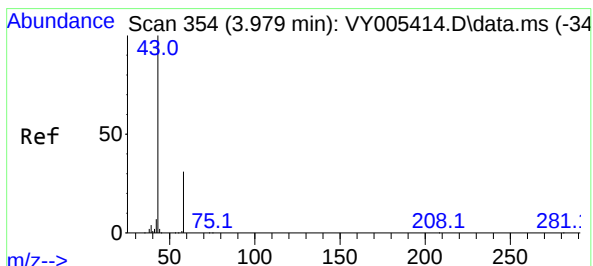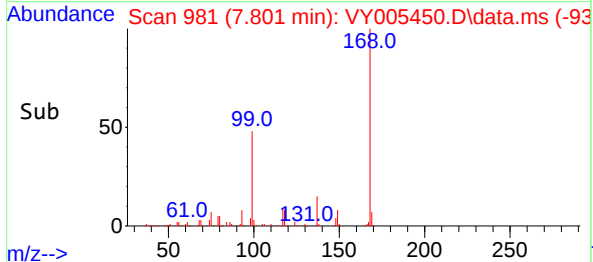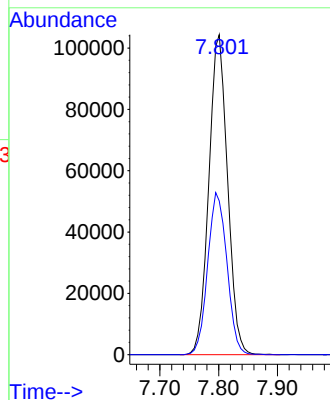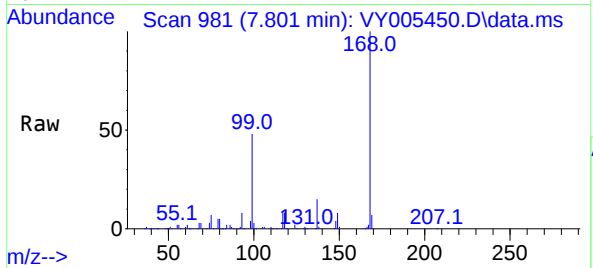

#16
Acetone
Concen: 24.202 ug/l
RT: 3.966 min Scan# 352
Delta R.T. -0.012 min
Lab File: VY005450.D
Acq: 26 Jul 2021 17:21

Tgt Ion: 43 Resp: 13623
Ion Ratio Lower Upper
43 100
58 31.8 24.5 36.7


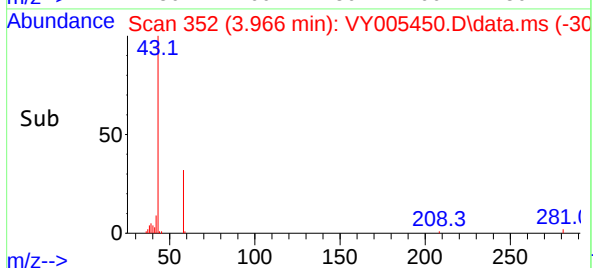
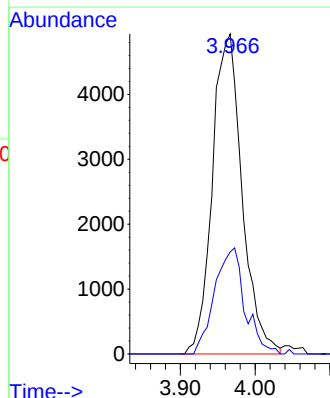
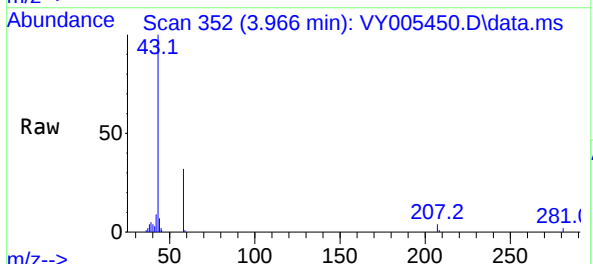


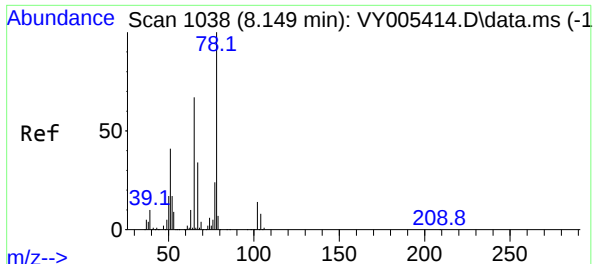

#33
1,2-Dichloroethane-d4
Concen: 52.298 ug/l
RT: 8.149 min Scan# 1038
Delta R.T. -0.000 min
Lab File: VY005450.D
Acq: 26 Jul 2021 17:21




Instrument :
MSVOA_Y
ClientSampleId :
COMP-3


Tgt Ion: 65 Resp: 128905
Ion Ratio Lower Upper
65 100
67 50.6 0.0 102.2

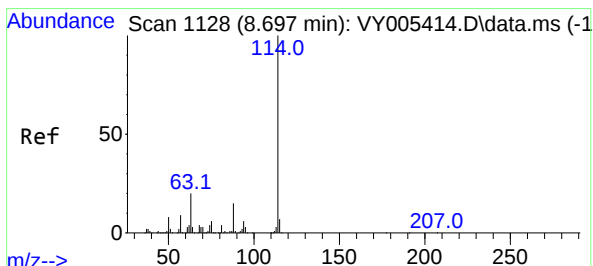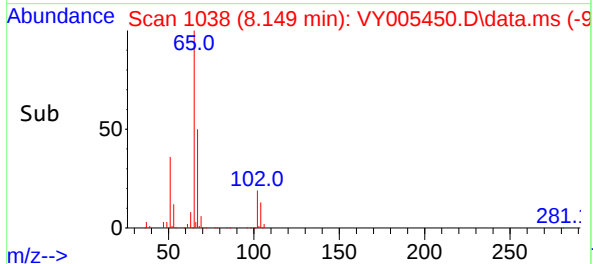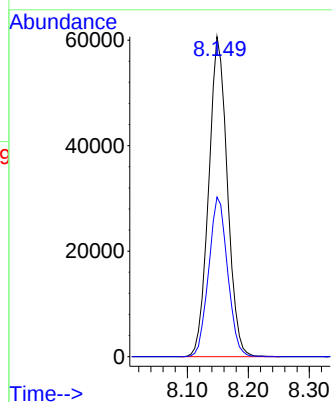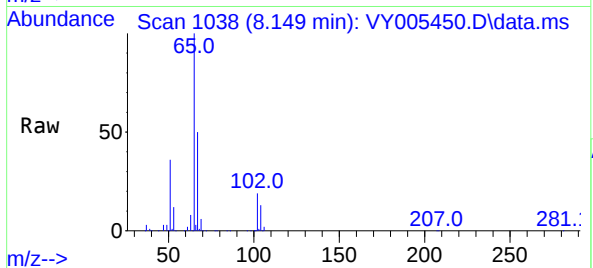

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.697 min Scan# 1128
Delta R.T. -0.000 min
Lab File: VY005450.D
Acq: 26 Jul 2021 17:21

Tgt Ion:114 Resp: 351305
Ion Ratio Lower Upper
114 100
63 20.9 0.0 39.0
88 15.7 0.0 30.8


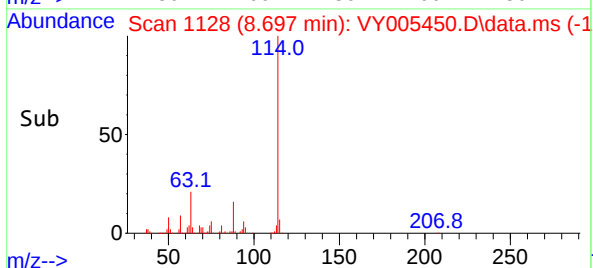
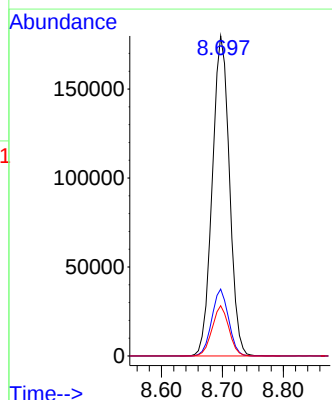
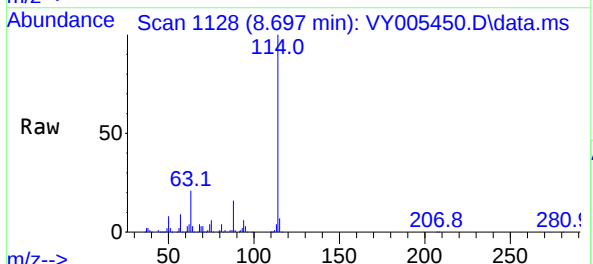


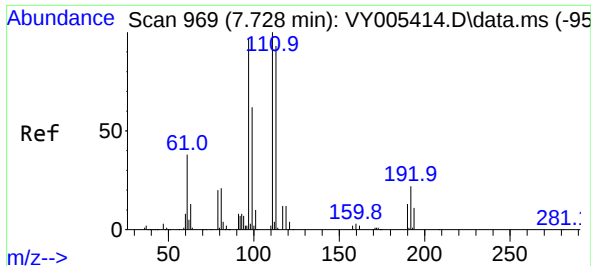

#35
Dibromofluoromethane
Concen: 59.044 ug/l
RT: 7.728 min Scan# 969
Delta R.T. -0.000 min
Lab File: VY005450.D
Acq: 26 Jul 2021 17:21




Instrument :
MSVOA_Y
ClientSampleId :
COMP-3


Tgt Ion:113 Resp: 119769
Ion Ratio Lower Upper
113 100
111 101.8 82.6 124.0
192 23.1 18.9 28.3

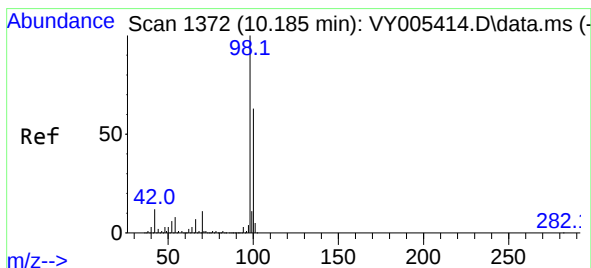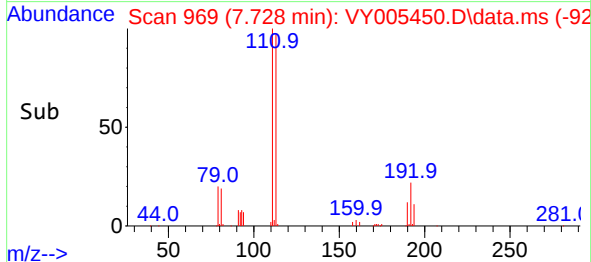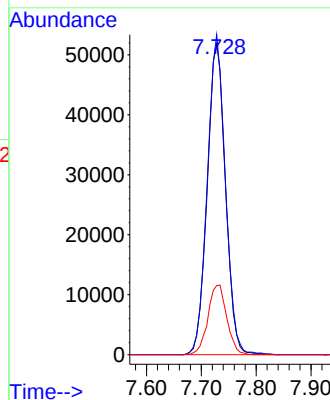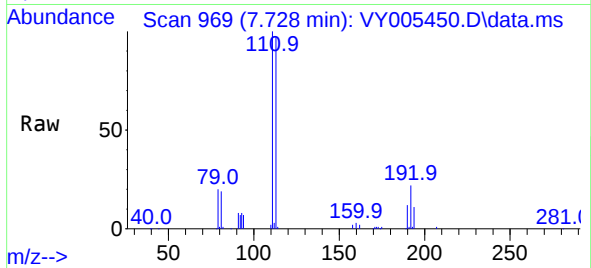

#50
Toluene-d8
Concen: 51.728 ug/l
RT: 10.185 min Scan# 1372
Delta R.T. -0.000 min
Lab File: VY005450.D
Acq: 26 Jul 2021 17:21

Tgt Ion: 98 Resp: 444730
Ion Ratio Lower Upper
98 100
100 63.6 50.9 76.3

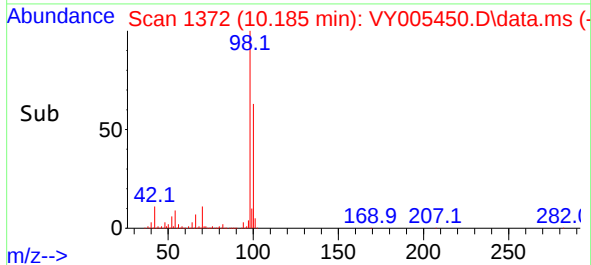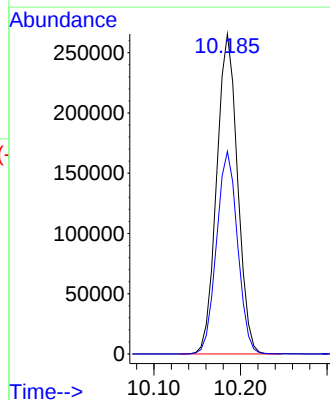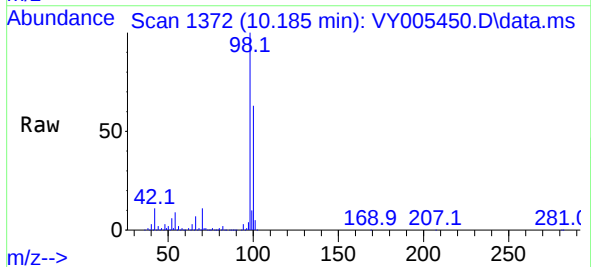




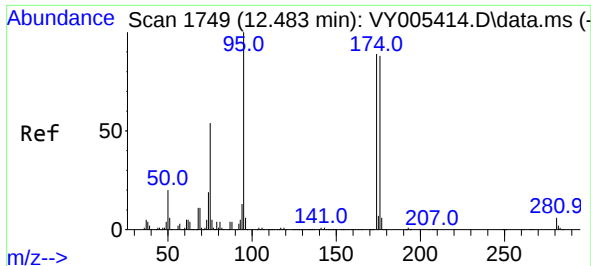


#62
4-Bromofluorobenzene
Concen: 55.014 ug/l
RT: 12.483 min Scan# 1749
Delta R.T. -0.000 min
Lab File: VY005450.D
Acq: 26 Jul 2021 17:21

Instrument :
MSVOA_Y
ClientSampleId :
COMP-3

Tgt Ion: 95 Resp: 156103




Ion	Ratio	Lower	Upper
95	100		
174	93.8	0.0	186.6
176	91.6	0.0	182.4

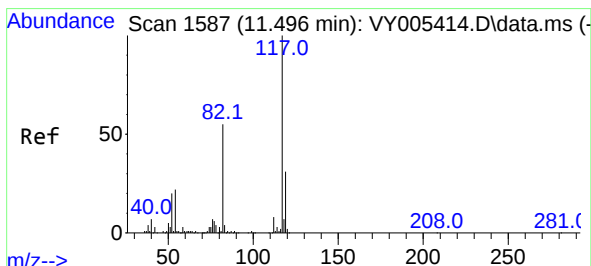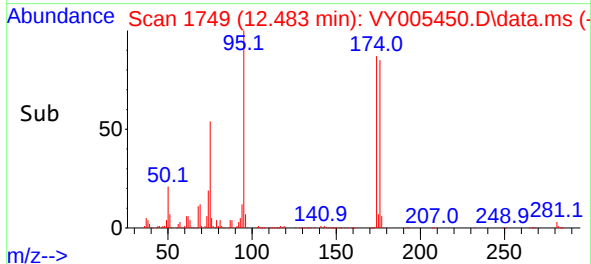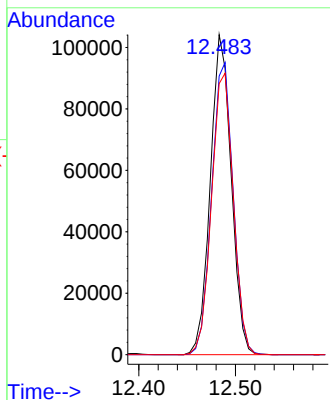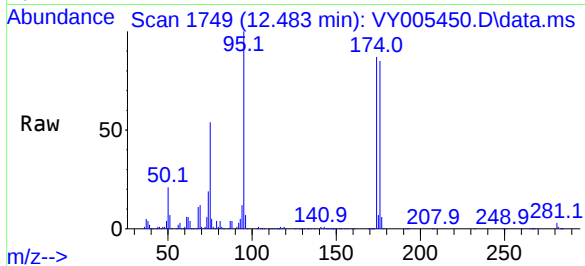


#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.496 min Scan# 1587
Delta R.T. -0.000 min
Lab File: VY005450.D
Acq: 26 Jul 2021 17:21

Tgt Ion: 117 Resp: 351967

Ion	Ratio	Lower	Upper
117	100		
82	54.4	43.8	65.6
119	32.5	24.8	37.2

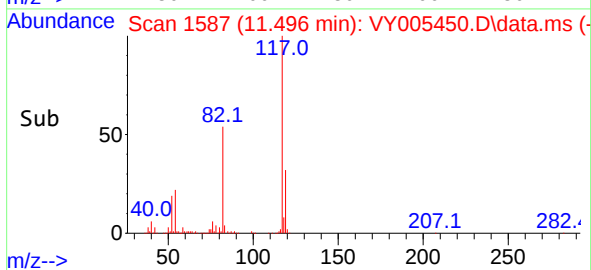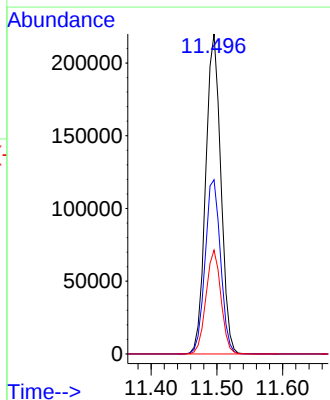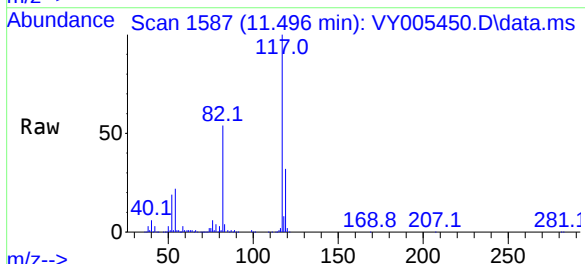

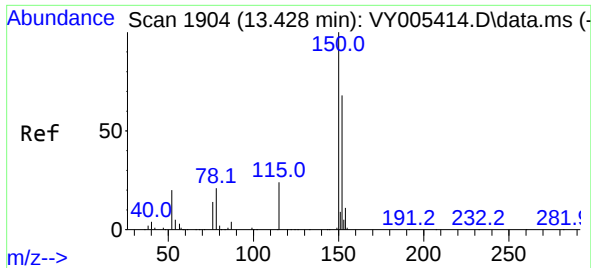

#72
 1,4-Dichlorobenzene-d4
 Concen: 50.000 ug/l
 RT: 13.428 min Scan# 1904
 Delta R.T. -0.000 min
 Lab File: VY005450.D
 Acq: 26 Jul 2021 17:21

Instrument :
 MSVOA_Y
 ClientSampleId :
 COMP-3

Tgt Ion:152 Resp: 179543
 Ion Ratio Lower Upper
 152 100
 115 54.4 27.7 83.1
 150 156.2 0.0 349.6

