
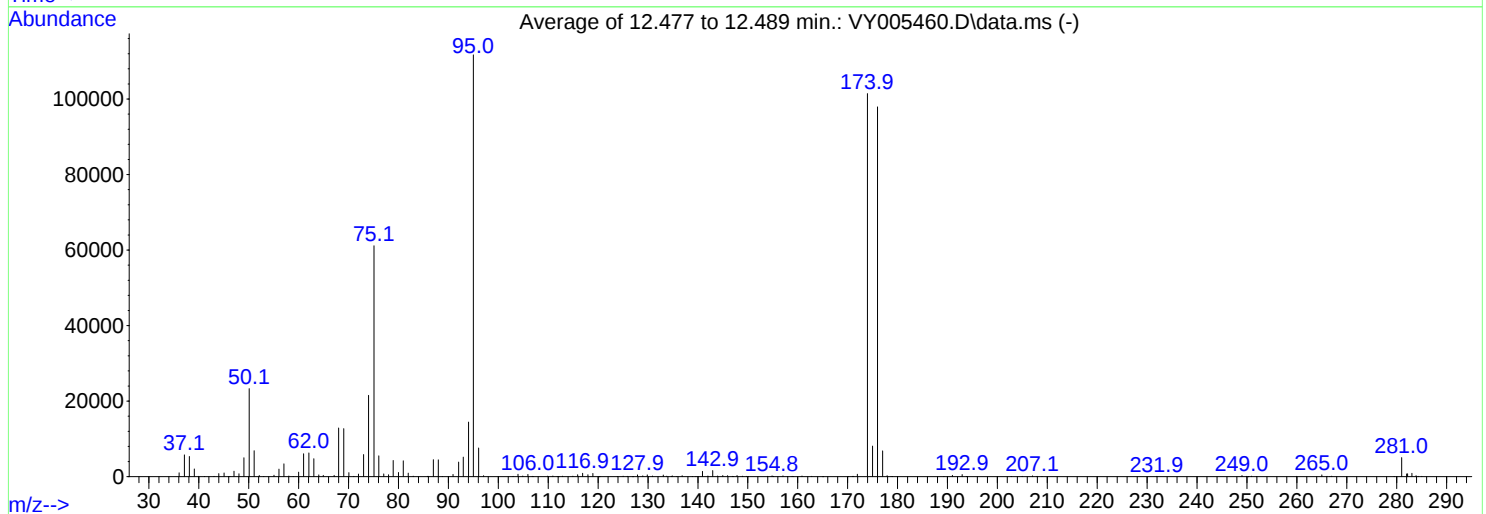


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY072721\
Data File : VY005460.D
Acq On : 27 Jul 2021 13:08
Operator : SY/MD
Sample : BFB
Misc : 5.00G/5ML/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y072221S.M
Title : SW846 8260
Last Update : Fri Jul 23 06:20:14 2021

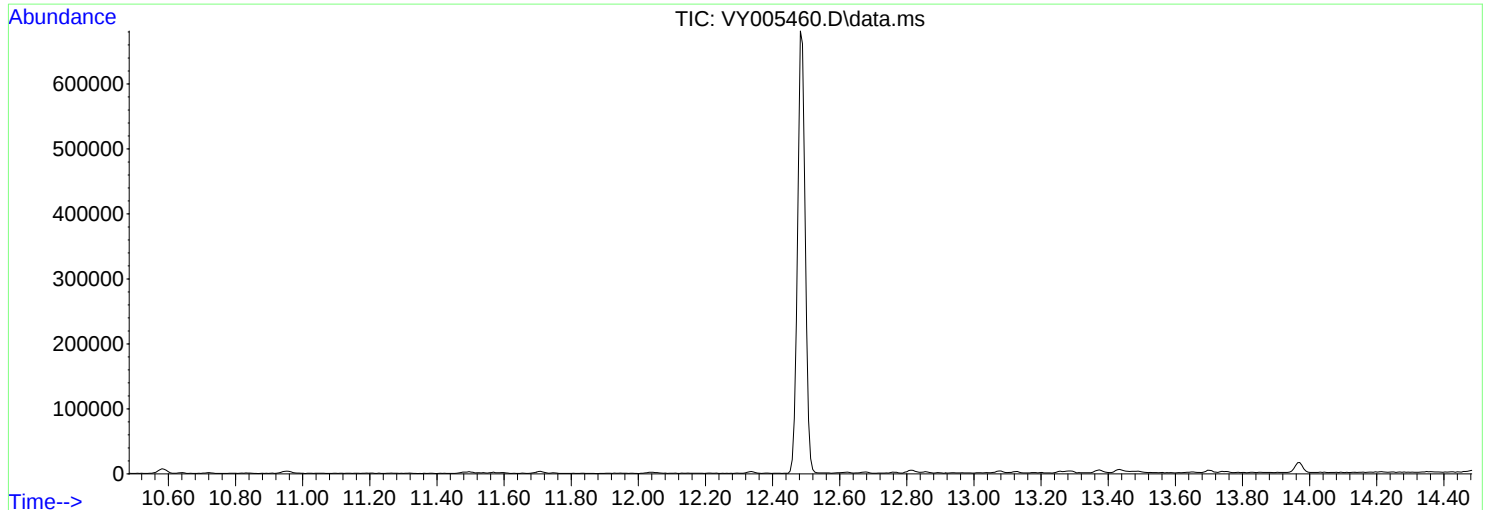

AutoFind: Scans 1748, 1749, 1750; Background Corrected with Scan 1740

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	20.9	23315	PASS
75	95	30	60	54.8	61165	PASS
95	95	100	100	100.0	111704	PASS
96	95	5	9	6.8	7584	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	90.8	101448	PASS
175	174	5	9	8.0	8095	PASS
176	174	95	101	96.5	97920	PASS
177	176	5	9	7.0	6812	PASS