


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY072722\
Data File : VY009712.D
Acq On : 27 Jul 2022 08:54
Operator : KP/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y072622S.M
Title : SW846 8260
Last Update : Wed Jul 27 04:24:58 2022

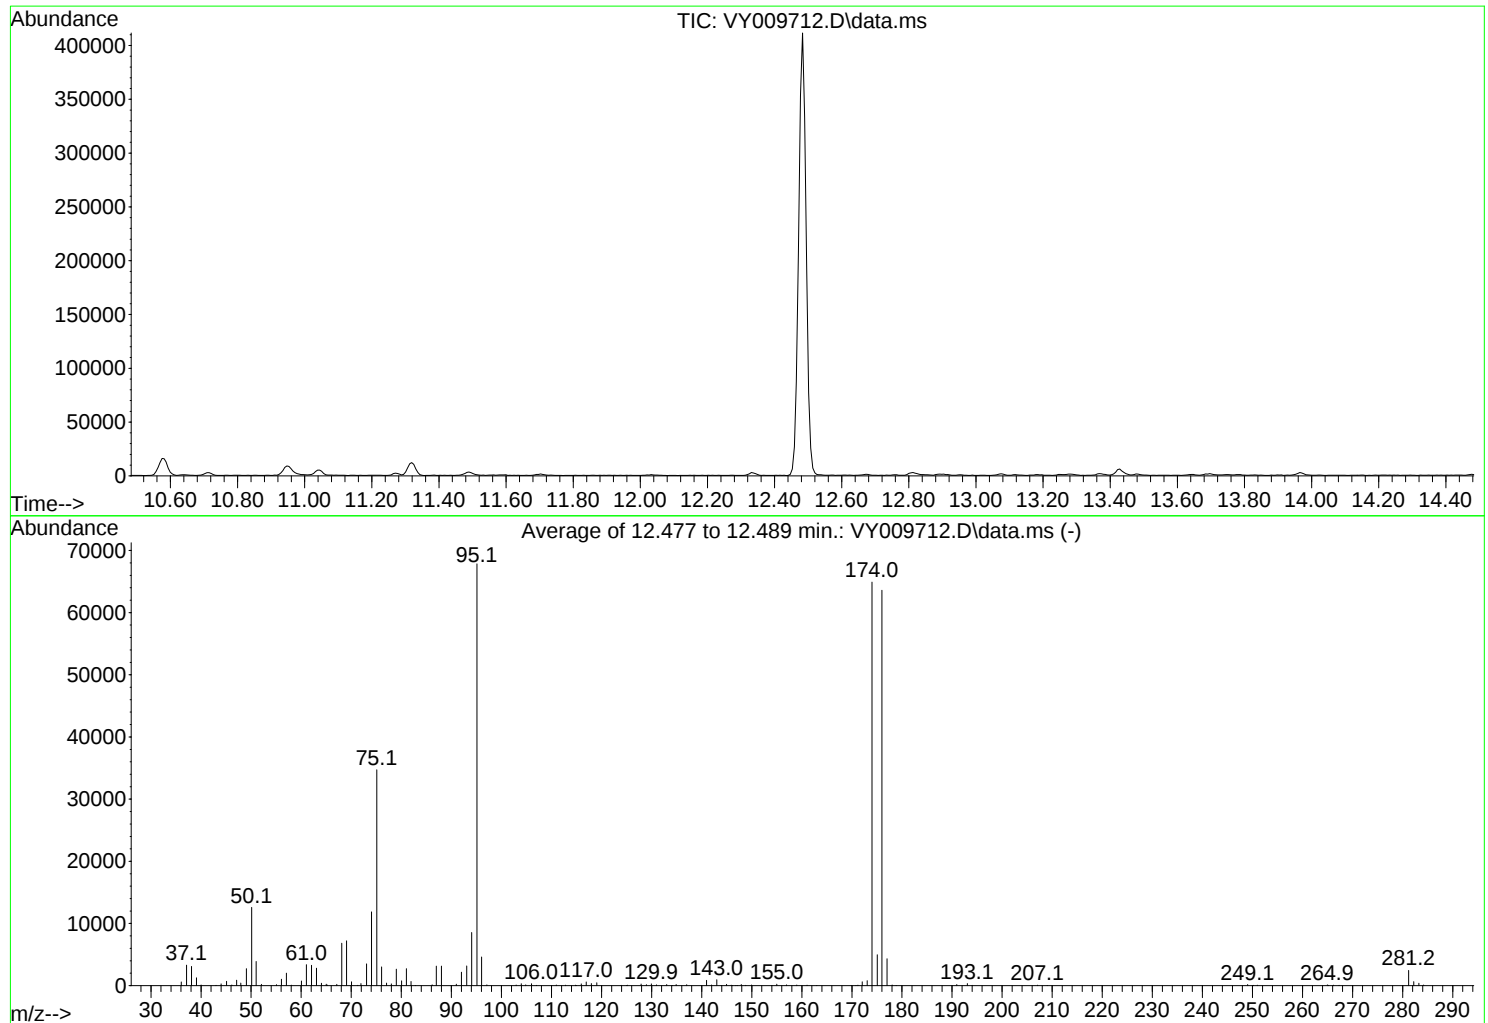

AutoFind: Scans 1748, 1749, 1750; Background Corrected with Scan 1740

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.5	12583	PASS
75	95	30	60	51.2	34712	PASS
95	95	100	100	100.0	67848	PASS
96	95	5	9	6.8	4610	PASS
173	174	0.00	2	1.2	805	PASS
174	95	50	100	95.7	64923	PASS
175	174	5	9	7.7	4974	PASS
176	174	95	101	98.0	63597	PASS
177	176	5	9	6.8	4313	PASS