
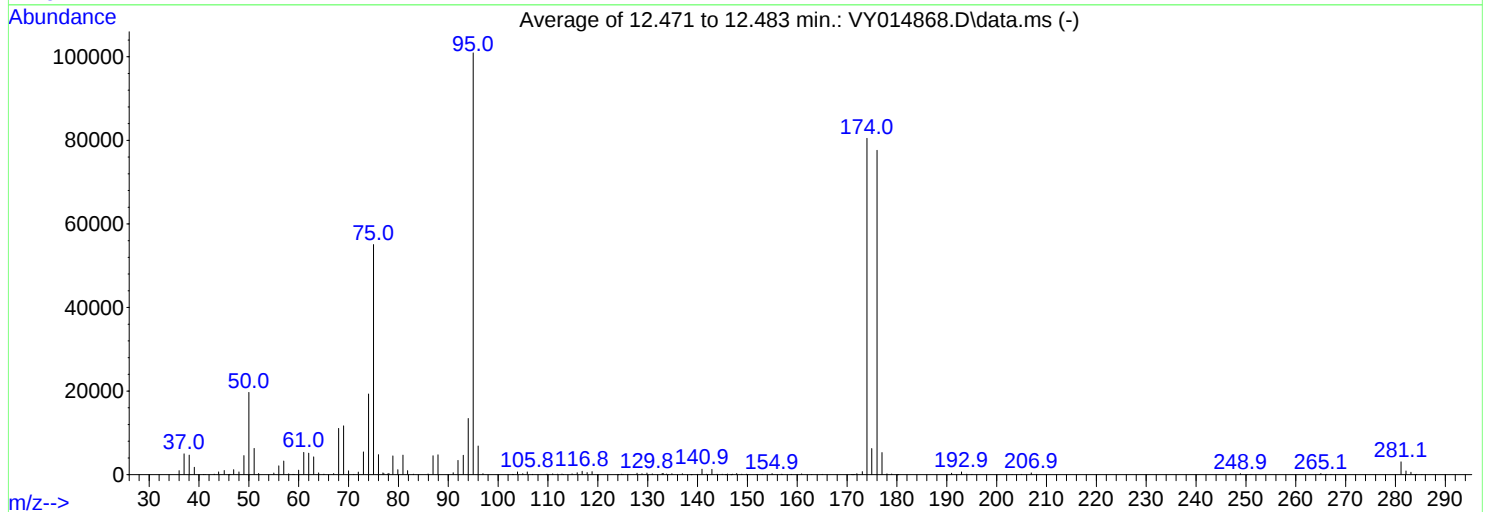


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY072723\
Data File : VY014868.D
Acq On : 27 Jul 2023 08:53
Operator : SY/MD
Sample : BFB
Misc : 5.02g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y071323S.M
Title : SW846 8260
Last Update : Fri Jul 14 02:09:50 2023

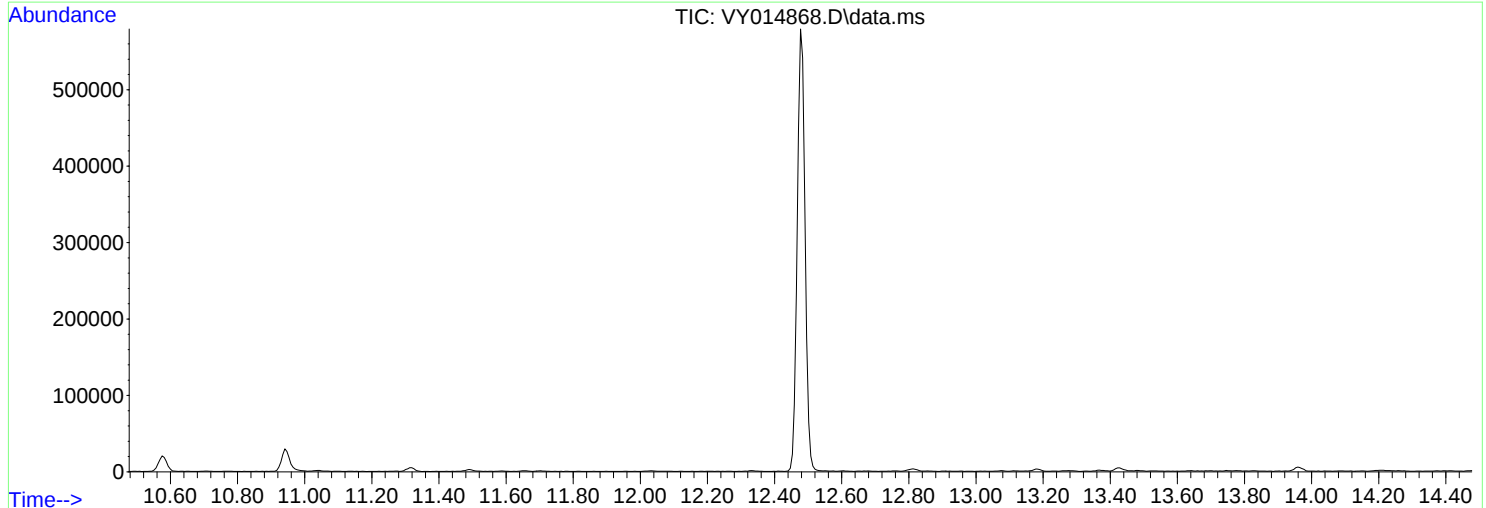

AutoFind: Scans 1747, 1748, 1749; Background Corrected with Scan 1739

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	19.5	19664	PASS
75	95	30	60	54.6	55072	PASS
95	95	100	100	100.0	100941	PASS
96	95	5	9	6.8	6849	PASS
173	174	0.00	2	0.9	734	PASS
174	95	50	100	79.7	80480	PASS
175	174	5	9	7.7	6236	PASS
176	174	95	101	96.5	77632	PASS
177	176	5	9	6.8	5290	PASS