


Data Path : Z:\VOASRV\HPCHEM1\MSVOA_Y\DATA\VY072820\
Data File : VY003369.D
Acq On : 28 Jul 2020 09:24
Operator : SY/MD
Sample : BFB
Misc : 5.00G/5ML/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_Y\METHODS\82Y071020S.M
Title : SW846 8260
Last Update : Fri Jul 10 13:18:03 2020

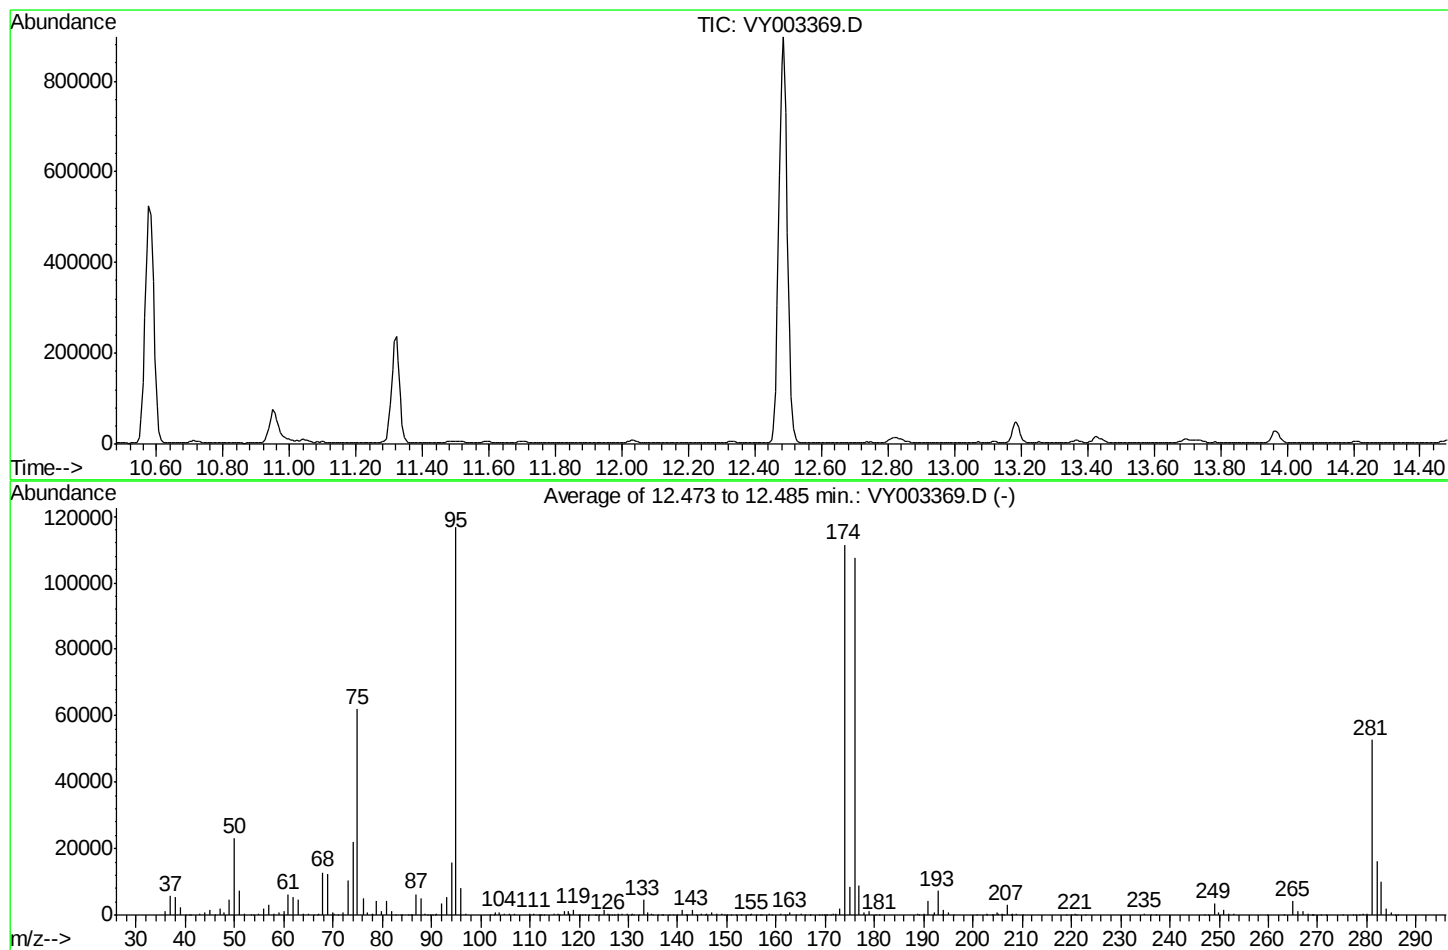

AutoFind: Scans 1761, 1762, 1763; Background Corrected with Scan 1753

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.7	23050	PASS
75	95	30	60	53.0	61896	PASS
95	95	100	100	100.0	116714	PASS
96	95	5	9	6.8	7970	PASS
173	174	0.00	2	1.6	1825	PASS
174	95	50	100	95.4	111394	PASS
175	174	5	9	7.8	8655	PASS
176	174	95	101	96.4	107344	PASS
177	176	5	9	8.2	8801	PASS