

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY072822\
 Data File : VY009758.D
 Acq On : 28 Jul 2022 17:59
 Operator : KP/MD
 Sample : N3895-02
 Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 RVE-40

Quant Time: Jul 29 02:57:52 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y072622S.M
 Quant Title : SW846 8260
 QLast Update : Wed Jul 27 04:24:58 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.783	168	159187	50.000	ug/l	# 0.00
34) 1,4-Difluorobenzene	8.685	114	286950	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.489	117	281086	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.422	152	130933	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.130	65	64672	62.308	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	124.620%
35) Dibromofluoromethane	7.710	113	61902	39.664	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	79.320%
50) Toluene-d8	10.173	98	245798	54.457	ug/l	0.00
Spiked Amount	50.000	Range	78 - 125	Recovery	=	108.920%
62) 4-Bromofluorobenzene	12.477	95	68353	33.031	ug/l	0.00
Spiked Amount	50.000	Range	50 - 146	Recovery	=	66.060%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY072822\
Data File : VY009758.D
Acq On : 28 Jul 2022 17:59
Operator : KP/MD
Sample : N3895-02
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
RVE-40

Quant Time: Jul 29 02:57:52 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y072622S.M
Quant Title : SW846 8260
QLast Update : Wed Jul 27 04:24:58 2022
Response via : Initial Calibration




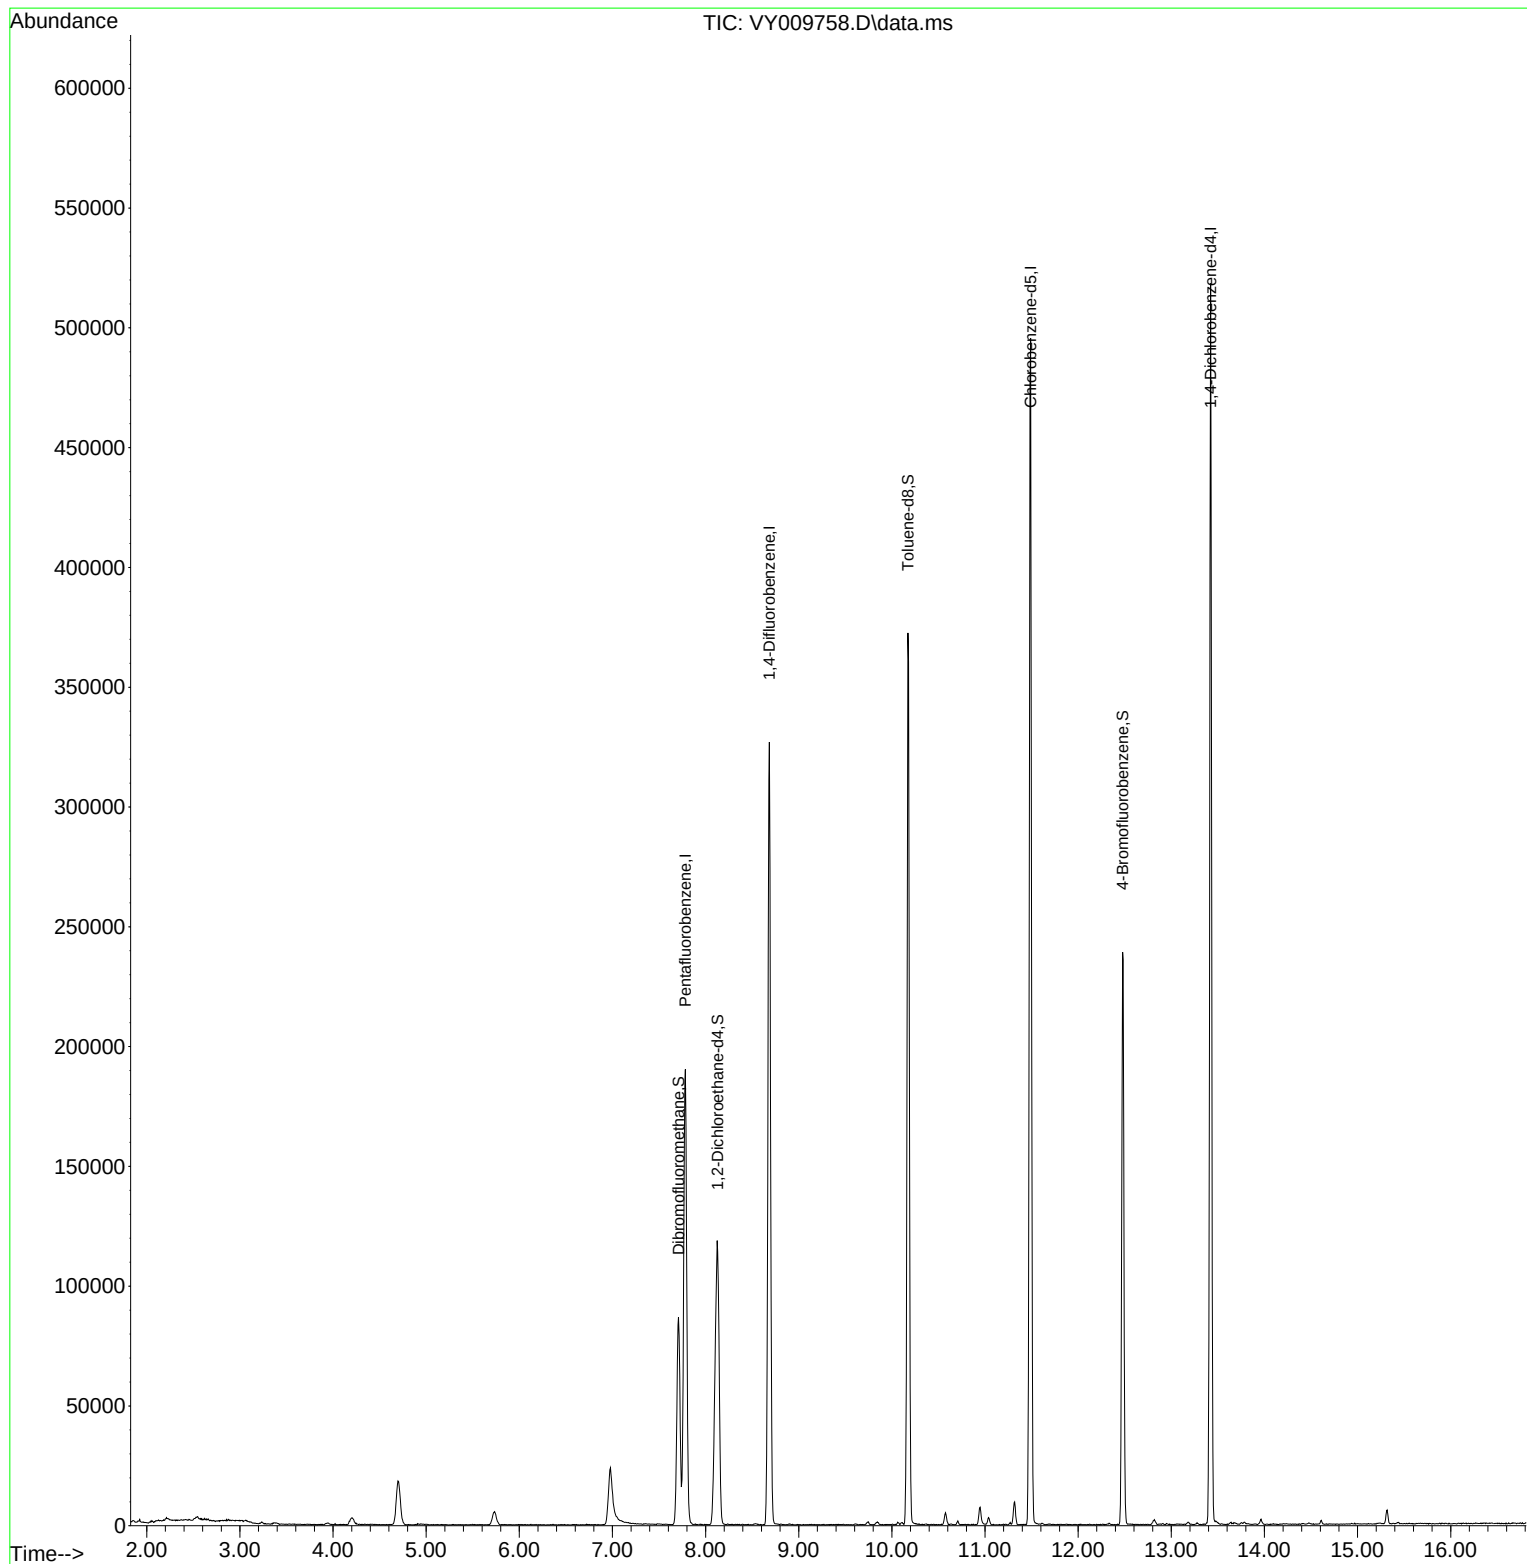


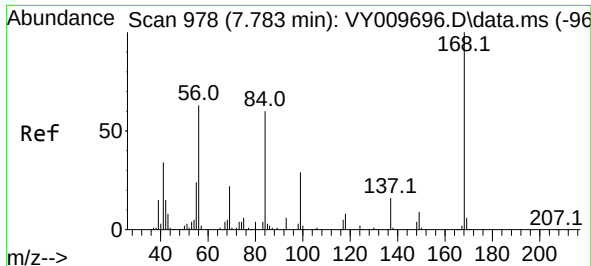

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.783 min Scan# 91
Delta R.T. -0.000 min
Lab File: VY009758.D
Acq: 28 Jul 2022 17:59




Instrument :
MSVOA_Y
ClientSampleId :
RVE-40


Tgt Ion:168 Resp: 159187
Ion Ratio Lower Upper
168 100
99 46.1 46.9 70.3#

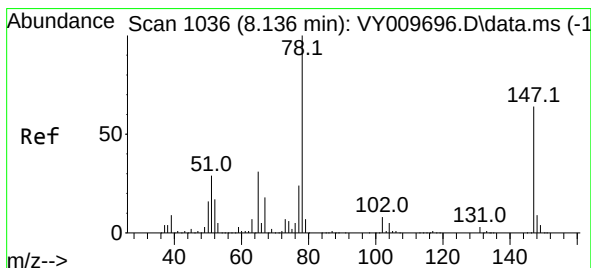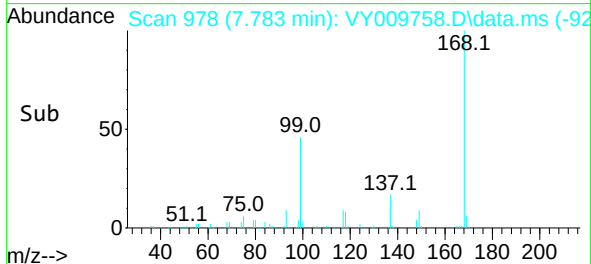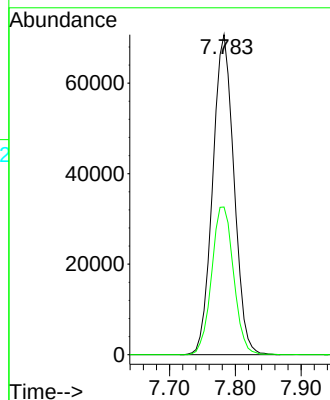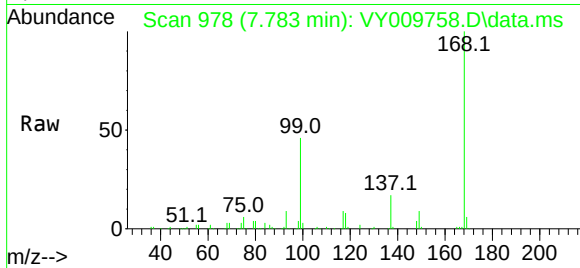

#33
1,2-Dichloroethane-d4
Concen: 62.308 ug/l
RT: 8.130 min Scan# 1035
Delta R.T. -0.006 min
Lab File: VY009758.D
Acq: 28 Jul 2022 17:59

Tgt Ion: 65 Resp: 64672
Ion Ratio Lower Upper
65 100
67 54.5 0.0 99.4

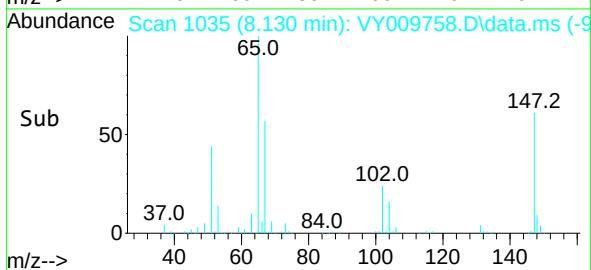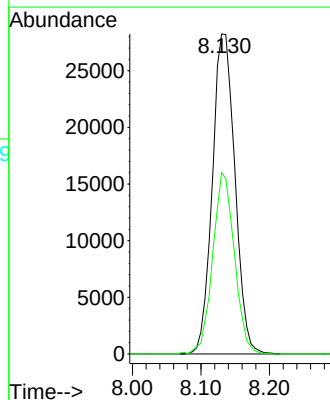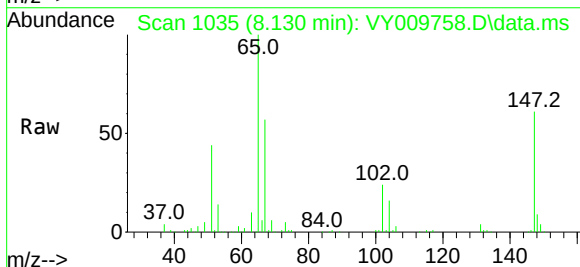

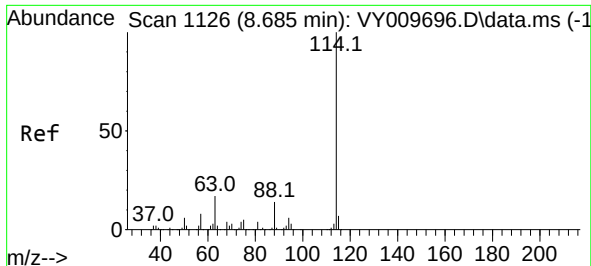

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.685 min Scan# 1126

Delta R.T. -0.000 min

Lab File: VY009758.D

Acq: 28 Jul 2022 17:59

Instrument :

MSVOA_Y

ClientSampleId :

RVE-40





Tgt Ion:114 Resp: 286950

Ion Ratio Lower Upper

114 100

63 17.9 0.0 43.2

88 13.7 0.0 31.8

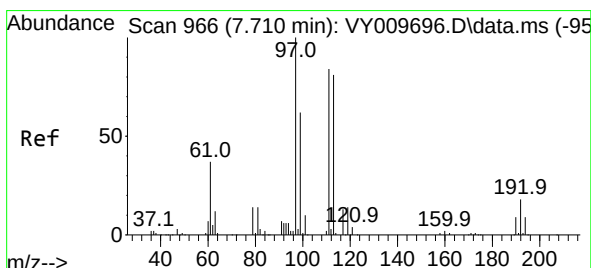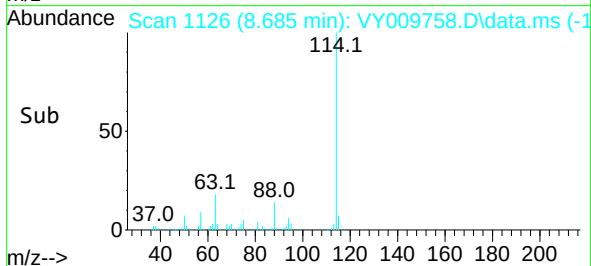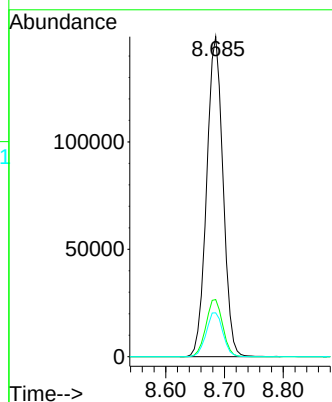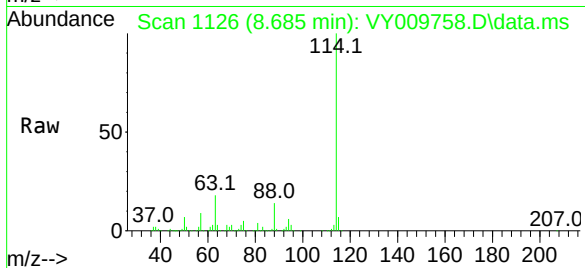

#35

Dibromofluoromethane

Concen: 39.664 ug/l

RT: 7.710 min Scan# 966

Delta R.T. -0.000 min

Lab File: VY009758.D

Acq: 28 Jul 2022 17:59




Tgt Ion:113 Resp: 61902


Ion Ratio Lower Upper

113 100

111 102.7 82.6 124.0

192 22.1 17.6 26.4


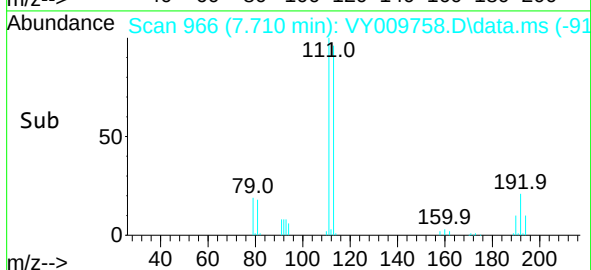
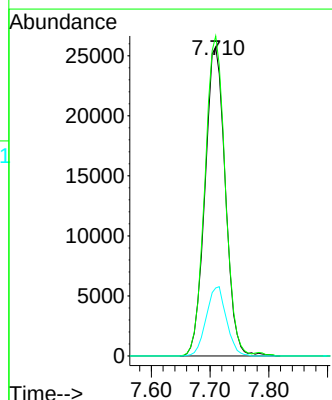
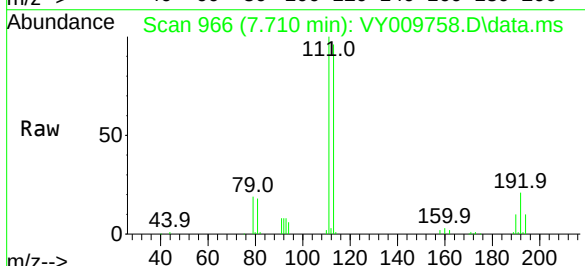


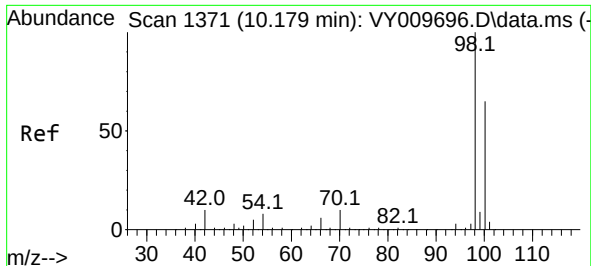

#50
Toluene-d8
Concen: 54.457 ug/l
RT: 10.173 min Scan# 11
Delta R.T. -0.006 min
Lab File: VY009758.D
Acq: 28 Jul 2022 17:59




Instrument :
MSVOA_Y
ClientSampleId :
RVE-40


Tgt Ion: 98 Resp: 245798
Ion Ratio Lower Upper
98 100
100 64.5 50.2 75.2

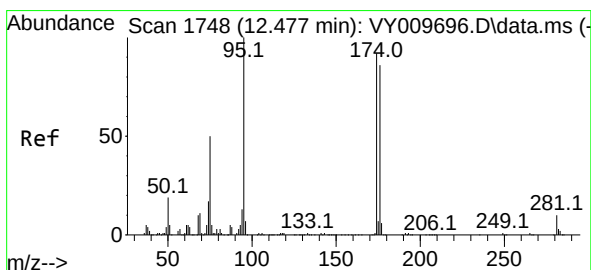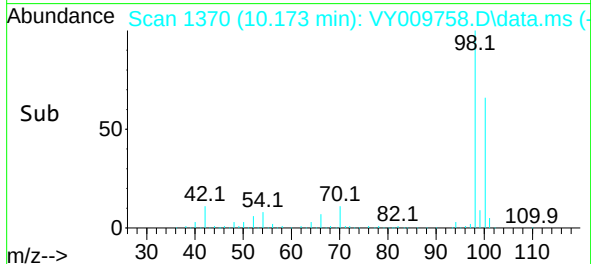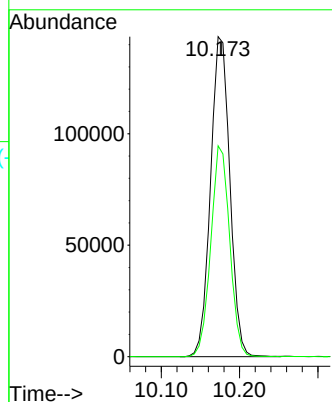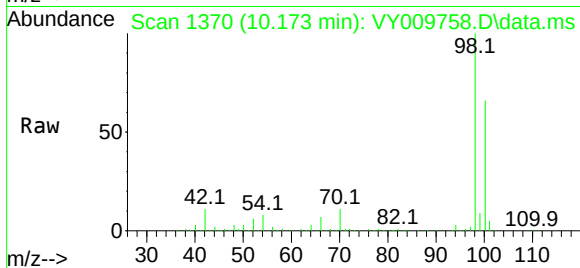

#62
4-Bromofluorobenzene
Concen: 33.031 ug/l
RT: 12.477 min Scan# 1748
Delta R.T. 0.000 min
Lab File: VY009758.D
Acq: 28 Jul 2022 17:59

Tgt Ion: 95 Resp: 68353
Ion Ratio Lower Upper
95 100
174 99.0 0.0 177.0
176 94.1 0.0 175.8


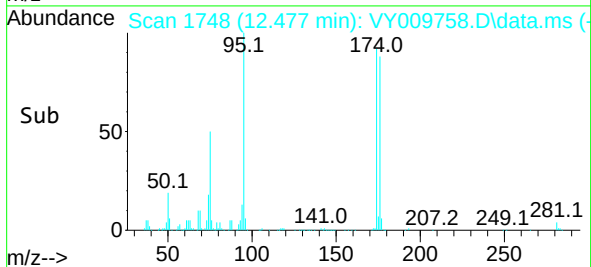
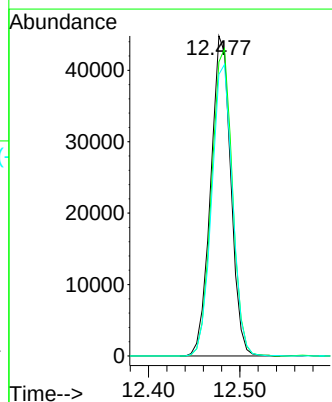
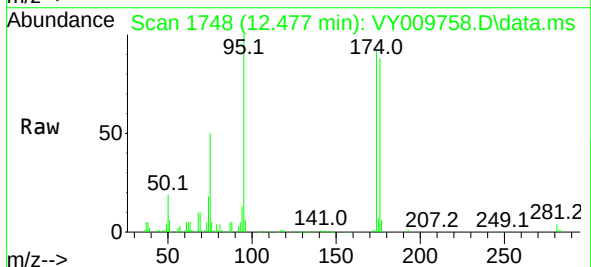


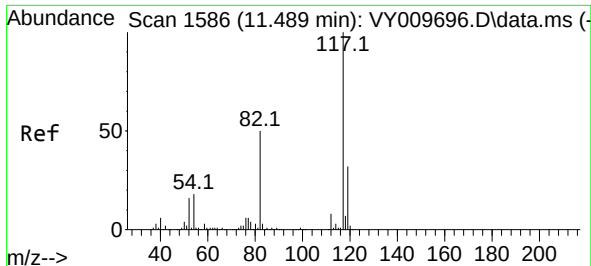

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.489 min Scan# 117
Delta R.T. 0.000 min
Lab File: VY009758.D
Acq: 28 Jul 2022 17:59

Instrument :
MSVOA_Y
ClientSampleId :
RVE-40

Tgt Ion:117 Resp: 281086
Ion Ratio Lower Upper
117 100
82 49.6 43.0 64.4
119 32.0 25.4 38.0

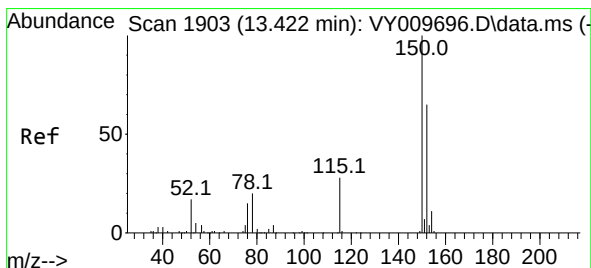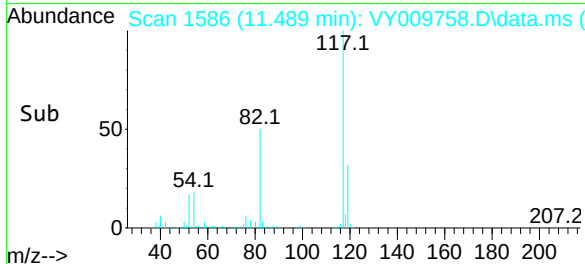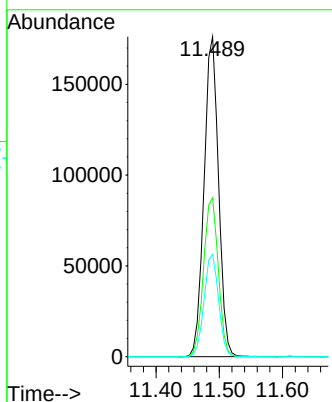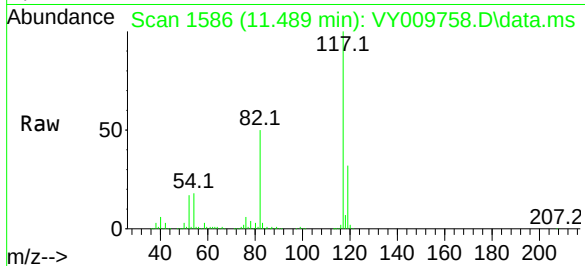

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.422 min Scan# 1903
Delta R.T. -0.000 min
Lab File: VY009758.D
Acq: 28 Jul 2022 17:59

Tgt Ion:152 Resp: 130933
Ion Ratio Lower Upper
152 100
115 54.0 28.2 84.7
150 156.7 0.0 347.6

