


Data Path : Z:\voasrv\HPCHEM1\MSVOA\_Y\Data\VY072822\  
 Data File : VY009737.D  
 Acq On : 28 Jul 2022 08:57  
 Operator : KP/MD  
 Sample : BFB  
 Misc : 5.00g/5.0mL/MSVOA\_Y/SOIL  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 MSVOA\_Y  
 ClientSampleId :  
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA\_Y\methods\82Y072622S.M  
 Title : SW846 8260  
 Last Update : Wed Jul 27 04:24:58 2022

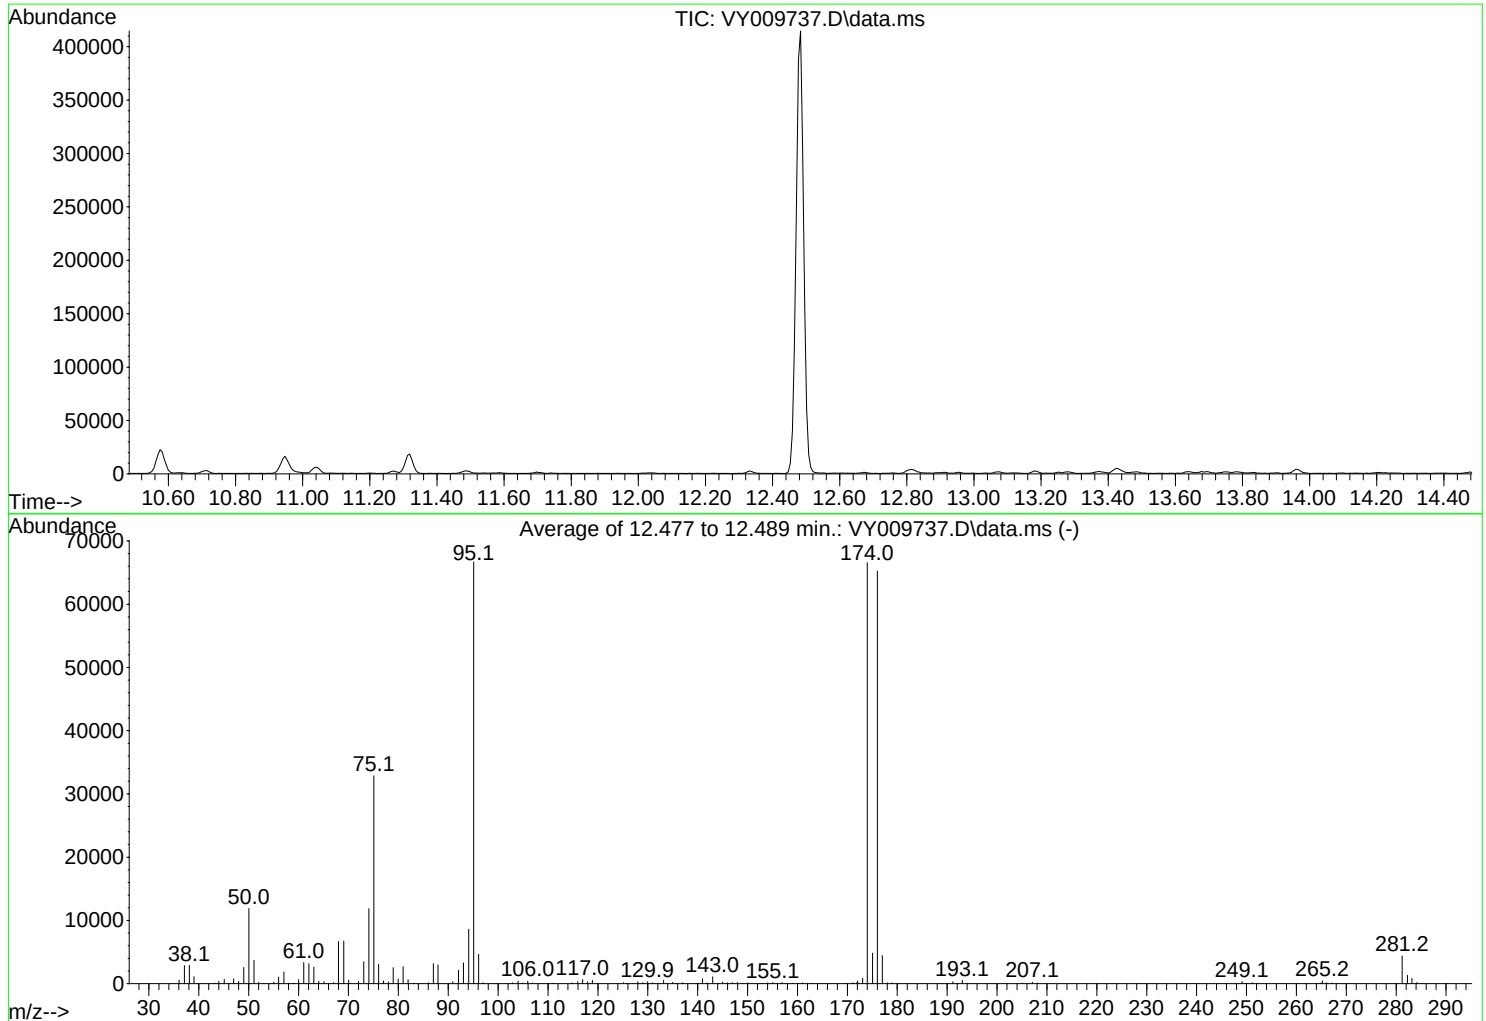

AutoFind: Scans 1748, 1749, 1750; Background Corrected with Scan 1740

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 50             | 95              | 15              | 40              | 17.8         | 11882      | PASS                |
| 75             | 95              | 30              | 60              | 49.3         | 32859      | PASS                |
| 95             | 95              | 100             | 100             | 100.0        | 66699      | PASS                |
| 96             | 95              | 5               | 9               | 6.9          | 4632       | PASS                |
| 173            | 174             | 0.00            | 2               | 1.2          | 832        | PASS                |
| 174            | 95              | 50              | 100             | 99.8         | 66579      | PASS                |
| 175            | 174             | 5               | 9               | 7.2          | 4823       | PASS                |
| 176            | 174             | 95              | 101             | 98.0         | 65240      | PASS                |
| 177            | 176             | 5               | 9               | 6.8          | 4435       | PASS                |