
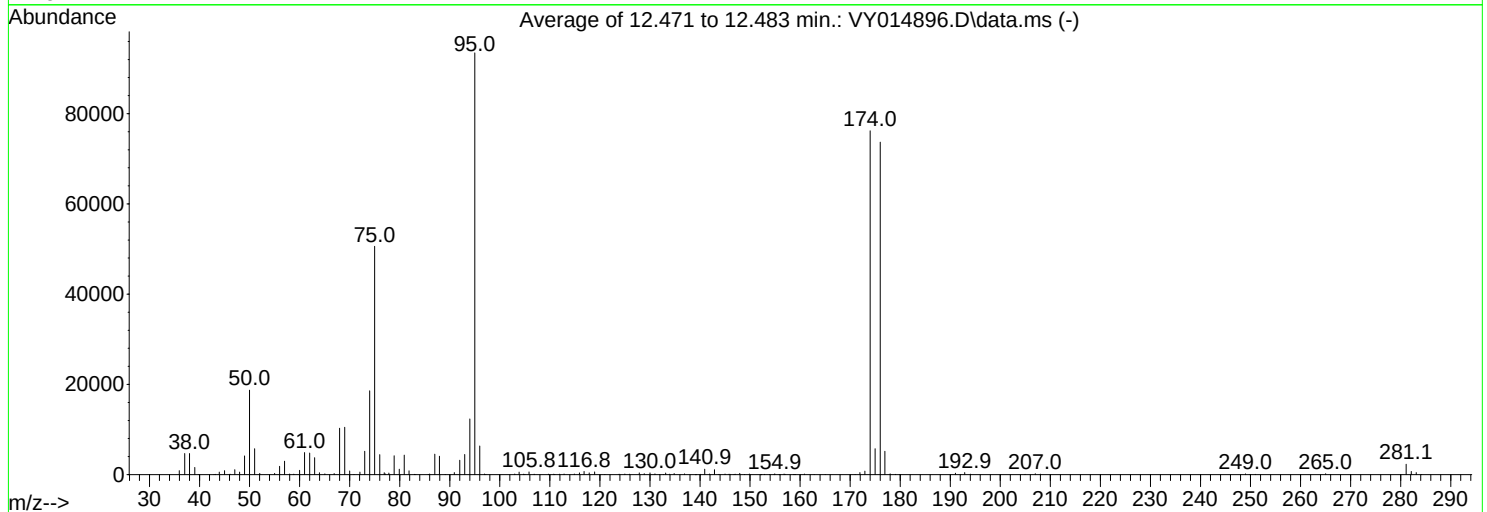


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY072823\
 Data File : VY014896.D
 Acq On : 28 Jul 2023 08:47
 Operator : SY/MD
 Sample : BFB
 Misc : 5.02g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y071323S.M
 Title : SW846 8260
 Last Update : Fri Jul 14 02:09:50 2023

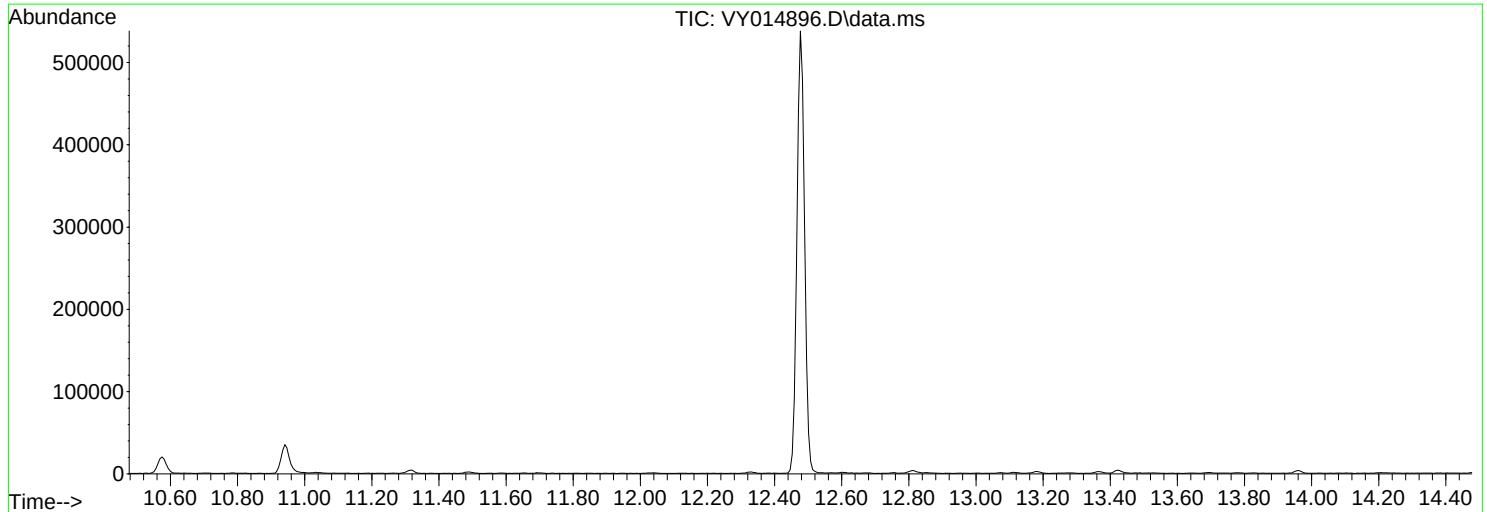

AutoFind: Scans 1747, 1748, 1749; Background Corrected with Scan 1739

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.0	18709	PASS
75	95	30	60	54.1	50595	PASS
95	95	100	100	100.0	93485	PASS
96	95	5	9	6.8	6343	PASS
173	174	0.00	2	1.0	776	PASS
174	95	50	100	81.5	76227	PASS
175	174	5	9	7.5	5746	PASS
176	174	95	101	96.7	73699	PASS
177	176	5	9	7.1	5199	PASS