

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY072922\
 Data File : VY009770.D
 Acq On : 29 Jul 2022 14:18
 Operator : KP/MD
 Sample : N3930-08
 Misc : 2.49g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 RVE-100

Quant Time: Aug 01 01:12:51 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y072622S.M
 Quant Title : SW846 8260
 QLast Update : Wed Jul 27 04:24:58 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.783	168	148965	50.000	ug/l	# 0.00
34) 1,4-Difluorobenzene	8.685	114	258879	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.489	117	253530	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.422	152	118179	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.136	65	63412	65.561	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	131.120%
35) Dibromofluoromethane	7.710	113	61231	43.489	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	86.980%
50) Toluene-d8	10.179	98	225010	55.325	ug/l	0.00
Spiked Amount	50.000	Range	78 - 125	Recovery	=	110.660%
62) 4-Bromofluorobenzene	12.477	95	70032	37.511	ug/l	0.00
Spiked Amount	50.000	Range	50 - 146	Recovery	=	75.020%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY072922\
Data File : VY009770.D
Acq On : 29 Jul 2022 14:18
Operator : KP/MD
Sample : N3930-08
Misc : 2.49g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
RVE-100

Quant Time: Aug 01 01:12:51 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y072622S.M
Quant Title : SW846 8260
QLast Update : Wed Jul 27 04:24:58 2022
Response via : Initial Calibration




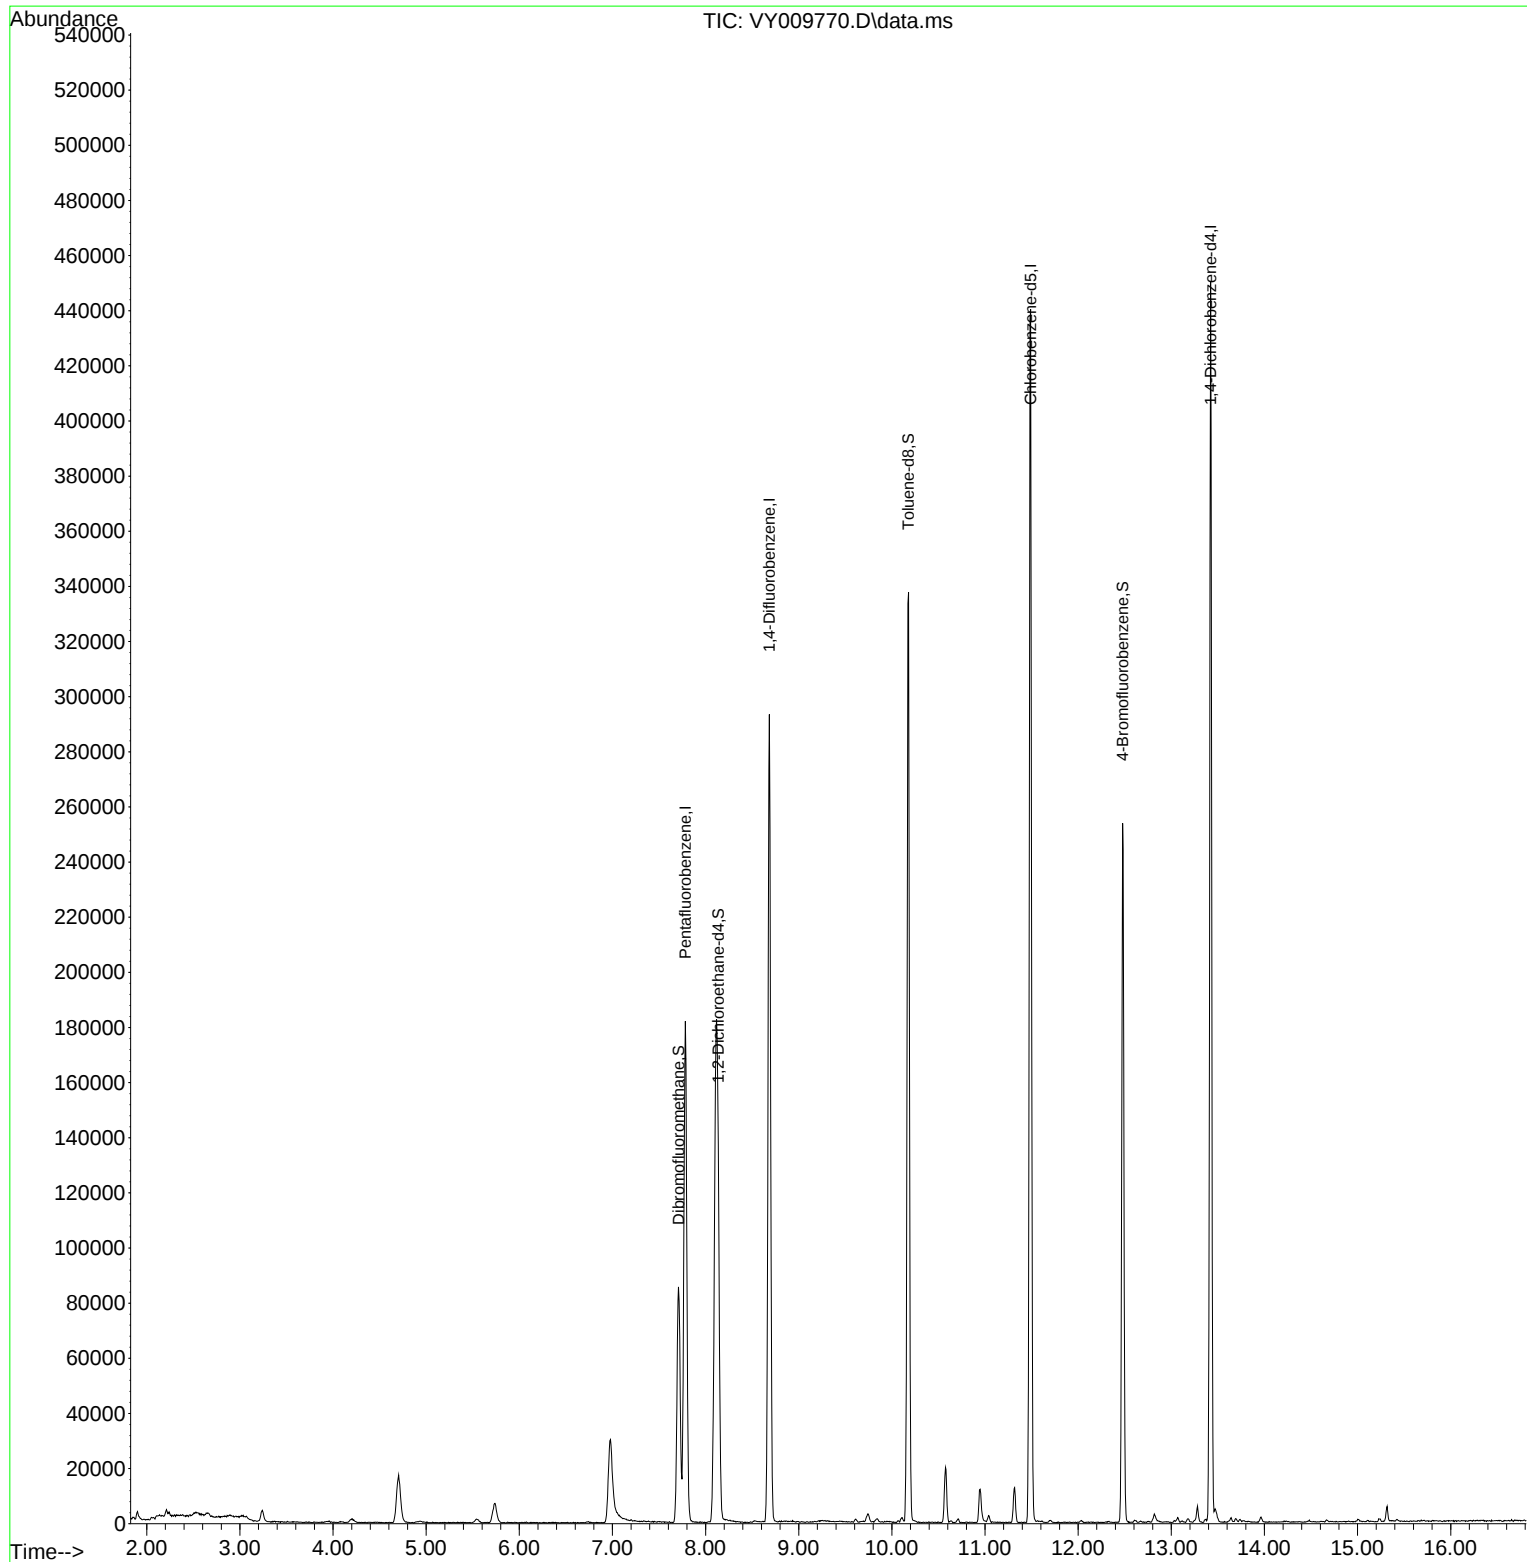


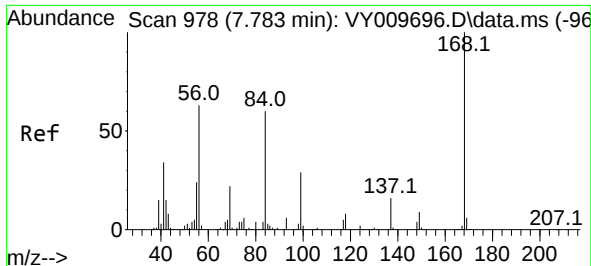

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.783 min Scan# 91
Delta R.T. -0.000 min
Lab File: VY009770.D
Acq: 29 Jul 2022 14:18




Instrument :
MSVOA_Y
ClientSampleId :
RVE-100


Tgt Ion:168 Resp: 148965
Ion Ratio Lower Upper
168 100
99 46.0 46.9 70.3#

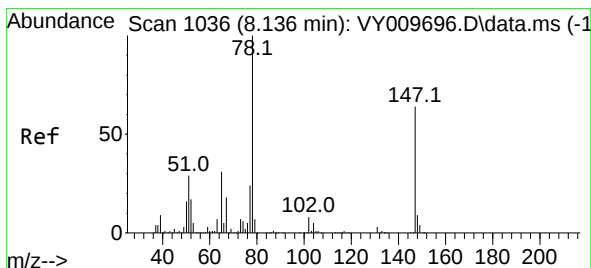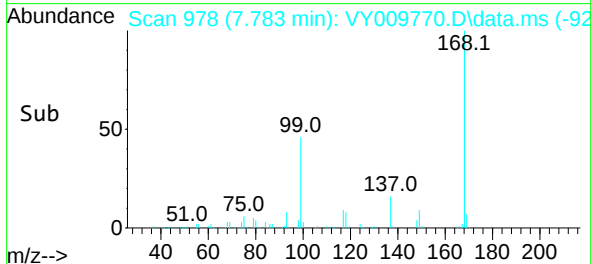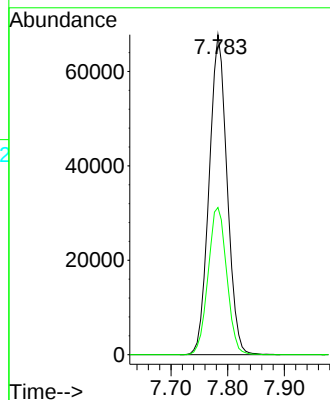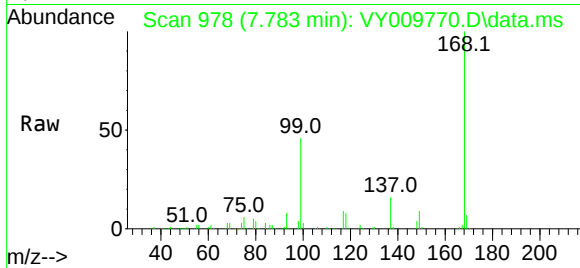

#33
1,2-Dichloroethane-d4
Concen: 65.561 ug/l
RT: 8.136 min Scan# 1036
Delta R.T. 0.000 min
Lab File: VY009770.D
Acq: 29 Jul 2022 14:18

Tgt Ion: 65 Resp: 63412
Ion Ratio Lower Upper
65 100
67 56.7 0.0 99.4

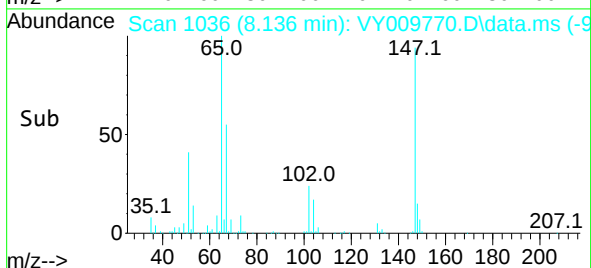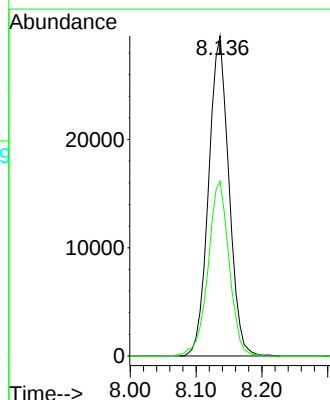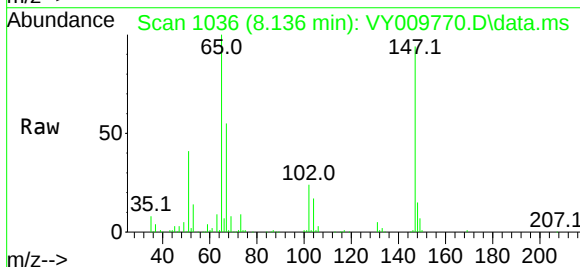

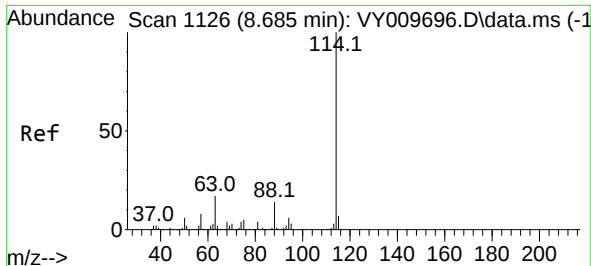

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.685 min Scan# 1126

Delta R.T. 0.000 min

Lab File: VY009770.D

Acq: 29 Jul 2022 14:18

Instrument :

MSVOA_Y

ClientSampleId :

RVE-100





Tgt Ion:114 Resp: 258879

Ion Ratio Lower Upper

114 100

63 17.2 0.0 43.2

88 13.3 0.0 31.8

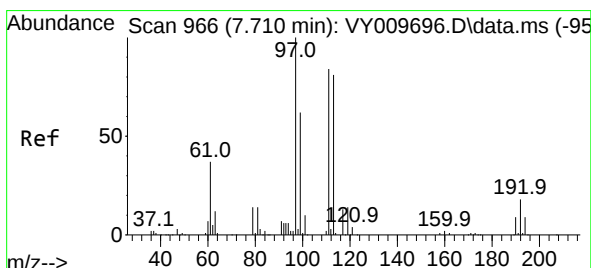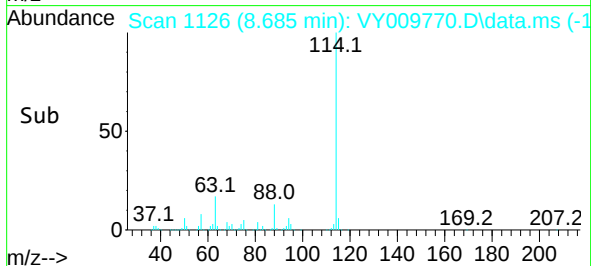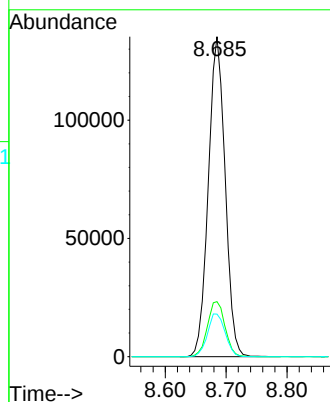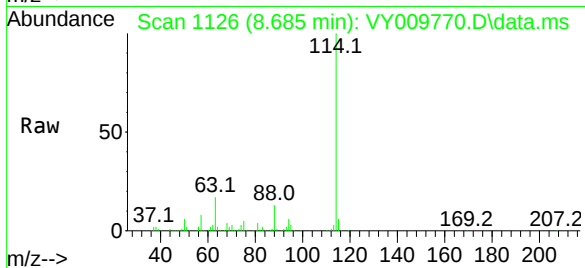

#35

Dibromofluoromethane

Concen: 43.489 ug/l

RT: 7.710 min Scan# 966

Delta R.T. -0.000 min

Lab File: VY009770.D

Acq: 29 Jul 2022 14:18




Tgt Ion:113 Resp: 61231


Ion Ratio Lower Upper

113 100

111 102.8 82.6 124.0

192 22.0 17.6 26.4


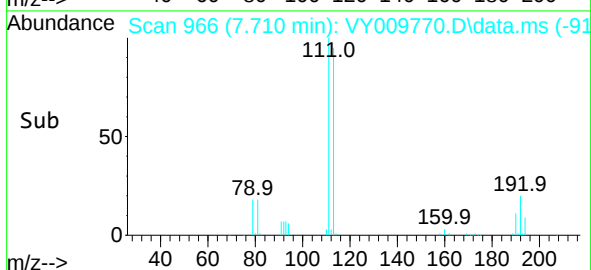
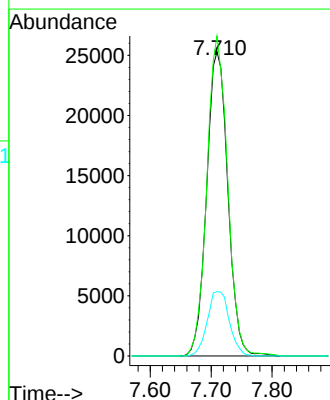
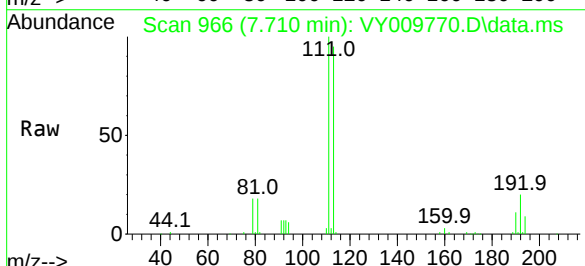


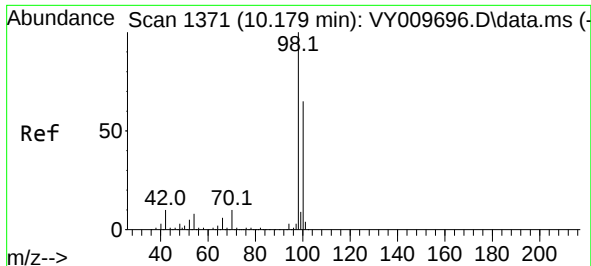

#50
Toluene-d8
Concen: 55.325 ug/l
RT: 10.179 min Scan# 1371
Delta R.T. -0.000 min
Lab File: VY009770.D
Acq: 29 Jul 2022 14:18




Instrument :
MSVOA_Y
ClientSampleId :
RVE-100


Tgt Ion: 98 Resp: 225010
Ion Ratio Lower Upper
98 100
100 64.3 50.2 75.2

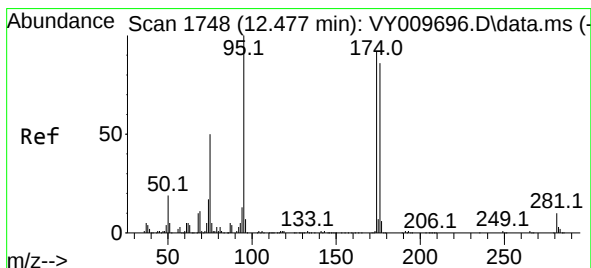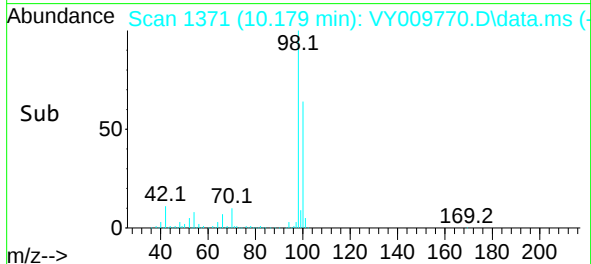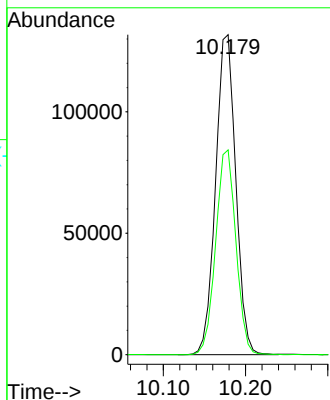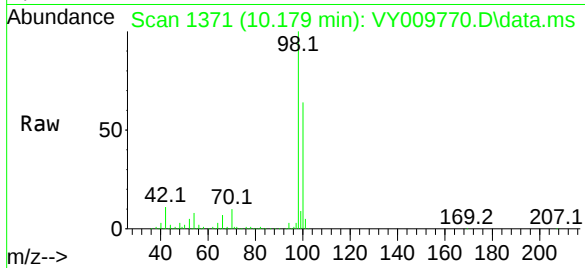

#62
4-Bromofluorobenzene
Concen: 37.511 ug/l
RT: 12.477 min Scan# 1748
Delta R.T. 0.000 min
Lab File: VY009770.D
Acq: 29 Jul 2022 14:18

Tgt Ion: 95 Resp: 70032
Ion Ratio Lower Upper
95 100
174 98.6 0.0 177.0
176 94.3 0.0 175.8

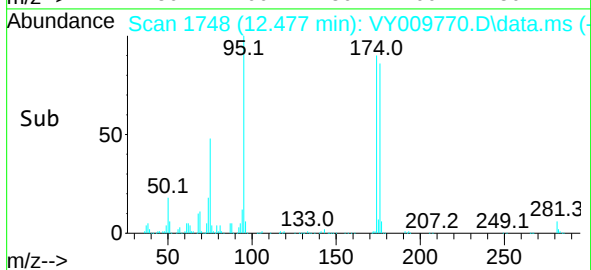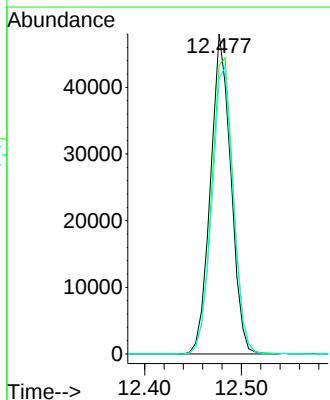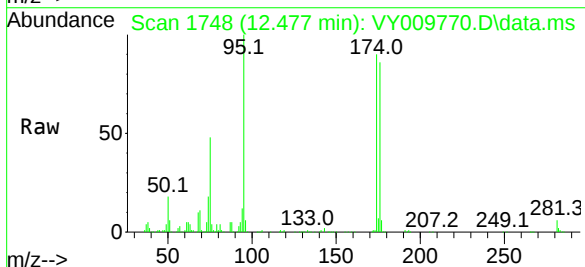

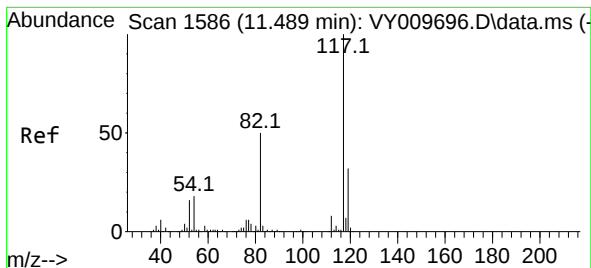

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.489 min Scan# 11

Delta R.T. 0.000 min

Lab File: VY009770.D

Acq: 29 Jul 2022 14:18

Instrument :

MSVOA_Y

ClientSampleId :

RVE-100





Tgt Ion:117 Resp: 253530

Ion Ratio Lower Upper

117 100

82 49.9 43.0 64.4

119 32.9 25.4 38.0

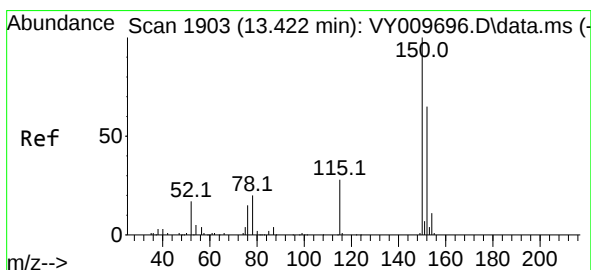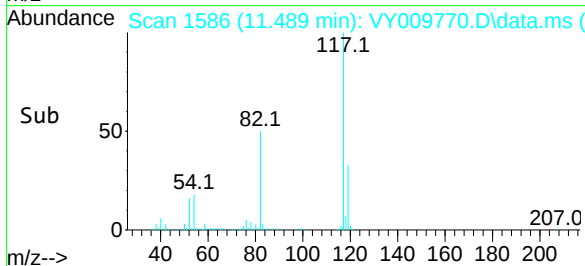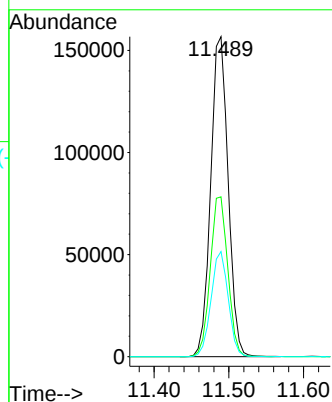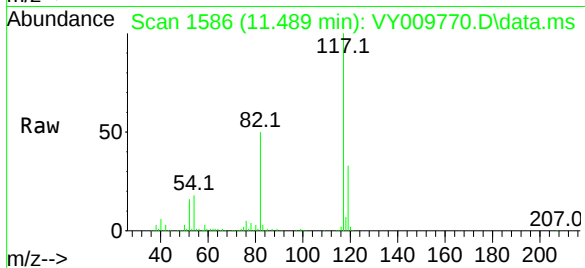

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.422 min Scan# 1903

Delta R.T. -0.000 min

Lab File: VY009770.D

Acq: 29 Jul 2022 14:18

Tgt Ion:152 Resp: 118179

Ion Ratio Lower Upper

152 100

115 53.1 28.2 84.7

150 157.5 0.0 347.6

