
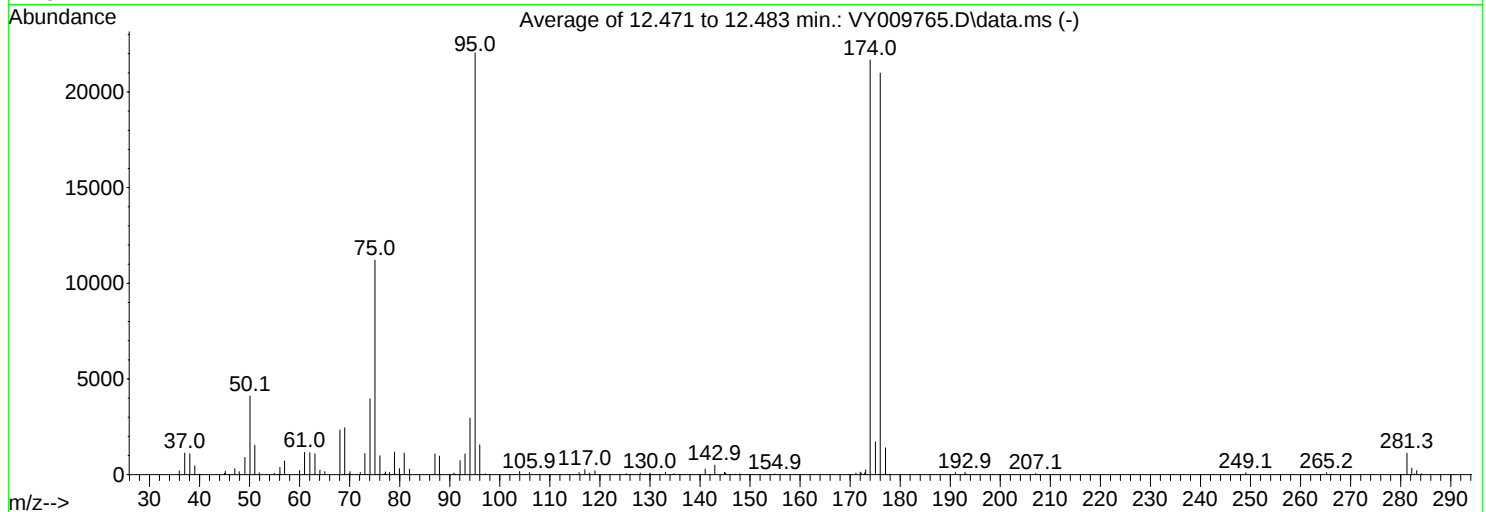


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY072922\
Data File : VY009765.D
Acq On : 29 Jul 2022 09:51
Operator : KP/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y072622S.M
Title : SW846 8260
Last Update : Wed Jul 27 04:24:58 2022

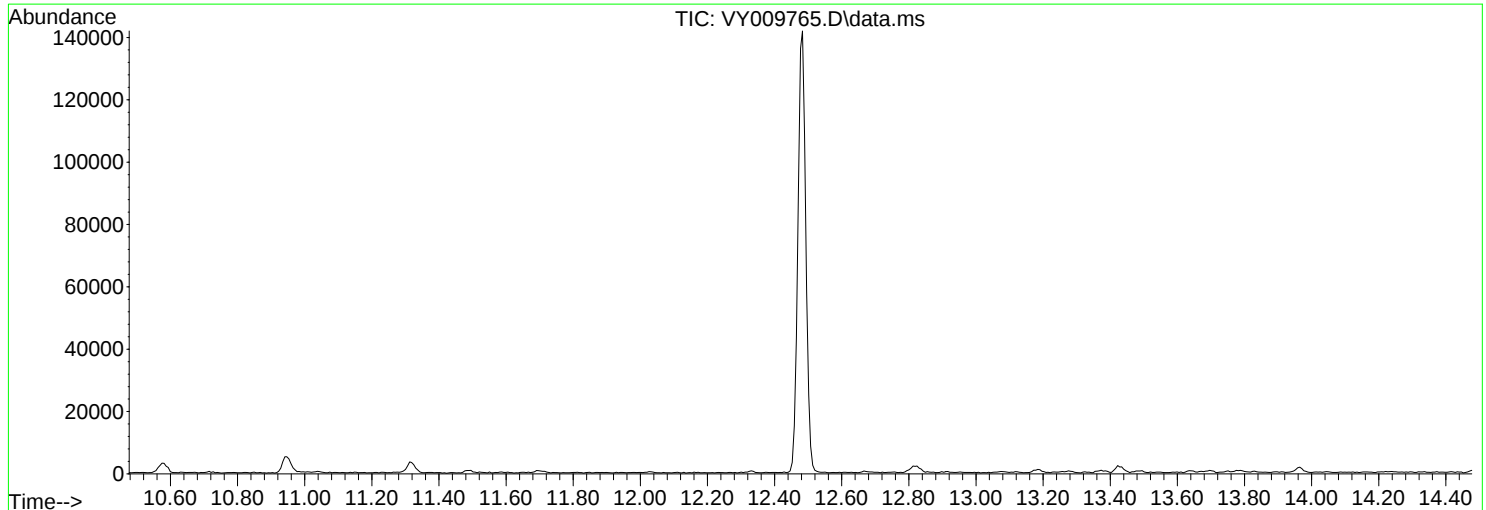

AutoFind: Scans 1747, 1748, 1749; Background Corrected with Scan 1740

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	18.7	4115	PASS
75	95	30	60	50.9	11213	PASS
95	95	100	100	100.0	22045	PASS
96	95	5	9	7.1	1555	PASS
173	174	0.00	2	1.1	249	PASS
174	95	50	100	98.3	21677	PASS
175	174	5	9	7.9	1715	PASS
176	174	95	101	96.8	20989	PASS
177	176	5	9	6.7	1406	PASS