



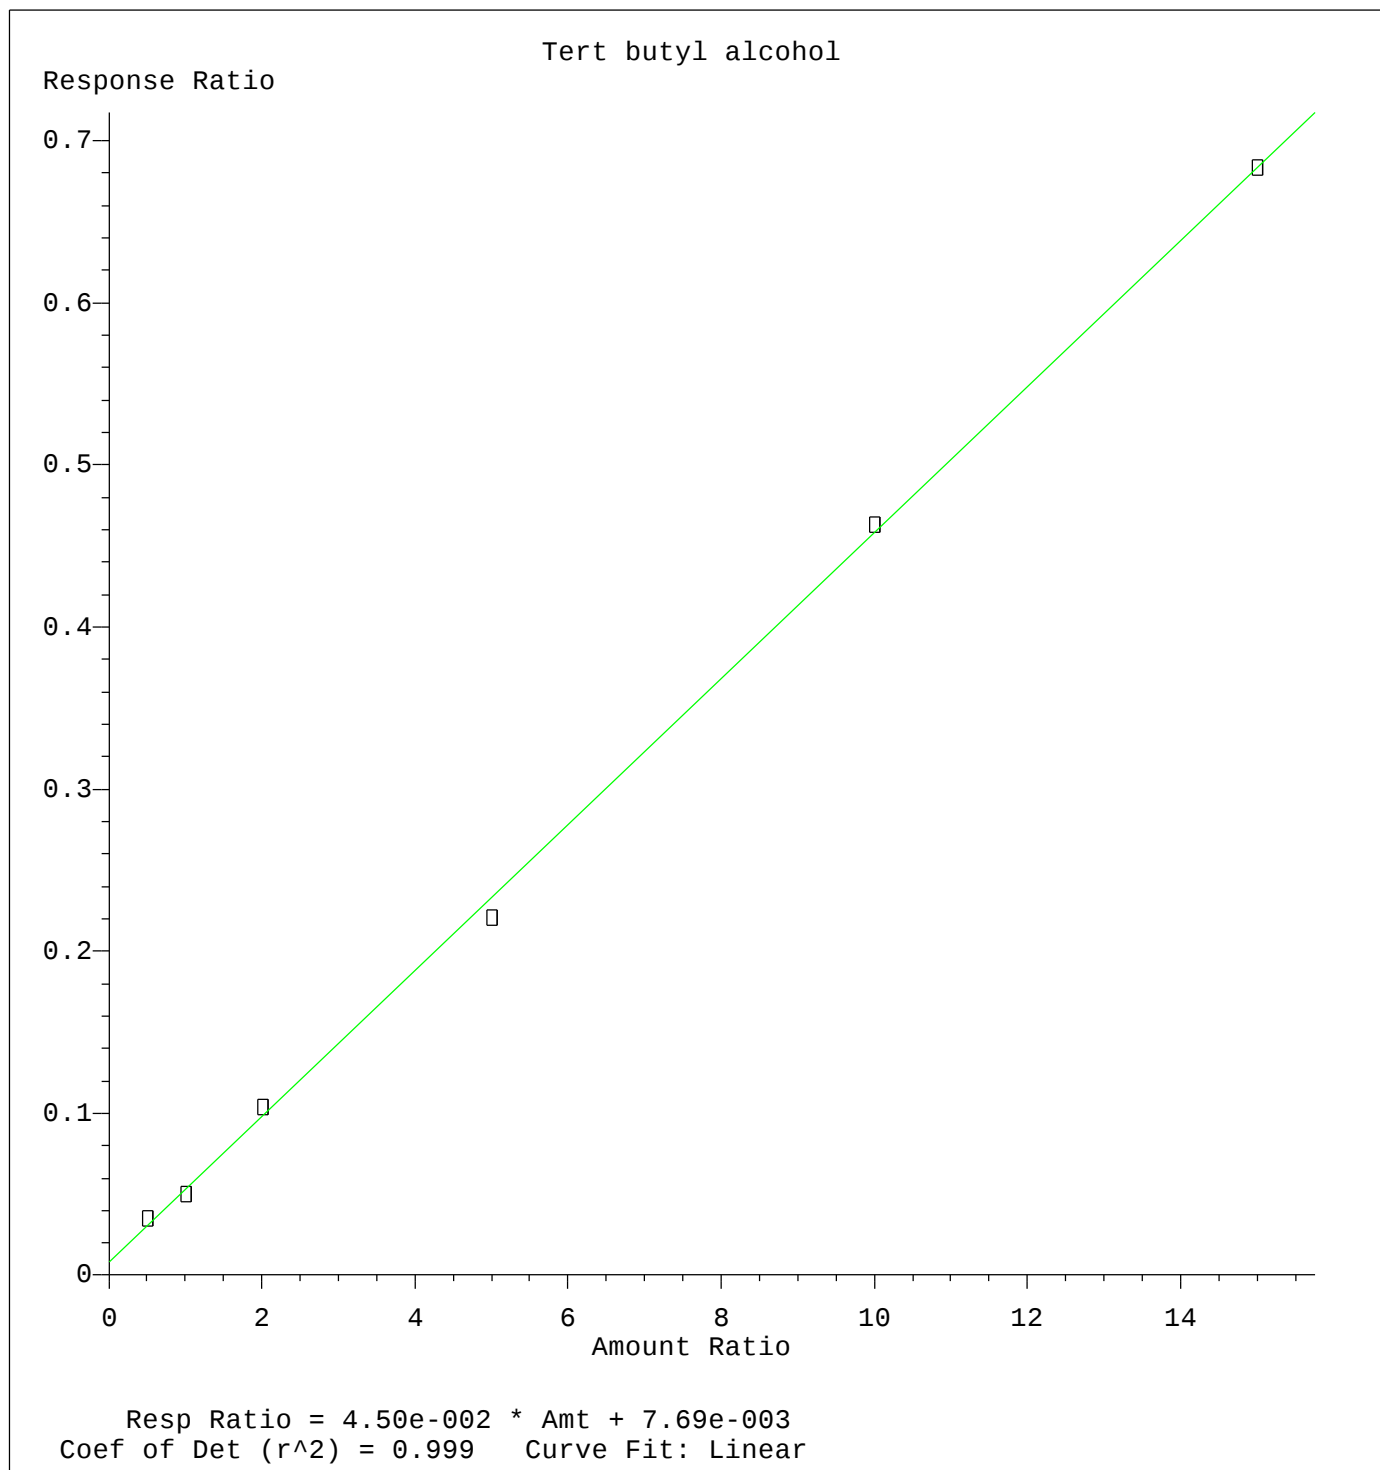

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_Y\METHODS\82Y073120S.M
Calibration Table Last Updated: Fri Jul 31 13:08:19 2020

Methylene Chloride

Response Ratio

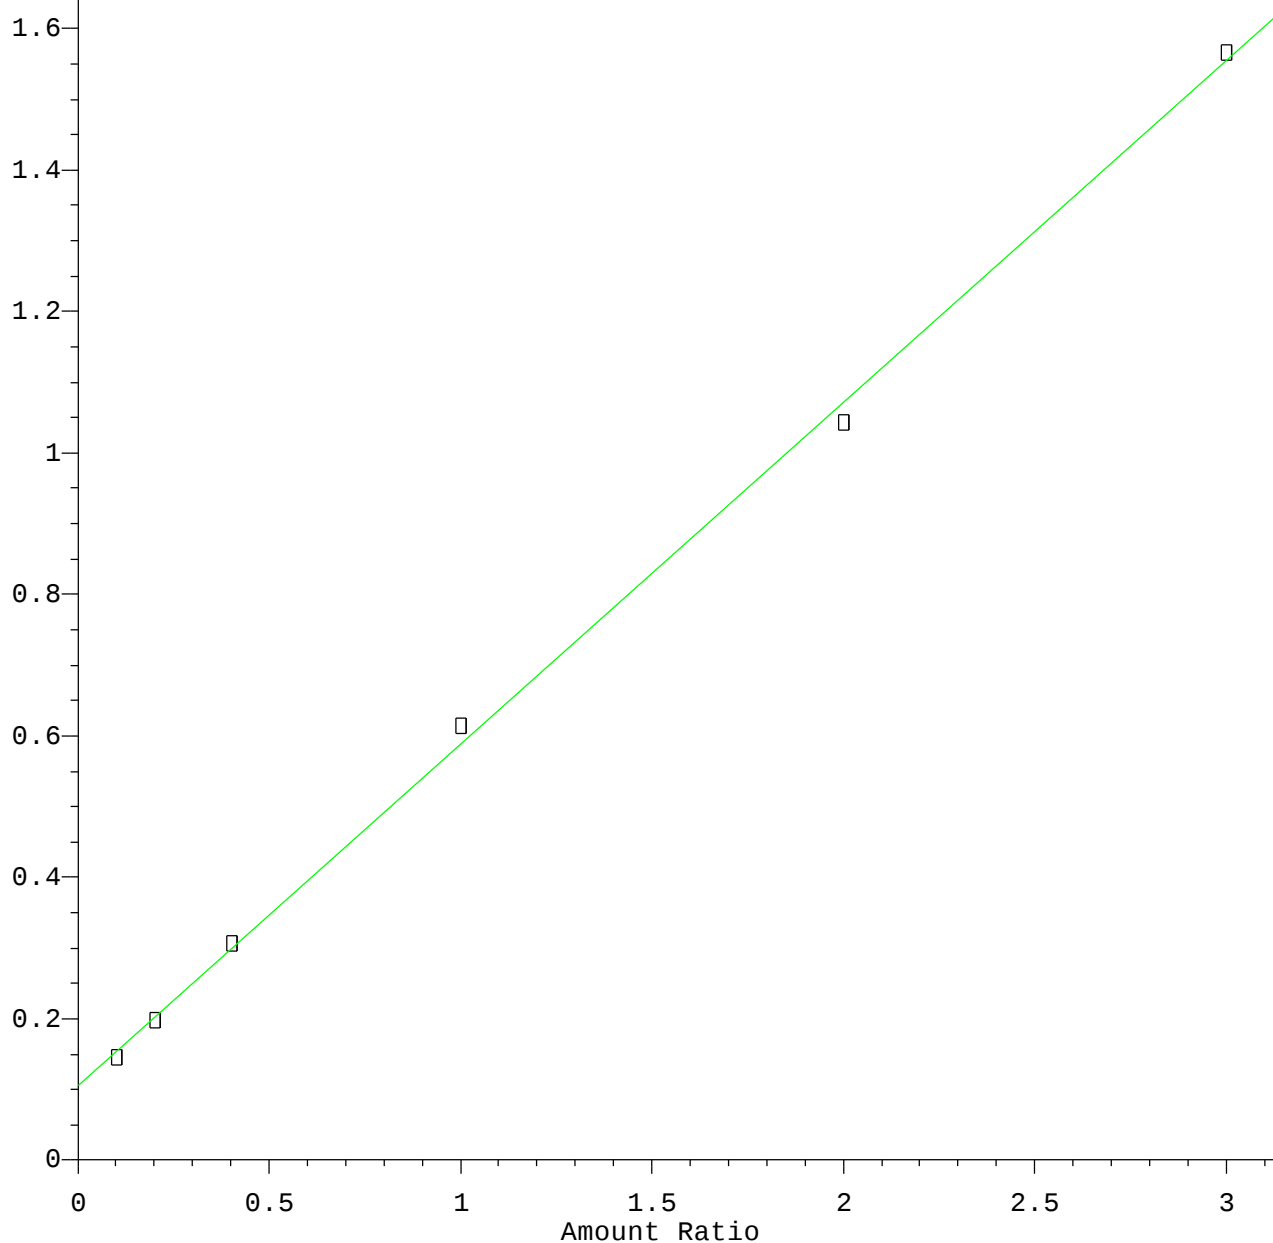

Resp Ratio = $4.83 \times 10^{-1} \times \text{Amt} + 1.05 \times 10^{-1}$
Coef of Det (r^2) = 0.999 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_Y\METHODS\82Y073120S.M
Calibration Table Last Updated: Fri Jul 31 13:08:51 2020