


Data Path : Z:\voasrv\HPCHEM1\MSVOA Y\Data\vv073120\
Data File : VY003379.D
Acq On : 31 Jul 2020 10:00
Operator : SY/MD
Sample : BFB
Misc : 5.00G/5ML/MSVOA Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_Y\METHODS\82Y073120S.M
Title : SW846 8260
Last Update : Fri Jul 31 13:09:26 2020

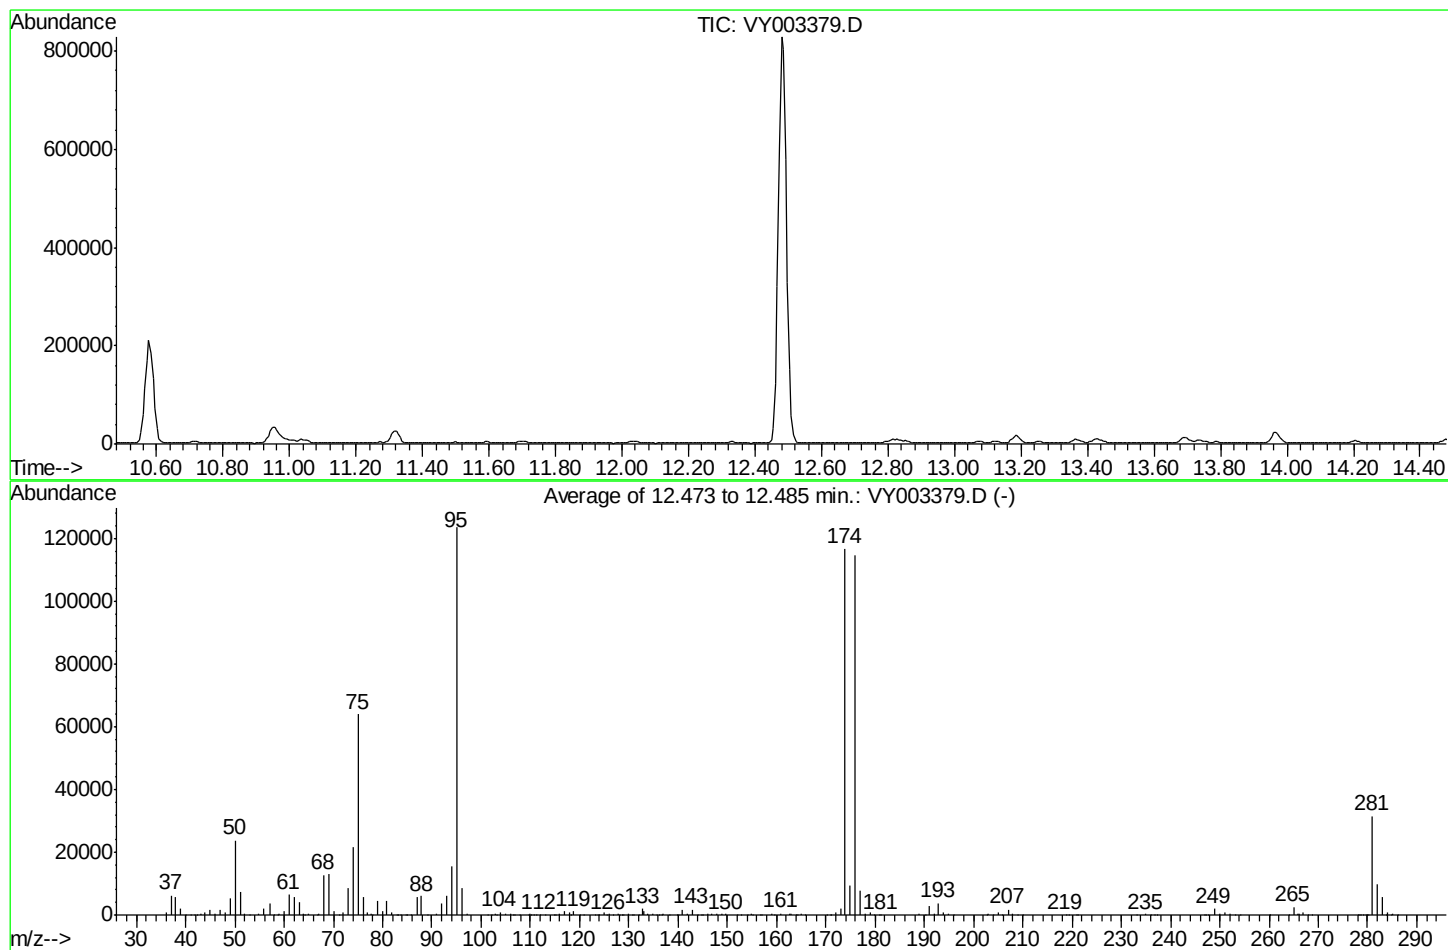

AutoFind: Scans 1761, 1762, 1763; Background Corrected with Scan 1753

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.2	23677	PASS
75	95	30	60	51.8	63989	PASS
95	95	100	100	100.0	123488	PASS
96	95	5	9	7.0	8613	PASS
173	174	0.00	2	1.6	1888	PASS
174	95	50	100	94.5	116712	PASS
175	174	5	9	8.0	9374	PASS
176	174	95	101	98.2	114592	PASS
177	176	5	9	6.9	7904	PASS