
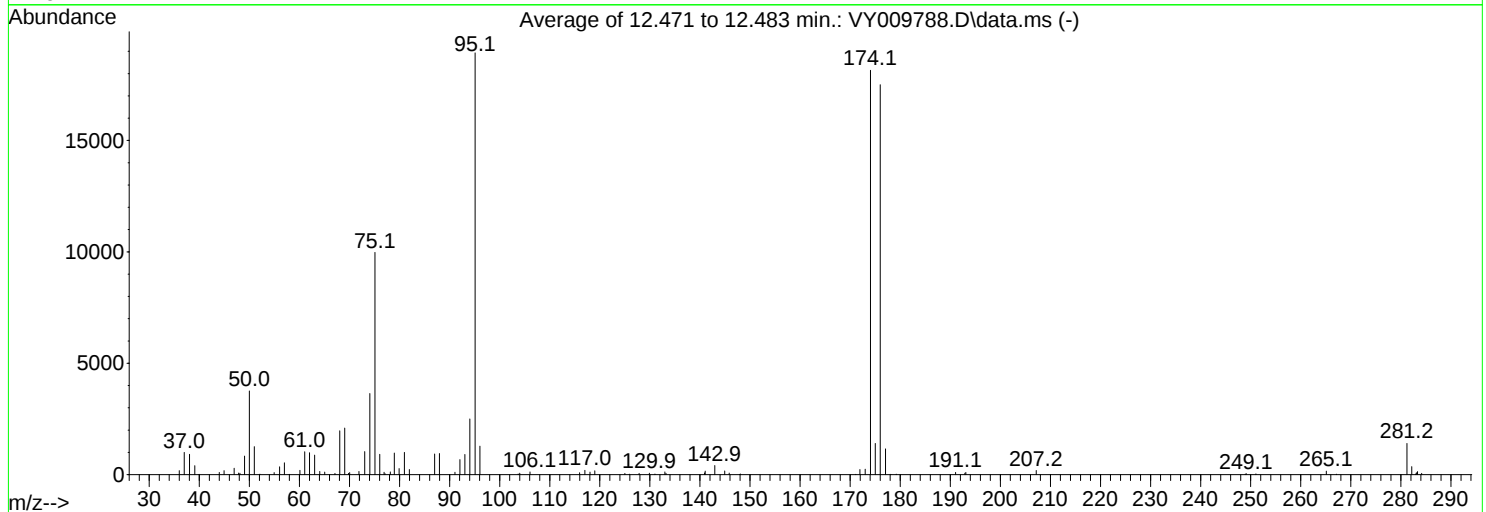


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY080122\
Data File : VY009788.D
Acq On : 01 Aug 2022 10:00
Operator : KP/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y072622S.M
Title : SW846 8260
Last Update : Wed Jul 27 04:24:58 2022

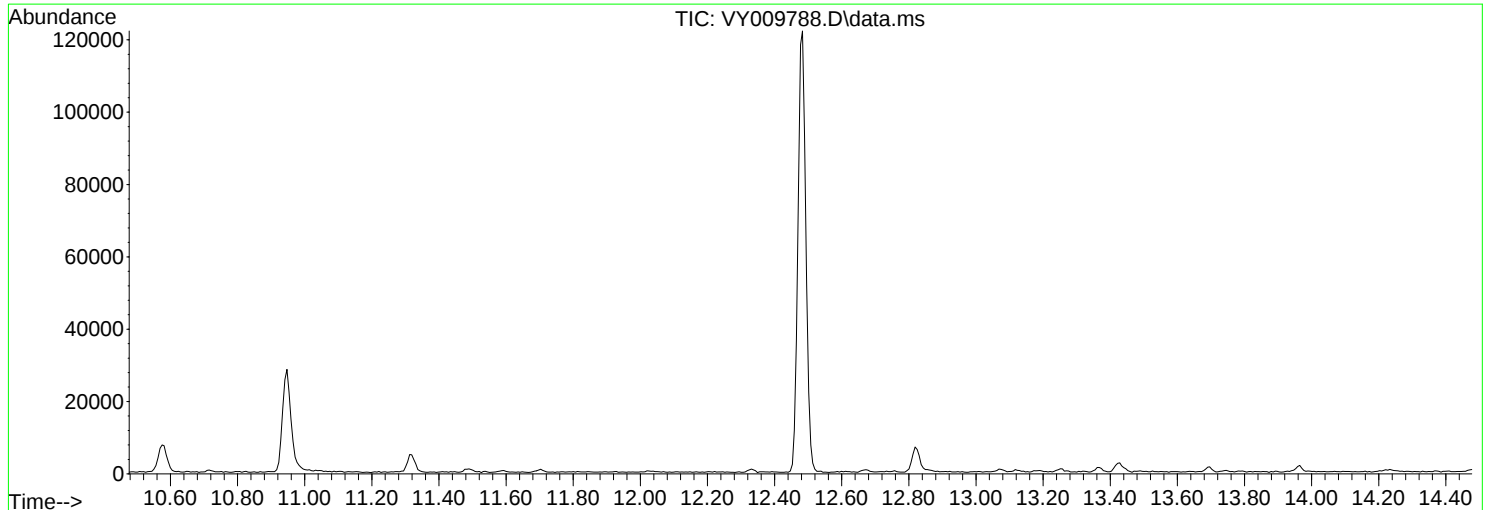

AutoFind: Scans 1747, 1748, 1749; Background Corrected with Scan 1740

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.8	3756	PASS
75	95	30	60	52.7	9972	PASS
95	95	100	100	100.0	18931	PASS
96	95	5	9	6.8	1278	PASS
173	174	0.00	2	1.3	245	PASS
174	95	50	100	95.9	18151	PASS
175	174	5	9	7.7	1398	PASS
176	174	95	101	96.4	17498	PASS
177	176	5	9	6.6	1154	PASS