

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY080223\
 Data File : VY014938.D
 Acq On : 02 Aug 2023 18:04
 Operator : SY/MD
 Sample : 03862-02
 Misc : 6.48g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 BUILDING-B-3-(5-10)

Quant Time: Aug 03 02:46:01 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y071323S.M
 Quant Title : SW846 8260
 QLast Update : Fri Jul 14 02:09:50 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	7.783	168	215751	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.685	114	379608	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.489	117	355730	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.422	152	156812	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.136	65	141796	57.674	ug/l	0.00
Spiked Amount 50.000	Range 50 - 163		Recovery = 115.340%			
35) Dibromofluoromethane	7.710	113	118388	48.992	ug/l	0.00
Spiked Amount 50.000	Range 54 - 147		Recovery = 97.980%			
50) Toluene-d8	10.173	98	449616	50.467	ug/l	0.00
Spiked Amount 50.000	Range 58 - 134		Recovery = 100.940%			
62) 4-Bromofluorobenzene	12.477	95	159703	46.750	ug/l	0.00
Spiked Amount 50.000	Range 30 - 143		Recovery = 93.500%			
Target Compounds					Qvalue	
10) Methyl Iodide	4.088	142	182	2.441	ug/l #	38
11) Tert butyl alcohol	4.954	59	590	Below Cal	#	89
13) Acrolein	3.729	56	360	1.401	ug/l #	70
16) Acetone	3.948	43	24122	30.962	ug/l #	89
17) Carbon Disulfide	4.186	76	53806	8.846	ug/l #	94
20) Methylene Chloride	4.710	84	26449	6.802	ug/l #	83
25) 2-Butanone	6.984	43	6280	5.510	ug/l	99
31) Cyclohexane	7.777	56	4765	1.168	ug/l #	17
36) 1,1-Dichloropropene	7.789	75	16852	4.663	ug/l #	50
37) Ethyl Acetate	6.984	43	6280	2.524	ug/l #	71
38) Carbon Tetrachloride	7.789	117	21907	5.735	ug/l #	15
52) Toluene	10.240	92	8172	1.243	ug/l	91
67) Ethyl Benzene	11.587	91	37632	2.750	ug/l	99
68) m/p-Xylenes	11.697	106	13880	2.657	ug/l	99
69) o-Xylene	12.026	106	32804	6.446	ug/l	99
73) Isopropylbenzene	12.325	105	84563	6.887	ug/l	100
76) 1,2,3-Trichloropropane	12.477	75	86683	43.768	ug/l #	100
78) n-propylbenzene	12.666	91	65695	4.440	ug/l	100
79) 2-Chlorotoluene	12.764	91	26383	3.096	ug/l #	40
80) 1,3,5-Trimethylbenzene	12.806	105	236045	23.019	ug/l	95
81) trans-1,4-Dichloro-2-b...	12.477	75	86683	84.743	ug/l #	11
82) 4-Chlorotoluene	12.806	91	25777	2.937	ug/l #	40
83) tert-Butylbenzene	13.117	119	58260	6.405	ug/l #	55
84) 1,2,4-Trimethylbenzene	13.117	105	507089	50.390	ug/l	98
85) sec-Butylbenzene	13.251	105	17218	1.290	ug/l #	77
86) p-Isopropyltoluene	13.367	119	153803	14.117	ug/l	98
89) n-Butylbenzene	13.660	91	116069	10.951	ug/l #	1
90) Hexachloroethane	13.965	117	109243	48.818	ug/l #	8
92) 1,2-Dibromo-3-Chloropr...	14.373	75	1557	2.908	ug/l #	3
95) Naphthalene	15.233	128	14441911	1953.922	ug/l #	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY080223\
Data File : VY014938.D
Acq On : 02 Aug 2023 18:04
Operator : SY/MD
Sample : 03862-02
Misc : 6.48g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BUILDING-B-3-(5-10)

Quant Time: Aug 03 02:46:01 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y071323S.M
Quant Title : SW846 8260
QLast Update : Fri Jul 14 02:09:50 2023
Response via : Initial Calibration




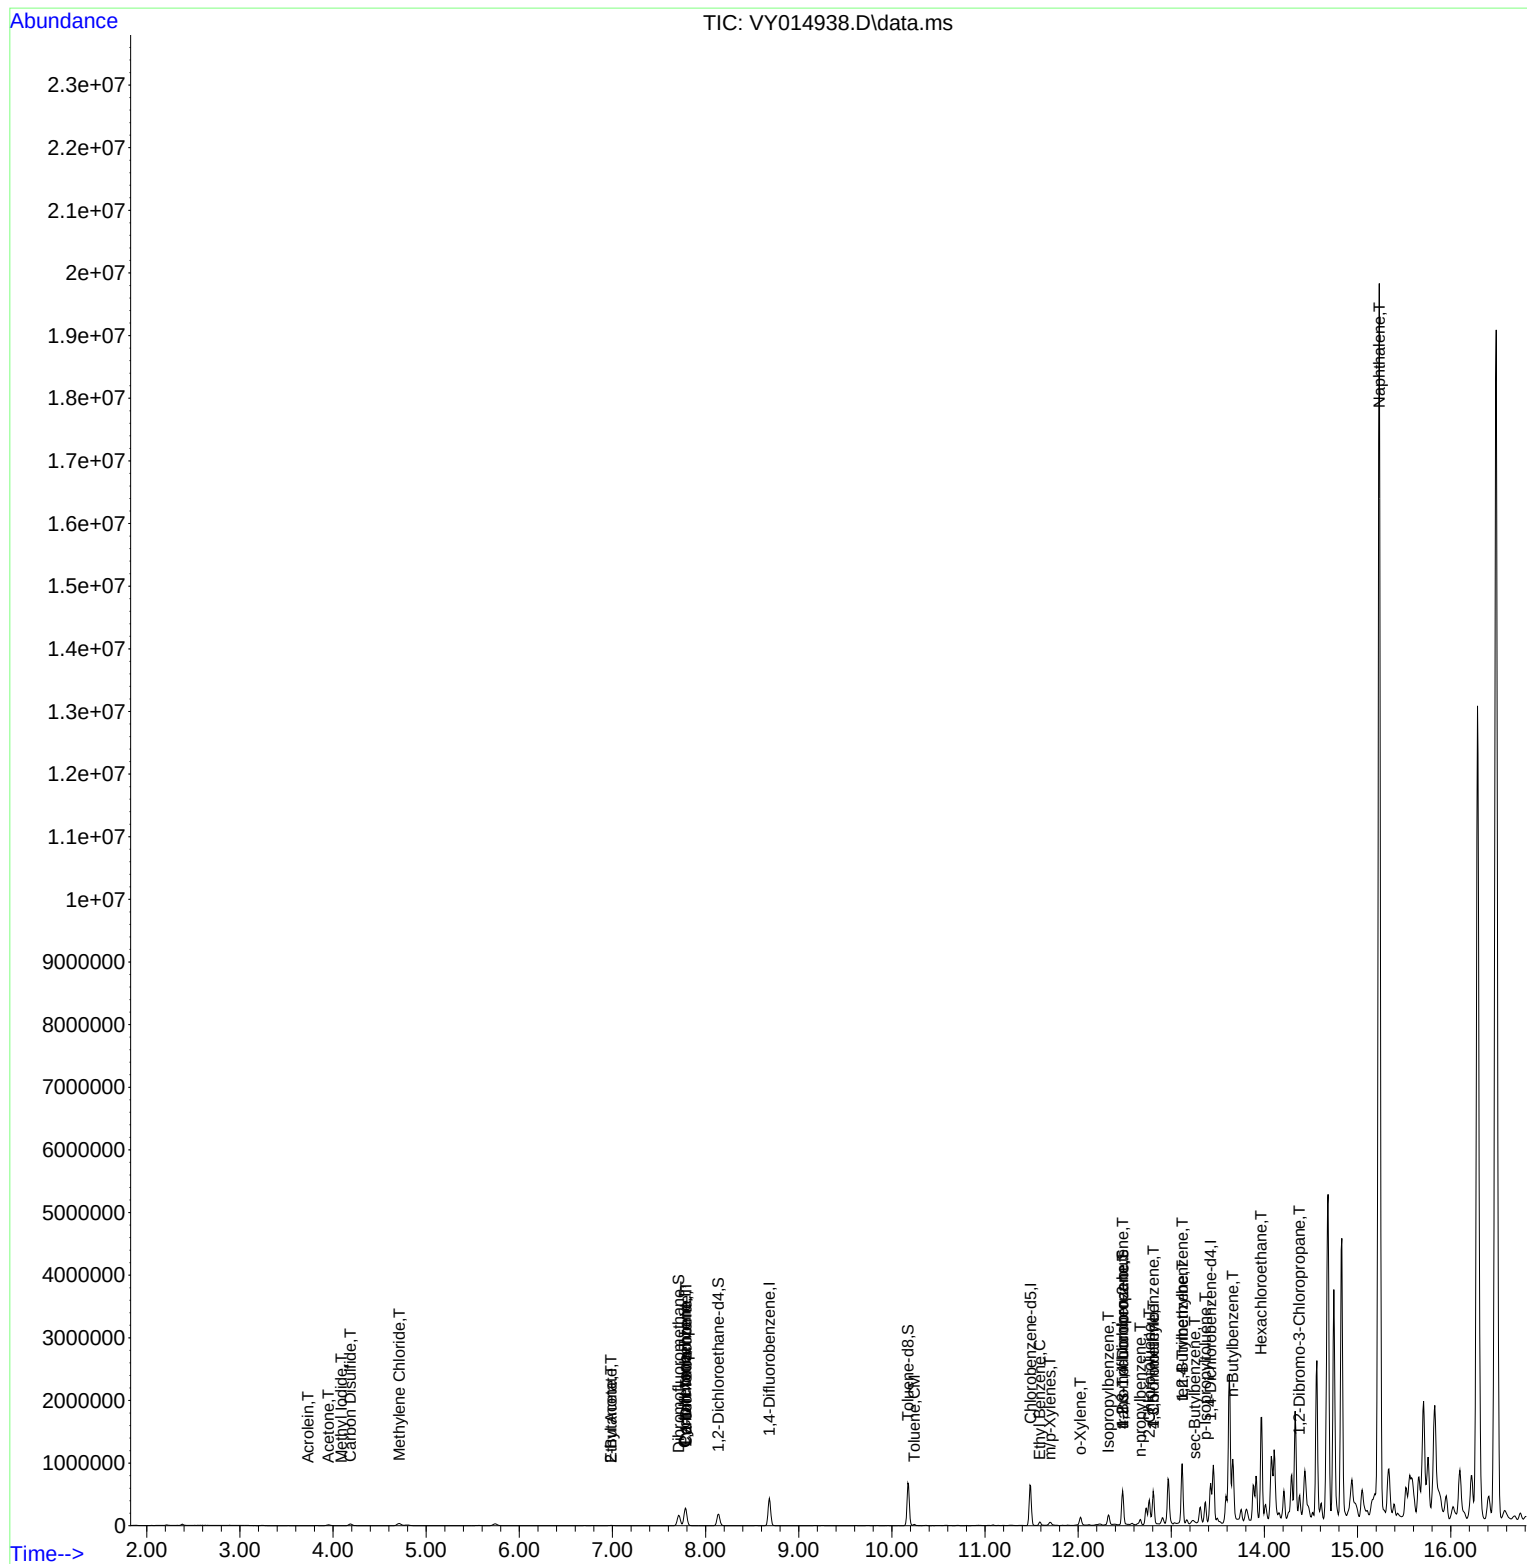




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.783 min Scan# 91
Delta R.T. -0.006 min
Lab File: VY014938.D
Acq: 02 Aug 2023 18:04




Instrument :
MSVOA_Y
ClientSampleId :
BUILDING-B-3-(5-10)


Tgt Ion:168 Resp: 215751
Ion Ratio Lower Upper
168 100
99 58.9 43.4 65.0



#10
Methyl Iodide
Concen: 2.441 ug/l
RT: 4.088 min Scan# 372
Delta R.T. 0.006 min
Lab File: VY014938.D
Acq: 02 Aug 2023 18:04

Tgt Ion:142 Resp: 182
Ion Ratio Lower Upper
142 100
127 0.0 37.6 56.4#
141 0.0 11.8 17.8#


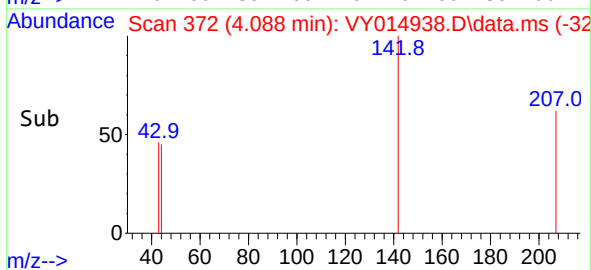






#13
Acrolein
Concen: 1.401 ug/l
RT: 3.729 min Scan# 312
Delta R.T. 0.006 min
Lab File: VY014938.D
Acq: 02 Aug 2023 18:04




Instrument :
MSVOA_Y
ClientSampleId :
BUILDING-B-3-(5-10)


Tgt Ion: 56 Resp: 360
Ion Ratio Lower Upper
56 100
55 46.1 57.0 85.4#



#16
Acetone
Concen: 30.962 ug/l
RT: 3.948 min Scan# 349
Delta R.T. 0.006 min
Lab File: VY014938.D
Acq: 02 Aug 2023 18:04

Tgt Ion: 43 Resp: 24122
Ion Ratio Lower Upper
43 100
58 34.2 22.7 34.1#


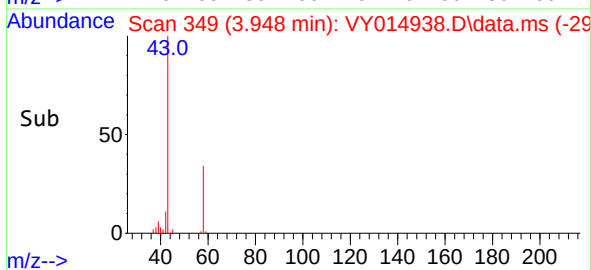






#17
Carbon Disulfide
Concen: 8.846 ug/l
RT: 4.186 min Scan# 388
Delta R.T. -0.000 min
Lab File: VY014938.D
Acq: 02 Aug 2023 18:04




Instrument :
MSVOA_Y
ClientSampleId :
BUILDING-B-3-(5-10)


Tgt Ion: 76 Resp: 53806
Ion Ratio Lower Upper
76 100
78 10.8 7.0 10.4#

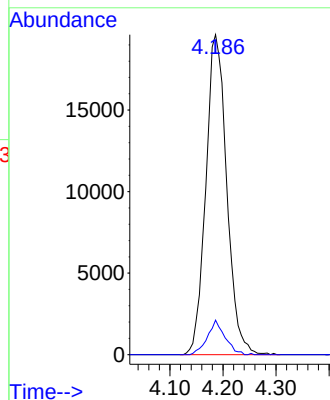

#20
Methylene Chloride
Concen: 6.802 ug/l
RT: 4.710 min Scan# 474
Delta R.T. 0.006 min
Lab File: VY014938.D
Acq: 02 Aug 2023 18:04

Tgt Ion: 84 Resp: 26449
Ion Ratio Lower Upper
84 100
49 107.3 106.9 160.3
51 29.8 33.2 49.8#
86 59.0 51.0 76.6



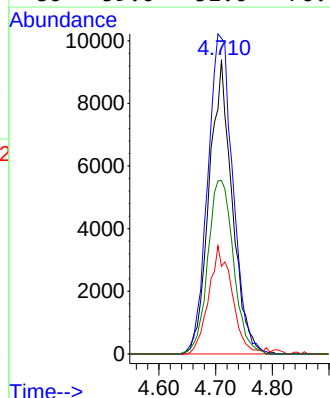





#25
2-Butanone
Concen: 5.510 ug/l
RT: 6.984 min Scan# 846
Delta R.T. 0.006 min
Lab File: VY014938.D
Acq: 02 Aug 2023 18:04




Instrument :
MSVOA_Y
ClientSampleId :
BUILDING-B-3-(5-10)


Tgt Ion: 43 Resp: 6280
Ion Ratio Lower Upper
43 100
72 25.0 20.5 30.7

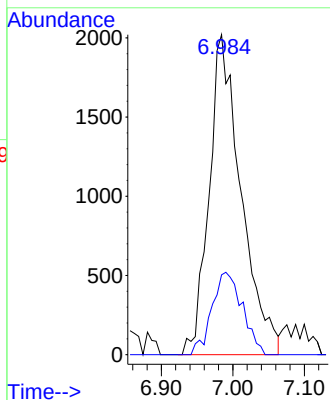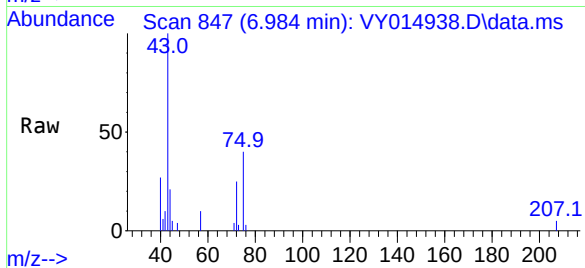

#31
Cyclohexane
Concen: 1.168 ug/l
RT: 7.777 min Scan# 977
Delta R.T. -0.000 min
Lab File: VY014938.D
Acq: 02 Aug 2023 18:04

Tgt Ion: 56 Resp: 4765
Ion Ratio Lower Upper
56 100
69 138.1 27.8 41.6#
84 121.4 66.4 99.6#

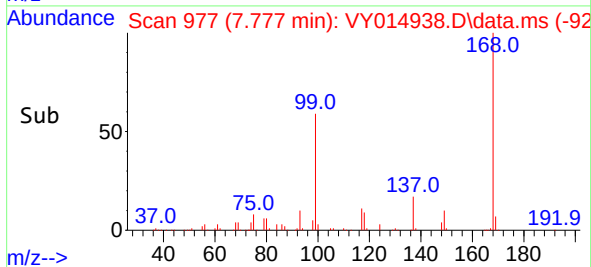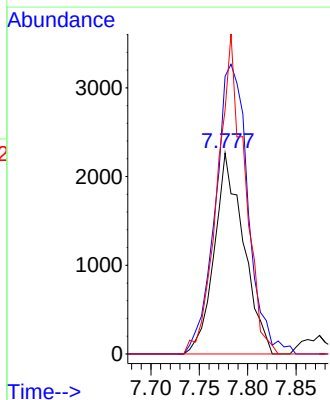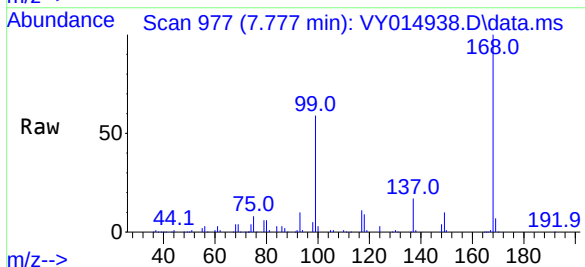



#33

1,2-Dichloroethane-d4

Concen: 57.674 ug/l

RT: 8.136 min Scan# 1036

Delta R.T. 0.000 min

Lab File: VY014938.D

Acq: 02 Aug 2023 18:04

Instrument :

MSVOA_Y

ClientSampleId :





BUILDING-B-3-(5-10)

Tgt Ion: 65 Resp: 141796

Ion Ratio Lower Upper

65 100

67 52.2 0.0 101.8

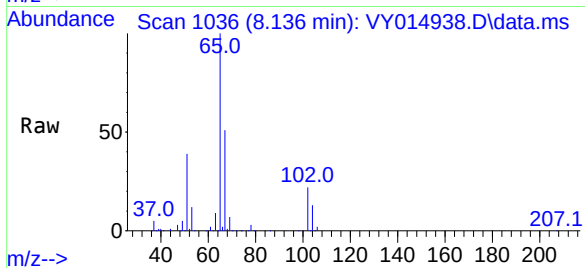

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.685 min Scan# 1126

Delta R.T. -0.000 min

Lab File: VY014938.D

Acq: 02 Aug 2023 18:04




Tgt Ion: 114 Resp: 379608


Ion Ratio Lower Upper

114 100

63 19.2 0.0 42.4

88 15.0 0.0 30.6


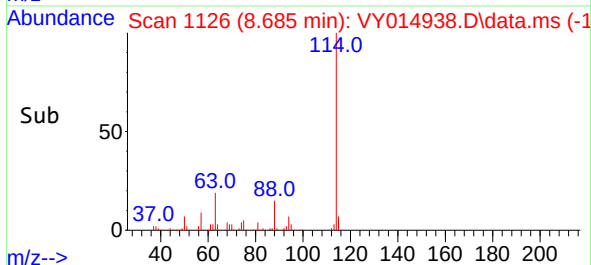
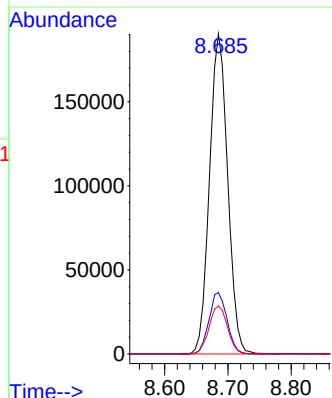
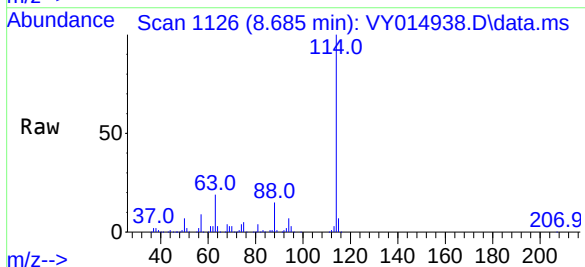




#35
Dibromofluoromethane
Concen: 48.992 ug/l
RT: 7.710 min Scan# 910
Delta R.T. -0.006 min
Lab File: VY014938.D
Acq: 02 Aug 2023 18:04




Instrument :
MSVOA_Y
ClientSampleId :
BUILDING-B-3-(5-10)


Tgt Ion:113 Resp: 118388
Ion Ratio Lower Upper
113 100
111 101.5 81.3 121.9
192 19.1 16.9 25.3

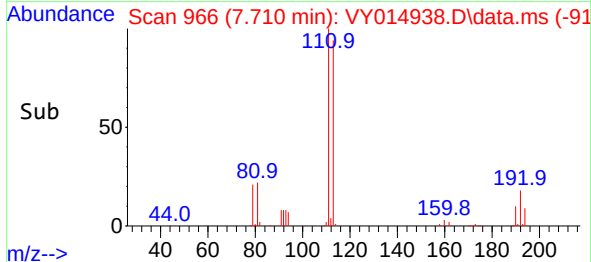

#36
1,1-Dichloropropene
Concen: 4.663 ug/l
RT: 7.789 min Scan# 979
Delta R.T. -0.122 min
Lab File: VY014938.D
Acq: 02 Aug 2023 18:04

Tgt Ion: 75 Resp: 16852
Ion Ratio Lower Upper
75 100
110 9.3 17.8 53.5#
77 0.0 24.4 36.6#

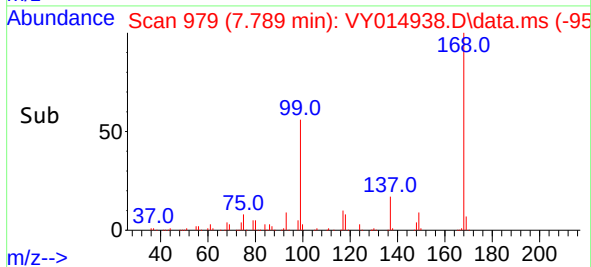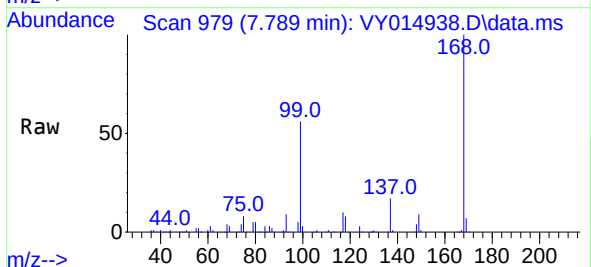



#37

Ethyl Acetate

Concen: 2.524 ug/l

RT: 6.984 min Scan# 84

Delta R.T. -0.086 min

Lab File: VY014938.D


Acq: 02 Aug 2023 18:04

Instrument :

MSVOA_Y

ClientSampleId :

BUILDING-B-3-(5-10)






Tgt Ion: 43 Resp: 6280

Ion Ratio Lower Upper

43 100

61 0.0 10.1 15.1#

70 0.0 7.1 10.7#

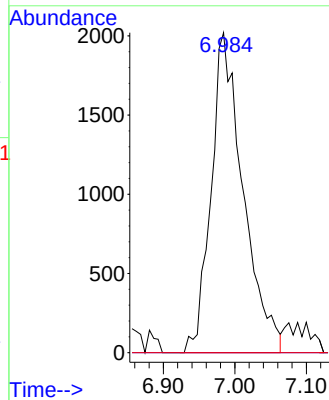

#38

Carbon Tetrachloride

Concen: 5.735 ug/l

RT: 7.789 min Scan# 979

Delta R.T. -0.110 min

Lab File: VY014938.D

Acq: 02 Aug 2023 18:04




Tgt Ion: 117 Resp: 21907


Ion Ratio Lower Upper

117 100

119 4.0 76.4 114.6#

121 0.0 25.8 38.6#


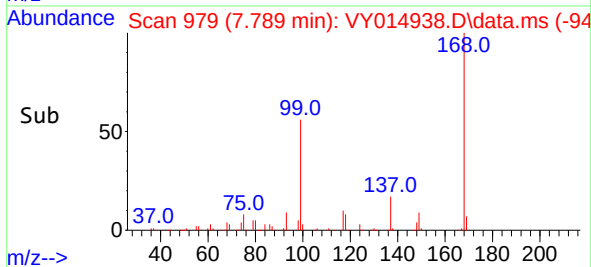
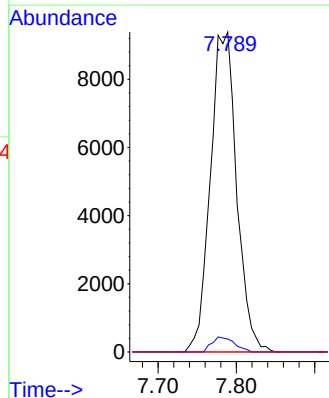
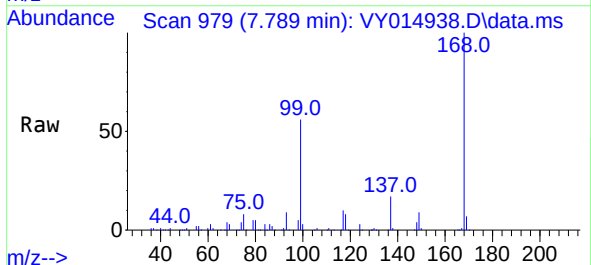




#50
Toluene-d8
Concen: 50.467 ug/l
RT: 10.173 min Scan# 1370
Delta R.T. -0.006 min
Lab File: VY014938.D
Acq: 02 Aug 2023 18:04




Instrument :
MSVOA_Y
ClientSampleId :
BUILDING-B-3-(5-10)


Tgt Ion: 98 Resp: 449616
Ion Ratio Lower Upper
98 100
100 65.5 50.1 75.1

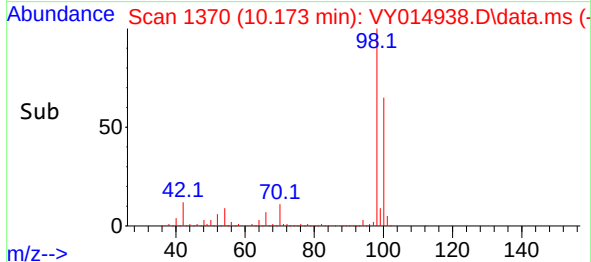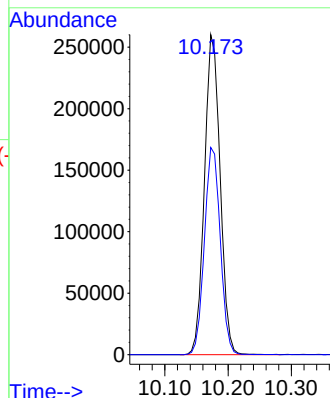

#52
Toluene
Concen: 1.243 ug/l
RT: 10.240 min Scan# 1381
Delta R.T. -0.000 min
Lab File: VY014938.D
Acq: 02 Aug 2023 18:04

Tgt Ion: 92 Resp: 8172
Ion Ratio Lower Upper
92 100
91 167.4 143.8 215.6



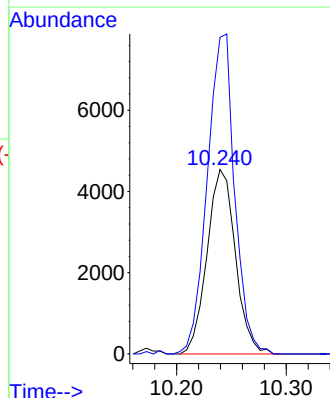





#62
4-Bromofluorobenzene
Concen: 46.750 ug/l
RT: 12.477 min Scan# 11
Delta R.T. 0.000 min
Lab File: VY014938.D
Acq: 02 Aug 2023 18:04




Instrument :
MSVOA_Y
ClientSampleId :
BUILDING-B-3-(5-10)


Tgt Ion: 95 Resp: 159703
Ion Ratio Lower Upper
95 100
174 83.6 0.0 178.2
176 80.2 0.0 173.8

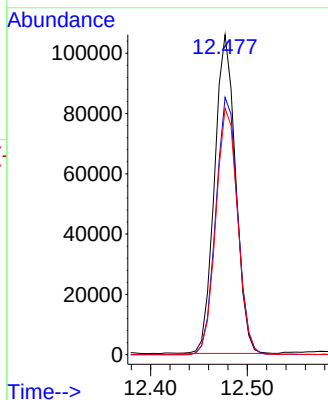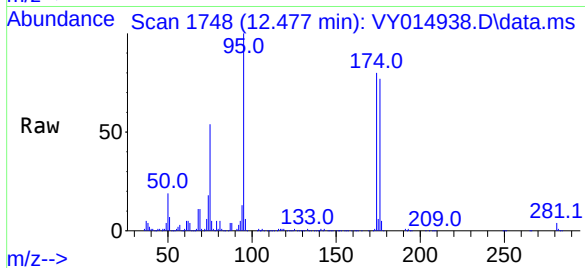

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.489 min Scan# 1586
Delta R.T. 0.000 min
Lab File: VY014938.D
Acq: 02 Aug 2023 18:04

Tgt Ion: 117 Resp: 355730
Ion Ratio Lower Upper
117 100
82 53.8 43.4 65.0
119 31.4 26.3 39.5

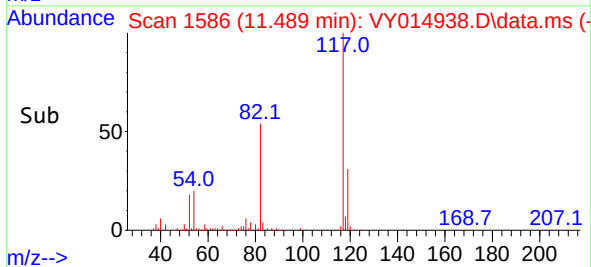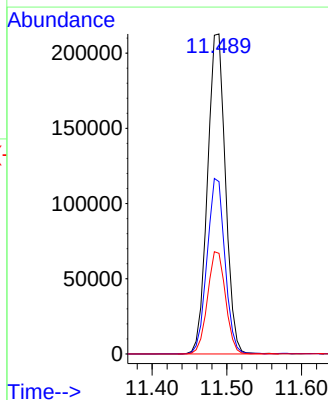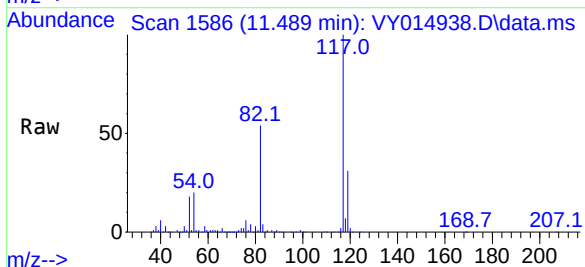



#67

Ethyl Benzene

Concen: 2.750 ug/l

RT: 11.587 min Scan# 1

Delta R.T. -0.006 min

Lab File: VY014938.D

Acq: 02 Aug 2023 18:04

Instrument :

MSVOA_Y

ClientSampleId :





BUILDING-B-3-(5-10)

Tgt Ion: 91 Resp: 37632

Ion Ratio Lower Upper

91 100

106 31.2 24.6 36.8

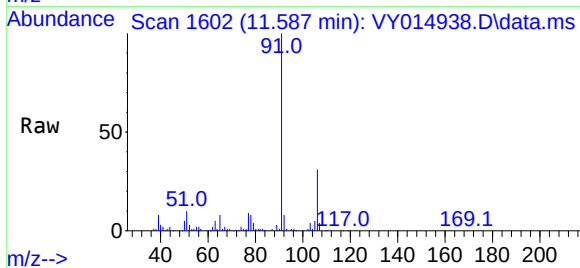

#68

m/p-Xylenes

Concen: 2.657 ug/l

RT: 11.697 min Scan# 1620

Delta R.T. -0.000 min

Lab File: VY014938.D




Acq: 02 Aug 2023 18:04


Tgt Ion:106 Resp: 13880

Ion Ratio Lower Upper

106 100

91 208.8 166.1 249.1

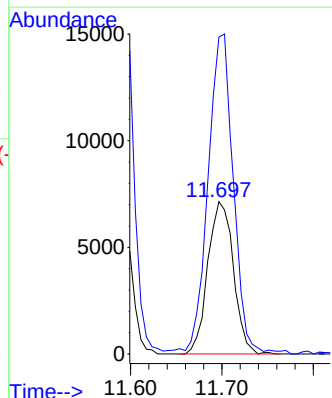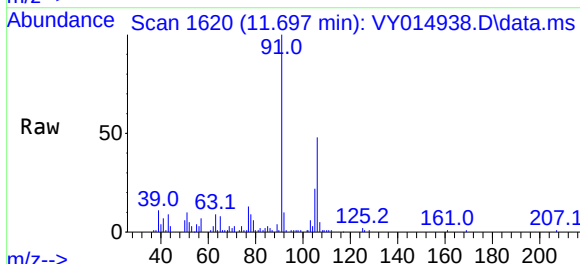



#69

o-Xylene

Concen: 6.446 ug/l

RT: 12.026 min Scan# 1

Delta R.T. -0.000 min

Lab File: VY014938.D

Acq: 02 Aug 2023 18:04

Instrument :

MSVOA_Y

ClientSampleId :


BUILDING-B-3-(5-10)

Tgt Ion:106 Resp: 32804




Ion Ratio Lower Upper

106 100

91 217.4 108.1 324.3

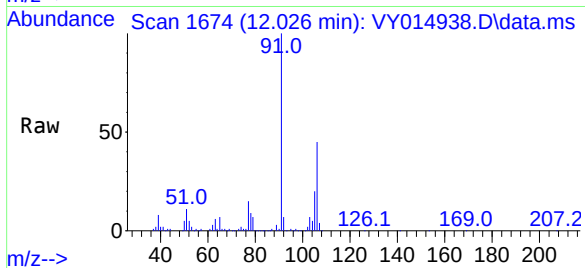

Abundance

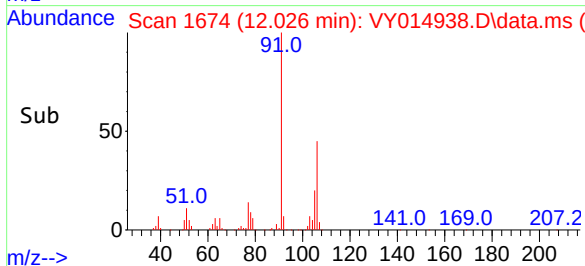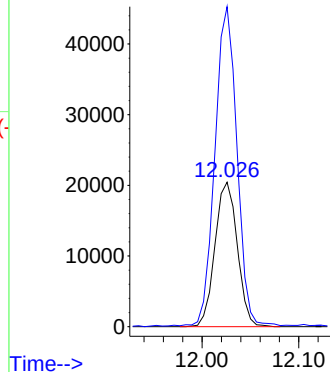

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.422 min Scan# 1903

Delta R.T. -0.000 min

Lab File: VY014938.D

Acq: 02 Aug 2023 18:04


Tgt Ion:152 Resp: 156812

Ion Ratio Lower Upper



152 100


115 69.7 28.8 86.5

150 159.1 0.0 348.8

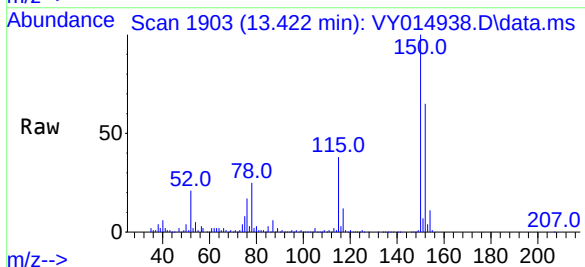

Abundance




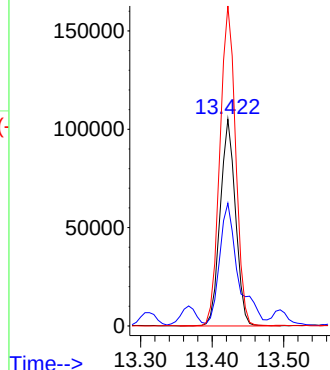




#73
Isopropylbenzene
Concen: 6.887 ug/l
RT: 12.325 min Scan# 1748
Delta R.T. -0.000 min
Lab File: VY014938.D
Acq: 02 Aug 2023 18:04




Instrument :
MSVOA_Y
ClientSampleId :
BUILDING-B-3-(5-10)


Tgt Ion:105 Resp: 84563
Ion Ratio Lower Upper
105 100
120 26.6 13.3 39.9

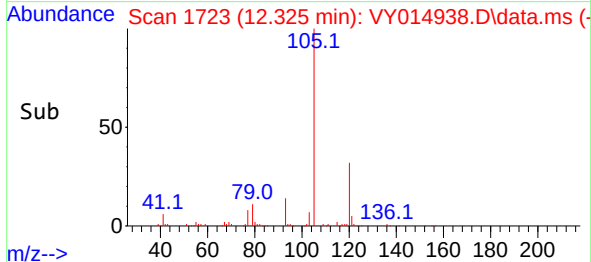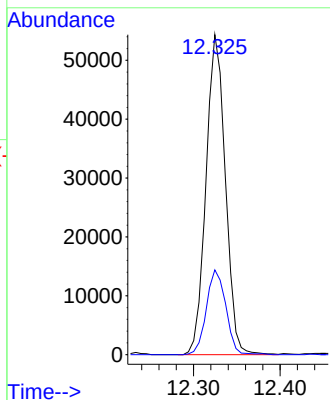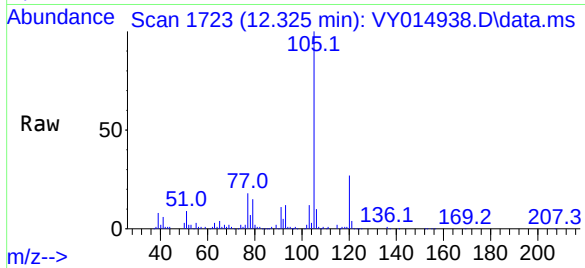

#76
1,2,3-Trichloropropane
Concen: 43.768 ug/l
RT: 12.477 min Scan# 1748
Delta R.T. -0.153 min
Lab File: VY014938.D
Acq: 02 Aug 2023 18:04

Tgt Ion: 75 Resp: 86683
Ion Ratio Lower Upper
75 100
77 1.6 0.0 0.0#


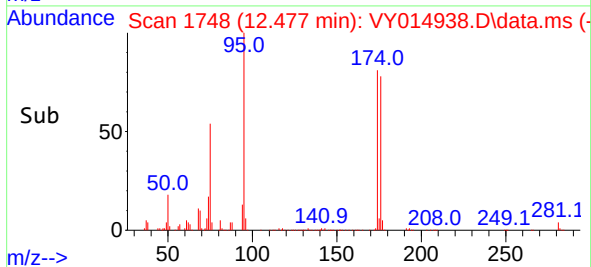
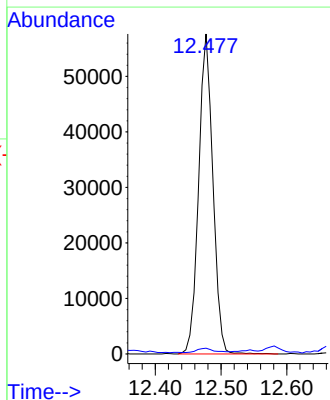
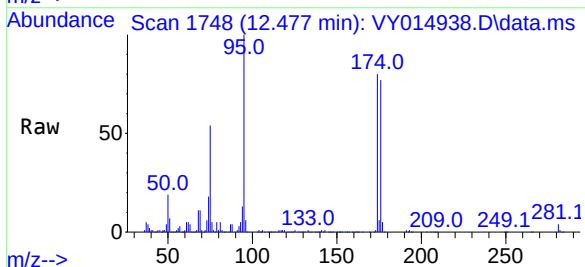




#78
n-propylbenzene
Concen: 4.440 ug/l
RT: 12.666 min Scan# 1779
Delta R.T. -0.000 min
Lab File: VY014938.D
Acq: 02 Aug 2023 18:04




Instrument :
MSVOA_Y
ClientSampleId :
BUILDING-B-3-(5-10)


Tgt Ion: 91 Resp: 65695
Ion Ratio Lower Upper
91 100
120 22.9 11.5 34.4

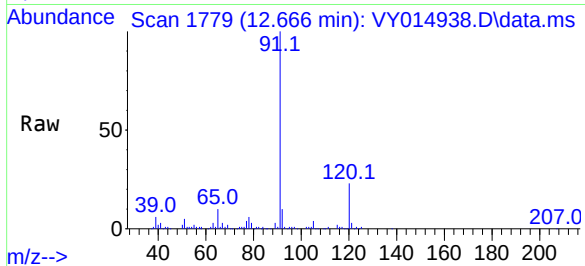

#79
2-Chlorotoluene
Concen: 3.096 ug/l
RT: 12.764 min Scan# 1795
Delta R.T. 0.013 min
Lab File: VY014938.D
Acq: 02 Aug 2023 18:04

Tgt Ion: 91 Resp: 26383
Ion Ratio Lower Upper
91 100
126 0.0 17.3 51.7#


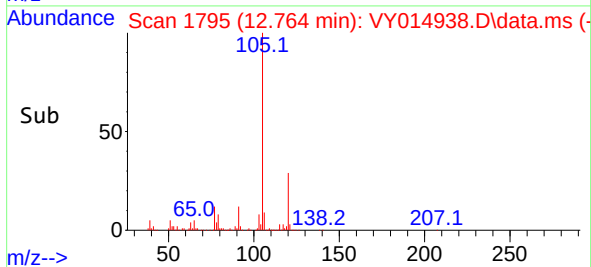

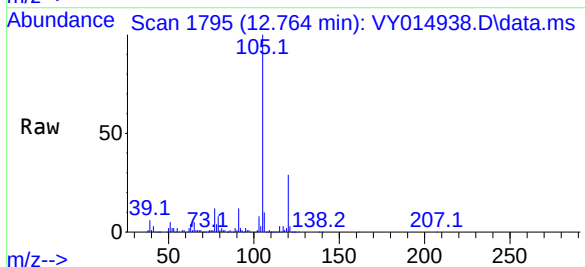




#80
1,3,5-Trimethylbenzene
Concen: 23.019 ug/l
RT: 12.806 min Scan# 11
Delta R.T. -0.006 min
Lab File: VY014938.D
Acq: 02 Aug 2023 18:04




Instrument :
MSVOA_Y
ClientSampleId :
BUILDING-B-3-(5-10)


Tgt Ion:105 Resp: 236045
Ion Ratio Lower Upper
105 100
120 51.4 23.9 71.7

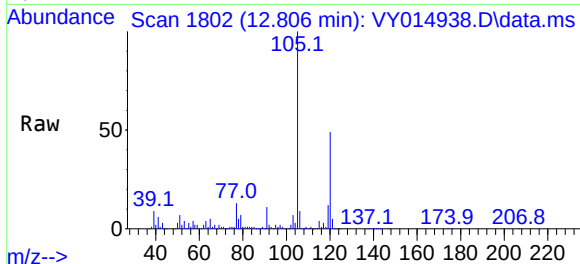

#81
trans-1,4-Dichloro-2-butene
Concen: 84.743 ug/l
RT: 12.477 min Scan# 1748
Delta R.T. 0.104 min
Lab File: VY014938.D
Acq: 02 Aug 2023 18:04

Tgt Ion: 75 Resp: 86683
Ion Ratio Lower Upper
75 100
53 0.3 77.8 116.8#
89 0.1 37.4 56.0#


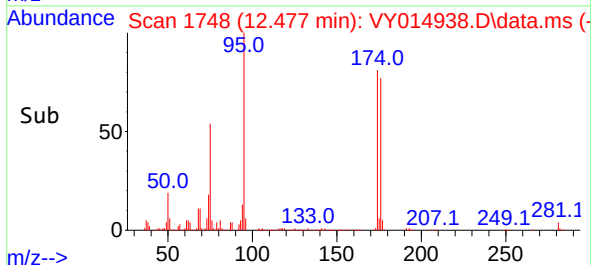
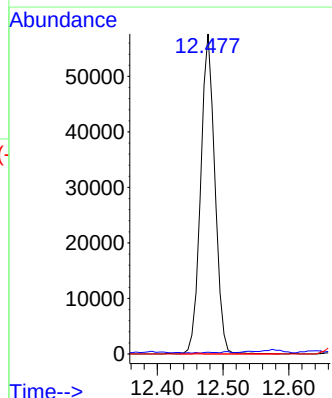
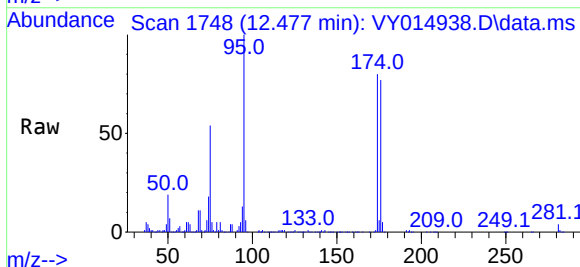




#82
4-Chlorotoluene
Concen: 2.937 ug/l
RT: 12.806 min Scan# 1802
Delta R.T. -0.043 min
Lab File: VY014938.D
Acq: 02 Aug 2023 18:04




Instrument :
MSVOA_Y
ClientSampleId :
BUILDING-B-3-(5-10)


Tgt Ion: 91 Resp: 25777
Ion Ratio Lower Upper
91 100
126 0.0 17.2 51.6#

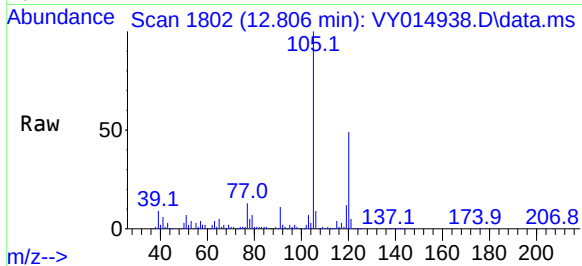

#83
tert-Butylbenzene
Concen: 6.405 ug/l
RT: 13.117 min Scan# 1853
Delta R.T. 0.042 min
Lab File: VY014938.D
Acq: 02 Aug 2023 18:04

Tgt Ion: 119 Resp: 58260
Ion Ratio Lower Upper
119 100
91 99.6 32.9 98.6#
134 0.0 13.0 38.9#


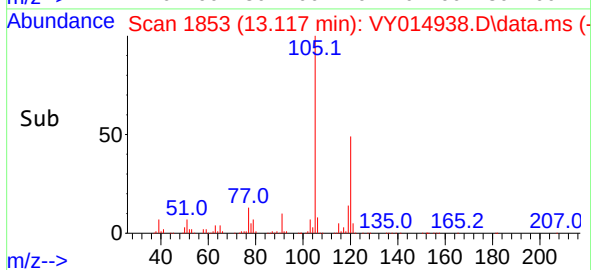

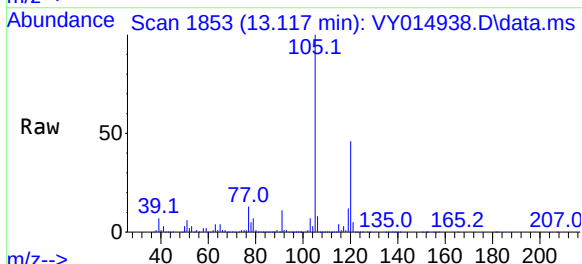




#84
1,2,4-Trimethylbenzene
Concen: 50.390 ug/l
RT: 13.117 min Scan# 1853
Delta R.T. 0.000 min
Lab File: VY014938.D
Acq: 02 Aug 2023 18:04




Instrument :
MSVOA_Y
ClientSampleId :
BUILDING-B-3-(5-10)


Tgt Ion:105 Resp: 507089
Ion Ratio Lower Upper
105 100
120 45.4 22.2 66.6

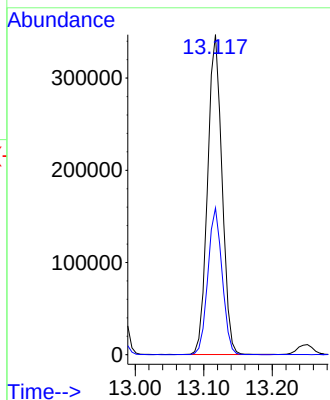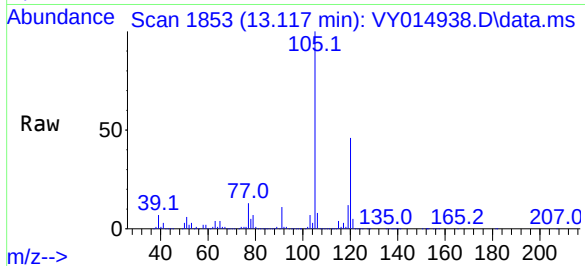

#85
sec-Butylbenzene
Concen: 1.290 ug/l
RT: 13.251 min Scan# 1875
Delta R.T. 0.000 min
Lab File: VY014938.D
Acq: 02 Aug 2023 18:04

Tgt Ion:105 Resp: 17218
Ion Ratio Lower Upper
105 100
134 31.2 10.2 30.6#


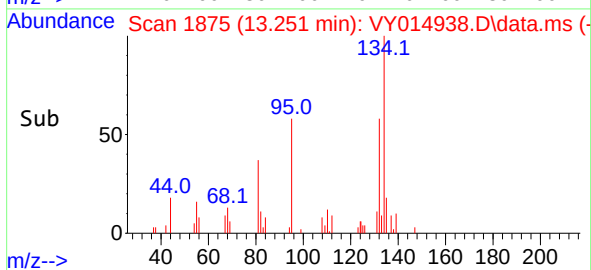
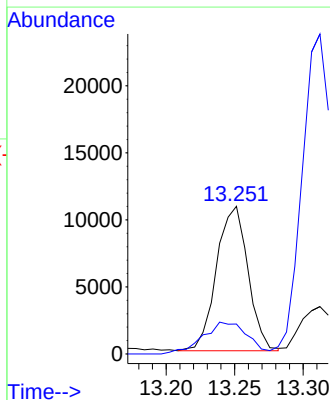
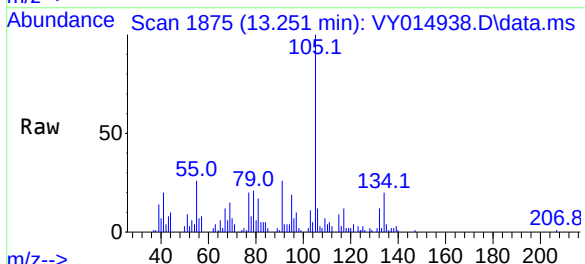




#86
p-Isopropyltoluene
Concen: 14.117 ug/l
RT: 13.367 min Scan# 1894
Delta R.T. 0.000 min
Lab File: VY014938.D
Acq: 02 Aug 2023 18:04




Instrument :
MSVOA_Y
ClientSampleId :
BUILDING-B-3-(5-10)


Tgt Ion:	119	Resp:	153803
Ion	Ratio	Lower	Upper
119	100		
134	26.4	13.3	39.8
91	26.9	12.4	37.4

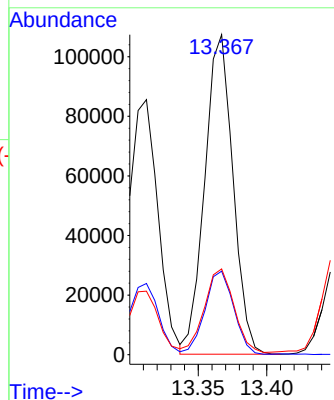

#89
n-Butylbenzene
Concen: 10.951 ug/l
RT: 13.660 min Scan# 1942
Delta R.T. -0.036 min
Lab File: VY014938.D
Acq: 02 Aug 2023 18:04

Tgt Ion:	91	Resp:	116069
Ion	Ratio	Lower	Upper
91	100		
92	3.0	25.4	76.0#
134	166.4	12.6	37.6#


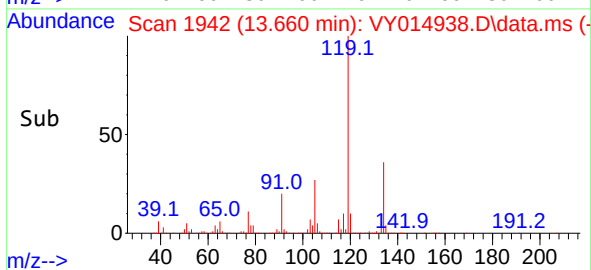
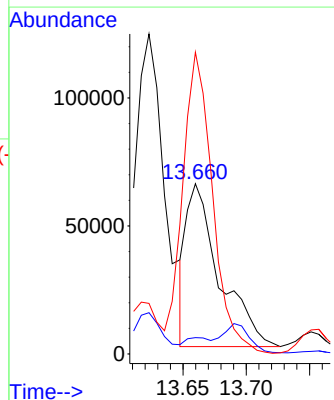





#90
Hexachloroethane
Concen: 48.818 ug/l
RT: 13.965 min Scan# 1991
Delta R.T. 0.006 min
Lab File: VY014938.D
Acq: 02 Aug 2023 18:04




Instrument :
MSVOA_Y
ClientSampleId :
BUILDING-B-3-(5-10)


Tgt Ion:117 Resp: 109243
Ion Ratio Lower Upper
117 100
201 0.0 41.6 124.8#

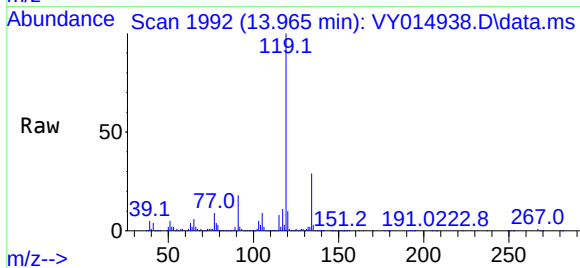

#92
1,2-Dibromo-3-Chloropropane
Concen: 2.908 ug/l
RT: 14.373 min Scan# 2059
Delta R.T. 0.018 min
Lab File: VY014938.D
Acq: 02 Aug 2023 18:04


Tgt Ion: 75 Resp: 1557
Ion Ratio Lower Upper
75 100
155 0.0 41.5 124.6#
157 0.0 51.8 155.5#

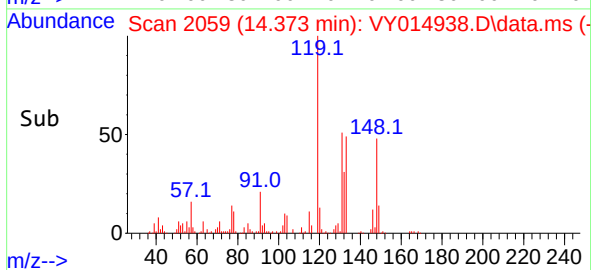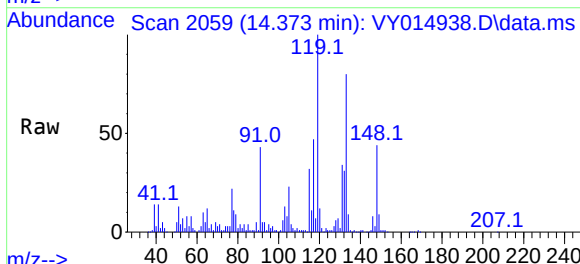



#95
Naphthalene
Concen: 1953.922 ug/l
RT: 15.233 min Scan# 21
Delta R.T. -0.000 min
Lab File: VY014938.D
Acq: 02 Aug 2023 18:04

Instrument :
MSVOA_Y
ClientSampleId :
BUILDING-B-3-(5-10)



Tgt Ion:128 Resp:14441911
Ion Ratio Lower Upper
128 100
127 15.0 10.8 16.2
129 13.5 8.6 13.0#

