



BFB

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY080223\
Data File : VY014927.D
Acq On : 02 Aug 2023 09:51
Operator : SY/MD
Sample : BFB
Misc : 5.02g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y071323S.M
Title : SW846 8260
Last Update : Fri Jul 14 02:09:50 2023

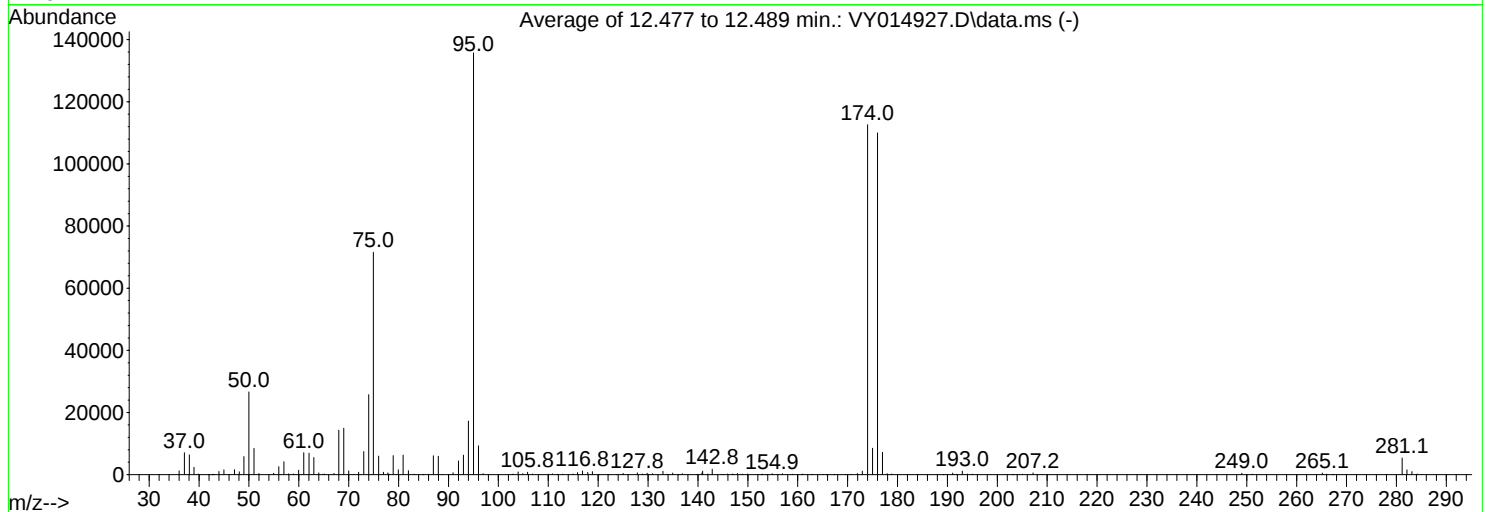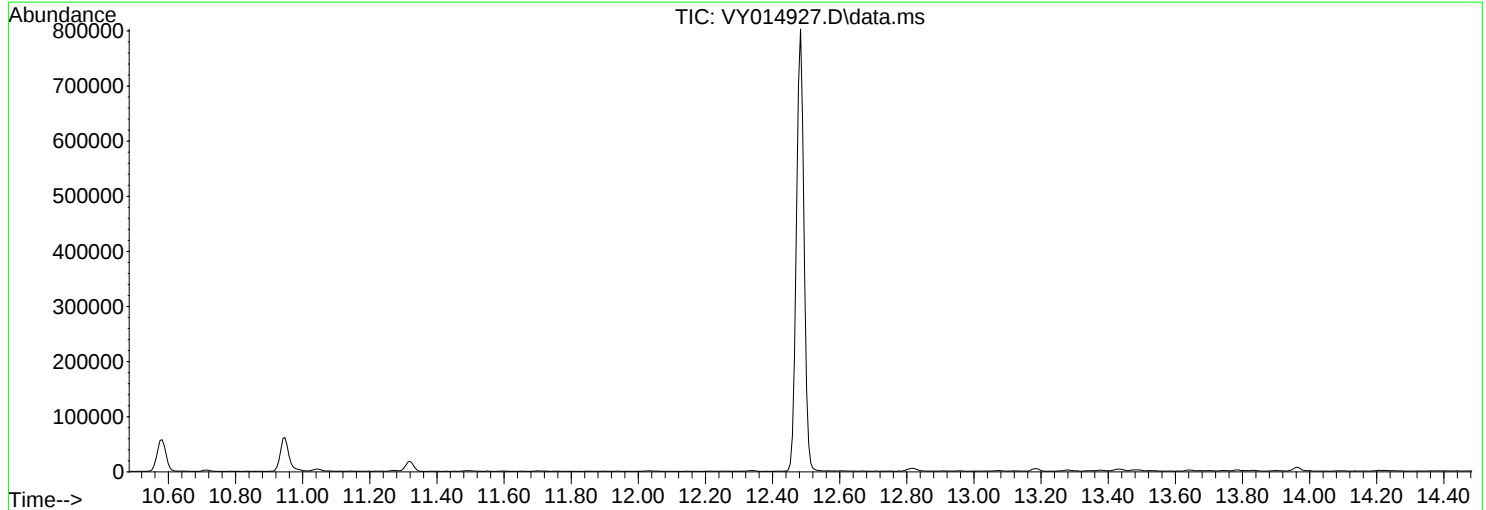

AutoFind: Scans 1748, 1749, 1750; Background Corrected with Scan 1740

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	19.6	26648	PASS
75	95	30	60	52.7	71564	PASS
95	95	100	100	100.0	135741	PASS
96	95	5	9	6.8	9254	PASS
173	174	0.00	2	1.0	1152	PASS
174	95	50	100	83.0	112635	PASS
175	174	5	9	7.5	8489	PASS
176	174	95	101	97.7	110003	PASS
177	176	5	9	6.6	7219	PASS