

Data Path : Z:\VOASRV\HPCHEM1\MSVOA Y\DATA\VY080320\
 Data File : VY003426.D
 Acq On : 03 Aug 2020 18:51
 Operator : SY/MD
 Sample : L3548-04
 Misc : 7.12G/5ML/MSVOA Y/SOIL
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 CRT-017

Quant Time: Aug 04 09:09:24 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_Y\METHODS\82Y073120S.M
 Quant Title : SW846 8260
 QLast Update : Fri Jul 31 13:09:26 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.80	168	443826	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.69	114	709949	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.49	117	662619	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.42	152	322929	50.00	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.14	65	233017	55.22	ug/l	0.00
Spiked Amount	50.000		Recovery	=	110.44%	
35) Dibromofluoromethane	7.72	113	223023	53.33	ug/l	0.00
Spiked Amount	50.000		Recovery	=	106.66%	
50) Toluene-d8	10.18	98	854301	52.17	ug/l	0.00
Spiked Amount	50.000		Recovery	=	104.34%	
62) 4-Bromofluorobenzene	12.48	95	283857	50.73	ug/l	0.00
Spiked Amount	50.000		Recovery	=	101.46%	


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA Y\DATA\VY080320\
Data File : VY003426.D
Acq On : 03 Aug 2020 18:51
Operator : SY/MD
Sample : L3548-04
Misc : 7.12G/5ML/MSVOA Y/SOIL
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
CRT-017

Quant Time: Aug 04 09:09:24 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_Y\METHODS\82Y073120S.M
Quant Title : SW846 8260
QLast Update : Fri Jul 31 13:09:26 2020
Response via : Initial Calibration

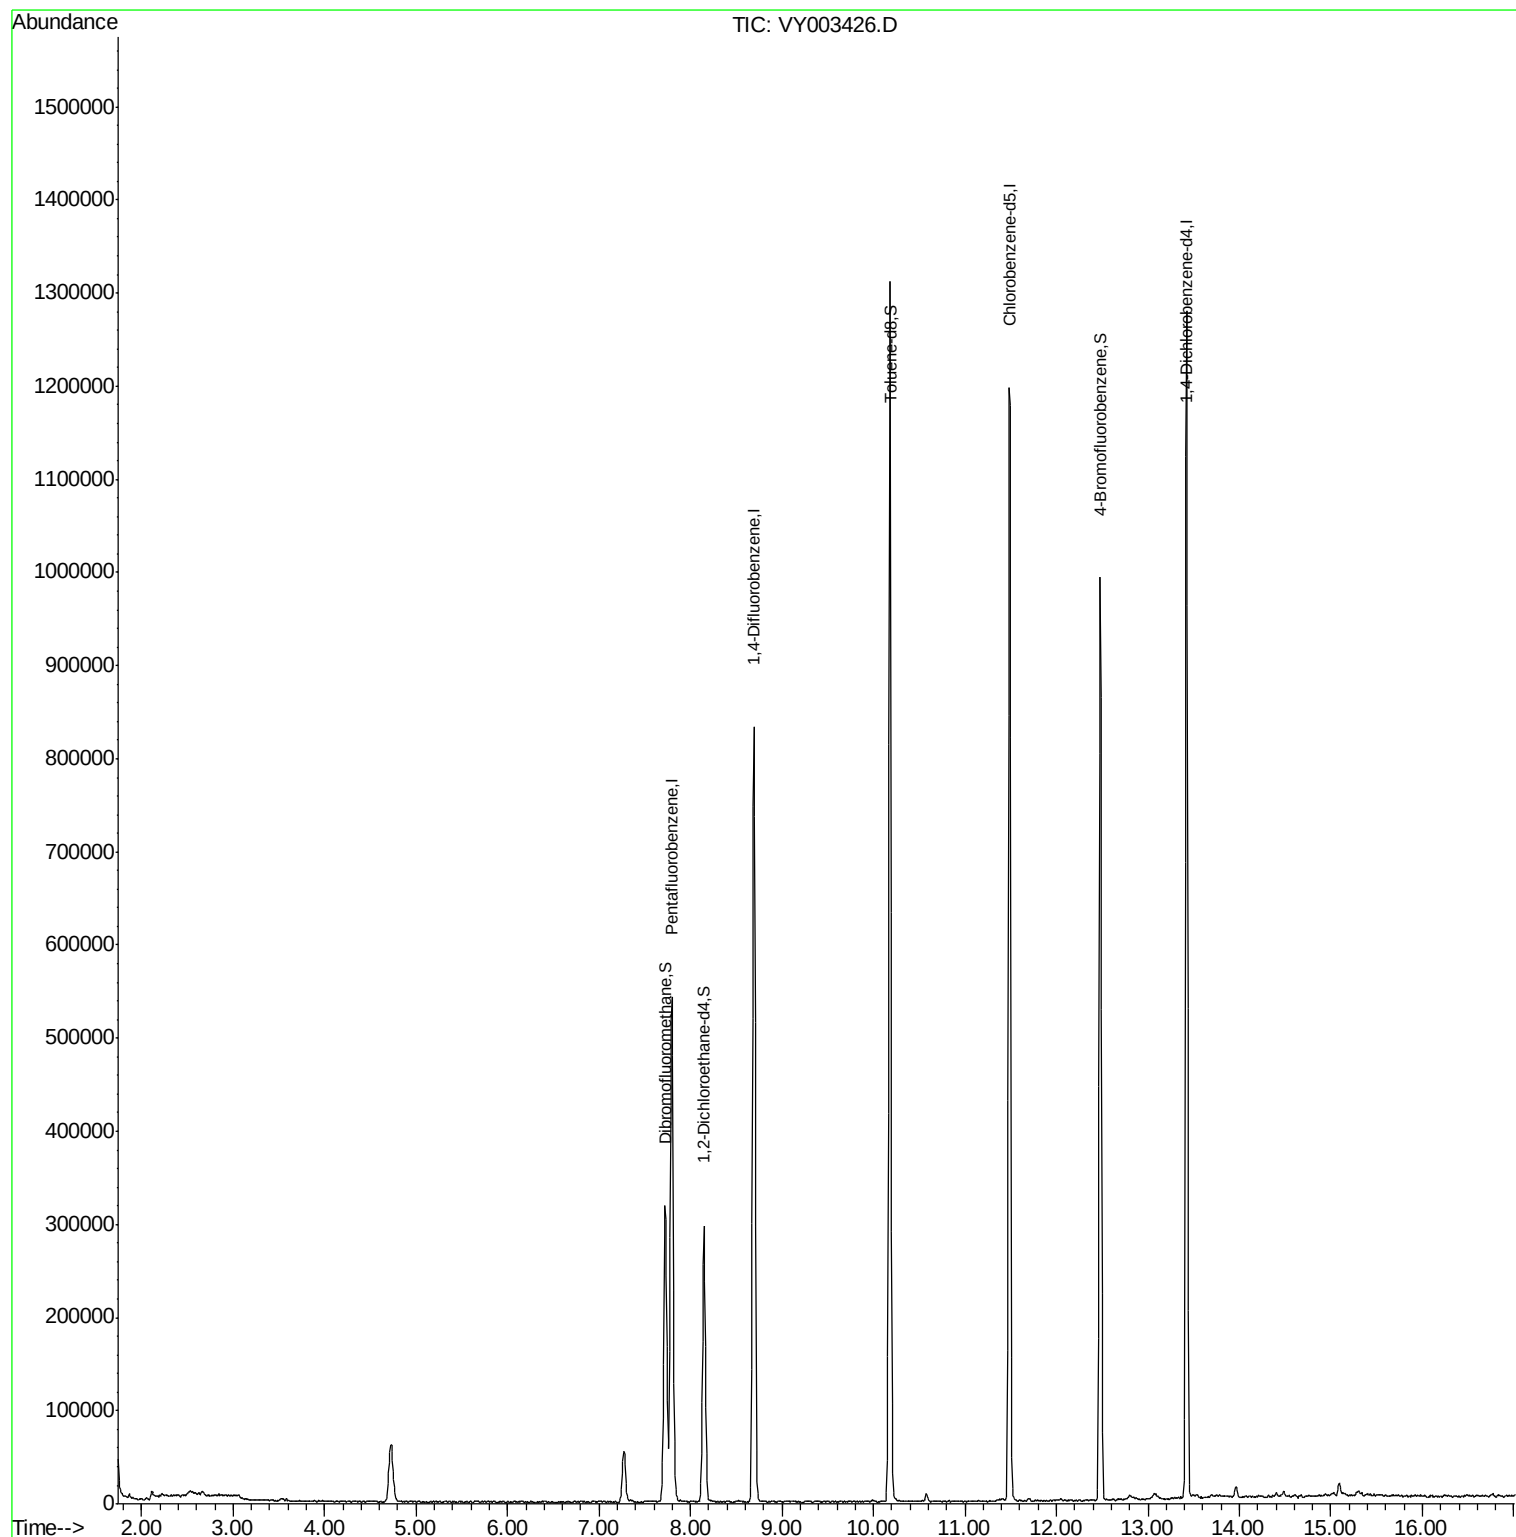

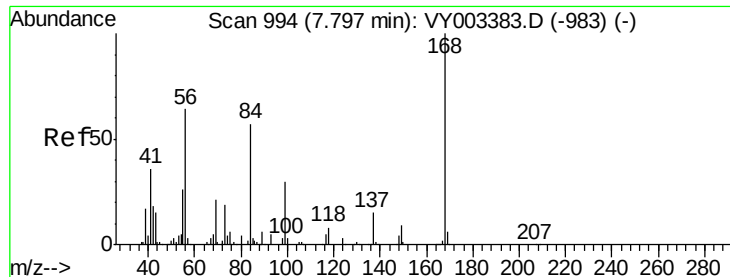

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.80 min Scan# 994

Delta R.T. -0.00 min

Lab File: VY003426.D

Acq: 03 Aug 2020 18:51

Instrument :

MSVOA_Y

ClientSampleId :


CRT-017

Tot Ion:168 Resp: 443826

Ion Ratio Lower Upper

168 100

99 50.4 38.8 58.2

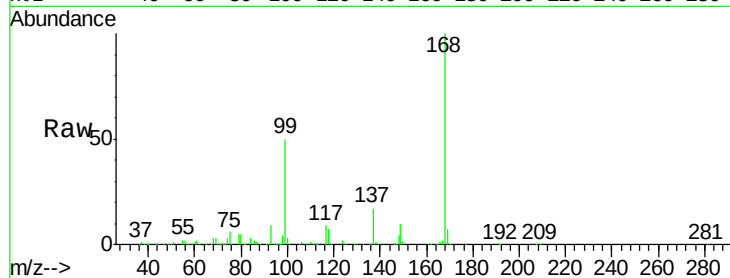

Abundance Ion 167.90 (167.60 to 168.60): VY003383.D (-983) (-)

Ion 98.90 (98.60 to 99.60): VY003383.D (-983) (-)

7.80

200000



150000

100000

50000

0

Time-->

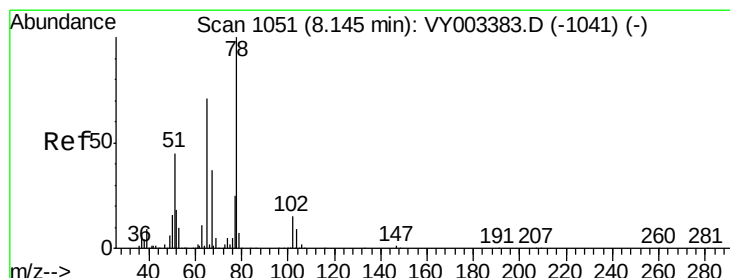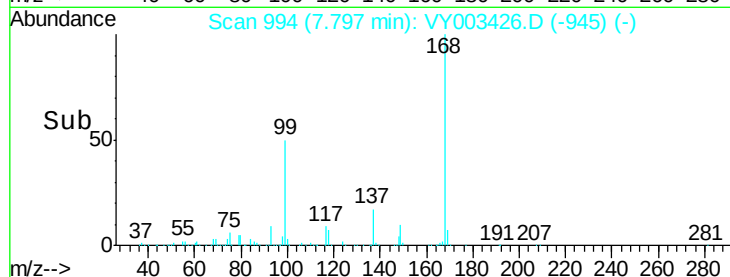

#33

1,2-Dichloroethane-d4

Concen: 55.218 ug/l

RT: 8.14 min Scan# 1051

Delta R.T. -0.00 min

Lab File: VY003426.D


Acq: 03 Aug 2020 18:51

Tgt Ion: 65 Resp: 233017

Ion Ratio Lower Upper

65 100

67 53.6 0.0 106.6

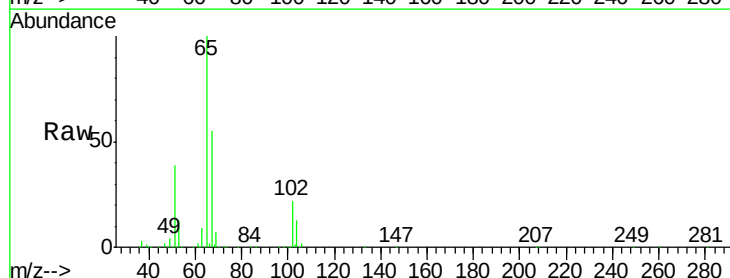

Abundance Ion 64.90 (64.60 to 65.60): VY003383.D (-1041) (-)

Ion 66.90 (66.60 to 67.60): VY003383.D (-1041) (-)

8.14

120000

100000

80000


60000


40000

20000

0

Time-->

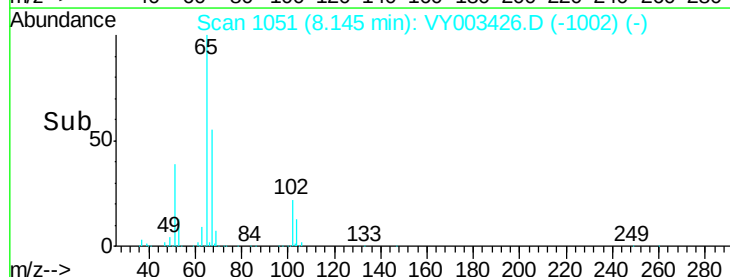


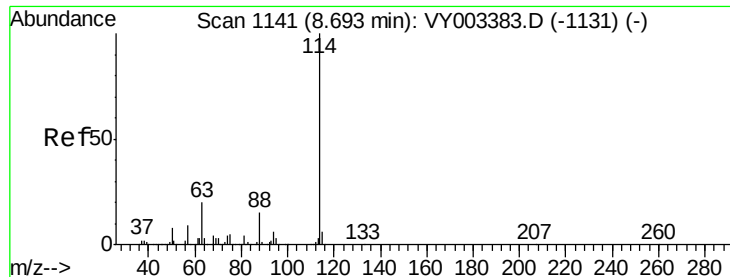




#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 8.69 min Scan# 1141
 Delta R.T. -0.00 min
 Lab File: VY003426.D
 Acq: 03 Aug 2020 18:51

Instrument :
 MSVOA_Y
 ClientSampleId :
 CRT-017

Tot Ion:114	Resp:	709949
Ion	Ratio	Lower Upper
114	100	
63	19.9	0.0 40.6
88	15.3	0.0 29.2

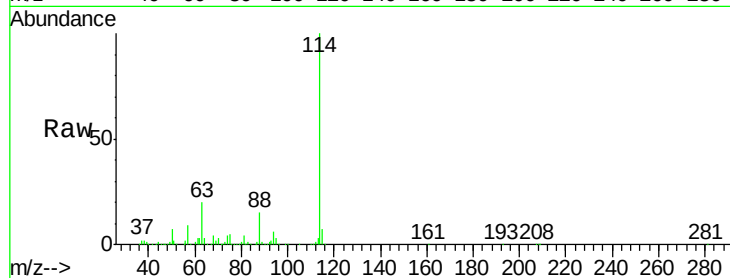


Abundance Ion 113.90 (113.60 to 114.60): V
 Ion 63.00 (62.70 to 63.70): VY0
 Ion 87.90 (87.60 to 88.60): VY0

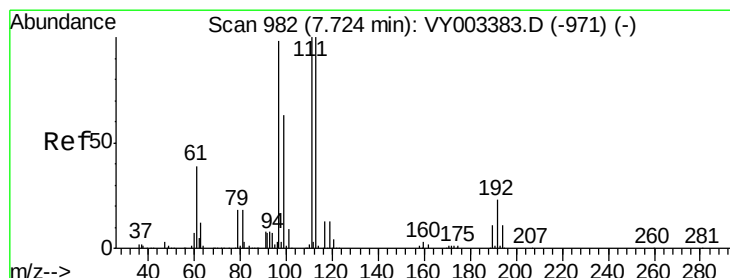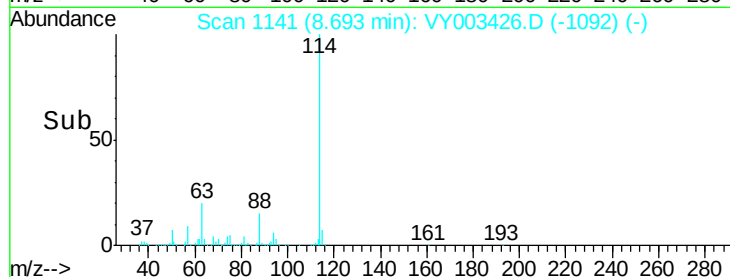
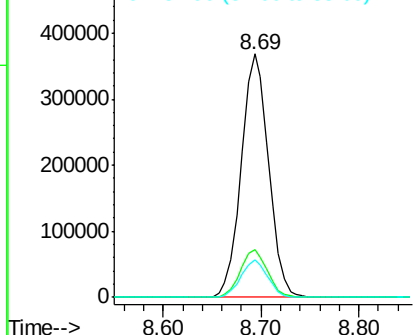



#35
 Dibromofluoromethane
 Concen: 53.329 ug/l
 RT: 7.72 min Scan# 982
 Delta R.T. -0.00 min
 Lab File: VY003426.D
 Acq: 03 Aug 2020 18:51

Tgt Ion:113	Resp:	223023
Ion	Ratio	Lower Upper
113	100	
111	103.1	83.0 124.4
192	22.8	18.8 28.2

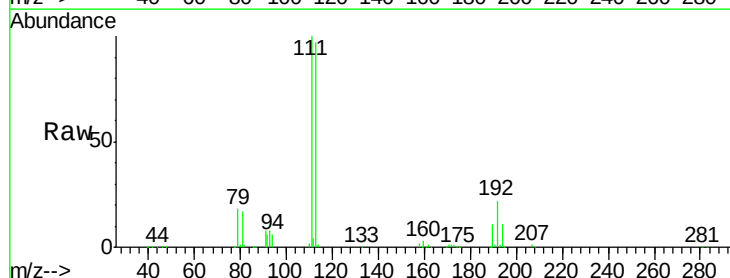

Abundance Ion 112.80 (112.50 to 113.50): V
 Ion 110.80 (110.50 to 111.50): V
 Ion 191.70 (191.40 to 192.40): V

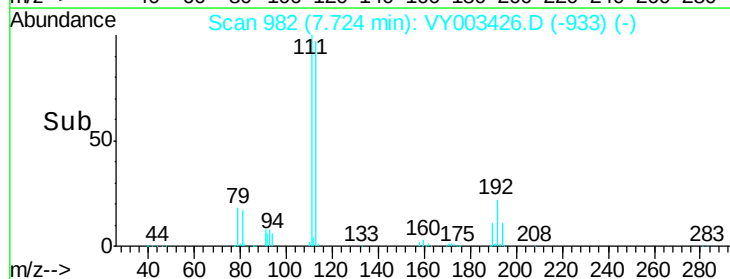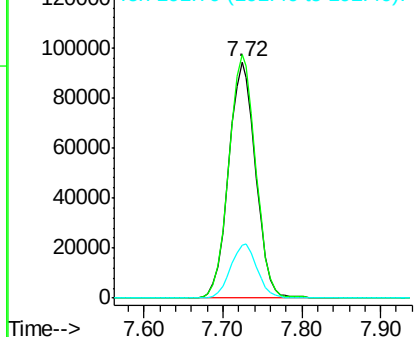

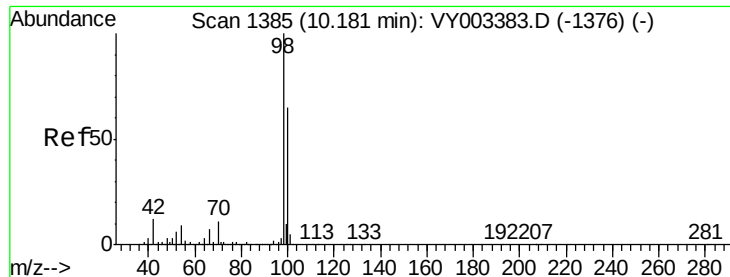

#50

Toluene-d8

Concen: 52.167 ug/l

RT: 10.18 min Scan# 1385

Delta R.T. -0.00 min

Lab File: VY003426.D

Acq: 03 Aug 2020 18:51

Instrument :

MSVOA_Y

ClientSampleId :





CRT-017

Tot Ion: 98 Resp: 854301

Ion Ratio Lower Upper

98 100

100 64.3 51.3 76.9

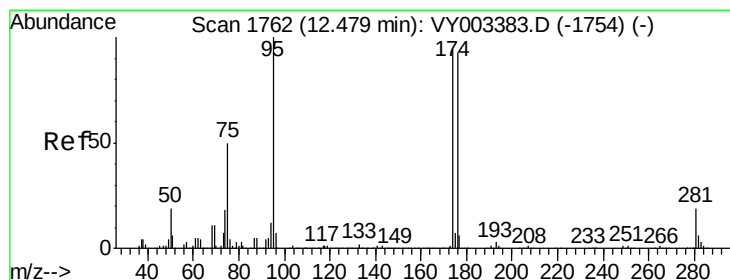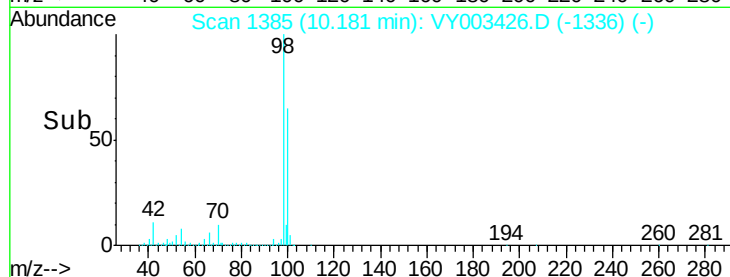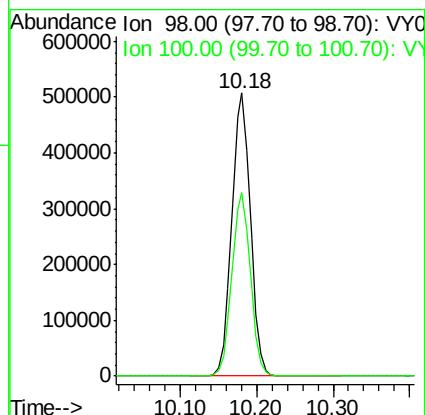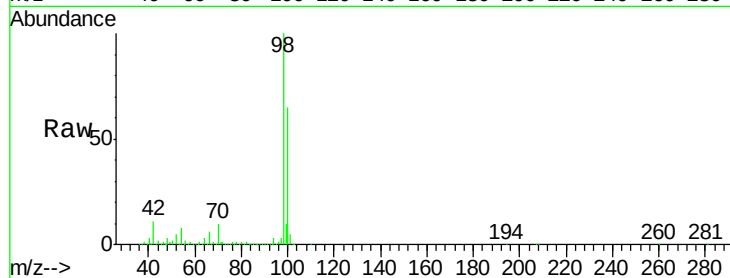

#62

4-Bromofluorobenzene

Concen: 50.731 ug/l

RT: 12.48 min Scan# 1762

Delta R.T. -0.00 min

Lab File: VY003426.D

Acq: 03 Aug 2020 18:51




Tgt Ion: 95 Resp: 283857


Ion Ratio Lower Upper

95 100

174 95.5 0.0 190.0

176 92.1 0.0 184.4


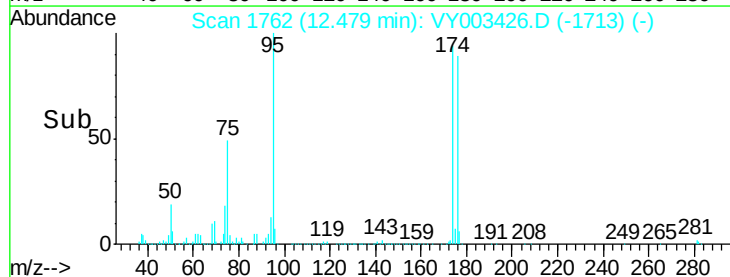
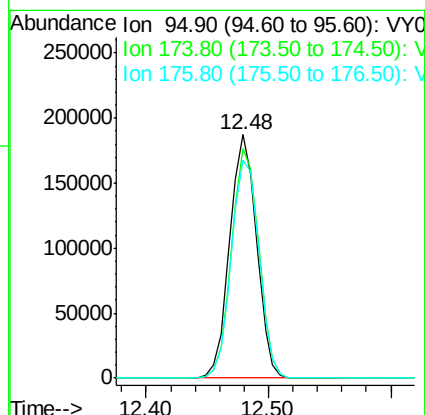
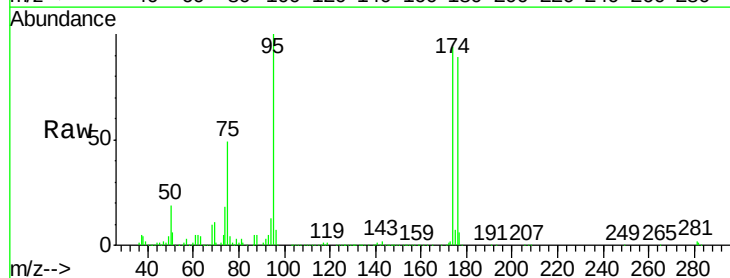


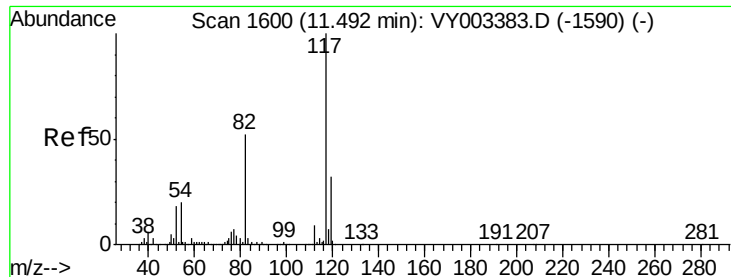

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.49 min Scan# 1599
Delta R.T. -0.01 min
Lab File: VY003426.D
Acq: 03 Aug 2020 18:51

Instrument :
MSVOA_Y
ClientSampleId :
CRT-017

Tot Ion:117 Resp: 662619
Ion Ratio Lower Upper
117 100
82 54.7 41.9 62.9
119 30.8 25.4 38.0

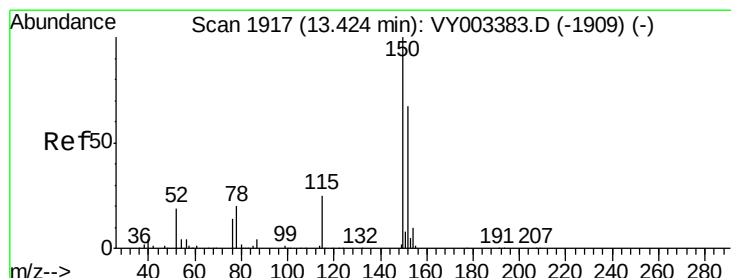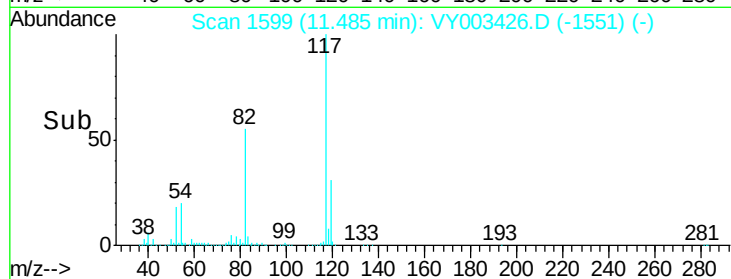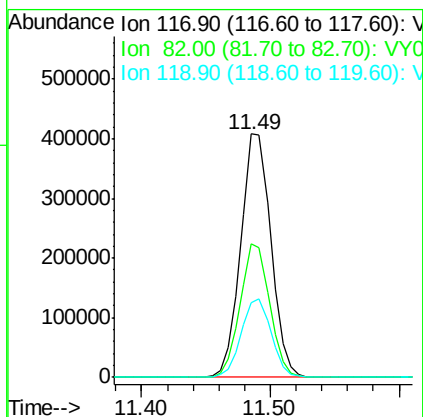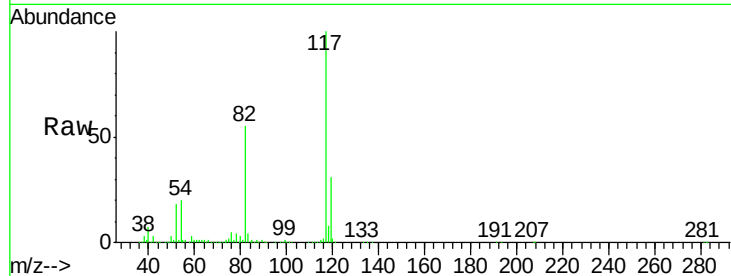

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.42 min Scan# 1917
Delta R.T. -0.00 min
Lab File: VY003426.D
Acq: 03 Aug 2020 18:51

Tgt Ion:152 Resp: 322929
Ion Ratio Lower Upper
152 100
115 55.6 27.2 81.5
150 159.9 0.0 346.8

