


Data Path : Z:\voasrv\HPCHEM1\MSVOA Y\Data\vv080320\
 Data File : VY003404.D
 Acq On : 03 Aug 2020 09:29
 Operator : SY/MD
 Sample : BFB
 Misc : 5.00G/5ML/MSVOA Y/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_Y\METHODS\82Y073120S.M
 Title : SW846 8260
 Last Update : Fri Jul 31 13:09:26 2020

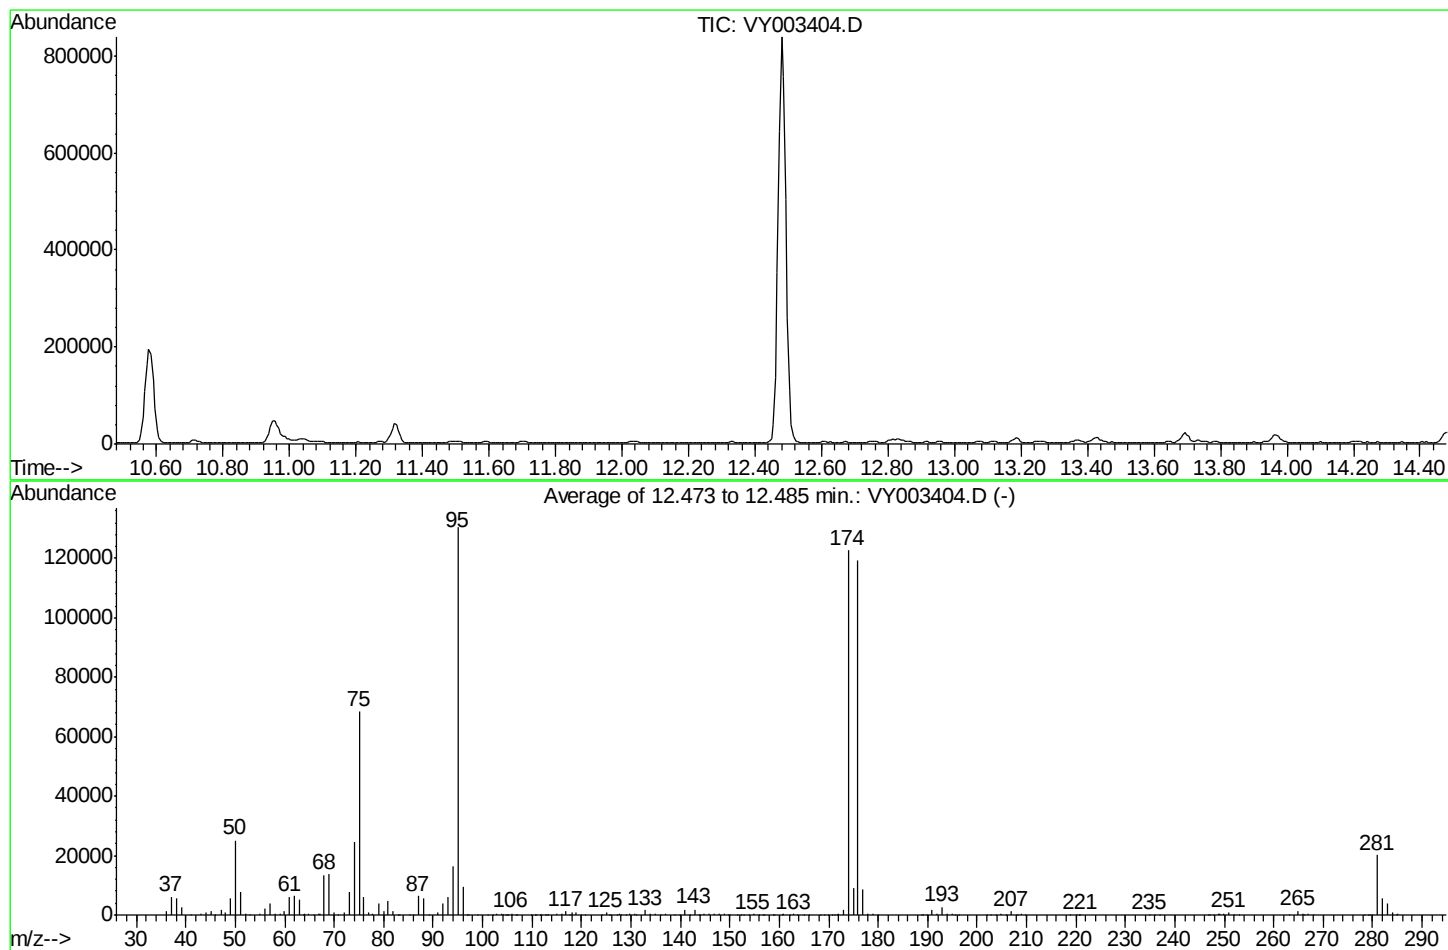

AutoFind: Scans 1761, 1762, 1763; Background Corrected with Scan 1753

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.3	25186	PASS
75	95	30	60	52.5	68416	PASS
95	95	100	100	100.0	130440	PASS
96	95	5	9	7.2	9353	PASS
173	174	0.00	2	1.5	1882	PASS
174	95	50	100	94.0	122584	PASS
175	174	5	9	7.4	9115	PASS
176	174	95	101	97.5	119520	PASS
177	176	5	9	7.2	8609	PASS