

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY080421\
 Data File : VY005531.D
 Acq On : 04 Aug 2021 12:42
 Operator : SY/MD
 Sample : M3271-01
 Misc : 5.01G/5ML/MSVOA_Y/SOIL
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :

Quant Time: Aug 05 06:38:26 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y080221S.M
 Quant Title : SW846 8260
 QLast Update : Tue Aug 03 04:52:05 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	7.801	168	7508	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.697	114	12085	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.490	117	11129	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.428	152	3774	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.149	65	4226	55.605	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	111.220%
35) Dibromofluoromethane	7.722	113	3257	48.137	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	96.280%
50) Toluene-d8	10.185	98	14512	51.141	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	=	102.280%
62) 4-Bromofluorobenzene	12.483	95	3910	41.609	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	=	83.220%
Target Compounds						
					Qvalue	
3) Chloromethane	2.119	50	96	1.303	ug/l #	42
4) Vinyl Chloride	2.278	62	270	3.060	ug/l #	42
5) Bromomethane	2.674	94	101	1.739	ug/l	98
6) Chloroethane	2.802	64	162	3.042	ug/l #	42
10) Methyl Iodide	4.107	142	785	9.834	ug/l #	86
16) Acetone	3.954	43	346	18.057	ug/l #	45
20) Methylene Chloride	4.716	84	573	1.684	ug/l #	71
21) trans-1,2-Dichloroethene	5.253	96	132	1.825	ug/l #	1
36) 1,1-Dichloropropene	7.801	75	513	4.526	ug/l #	41
38) Carbon Tetrachloride	7.807	117	599	4.862	ug/l #	13
64) Tetrachloroethene	10.727	164	187	2.207	ug/l #	1
68) m/p-Xylenes	11.703	106	307	1.946	ug/l #	54
76) 1,2,3-Trichloropropane	12.483	75	2189	55.971	ug/l #	100
78) n-propylbenzene	12.678	91	499	1.595	ug/l #	66
79) 2-Chlorotoluene	12.758	91	316	1.799	ug/l	88
80) 1,3,5-Trimethylbenzene	12.819	105	361	1.651	ug/l	92
81) trans-1,4-Dichloro-2-b...	12.483	75	2189	112.830	ug/l #	11
82) 4-Chlorotoluene	12.855	91	315	1.733	ug/l	92
83) tert-Butylbenzene	13.081	119	265	1.351	ug/l #	65
84) 1,2,4-Trimethylbenzene	13.129	105	440	2.040	ug/l	70
85) sec-Butylbenzene	13.257	105	401	1.417	ug/l #	66
86) p-Isopropyltoluene	13.373	119	476	1.959	ug/l #	76
87) 1,3-Dichlorobenzene	13.373	146	339	2.684	ug/l	83
88) 1,4-Dichlorobenzene	13.453	146	409	3.265	ug/l	90
89) n-Butylbenzene	13.696	91	392	1.781	ug/l	92
91) 1,2-Dichlorobenzene	13.739	146	327	2.931	ug/l #	83
92) 1,2-Dibromo-3-Chloropr...	14.416	75	41	4.269	ug/l #	1
93) 1,2,4-Trichlorobenzene	15.013	180	266	3.471	ug/l #	72
94) Hexachlorobutadiene	15.129	225	125	2.519	ug/l #	67
95) Naphthalene	15.245	128	463	3.065	ug/l #	69
96) 1,2,3-Trichlorobenzene	15.428	180	254	3.742	ug/l	78


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY080421\
Data File : VY005531.D
Acq On : 04 Aug 2021 12:42
Operator : SY/MD
Sample : M3271-01
Misc : 5.01G/5ML/MSVOA_Y/SOIL
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :

Quant Time: Aug 05 06:38:26 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y080221S.M
Quant Title : SW846 8260
QLast Update : Tue Aug 03 04:52:05 2021
Response via : Initial Calibration




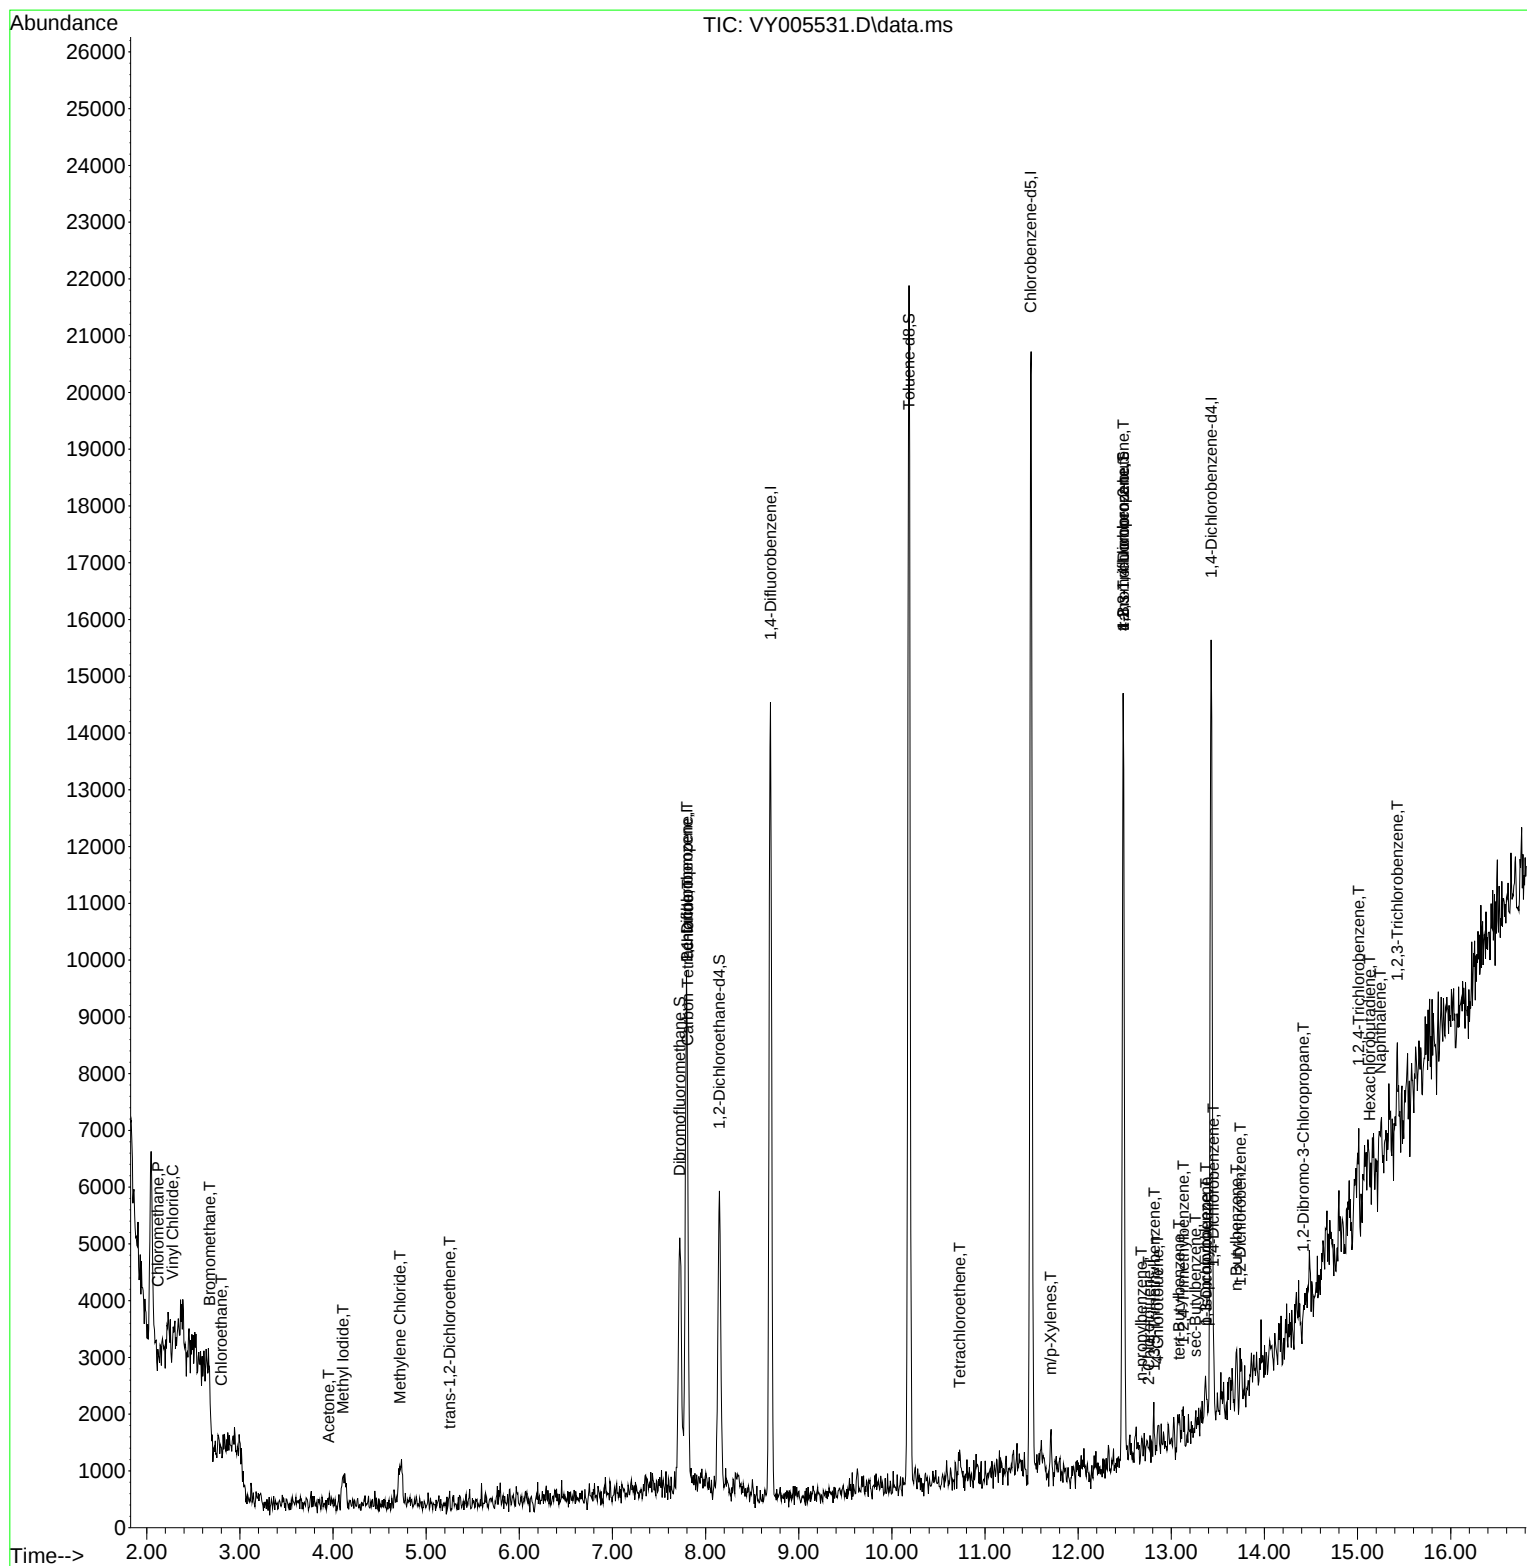




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.801 min Scan# 981
Delta R.T. 0.000 min
Lab File: VY005531.D
Acq: 04 Aug 2021 12:42




Instrument :
MSVOA_Y
ClientSampleId :


Tgt Ion:168 Resp: 7508
Ion Ratio Lower Upper
168 100
99 43.7 38.9 58.3



#3
Chloromethane
Concen: 1.303 ug/l
RT: 2.119 min Scan# 49
Delta R.T. -0.000 min
Lab File: VY005531.D
Acq: 04 Aug 2021 12:42

Tgt Ion: 50 Resp: 96
Ion Ratio Lower Upper
50 100
52 0.0 26.4 39.6#


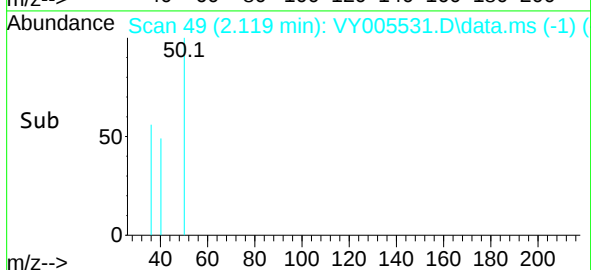
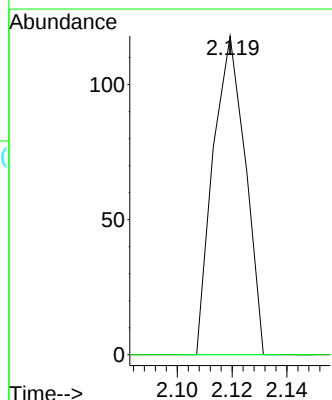



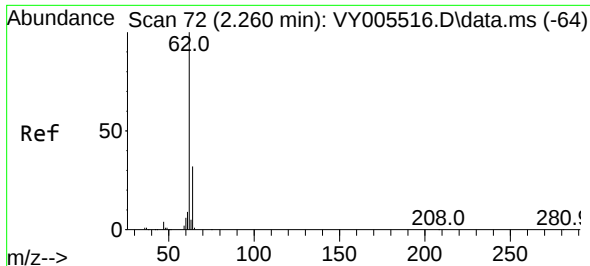

#4
 Vinyl Chloride
 Concen: 3.060 ug/l
 RT: 2.278 min Scan# 75
 Delta R.T. 0.018 min
 Lab File: VY005531.D
 Acq: 04 Aug 2021 12:42




Instrument :
 MSVOA_Y
 ClientSampled :


Tgt Ion: 62 Resp: 270
 Ion Ratio Lower Upper
 62 100
 64 0.0 25.9 38.9#

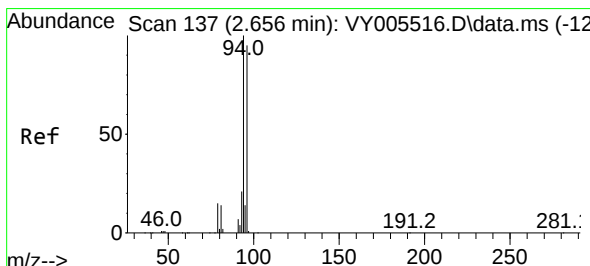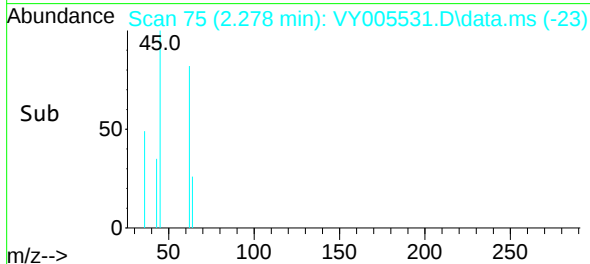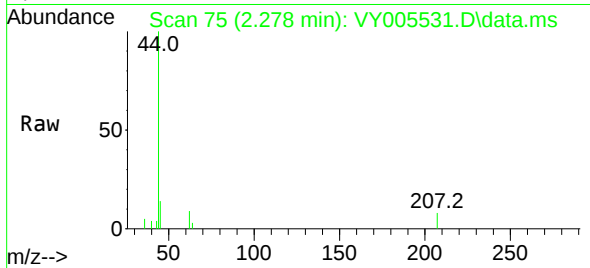

#5
 Bromomethane
 Concen: 1.739 ug/l
 RT: 2.674 min Scan# 140
 Delta R.T. 0.018 min
 Lab File: VY005531.D
 Acq: 04 Aug 2021 12:42


Tgt Ion: 94 Resp: 101
 Ion Ratio Lower Upper
 94 100
 96 92.9 75.7 113.5

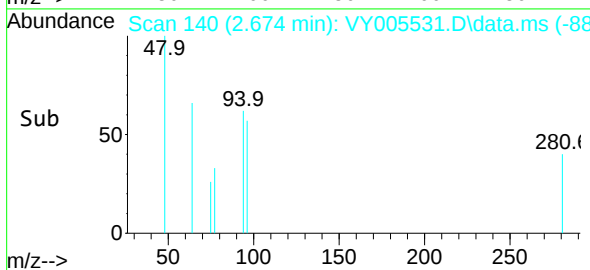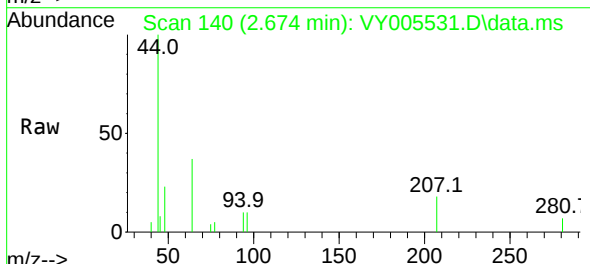






#6
Chloroethane
Concen: 3.042 ug/l
RT: 2.802 min Scan# 161
Delta R.T. -0.000 min
Lab File: VY005531.D
Acq: 04 Aug 2021 12:42


Instrument :
MSVOA_Y
ClientSampled :





Tgt Ion: 64 Resp: 162
Ion Ratio Lower Upper
64 100
66 0.0 26.1 39.1#




#10
Methyl Iodide
Concen: 9.834 ug/l
RT: 4.107 min Scan# 375
Delta R.T. 0.006 min
Lab File: VY005531.D
Acq: 04 Aug 2021 12:42



Tgt Ion: 142 Resp: 785
Ion Ratio Lower Upper
142 100
127 53.6 36.6 54.8
141 6.2 12.2 18.4#



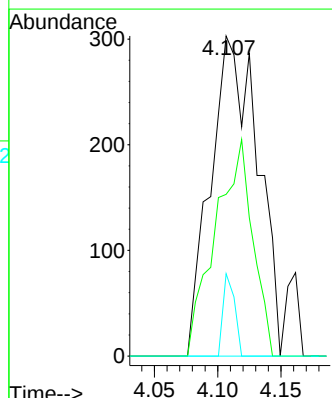





#16
Acetone
Concen: 18.057 ug/l
RT: 3.954 min Scan# 350
Delta R.T. -0.006 min
Lab File: VY005531.D
Acq: 04 Aug 2021 12:42




Instrument :
MSVOA_Y
ClientSampled :


Tgt Ion: 43 Resp: 346
Ion Ratio Lower Upper
43 100
58 0.0 23.8 35.6#

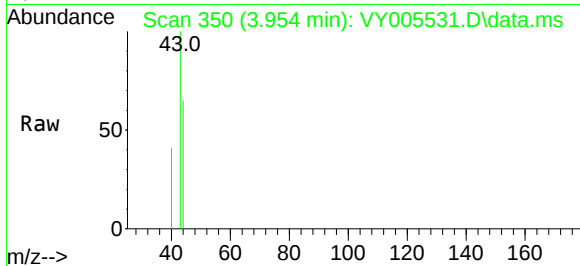

#20
Methylene Chloride
Concen: 1.684 ug/l
RT: 4.716 min Scan# 475
Delta R.T. -0.013 min
Lab File: VY005531.D
Acq: 04 Aug 2021 12:42


Tgt Ion: 84 Resp: 573
Ion Ratio Lower Upper
84 100
49 102.3 105.8 158.6#
51 0.0 33.4 50.2#
86 56.3 54.2 81.4

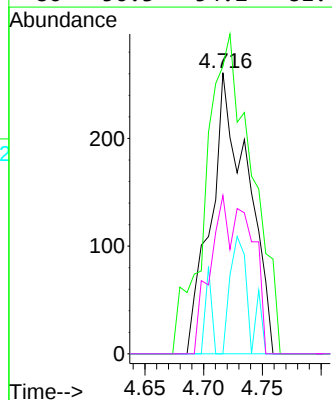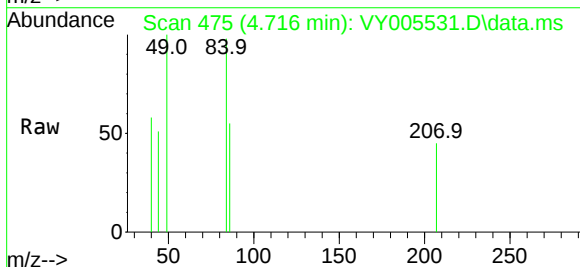






#21
trans-1,2-Dichloroethene
Concen: 1.825 ug/l
RT: 5.253 min Scan# 563
Delta R.T. 0.018 min
Lab File: VY005531.D
Acq: 04 Aug 2021 12:42

Instrument :
MSVOA_Y
ClientSampled :







Tgt Ion: 96 Resp: 132
Ion Ratio Lower Upper
96 100
61 0.0 112.6 168.8#
98 0.0 52.2 78.4#



#33
1,2-Dichloroethane-d4
Concen: 55.605 ug/l
RT: 8.149 min Scan# 1038
Delta R.T. -0.000 min
Lab File: VY005531.D
Acq: 04 Aug 2021 12:42

Tgt Ion: 65 Resp: 4226
Ion Ratio Lower Upper
65 100
67 50.7 0.0 103.4









#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.697 min Scan# 1128
Delta R.T. -0.000 min
Lab File: VY005531.D
Acq: 04 Aug 2021 12:42




Instrument :
MSVOA_Y
ClientSampleId :


Tgt Ion:	114	Resp:	12085
Ion Ratio	Lower	Upper	
114	100		
63	21.7	0.0	39.2
88	14.5	0.0	30.8

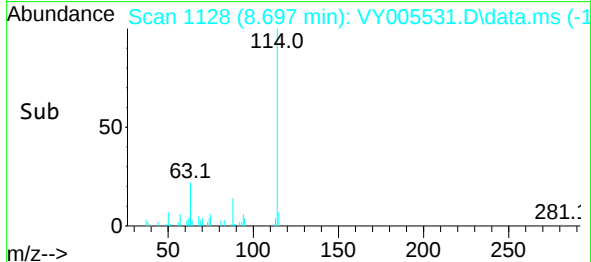

#35
Dibromofluoromethane
Concen: 48.137 ug/l
RT: 7.722 min Scan# 968
Delta R.T. -0.006 min
Lab File: VY005531.D
Acq: 04 Aug 2021 12:42

Tgt Ion:	113	Resp:	3257
Ion Ratio	Lower	Upper	
113	100		
111	99.8	81.9	122.9
192	24.5	19.2	28.8



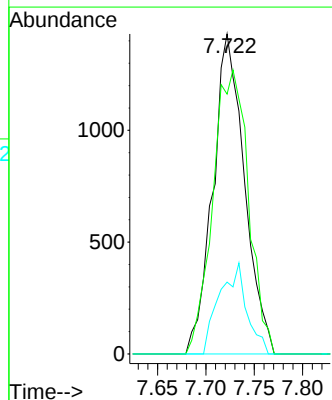
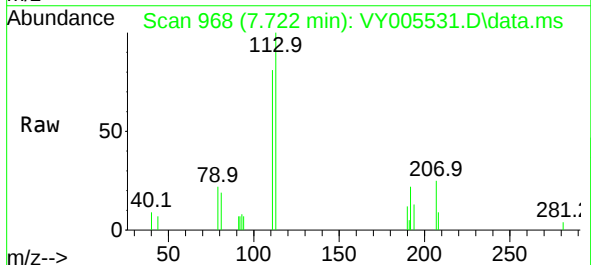




#36
 1,1-Dichloropropene
 Concen: 4.526 ug/l
 RT: 7.801 min Scan# 981
 Delta R.T. -0.122 min
 Lab File: VY005531.D
 Acq: 04 Aug 2021 12:42




Instrument :
 MSVOA_Y
 ClientSampleId :


Tgt Ion: 75	Resp: 513
Ion Ratio	Lower Upper
75 100	
110 0.0	18.1 54.1#
77 0.0	25.1 37.7#

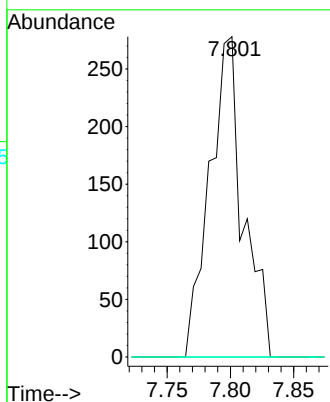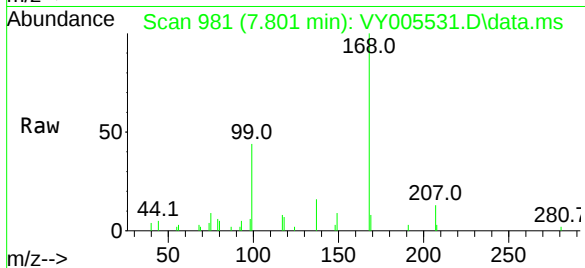

#38
 Carbon Tetrachloride
 Concen: 4.862 ug/l
 RT: 7.807 min Scan# 982
 Delta R.T. -0.104 min
 Lab File: VY005531.D
 Acq: 04 Aug 2021 12:42

Tgt Ion: 117	Resp: 599
Ion Ratio	Lower Upper
117 100	
119 0.0	75.4 113.0#
121 0.0	25.1 37.7#



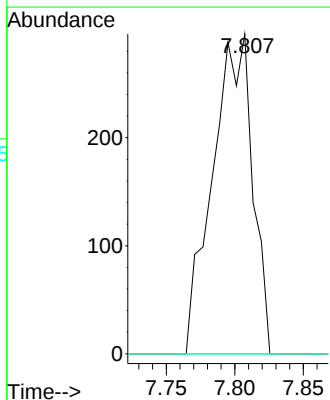
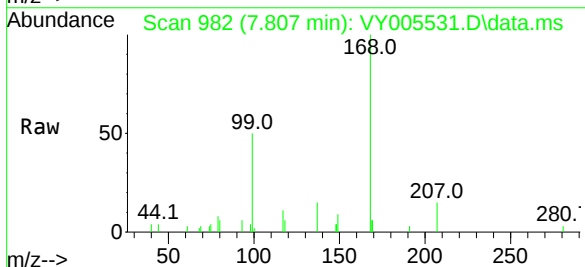


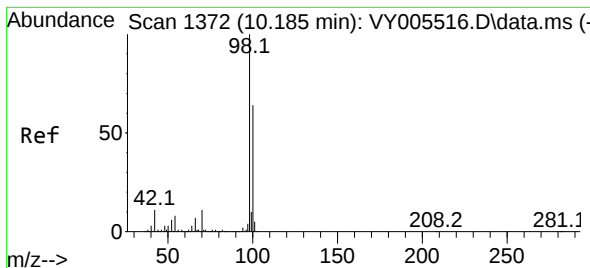

#50
Toluene-d8
Concen: 51.141 ug/l
RT: 10.185 min Scan# 1372
Delta R.T. -0.000 min
Lab File: VY005531.D
Acq: 04 Aug 2021 12:42




Instrument :
MSVOA_Y
ClientSampled :


Tgt Ion: 98 Resp: 14512
Ion Ratio Lower Upper
98 100
100 61.5 51.3 76.9

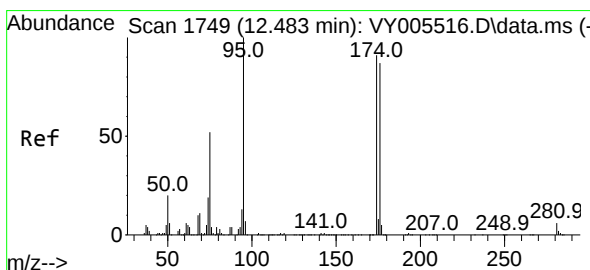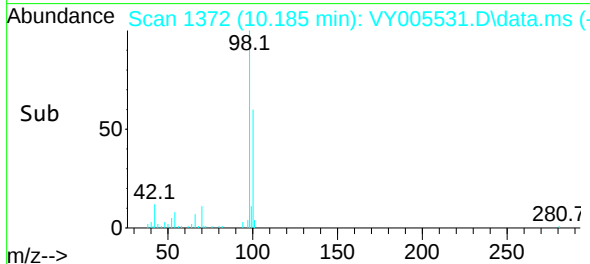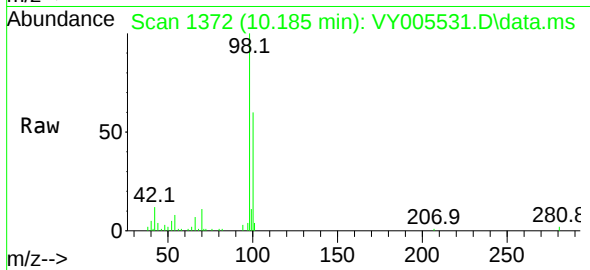

#62
4-Bromofluorobenzene
Concen: 41.609 ug/l
RT: 12.483 min Scan# 1749
Delta R.T. -0.000 min
Lab File: VY005531.D
Acq: 04 Aug 2021 12:42

Tgt Ion: 95 Resp: 3910
Ion Ratio Lower Upper
95 100
174 102.3 0.0 191.4
176 101.0 0.0 183.6


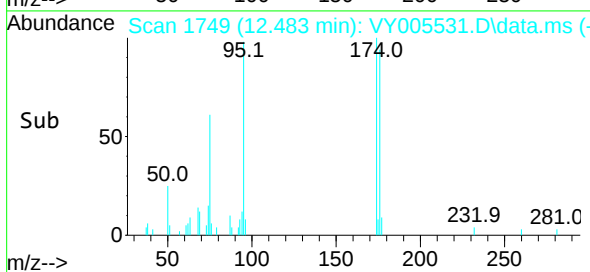

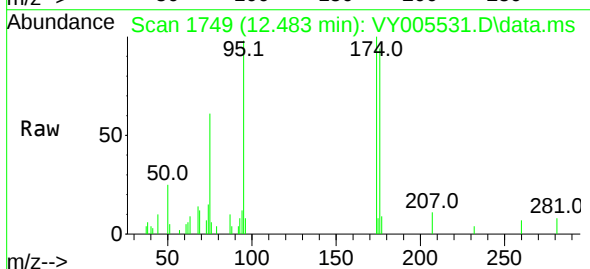


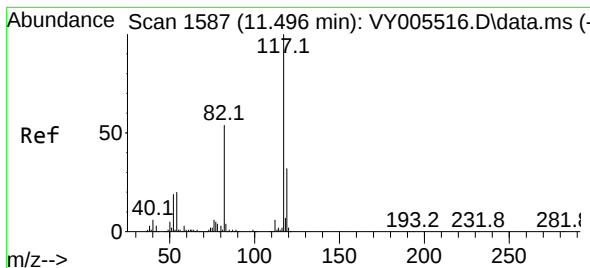

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.490 min Scan# 1586
Delta R.T. -0.006 min
Lab File: VY005531.D
Acq: 04 Aug 2021 12:42




Instrument :
MSVOA_Y
ClientSampleId :


Tgt Ion:	117	Resp:	11129
Ion	Ratio	Lower	Upper
117	100		
82	53.2	43.5	65.3
119	32.3	25.5	38.3

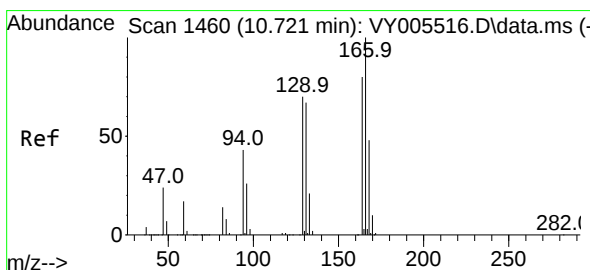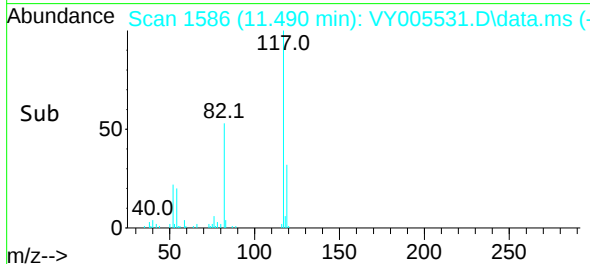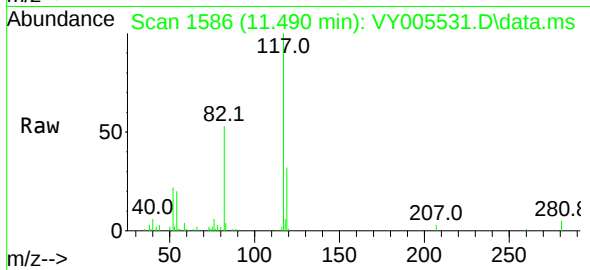

#64
Tetrachloroethene
Concen: 2.207 ug/l
RT: 10.727 min Scan# 1461
Delta R.T. 0.006 min
Lab File: VY005531.D
Acq: 04 Aug 2021 12:42

Tgt Ion:	164	Resp:	187
Ion	Ratio	Lower	Upper
164	100		
166	0.0	99.8	149.8#
129	0.0	70.1	105.1#
131	0.0	67.4	101.0#


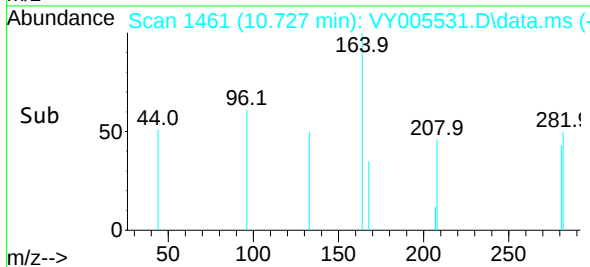
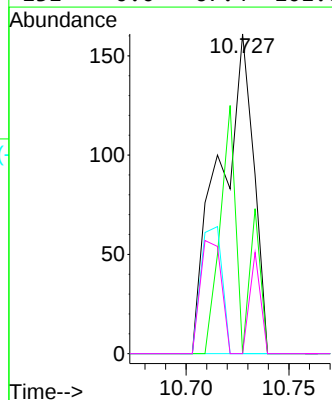
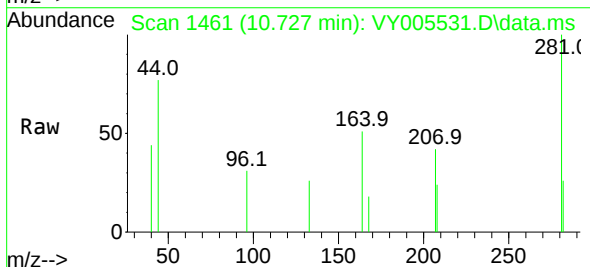




#68
m/p-Xylenes
Concen: 1.946 ug/l
RT: 11.703 min Scan# 1621
Delta R.T. -0.006 min
Lab File: VY005531.D
Acq: 04 Aug 2021 12:42




Instrument :
MSVOA_Y
ClientSampleId :


Tgt Ion:106 Resp: 307
Ion Ratio Lower Upper
106 100
91 129.3 159.6 239.4#



#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.428 min Scan# 1904
Delta R.T. -0.000 min
Lab File: VY005531.D
Acq: 04 Aug 2021 12:42

Tgt Ion:152 Resp: 3774
Ion Ratio Lower Upper
152 100
115 52.4 27.3 81.9
150 159.2 0.0 350.2


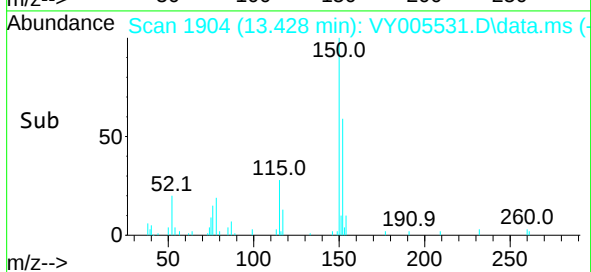






#76
1,2,3-Trichloropropane
Concen: 55.971 ug/l
RT: 12.483 min Scan# 1749
Delta R.T. -0.152 min
Lab File: VY005531.D
Acq: 04 Aug 2021 12:42




Instrument :
MSVOA_Y
ClientSampled :


Tgt Ion: 75 Resp: 2189
Ion Ratio Lower Upper
75 100
77 0.0 0.0 0.0

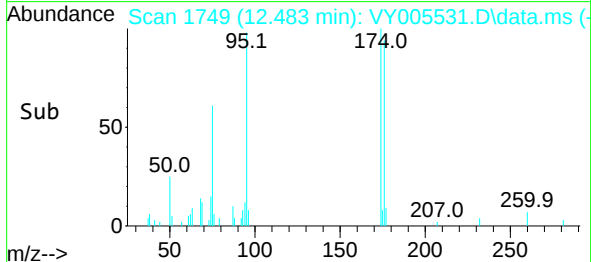

#78
n-propylbenzene
Concen: 1.595 ug/l
RT: 12.678 min Scan# 1781
Delta R.T. 0.006 min
Lab File: VY005531.D
Acq: 04 Aug 2021 12:42

Tgt Ion: 91 Resp: 499
Ion Ratio Lower Upper
91 100
120 7.0 11.9 35.9#









#79
2-Chlorotoluene
Concen: 1.799 ug/l
RT: 12.758 min Scan# 1794
Delta R.T. -0.000 min
Lab File: VY005531.D
Acq: 04 Aug 2021 12:42




Instrument :
MSVOA_Y
ClientSampled :


Tgt Ion: 91 Resp: 316
Ion Ratio Lower Upper
91 100
126 28.2 17.5 52.6

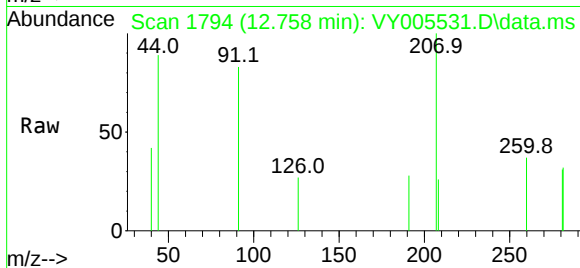

#80
1,3,5-Trimethylbenzene
Concen: 1.651 ug/l
RT: 12.819 min Scan# 1804
Delta R.T. -0.000 min
Lab File: VY005531.D
Acq: 04 Aug 2021 12:42

Tgt Ion: 105 Resp: 361
Ion Ratio Lower Upper
105 100
120 44.3 25.0 75.0




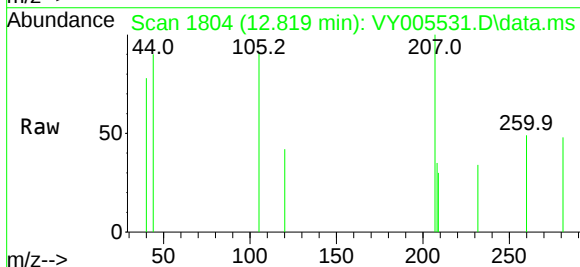




#81
 trans-1,4-Dichloro-2-butene
 Concen: 112.830 ug/l
 RT: 12.483 min Scan# 1749
 Delta R.T. 0.104 min
 Lab File: VY005531.D
 Acq: 04 Aug 2021 12:42




Instrument :
 MSVOA_Y
 ClientSampled :


Tgt Ion: 75 Resp: 2189
 Ion Ratio Lower Upper
 75 100
 53 0.0 76.7 115.1#
 89 0.0 38.4 57.6#

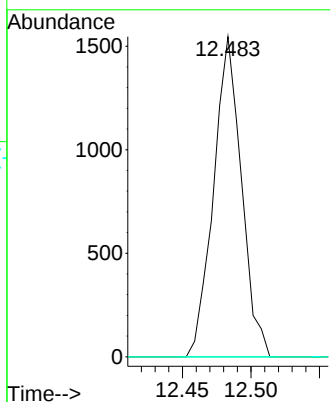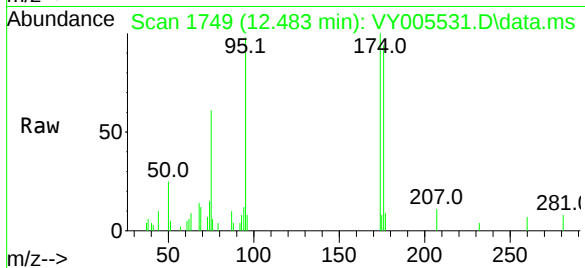

#82
 4-Chlorotoluene
 Concen: 1.733 ug/l
 RT: 12.855 min Scan# 1810
 Delta R.T. -0.006 min
 Lab File: VY005531.D
 Acq: 04 Aug 2021 12:42

Tgt Ion: 91 Resp: 315
 Ion Ratio Lower Upper
 91 100
 126 30.2 17.5 52.5



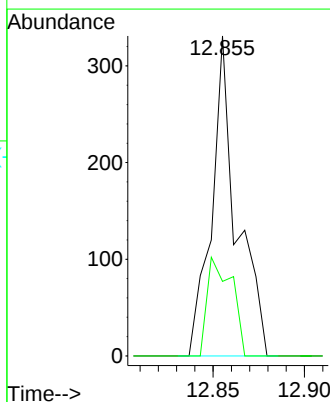
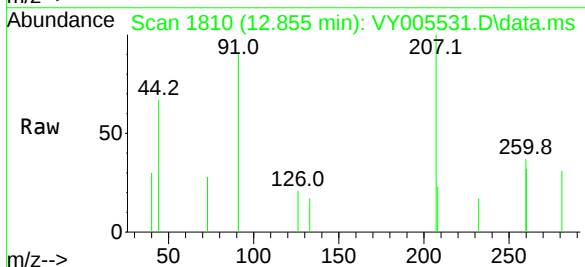




#83
tert-Butylbenzene
Concen: 1.351 ug/l
RT: 13.081 min Scan# 1847
Delta R.T. -0.000 min
Lab File: VY005531.D
Acq: 04 Aug 2021 12:42




Instrument :
MSVOA_Y
ClientSampled :


Tgt Ion:119 Resp: 265
Ion Ratio Lower Upper
119 100
91 30.9 31.9 95.9#
134 17.4 13.4 40.2

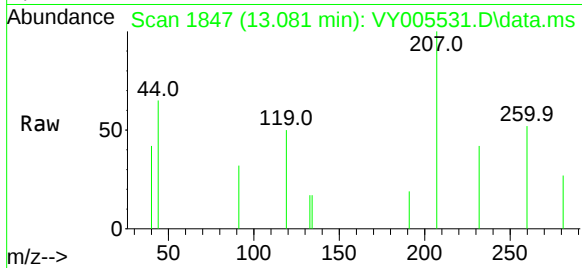

#84
1,2,4-Trimethylbenzene
Concen: 2.040 ug/l
RT: 13.129 min Scan# 1855
Delta R.T. 0.006 min
Lab File: VY005531.D
Acq: 04 Aug 2021 12:42

Tgt Ion:105 Resp: 440
Ion Ratio Lower Upper
105 100
120 26.1 22.9 68.5


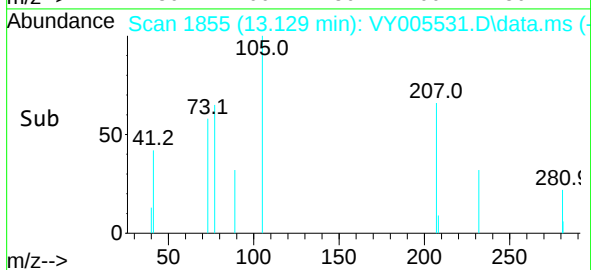

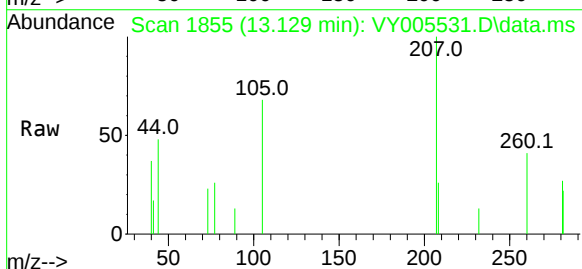




#85
 sec-Butylbenzene
 Concen: 1.417 ug/l
 RT: 13.257 min Scan# 1876
 Delta R.T. -0.000 min
 Lab File: VY005531.D
 Acq: 04 Aug 2021 12:42




Instrument :
 MSVOA_Y
 ClientSampled :


Tgt Ion:105 Resp: 401
 Ion Ratio Lower Upper
 105 100
 134 5.2 10.5 31.5#

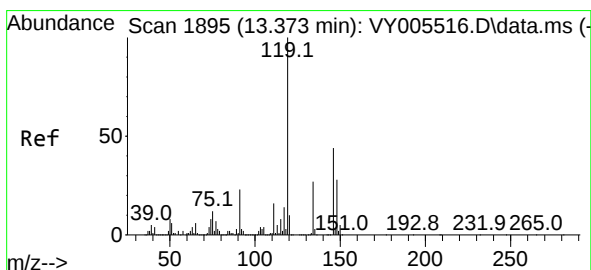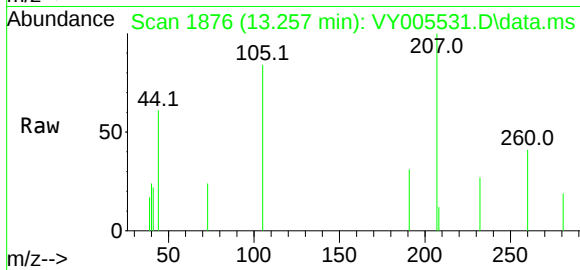

#86
 p-Isopropyltoluene
 Concen: 1.959 ug/l
 RT: 13.373 min Scan# 1895
 Delta R.T. -0.000 min
 Lab File: VY005531.D
 Acq: 04 Aug 2021 12:42

Tgt Ion:119 Resp: 476
 Ion Ratio Lower Upper
 119 100
 134 13.4 13.6 40.7#
 91 12.8 11.6 34.7

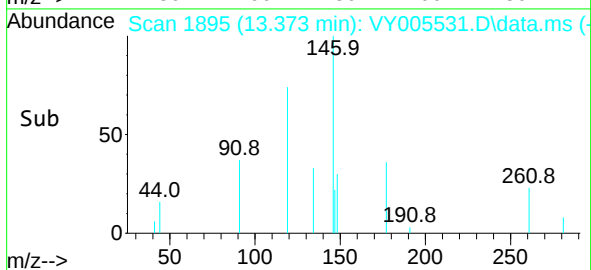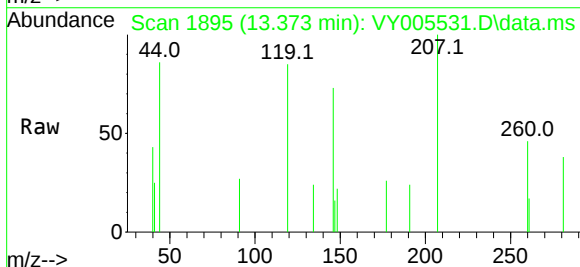







#87

1,3-Dichlorobenzene
Concen: 2.684 ug/l
RT: 13.373 min Scan# 1895
Delta R.T. 0.006 min
Lab File: VY005531.D
Acq: 04 Aug 2021 12:42

Instrument :
MSVOA_Y
ClientSampled :




Tgt Ion:146 Resp: 339
Ion Ratio Lower Upper
146 100
111 19.2 18.6 56.0
148 71.1 31.7 95.1

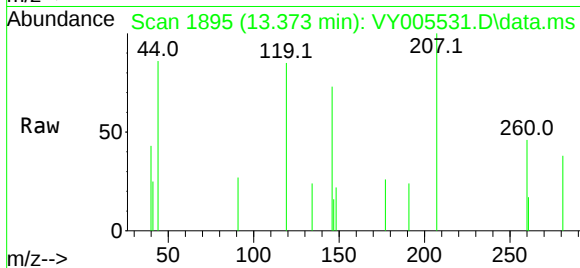


#88

1,4-Dichlorobenzene
Concen: 3.265 ug/l
RT: 13.453 min Scan# 1908
Delta R.T. -0.000 min
Lab File: VY005531.D
Acq: 04 Aug 2021 12:42

Tgt Ion:146 Resp: 409
Ion Ratio Lower Upper
146 100
111 39.4 18.1 54.3
148 53.8 31.8 95.3




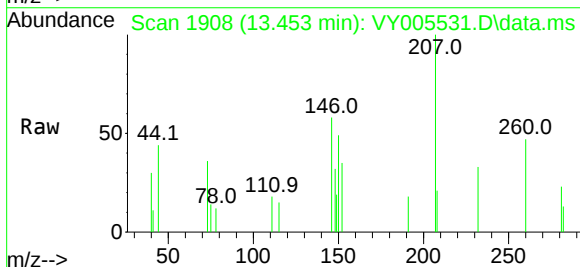




#89
n-Butylbenzene
Concen: 1.781 ug/l
RT: 13.696 min Scan# 1948
Delta R.T. -0.006 min
Lab File: VY005531.D
Acq: 04 Aug 2021 12:42




Instrument :
MSVOA_Y
ClientSampleId :


Tgt Ion: 91	Resp:	392
Ion	Ratio	Lower Upper
91	100	
92	47.7	26.7 80.1
134	31.1	13.8 41.4

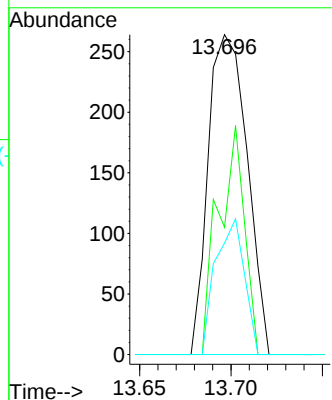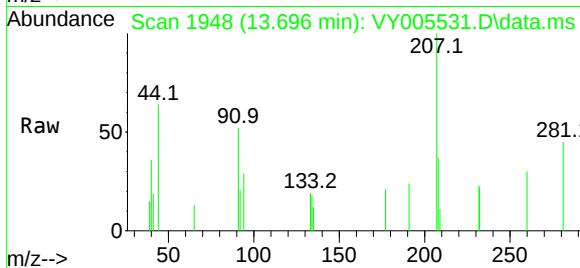

#91
1,2-Dichlorobenzene
Concen: 2.931 ug/l
RT: 13.739 min Scan# 1955
Delta R.T. -0.006 min
Lab File: VY005531.D
Acq: 04 Aug 2021 12:42

Tgt Ion: 146	Resp:	327
Ion	Ratio	Lower Upper
146	100	
111	15.3	19.4 58.2
148	66.7	31.9 95.5



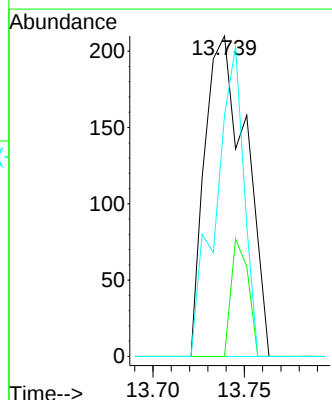
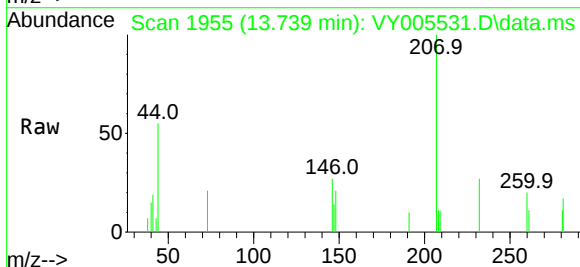


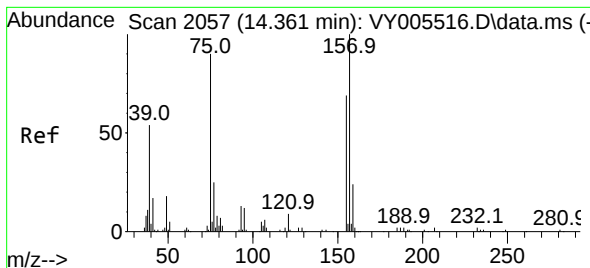

#92
 1,2-Dibromo-3-Chloropropane
 Concen: 4.269 ug/l
 RT: 14.416 min Scan# 2066
 Delta R.T. 0.055 min
 Lab File: VY005531.D
 Acq: 04 Aug 2021 12:42




Instrument :
 MSVOA_Y
 ClientSampleId :


Tgt Ion: 75 Resp: 41
 Ion Ratio Lower Upper
 75 100
 155 0.0 42.4 127.1#
 157 0.0 56.0 168.2#

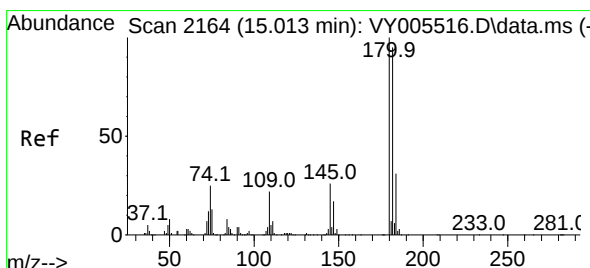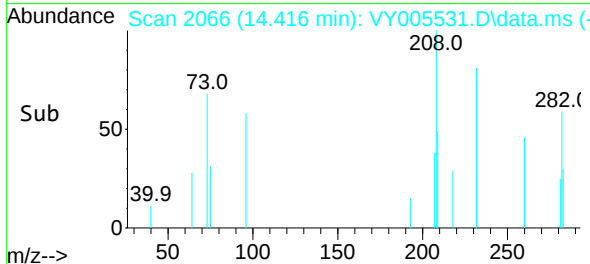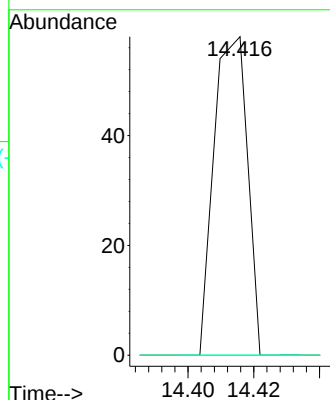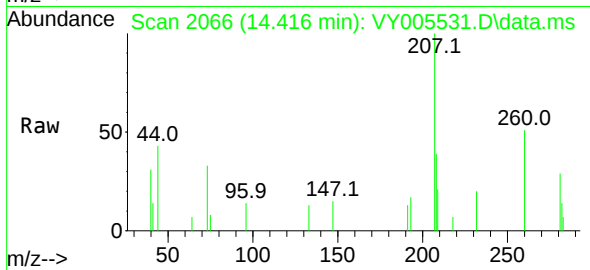

#93
 1,2,4-Trichlorobenzene
 Concen: 3.471 ug/l
 RT: 15.013 min Scan# 2164
 Delta R.T. -0.000 min
 Lab File: VY005531.D
 Acq: 04 Aug 2021 12:42

Tgt Ion: 180 Resp: 266
 Ion Ratio Lower Upper
 180 100
 182 71.4 47.8 143.4
 145 7.1 14.0 42.0#


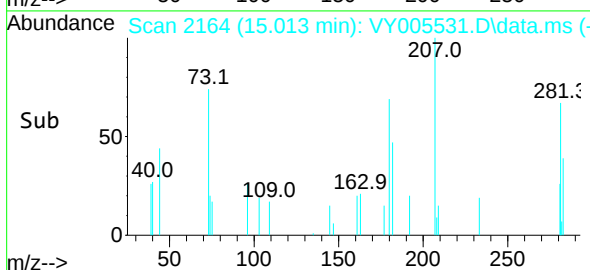
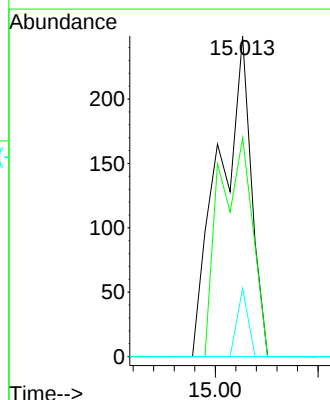
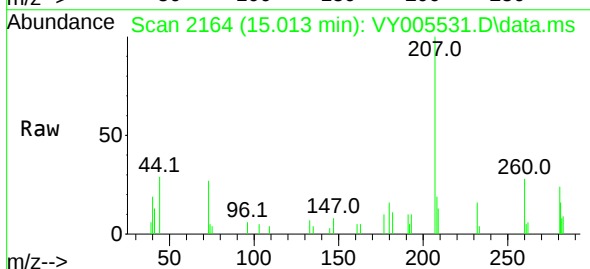




#94
Hexachlorobutadiene
Concen: 2.519 ug/l
RT: 15.129 min Scan# 2183
Delta R.T. 0.012 min
Lab File: VY005531.D
Acq: 04 Aug 2021 12:42




Instrument :
MSVOA_Y
ClientSampleId :


Tgt Ion:225 Resp: 125
Ion Ratio Lower Upper
225 100
223 56.0 31.4 94.0
227 19.2 32.2 96.6#

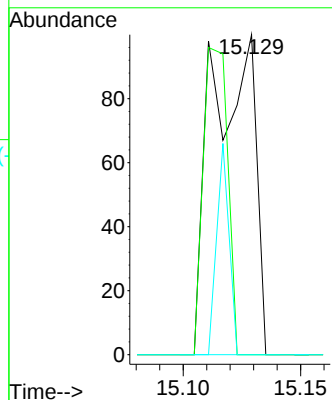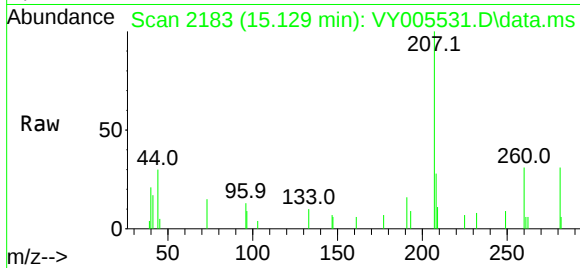

#95
Naphthalene
Concen: 3.065 ug/l
RT: 15.245 min Scan# 2202
Delta R.T. 0.006 min
Lab File: VY005531.D
Acq: 04 Aug 2021 12:42


Tgt Ion:128 Resp: 463
Ion Ratio Lower Upper
128 100
127 0.0 10.6 15.8#
129 0.0 8.7 13.1#

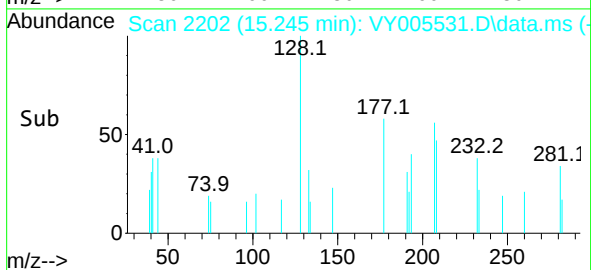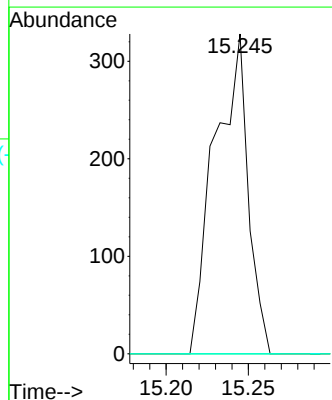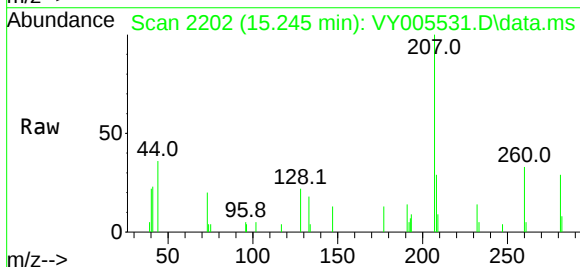



#96
 1,2,3-Trichlorobenzene
 Concen: 3.742 ug/l
 RT: 15.428 min Scan# 2232
 Delta R.T. -0.000 min
 Lab File: VY005531.D
 Acq: 04 Aug 2021 12:42

Instrument :
 MSVOA_Y
 ClientSampleId :

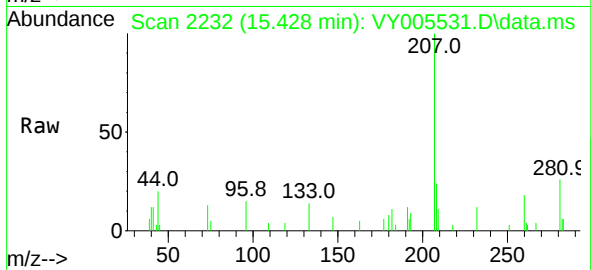

Tgt Ion:	180	Resp:	254
Ion	Ratio	Lower	Upper
180	100		
182	116.1	47.9	143.6
145	15.7	14.6	44.0

