
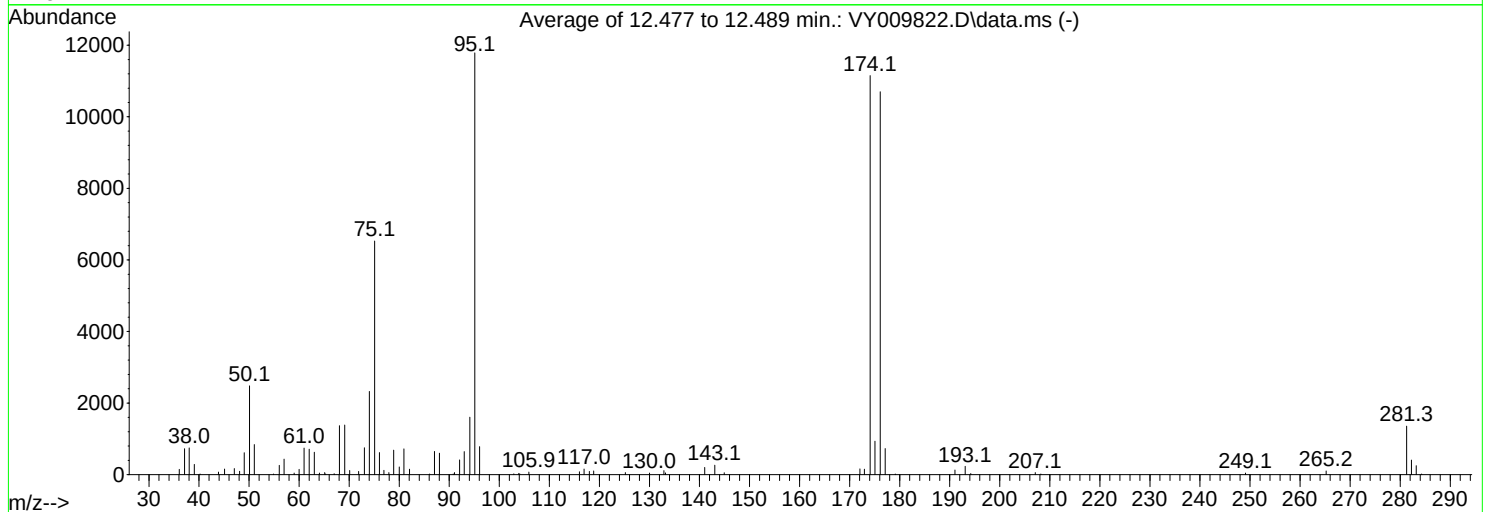


Data Path : Z:\voasrv\HPCHEM1\MSVOA\_Y\Data\VY080422\  
 Data File : VY009822.D  
 Acq On : 04 Aug 2022 10:07  
 Operator : KP/MD  
 Sample : BFB  
 Misc : 5.00g/5.0mL/MSVOA\_Y/SOIL  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 MSVOA\_Y  
 ClientSampleId :  
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA\_Y\methods\82Y080322S.M  
 Title : SW846 8260  
 Last Update : Thu Aug 04 02:27:45 2022

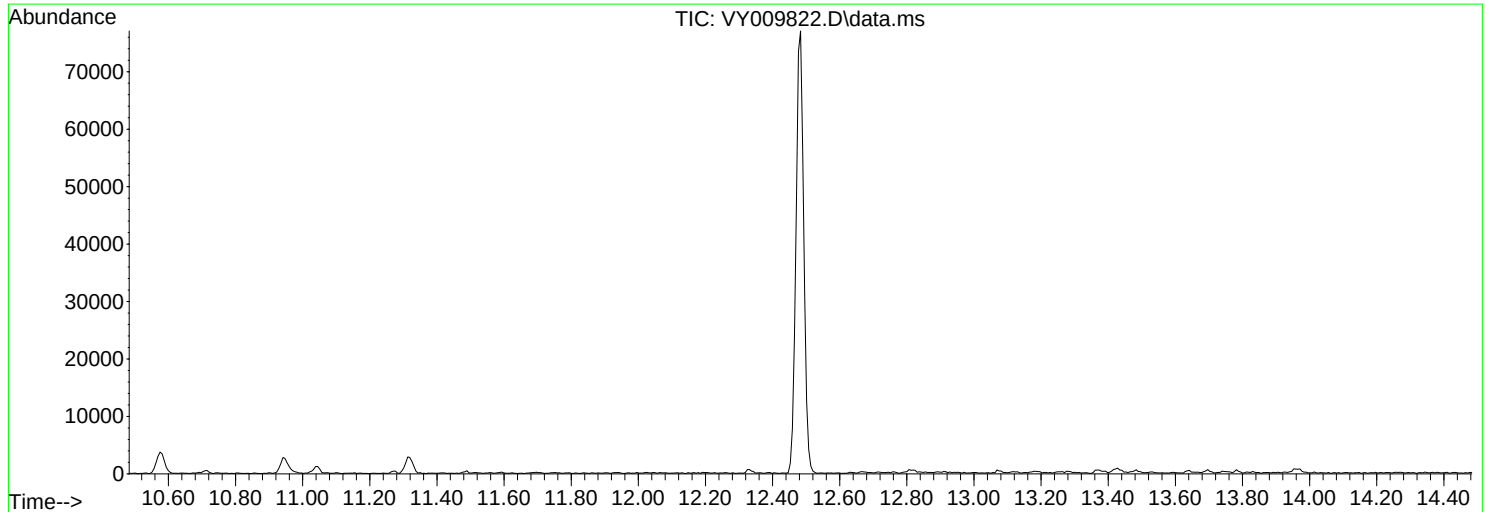

AutoFind: Scans 1748, 1749, 1750; Background Corrected with Scan 1741

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 50             | 95              | 15              | 40              | 21.1         | 2482       | PASS                |
| 75             | 95              | 30              | 60              | 55.4         | 6526       | PASS                |
| 95             | 95              | 100             | 100             | 100.0        | 11787      | PASS                |
| 96             | 95              | 5               | 9               | 6.7          | 784        | PASS                |
| 173            | 174             | 0.00            | 2               | 1.4          | 154        | PASS                |
| 174            | 95              | 50              | 100             | 94.6         | 11153      | PASS                |
| 175            | 174             | 5               | 9               | 8.4          | 936        | PASS                |
| 176            | 174             | 95              | 101             | 95.9         | 10700      | PASS                |
| 177            | 176             | 5               | 9               | 6.8          | 728        | PASS                |