

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY080521\
 Data File : VY0805545.D
 Acq On : 05 Aug 2021 11:04
 Operator : SY/MD
 Sample : VY0805SBL01
 Misc : 5.00G/5ML/MSVOA_Y/SOIL
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 VY0805SBL01

Quant Time: Aug 06 04:36:17 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y080221S.M
 Quant Title : SW846 8260
 QLast Update : Tue Aug 03 04:52:05 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.801	168	301474	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.697	114	448326	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.496	117	400310	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.428	152	202478	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.149	65	152817	50.077	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	= 100.160%	
35) Dibromofluoromethane	7.722	113	128134	51.048	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	= 102.100%	
50) Toluene-d8	10.185	98	529170	50.268	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	= 100.540%	
62) 4-Bromofluorobenzene	12.483	95	172455	49.470	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	= 98.940%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY080521\
Data File : VY005545.D
Acq On : 05 Aug 2021 11:04
Operator : SY/MD
Sample : VY0805SBL01
Misc : 5.00G/5ML/MSVOA_Y/SOIL
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
VY0805SBL01

Quant Time: Aug 06 04:36:17 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y080221S.M
Quant Title : SW846 8260
QLast Update : Tue Aug 03 04:52:05 2021
Response via : Initial Calibration




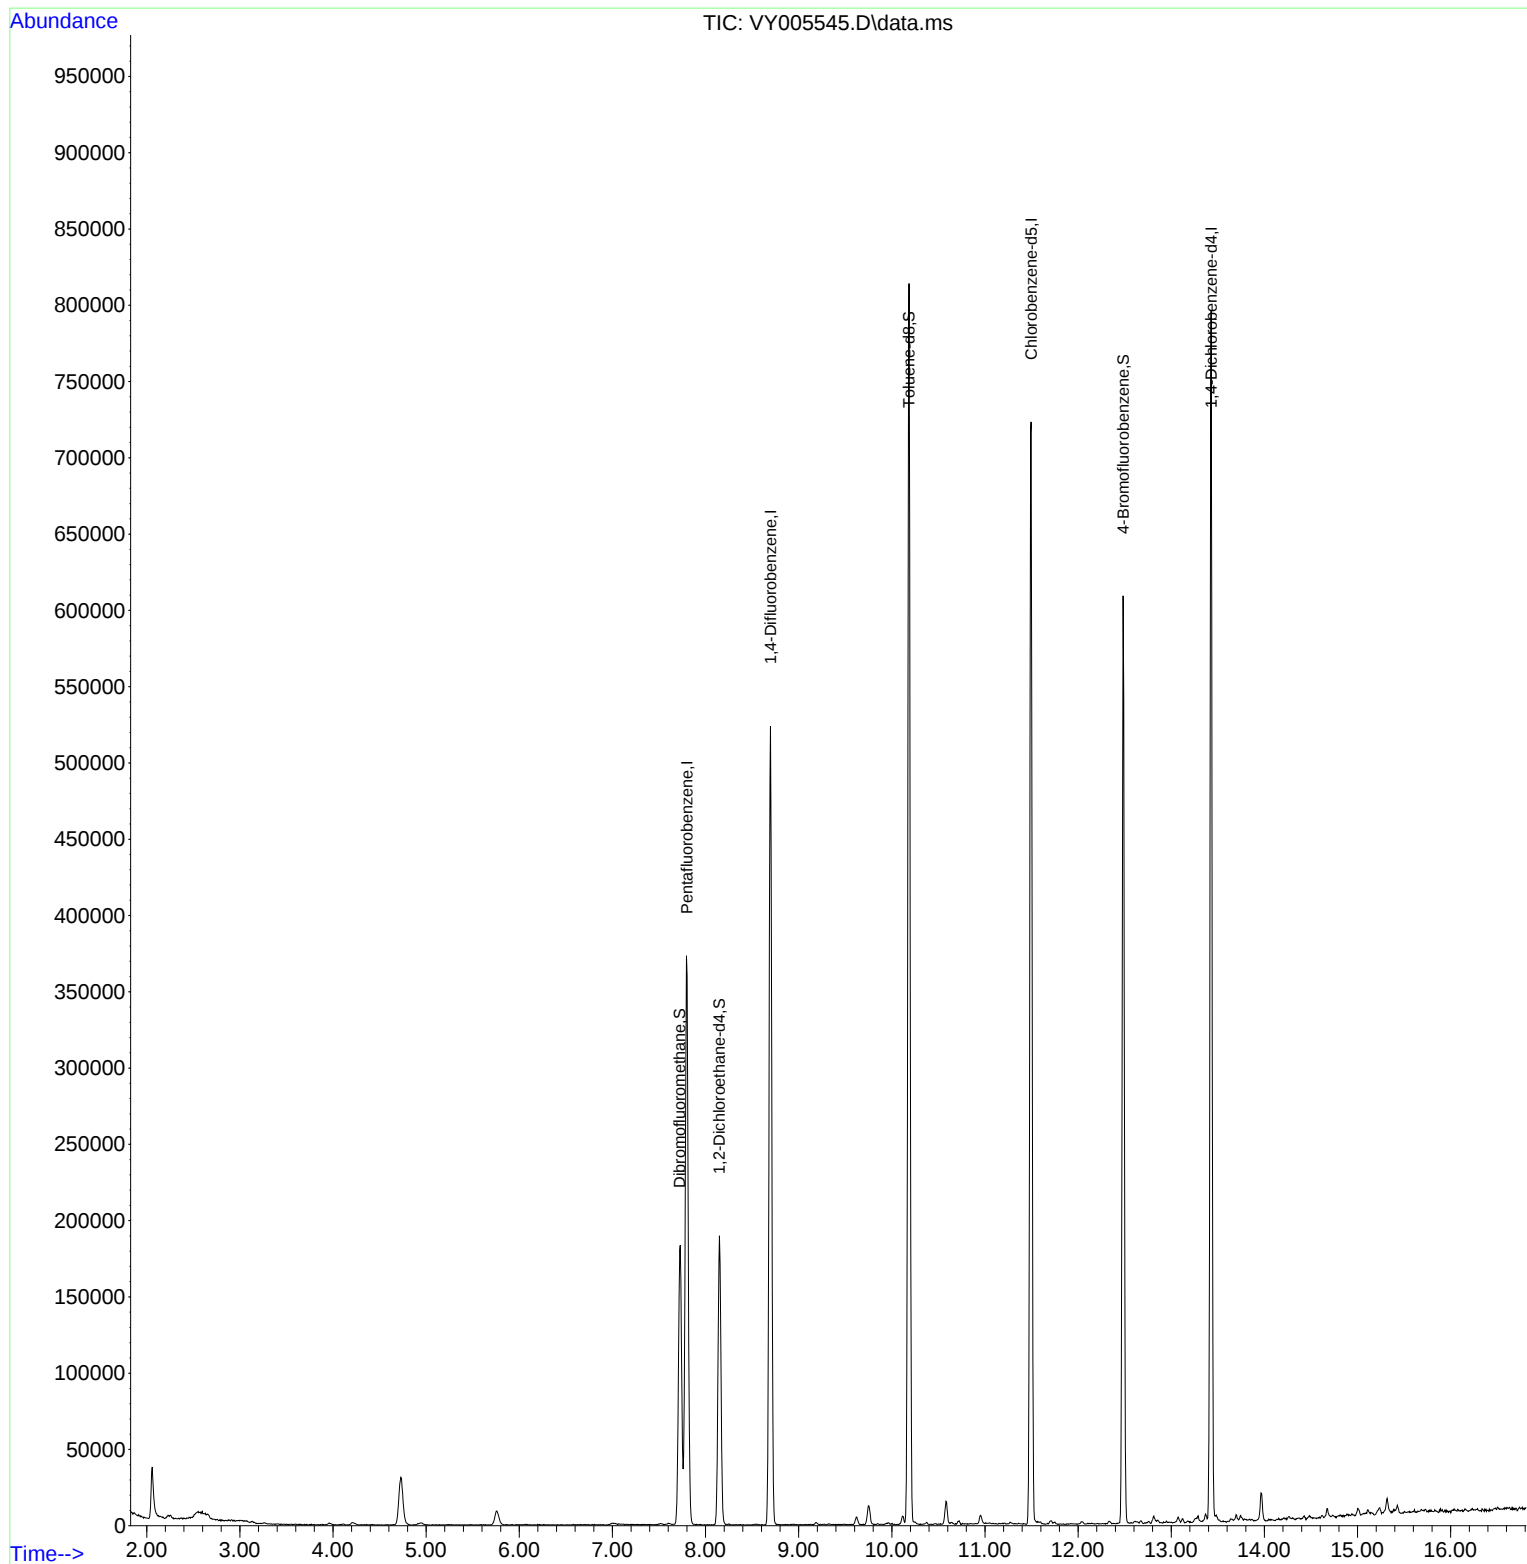


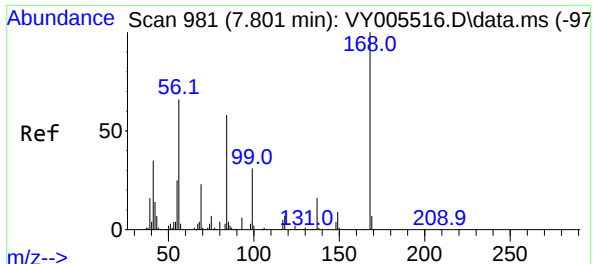

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.801 min Scan# 981
Delta R.T. 0.000 min
Lab File: VY005545.D
Acq: 05 Aug 2021 11:04




Instrument :
MSVOA_Y
ClientSampleId :
VY0805SBL01


Tgt Ion:168 Resp: 301474
Ion Ratio Lower Upper
168 100
99 49.9 38.9 58.3

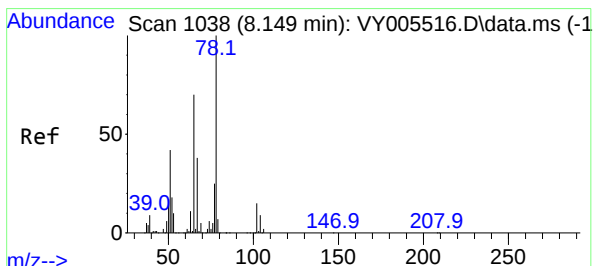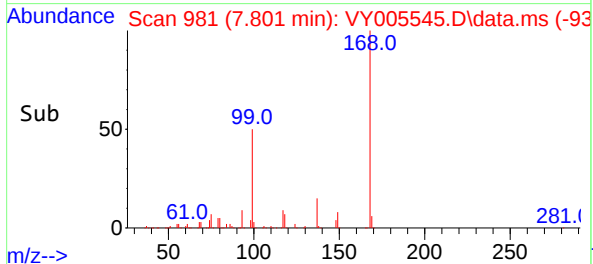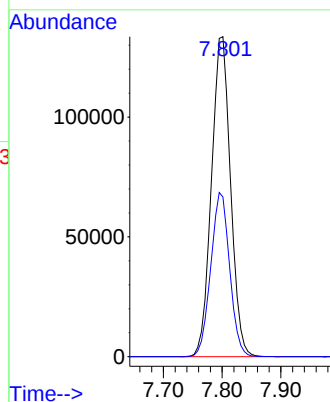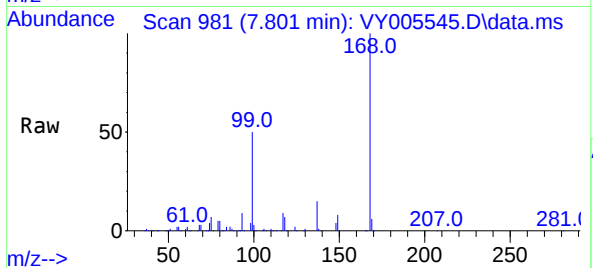

#33
1,2-Dichloroethane-d4
Concen: 50.077 ug/l
RT: 8.149 min Scan# 1038
Delta R.T. 0.000 min
Lab File: VY005545.D
Acq: 05 Aug 2021 11:04

Tgt Ion: 65 Resp: 152817
Ion Ratio Lower Upper
65 100
67 51.5 0.0 103.4


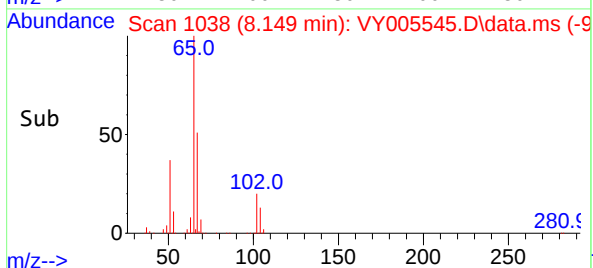
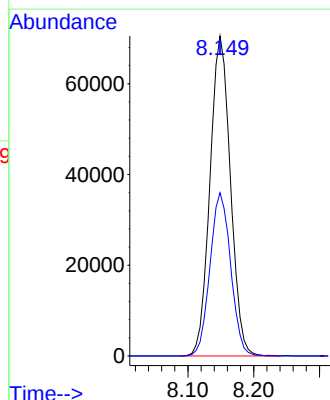
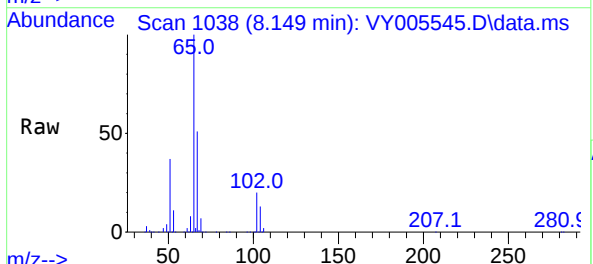


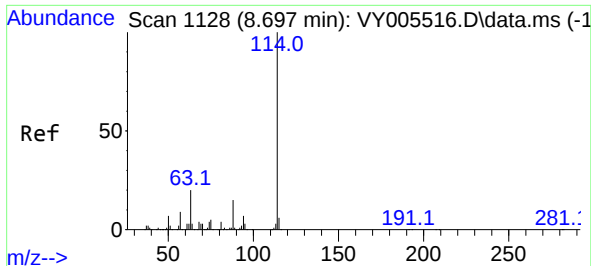

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.697 min Scan# 1128
Delta R.T. 0.000 min
Lab File: VY005545.D
Acq: 05 Aug 2021 11:04




Instrument :
MSVOA_Y
ClientSampleId :
VY0805SBL01

Tgt Ion:	114	Resp:	448326
Ion	Ratio	Lower	Upper
114	100		
63	20.4	0.0	39.2
88	15.4	0.0	30.8

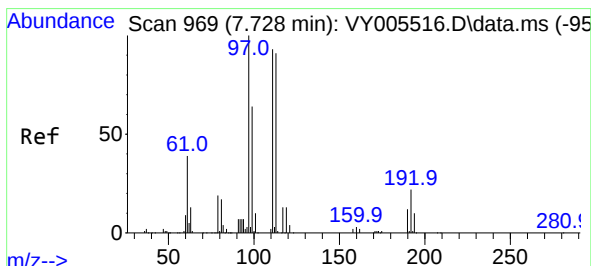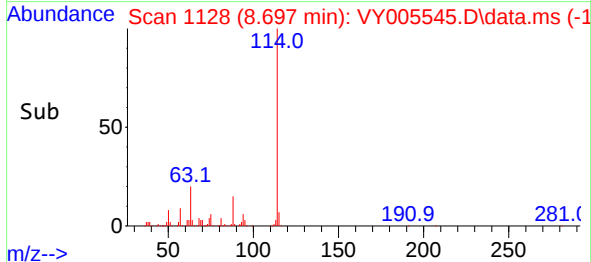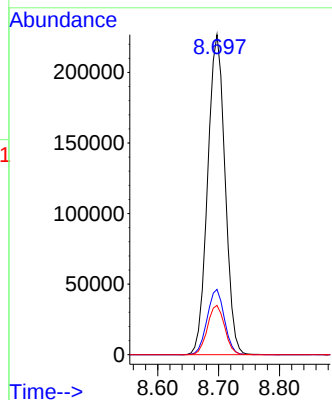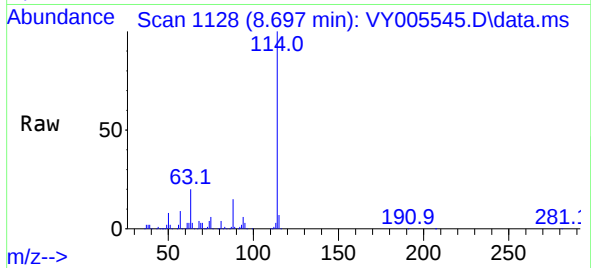

#35
Dibromofluoromethane
Concen: 51.048 ug/l
RT: 7.722 min Scan# 968
Delta R.T. -0.006 min
Lab File: VY005545.D
Acq: 05 Aug 2021 11:04

Tgt Ion:	113	Resp:	128134
Ion	Ratio	Lower	Upper
113	100		
111	102.5	81.9	122.9
192	23.5	19.2	28.8


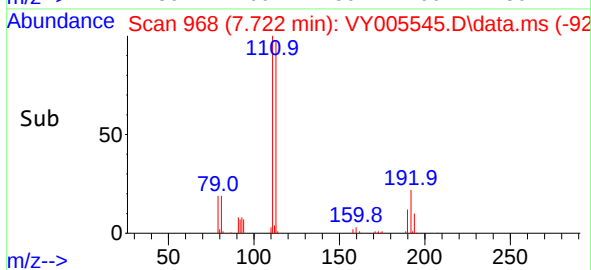
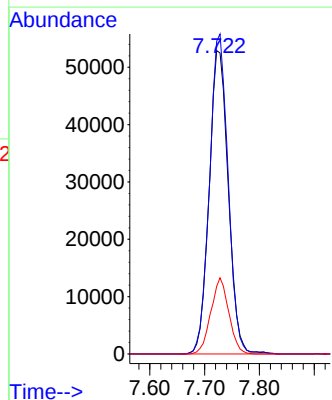
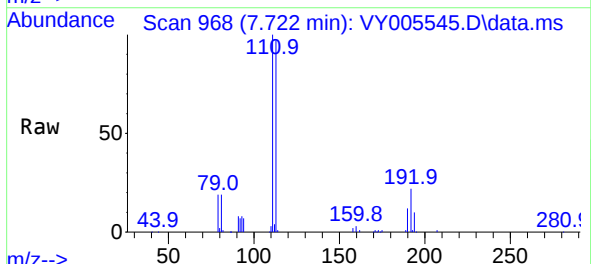




#50
Toluene-d8
Concen: 50.268 ug/l
RT: 10.185 min Scan# 1372
Delta R.T. 0.000 min
Lab File: VY005545.D
Acq: 05 Aug 2021 11:04




Instrument :
MSVOA_Y
ClientSampleId :
VY0805SBL01


Tgt Ion: 98 Resp: 529170
Ion Ratio Lower Upper
98 100
100 63.7 51.3 76.9

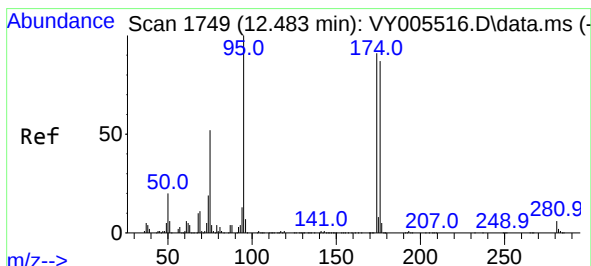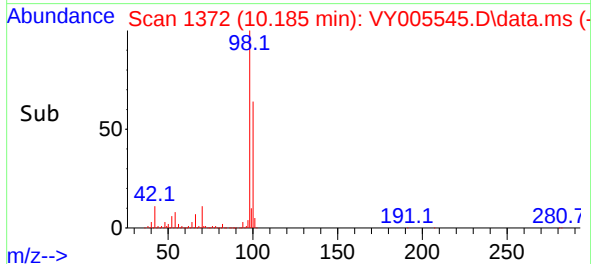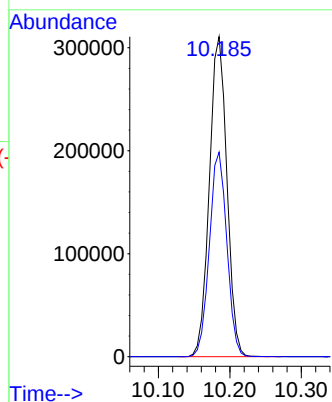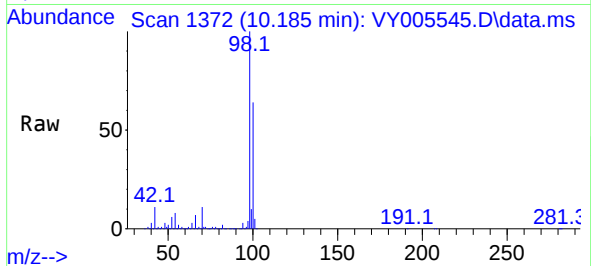

#62
4-Bromofluorobenzene
Concen: 49.470 ug/l
RT: 12.483 min Scan# 1749
Delta R.T. 0.000 min
Lab File: VY005545.D
Acq: 05 Aug 2021 11:04

Tgt Ion: 95 Resp: 172455
Ion Ratio Lower Upper
95 100
174 92.5 0.0 191.4
176 89.9 0.0 183.6


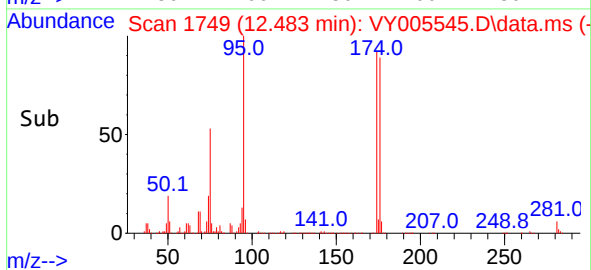
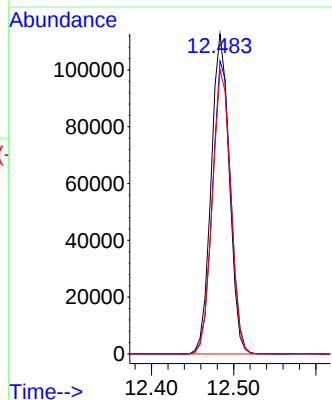
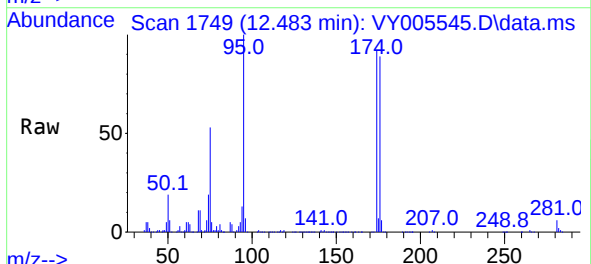


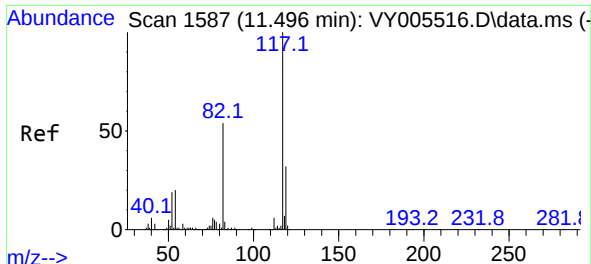

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.496 min Scan# 1587
Delta R.T. 0.000 min
Lab File: VY005545.D
Acq: 05 Aug 2021 11:04

Instrument :
MSVOA_Y
ClientSampleId :
VY0805SBL01

Tgt Ion:117 Resp: 400310
Ion Ratio Lower Upper
117 100
82 55.3 43.5 65.3
119 32.7 25.5 38.3

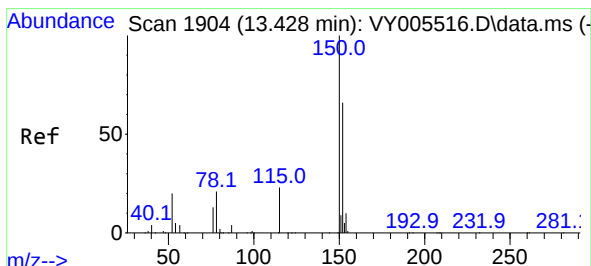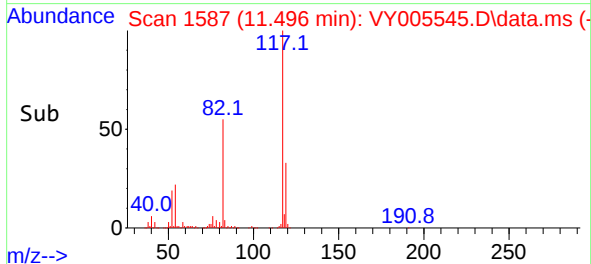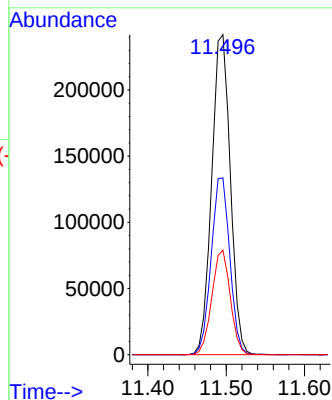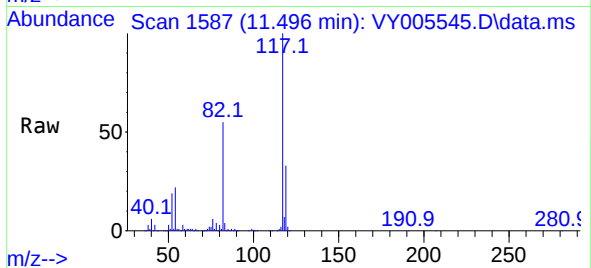

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.428 min Scan# 1904
Delta R.T. 0.000 min
Lab File: VY005545.D
Acq: 05 Aug 2021 11:04

Tgt Ion:152 Resp: 202478
Ion Ratio Lower Upper
152 100
115 55.3 27.3 81.9
150 157.3 0.0 350.2

