

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY080621\
 Data File : VY005574.D
 Acq On : 06 Aug 2021 16:35
 Operator : SY/MD
 Sample : M3310-01
 Misc : 5.07G/5ML/MSVOA_Y/SOIL
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 NB-08-080521

Quant Time: Aug 07 06:19:56 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y080221S.M
 Quant Title : SW846 8260
 QLast Update : Tue Aug 03 04:52:05 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.801	168	228936	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.697	114	386128	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.496	117	380500	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.428	152	191275	50.00	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.149	65	128700	55.54	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	111.08%
35) Dibromofluoromethane	7.728	113	113925	52.70	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	105.40%
50) Toluene-d8	10.185	98	491924	54.26	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	=	108.52%
62) 4-Bromofluorobenzene	12.483	95	169416	56.43	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	=	112.86%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY080621\
Data File : VY005574.D
Acq On : 06 Aug 2021 16:35
Operator : SY/MD
Sample : M3310-01
Misc : 5.07G/5ML/MSVOA_Y/SOIL
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
NB-08-080521

Quant Time: Aug 07 06:19:56 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y080221S.M
Quant Title : SW846 8260
QLast Update : Tue Aug 03 04:52:05 2021
Response via : Initial Calibration




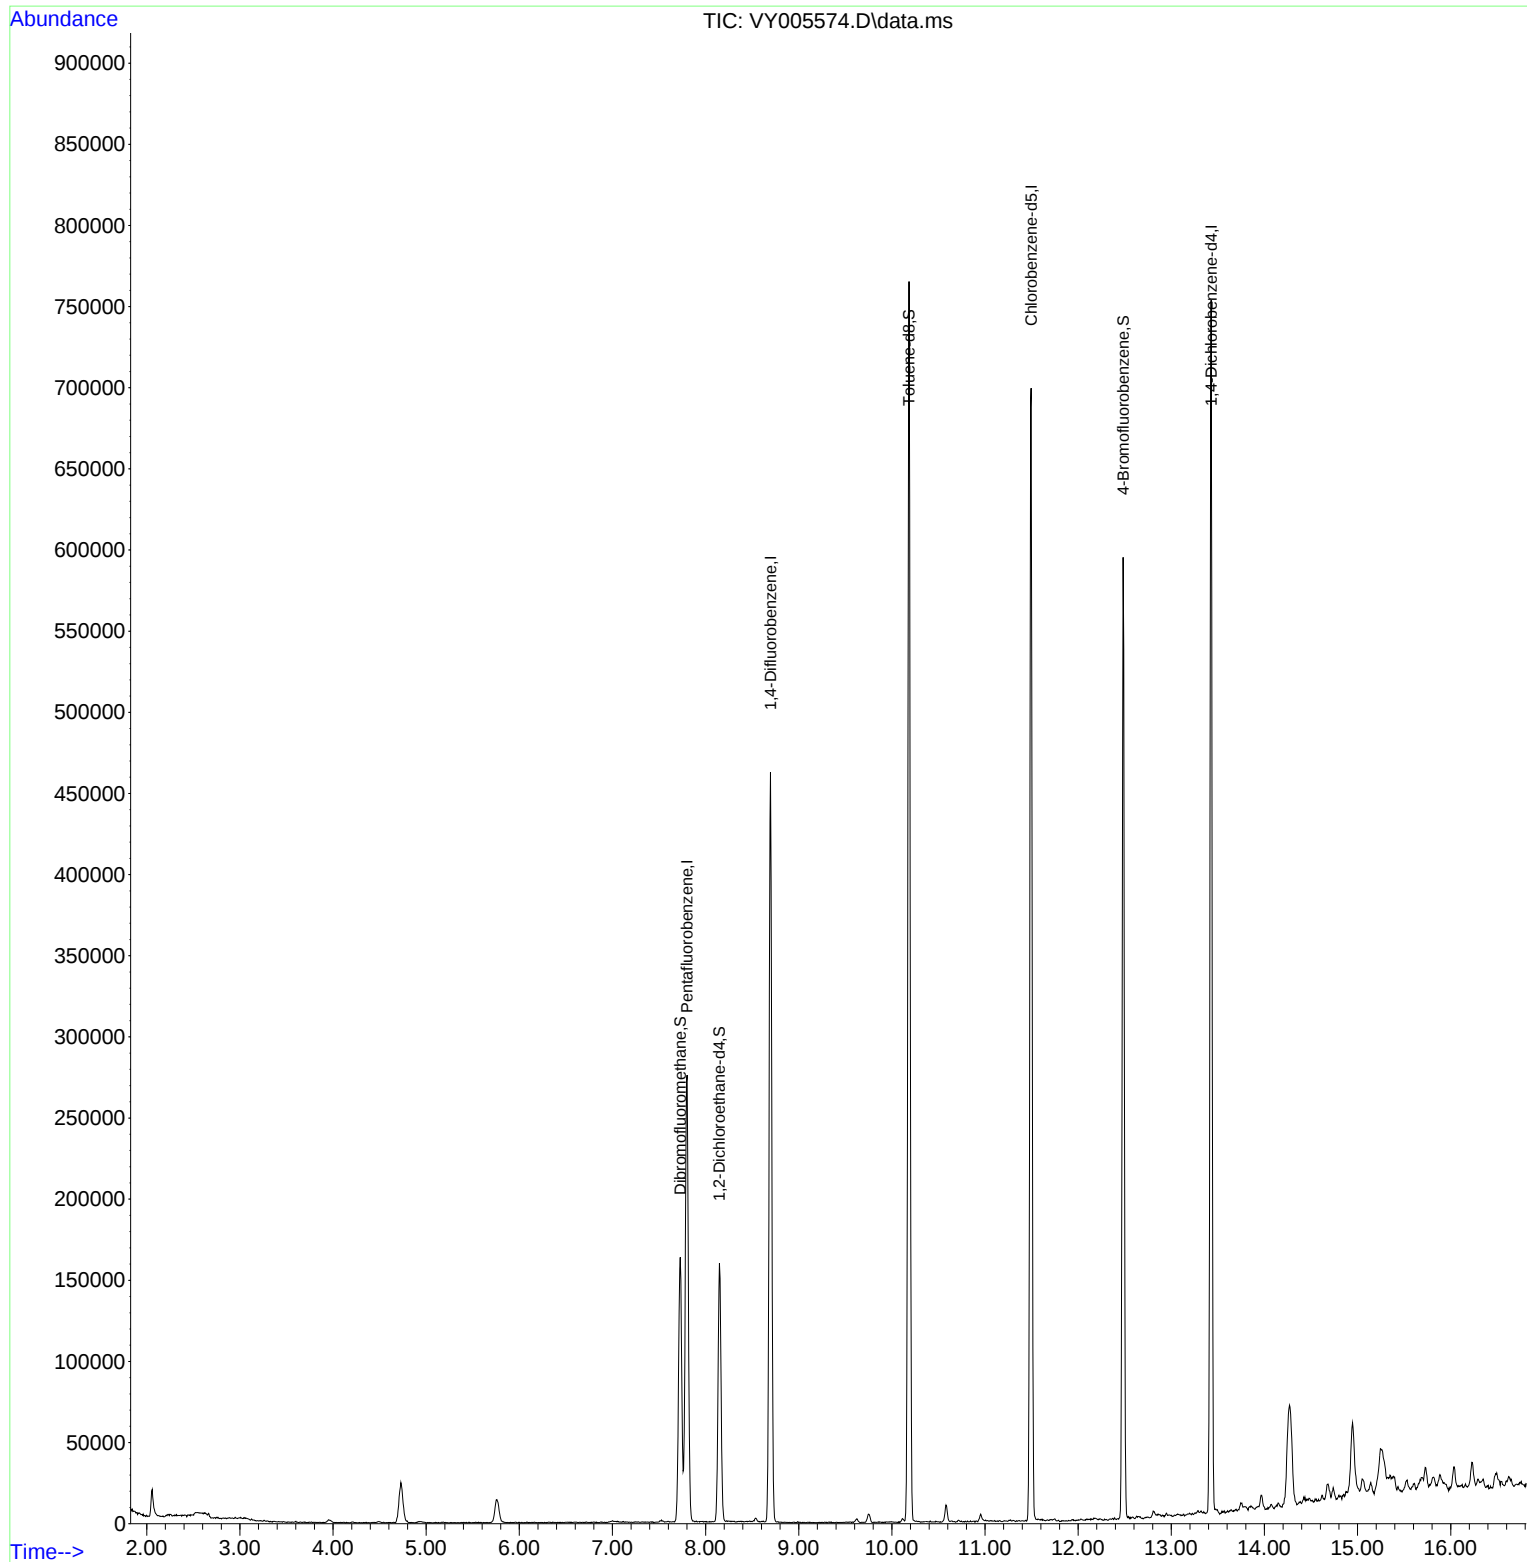


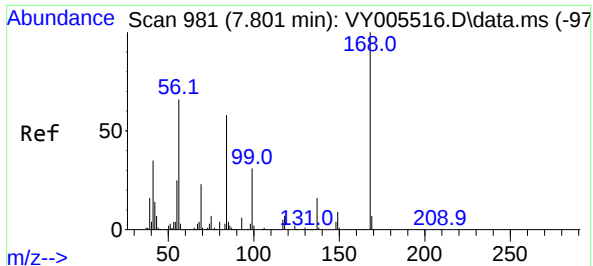

#1
Pentafluorobenzene
Concen: 50.00 ug/l
RT: 7.801 min Scan# 981
Delta R.T. 0.000 min
Lab File: VY005574.D
Acq: 06 Aug 2021 16:35




Instrument :
MSVOA_Y
ClientSampleId :
NB-08-080521


Tgt Ion:168 Resp: 228936
Ion Ratio Lower Upper
168 100
99 49.8 38.9 58.3

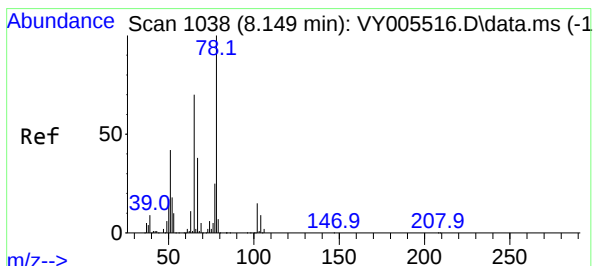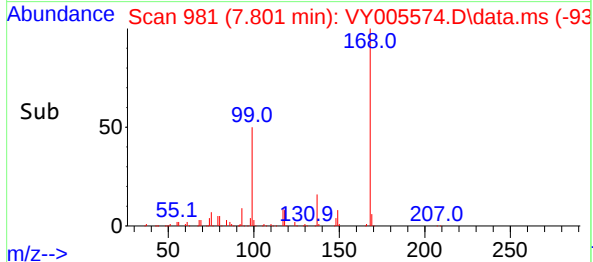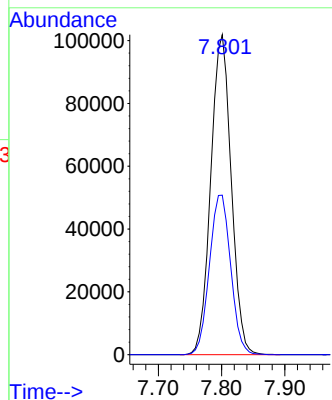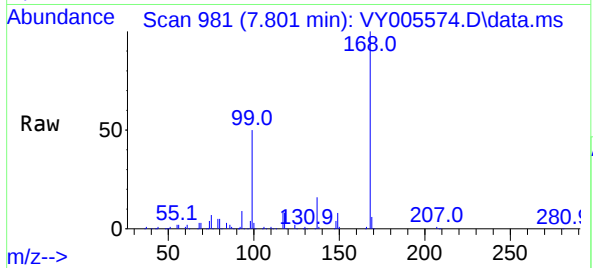

#33
1,2-Dichloroethane-d4
Concen: 55.54 ug/l
RT: 8.149 min Scan# 1038
Delta R.T. -0.000 min
Lab File: VY005574.D
Acq: 06 Aug 2021 16:35

Tgt Ion: 65 Resp: 128700
Ion Ratio Lower Upper
65 100
67 51.9 0.0 103.4


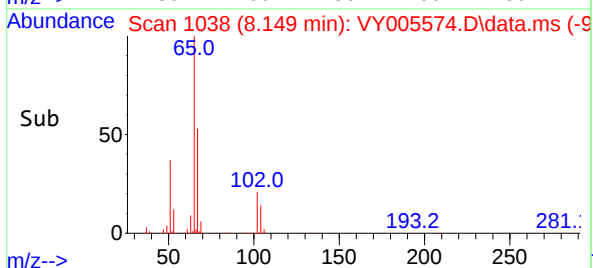
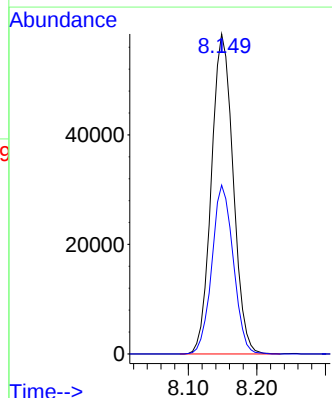
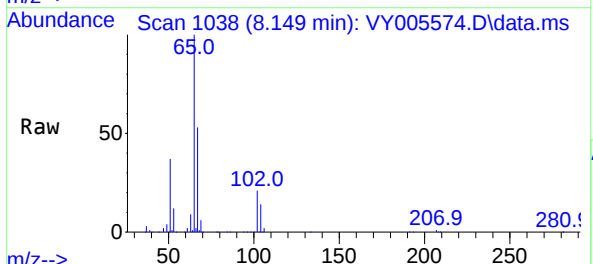


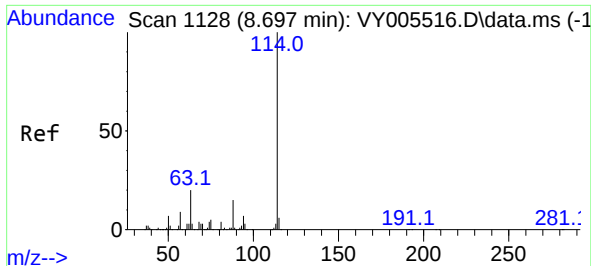

#34
1,4-Difluorobenzene
Concen: 50.00 ug/l
RT: 8.697 min Scan# 1128
Delta R.T. -0.000 min
Lab File: VY005574.D
Acq: 06 Aug 2021 16:35




Instrument :
MSVOA_Y
ClientSampleId :
NB-08-080521

Tgt Ion:	114	Resp:	386128
Ion	Ratio	Lower	Upper
114	100		
63	21.0	0.0	39.2
88	15.3	0.0	30.8

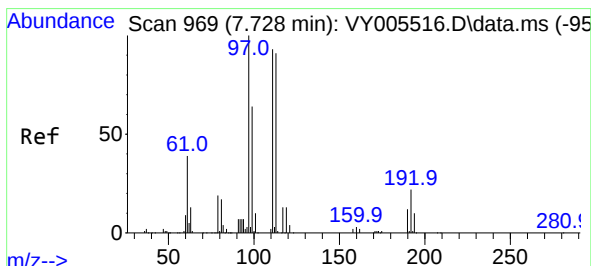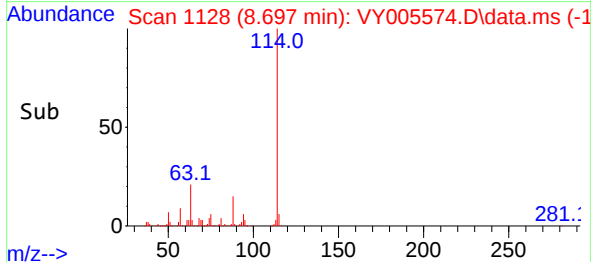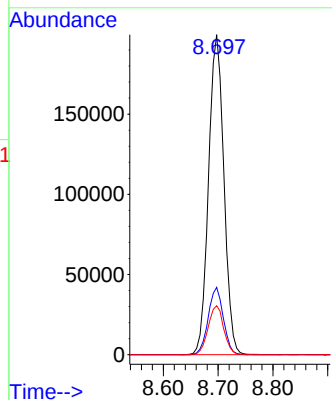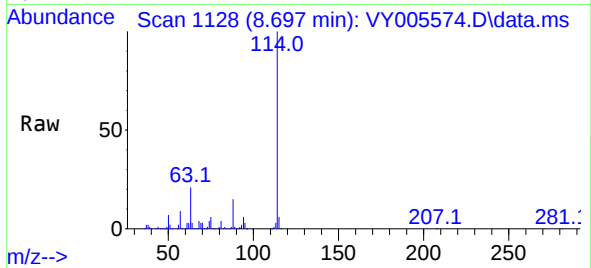

#35
Dibromofluoromethane
Concen: 52.70 ug/l
RT: 7.728 min Scan# 969
Delta R.T. -0.000 min
Lab File: VY005574.D
Acq: 06 Aug 2021 16:35

Tgt Ion:	113	Resp:	113925
Ion	Ratio	Lower	Upper
113	100		
111	102.2	81.9	122.9
192	23.4	19.2	28.8


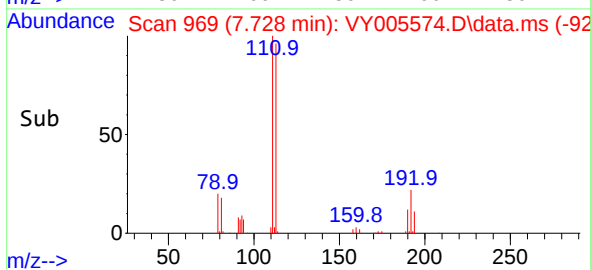
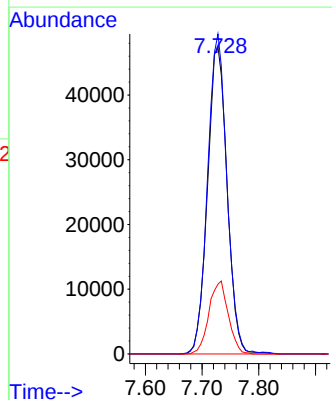
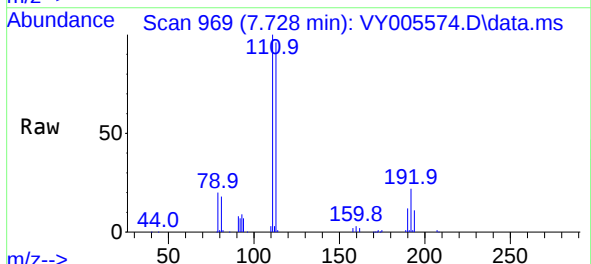




#50
Toluene-d8
Concen: 54.26 ug/l
RT: 10.185 min Scan# 1372
Delta R.T. -0.000 min
Lab File: VY005574.D
Acq: 06 Aug 2021 16:35




Instrument :
MSVOA_Y
ClientSampleId :
NB-08-080521


Tgt Ion: 98 Resp: 491924
Ion Ratio Lower Upper
98 100
100 62.8 51.3 76.9

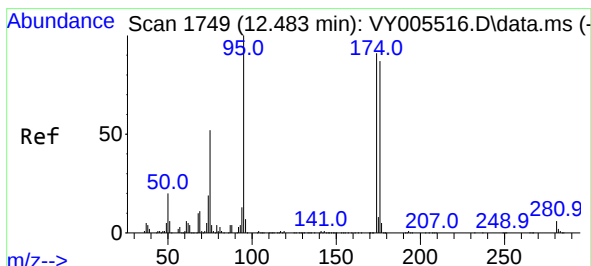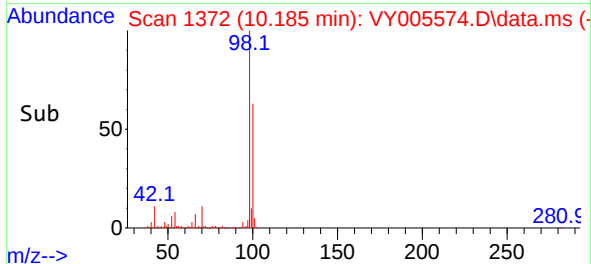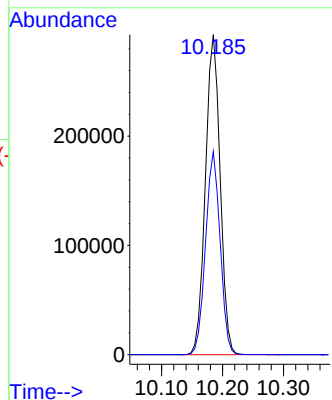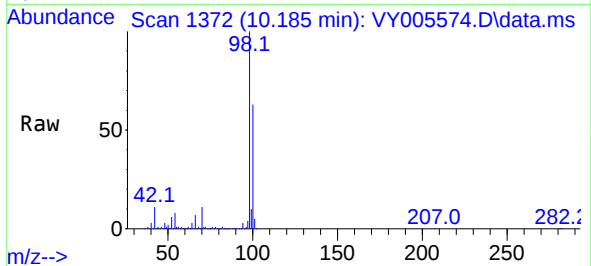

#62
4-Bromofluorobenzene
Concen: 56.43 ug/l
RT: 12.483 min Scan# 1749
Delta R.T. -0.000 min
Lab File: VY005574.D
Acq: 06 Aug 2021 16:35

Tgt Ion: 95 Resp: 169416
Ion Ratio Lower Upper
95 100
174 93.4 0.0 191.4
176 90.1 0.0 183.6


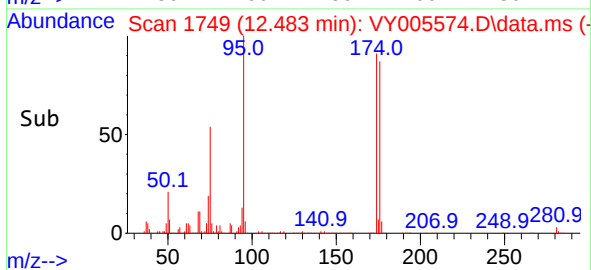
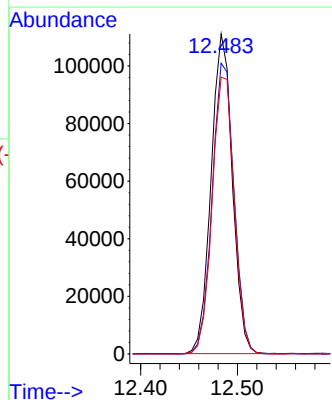
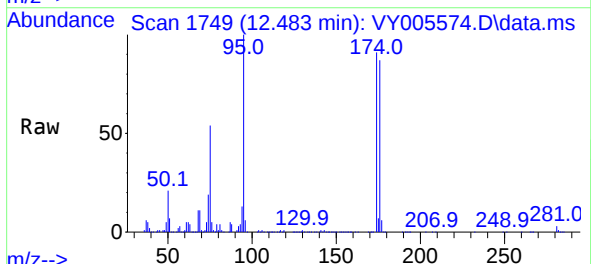


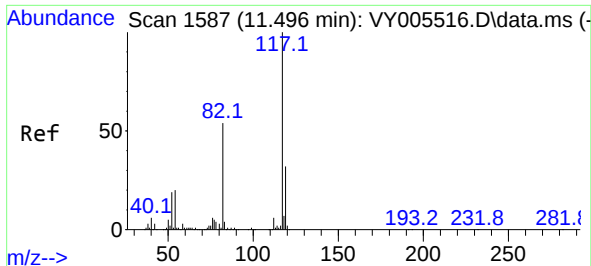

#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 11.496 min Scan# 1587
Delta R.T. -0.000 min
Lab File: VY005574.D
Acq: 06 Aug 2021 16:35

Instrument :
MSVOA_Y
ClientSampleId :
NB-08-080521

Tgt Ion:	117	Resp:	380500
Ion	Ratio	Lower	Upper
117	100		
82	55.1	43.5	65.3
119	31.8	25.5	38.3

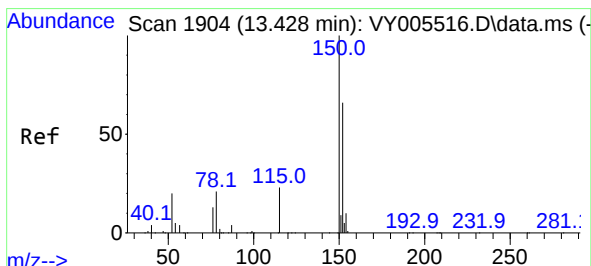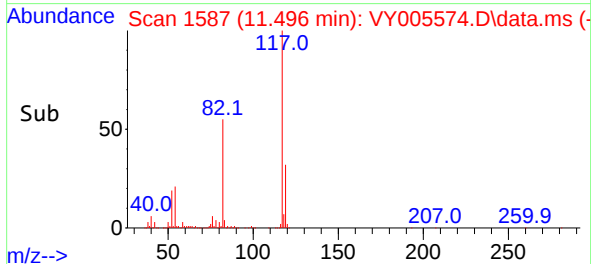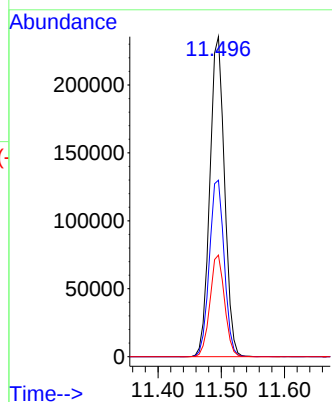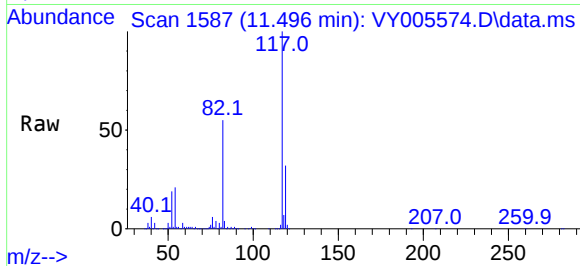

#72
1,4-Dichlorobenzene-d4
Concen: 50.00 ug/l
RT: 13.428 min Scan# 1904
Delta R.T. -0.000 min
Lab File: VY005574.D
Acq: 06 Aug 2021 16:35

Tgt Ion:	152	Resp:	191275
Ion	Ratio	Lower	Upper
152	100		
115	56.1	27.3	81.9
150	158.0	0.0	350.2

