



BFB

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY080723\
Data File : VY014963.D
Acq On : 07 Aug 2023 13:25
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y080723S.M
Title : SW846 8260
Last Update : Tue Aug 08 07:44:56 2023

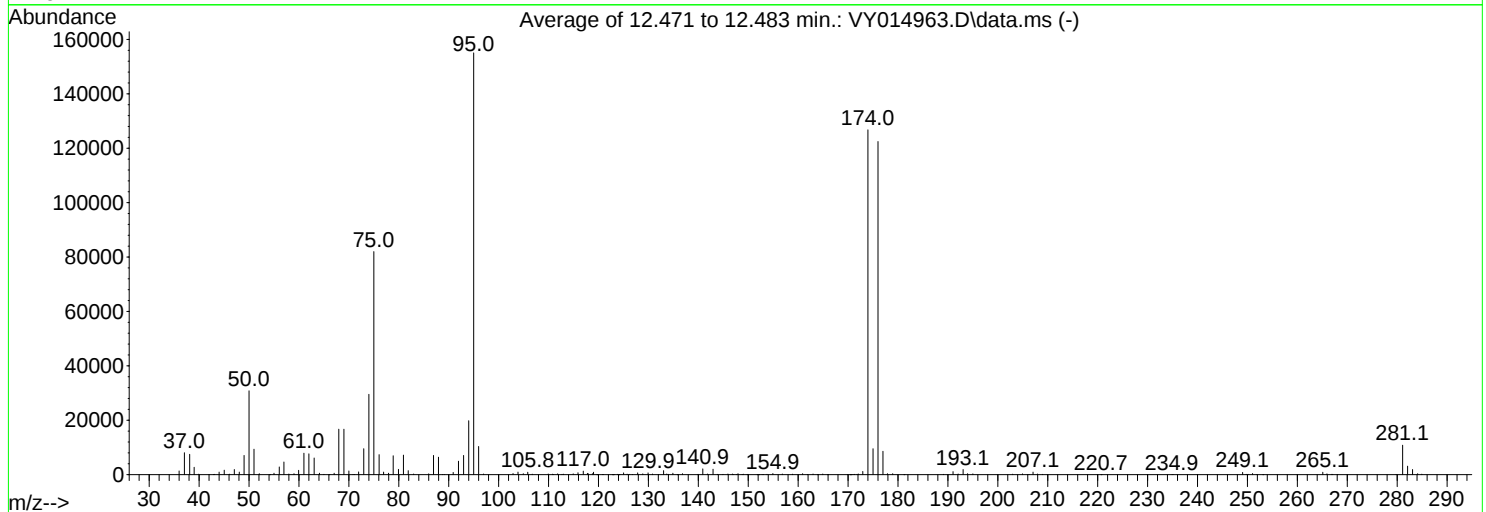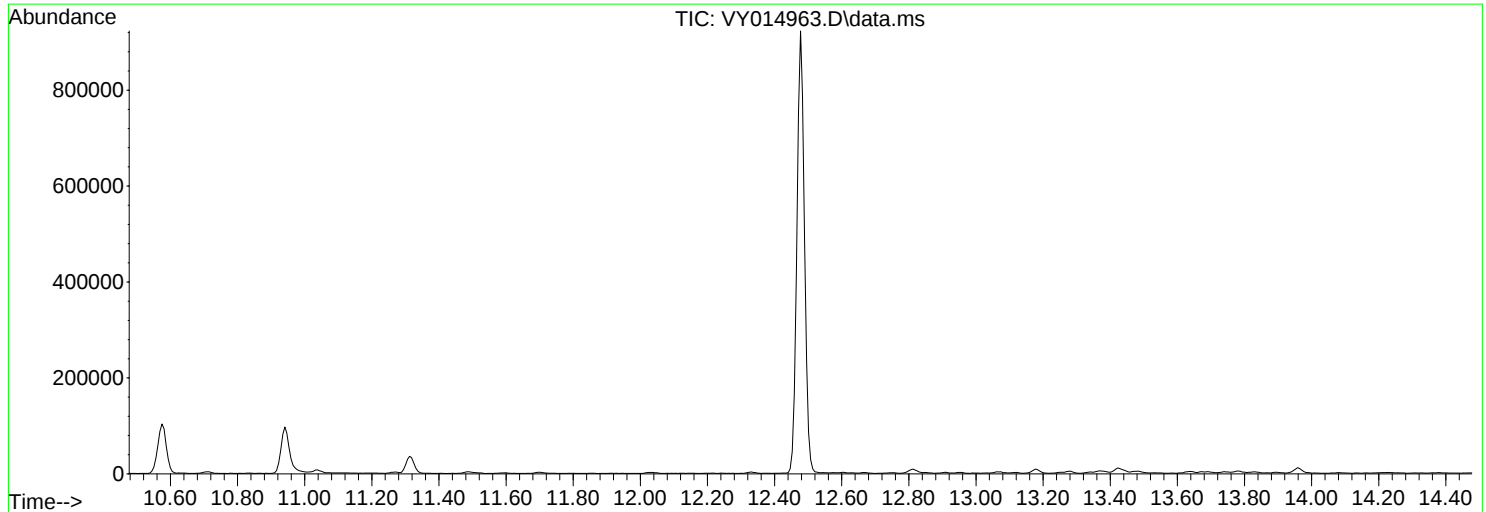

AutoFind: Scans 1747, 1748, 1749; Background Corrected with Scan 1739

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.9	30800	PASS
75	95	30	60	52.9	82003	PASS
95	95	100	100	100.0	155072	PASS
96	95	5	9	6.7	10363	PASS
173	174	0.00	2	0.9	1187	PASS
174	95	50	100	81.7	126752	PASS
175	174	5	9	7.5	9543	PASS
176	174	95	101	96.6	122469	PASS
177	176	5	9	7.0	8595	PASS