
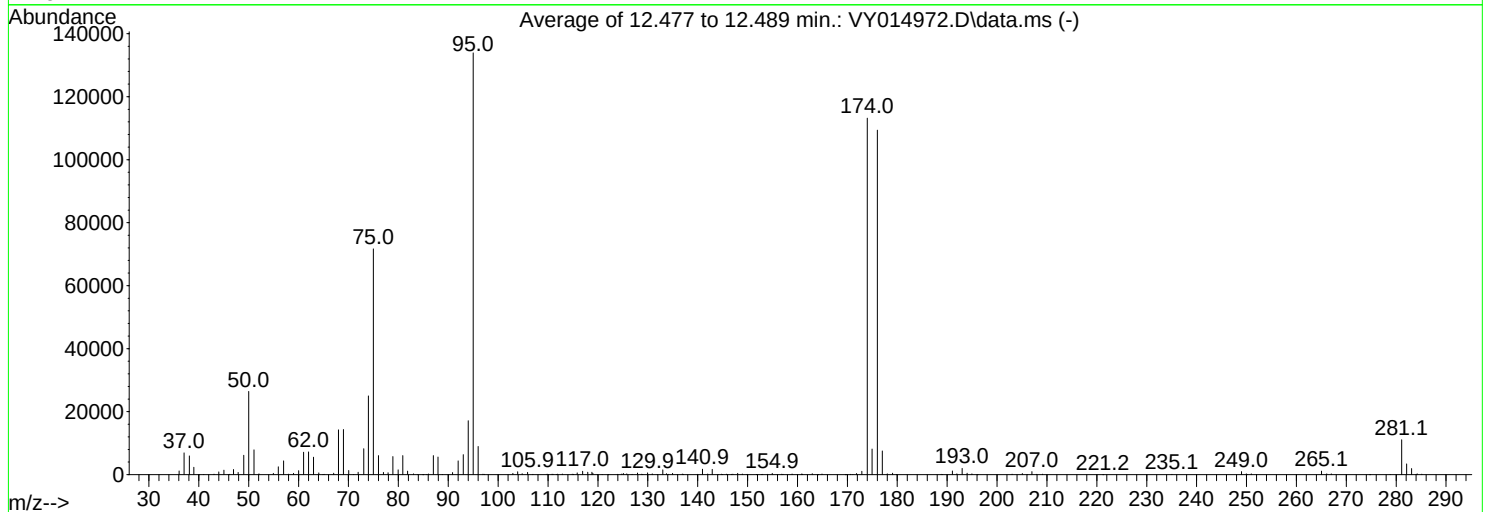


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY080823\
Data File : VY014972.D
Acq On : 08 Aug 2023 08:55
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y063023S.M
Title : SW846 8260
Last Update : Fri Jun 30 19:02:11 2023

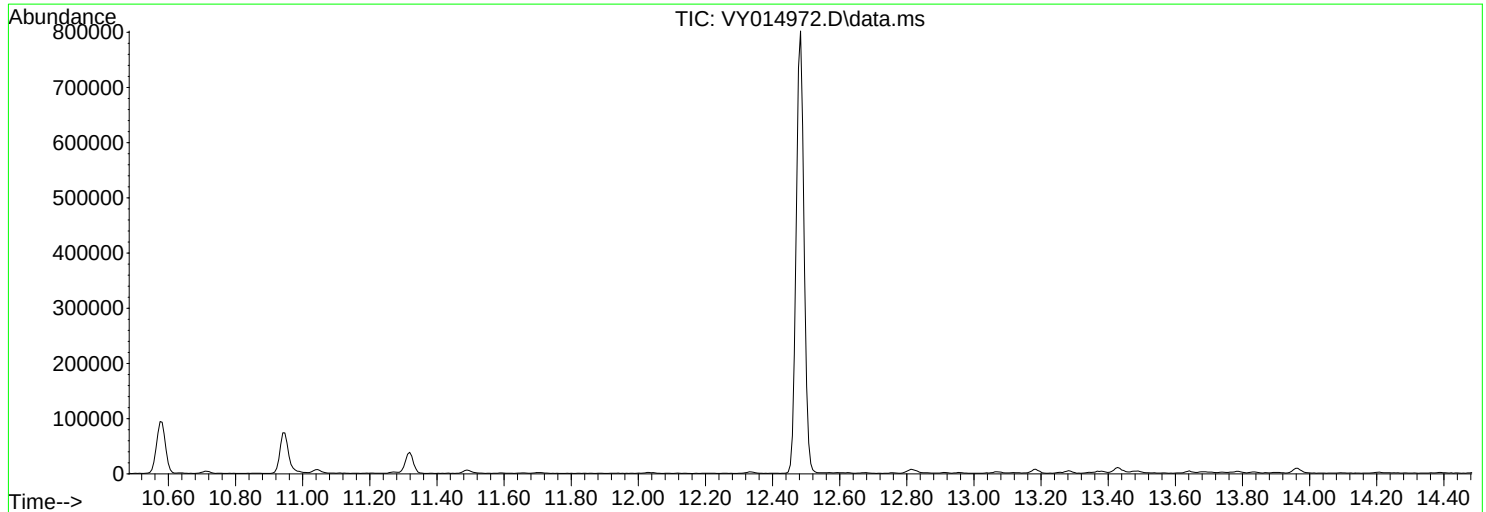

AutoFind: Scans 1748, 1749, 1750; Background Corrected with Scan 1740

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	19.7	26408	PASS
75	95	30	60	53.5	71683	PASS
95	95	100	100	100.0	133920	PASS
96	95	5	9	6.7	8957	PASS
173	174	0.00	2	1.0	1095	PASS
174	95	50	100	84.5	113211	PASS
175	174	5	9	7.2	8115	PASS
176	174	95	101	96.6	109405	PASS
177	176	5	9	6.9	7547	PASS