

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY081021\
 Data File : VY005582.D
 Acq On : 10 Aug 2021 09:27
 Operator : SY/MD
 Sample : VY0810SBL01
 Misc : 5.00G/5ML/MSVOA_Y/SOIL
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 VY0810SBL01

Quant Time: Aug 11 03:35:10 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y080221S.M
 Quant Title : SW846 8260
 QLast Update : Tue Aug 03 04:52:05 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.795	168	263182	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.697	114	390087	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.489	117	347697	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.428	152	176170	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.149	65	139897	52.513	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	105.020%
35) Dibromofluoromethane	7.722	113	118027	54.042	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	108.080%
50) Toluene-d8	10.185	98	475192	51.879	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	=	103.760%
62) 4-Bromofluorobenzene	12.483	95	156811	51.698	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	=	103.400%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY081021\
Data File : VY005582.D
Acq On : 10 Aug 2021 09:27
Operator : SY/MD
Sample : VY0810SBL01
Misc : 5.00G/5ML/MSVOA_Y/SOIL
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
VY0810SBL01

Quant Time: Aug 11 03:35:10 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y080221S.M
Quant Title : SW846 8260
QLast Update : Tue Aug 03 04:52:05 2021
Response via : Initial Calibration




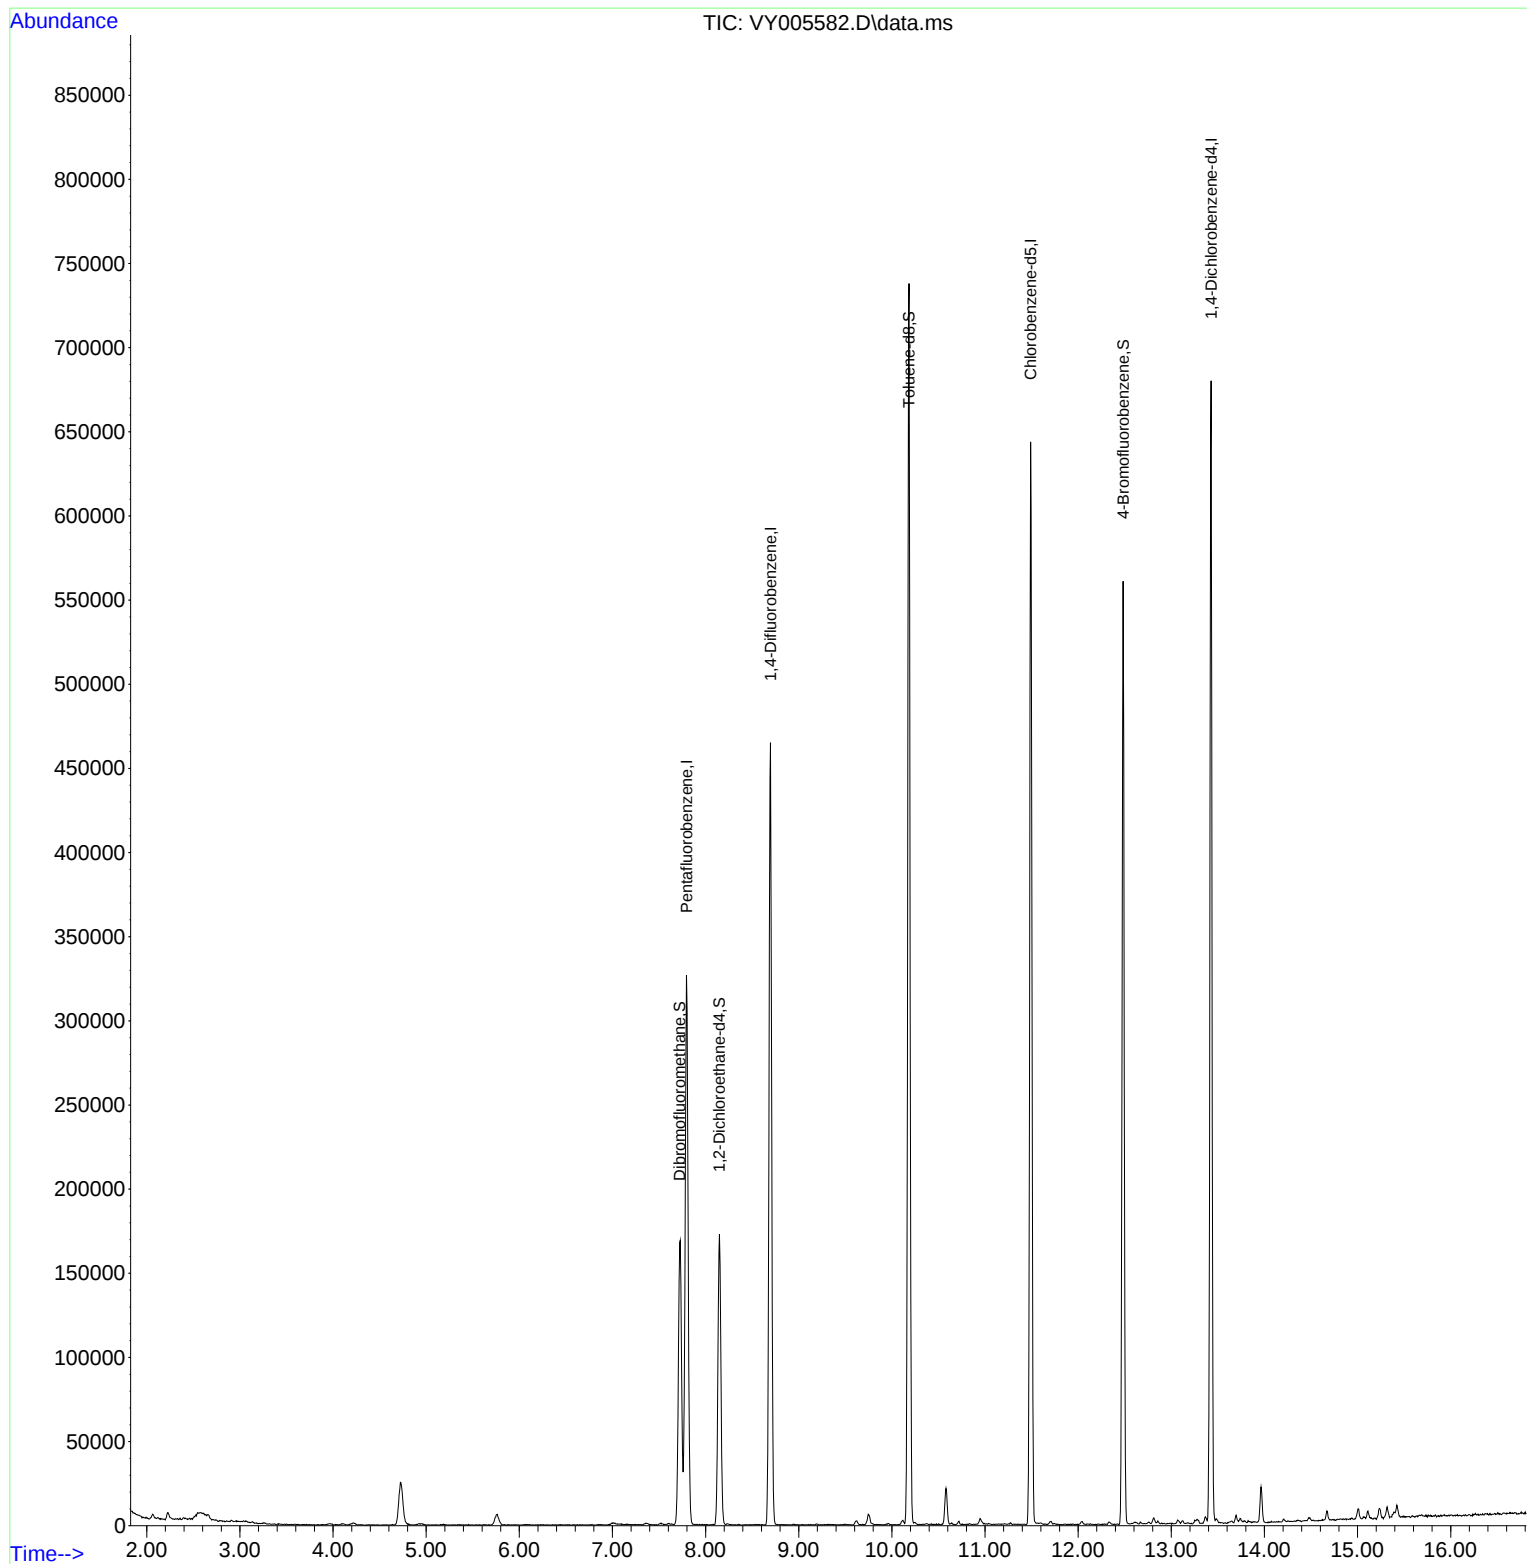


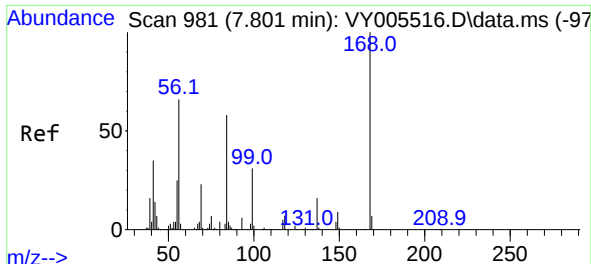

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.795 min Scan# 980
Delta R.T. -0.006 min
Lab File: VY005582.D
Acq: 10 Aug 2021 09:27




Instrument :
MSVOA_Y
ClientSampleId :
VY0810SBL01


Tgt Ion:168 Resp: 263182
Ion Ratio Lower Upper
168 100
99 51.9 38.9 58.3

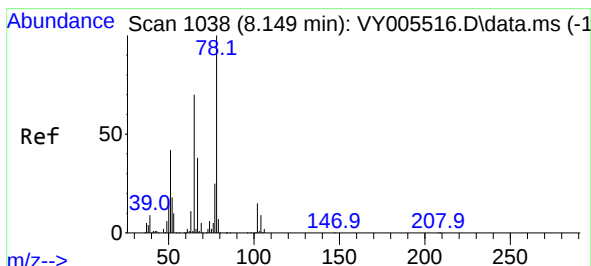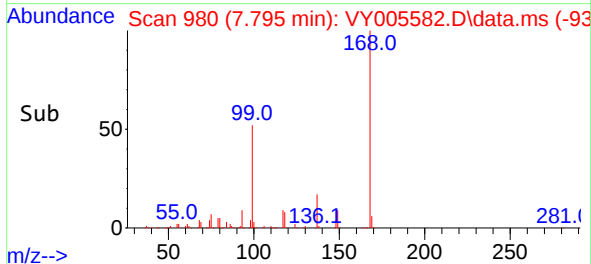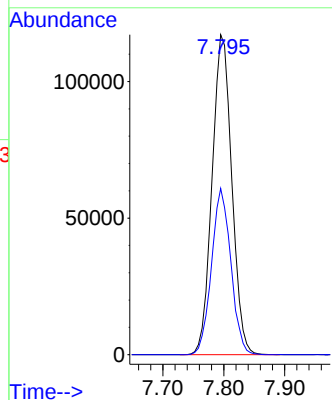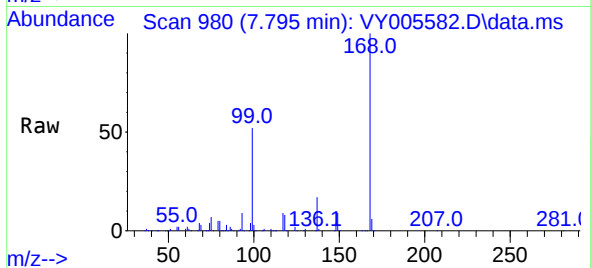

#33
1,2-Dichloroethane-d4
Concen: 52.513 ug/l
RT: 8.149 min Scan# 1038
Delta R.T. -0.000 min
Lab File: VY005582.D
Acq: 10 Aug 2021 09:27

Tgt Ion: 65 Resp: 139897
Ion Ratio Lower Upper
65 100
67 51.0 0.0 103.4

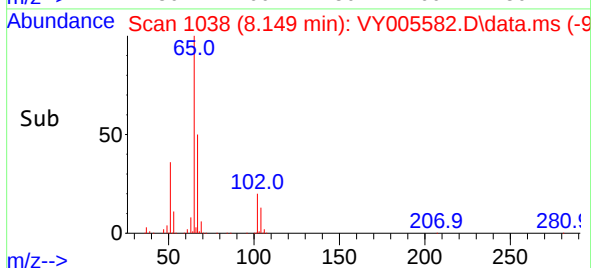
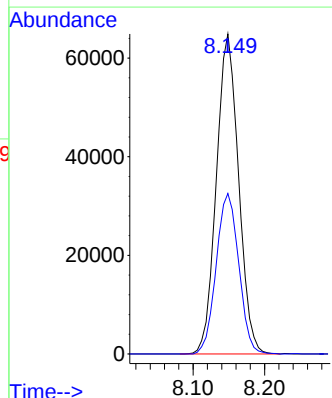
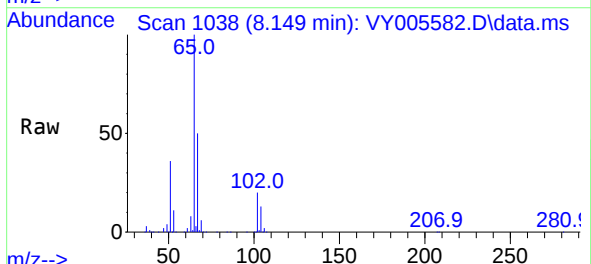


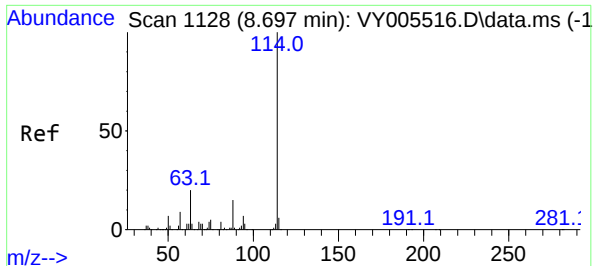

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.697 min Scan# 1128
Delta R.T. -0.000 min
Lab File: VY005582.D
Acq: 10 Aug 2021 09:27




Instrument :
MSVOA_Y
ClientSampleId :
VY0810SBL01


Tgt Ion:	114	Resp:	390087
Ion	Ratio	Lower	Upper
114	100		
63	19.7	0.0	39.2
88	15.1	0.0	30.8

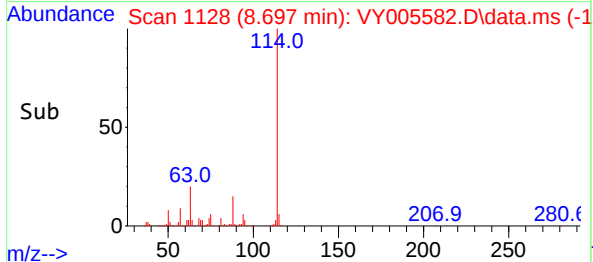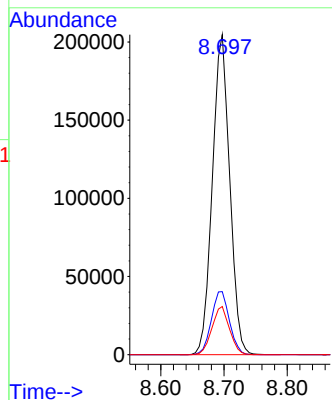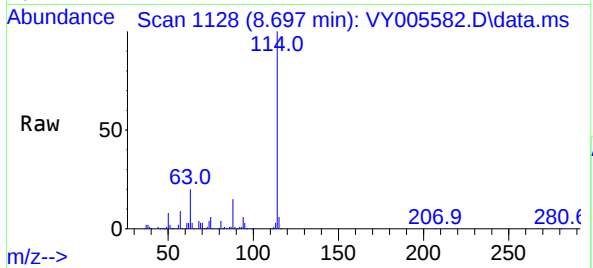

#35
Dibromofluoromethane
Concen: 54.042 ug/l
RT: 7.722 min Scan# 968
Delta R.T. -0.006 min
Lab File: VY005582.D
Acq: 10 Aug 2021 09:27

Tgt Ion:	113	Resp:	118027
Ion	Ratio	Lower	Upper
113	100		
111	100.9	81.9	122.9
192	23.7	19.2	28.8


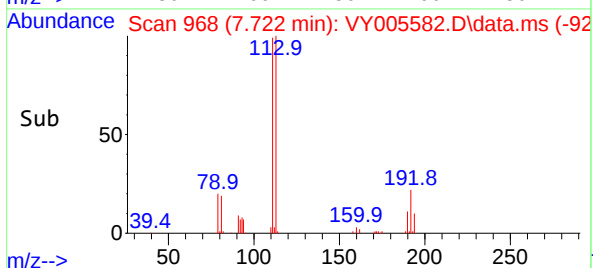
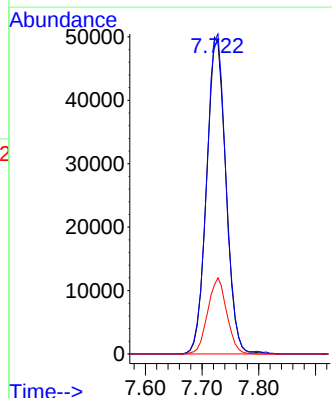
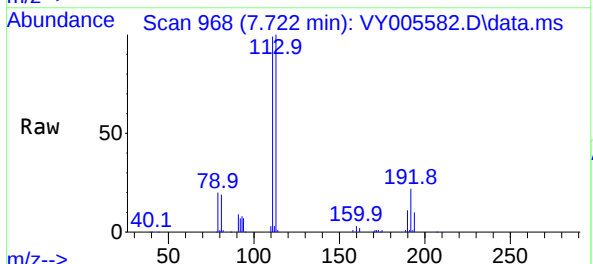


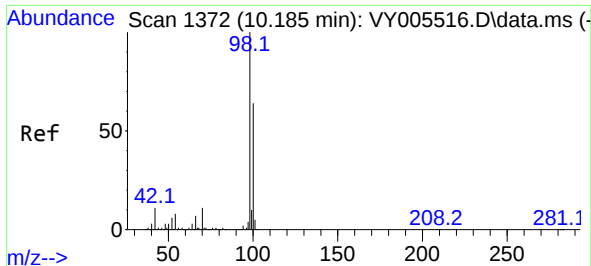

#50
Toluene-d8
Concen: 51.879 ug/l
RT: 10.185 min Scan# 1372
Delta R.T. -0.000 min
Lab File: VY005582.D
Acq: 10 Aug 2021 09:27




Instrument :
MSVOA_Y
ClientSampleId :
VY0810SBL01


Tgt Ion: 98 Resp: 475192
Ion Ratio Lower Upper
98 100
100 63.7 51.3 76.9

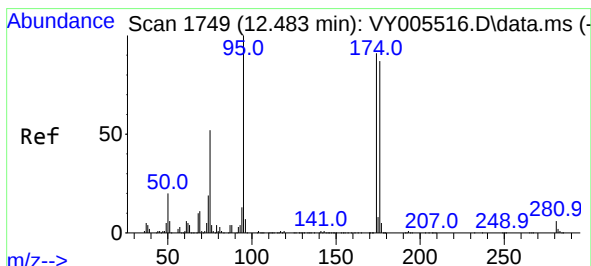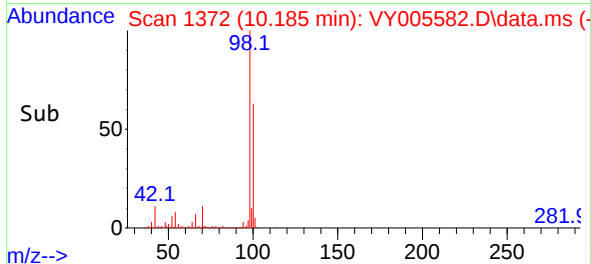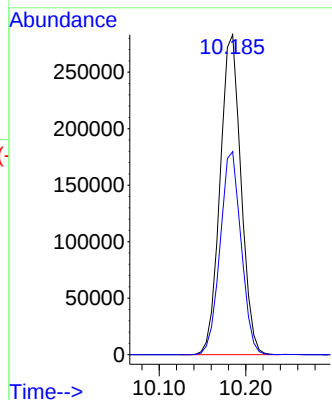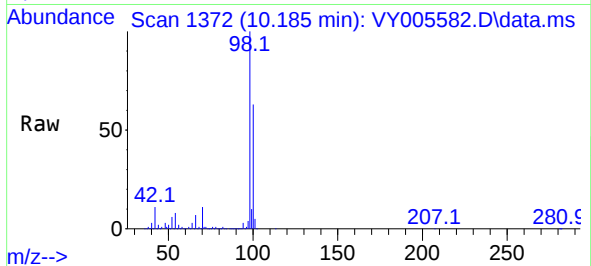

#62
4-Bromofluorobenzene
Concen: 51.698 ug/l
RT: 12.483 min Scan# 1749
Delta R.T. -0.000 min
Lab File: VY005582.D
Acq: 10 Aug 2021 09:27

Tgt Ion: 95 Resp: 156811
Ion Ratio Lower Upper
95 100
174 93.0 0.0 191.4
176 91.3 0.0 183.6

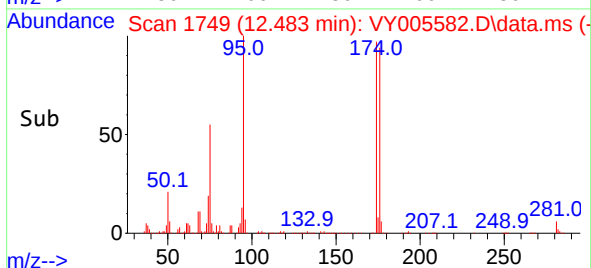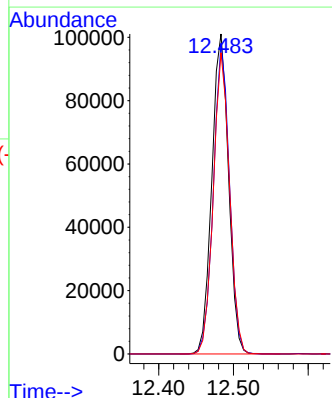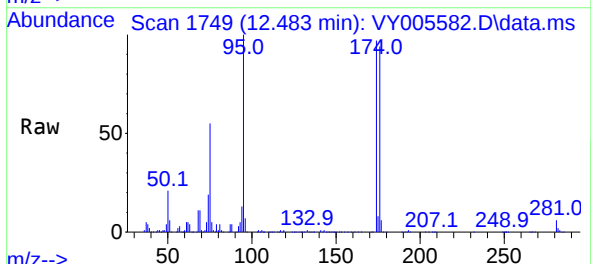




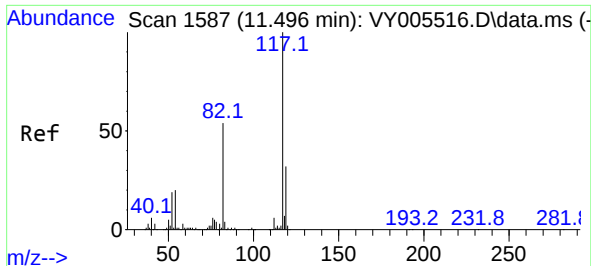


#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.489 min Scan# 1586
Delta R.T. -0.006 min
Lab File: VY005582.D
Acq: 10 Aug 2021 09:27

Instrument :
MSVOA_Y
ClientSampleId :
VY0810SBL01

Tgt Ion:117 Resp: 347697

Ion	Ratio	Lower	Upper
117	100		
82	56.4	43.5	65.3
119	32.5	25.5	38.3

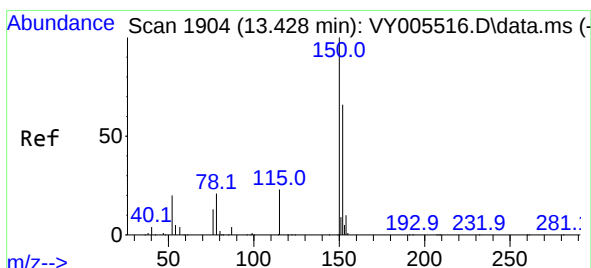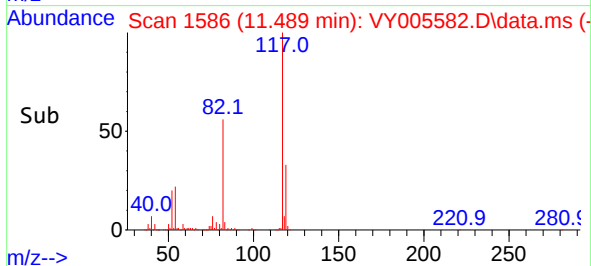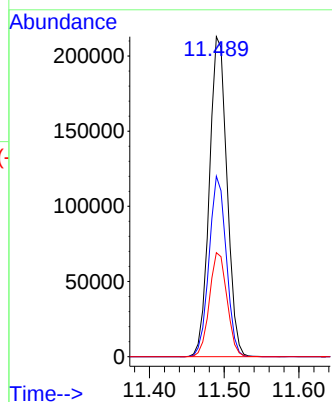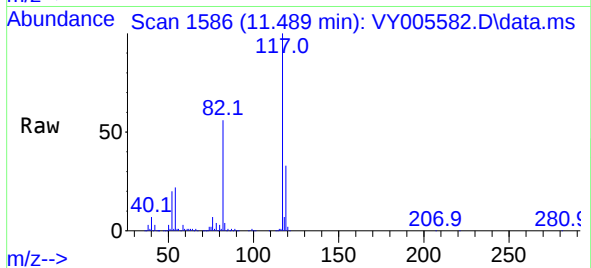

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.428 min Scan# 1904
Delta R.T. -0.000 min
Lab File: VY005582.D
Acq: 10 Aug 2021 09:27

Tgt Ion:152 Resp: 176170

Ion	Ratio	Lower	Upper
152	100		
115	54.6	27.3	81.9
150	156.7	0.0	350.2

