
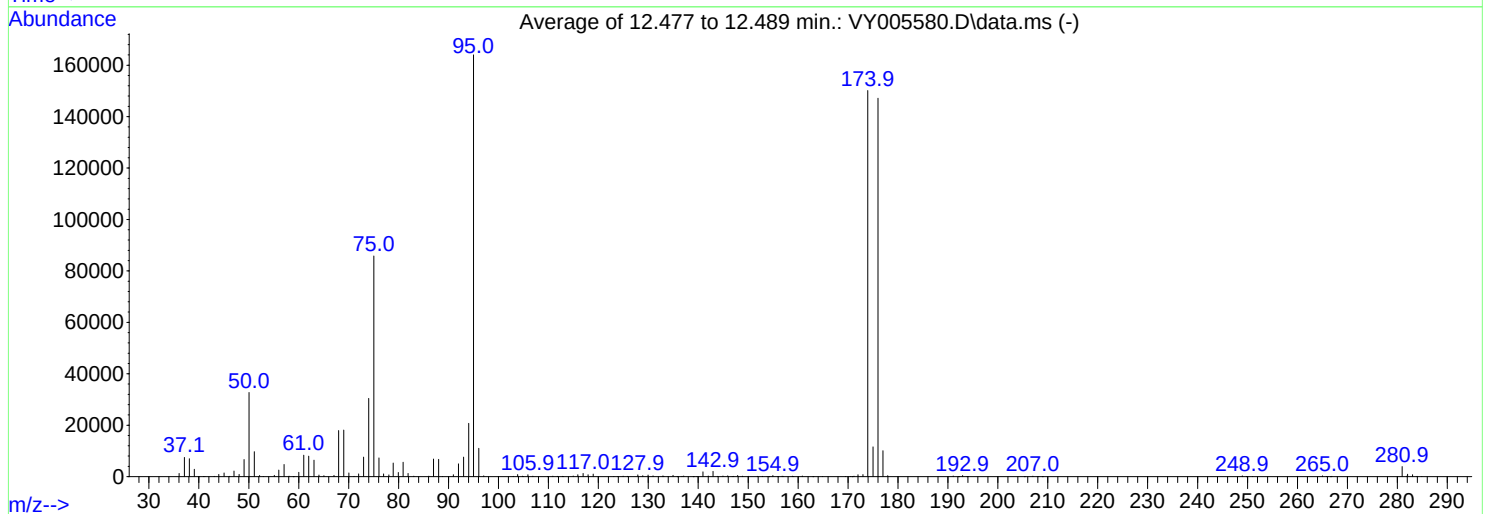


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY081021\
 Data File : VY005580.D
 Acq On : 10 Aug 2021 08:25
 Operator : SY/MD
 Sample : BFB
 Misc : 5.00G/5ML/MSVOA_Y/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y080221S.M
 Title : SW846 8260
 Last Update : Tue Aug 03 04:52:05 2021

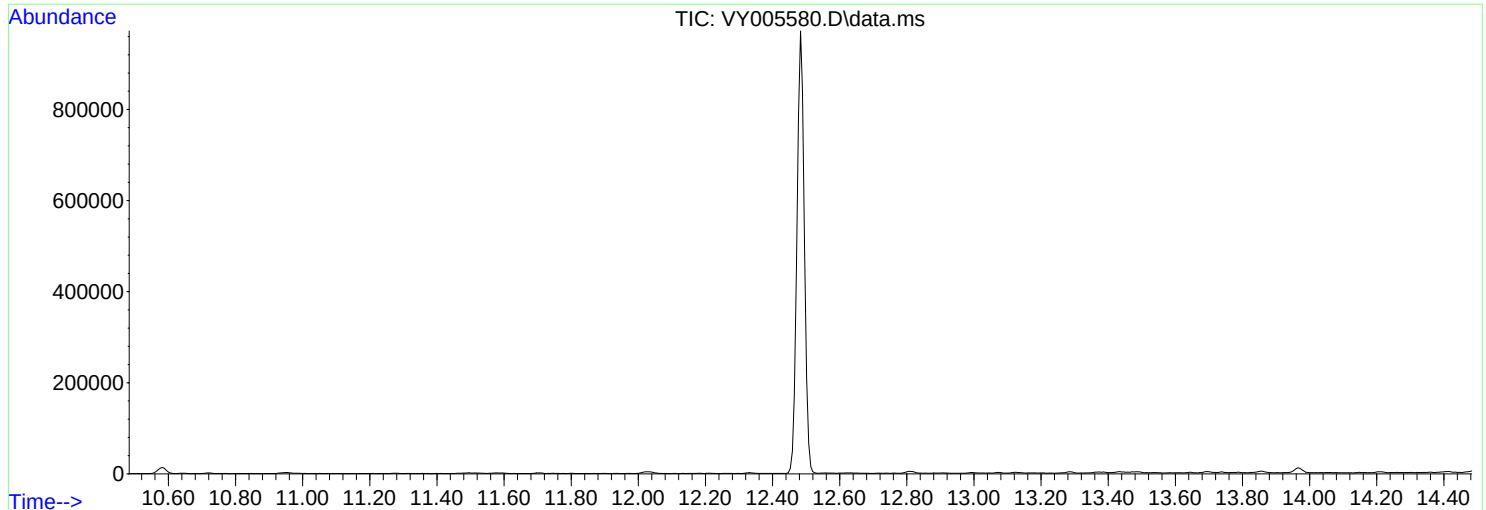

AutoFind: Scans 1748, 1749, 1750; Background Corrected with Scan 1739

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.9	32704	PASS
75	95	30	60	52.3	85821	PASS
95	95	100	100	100.0	164032	PASS
96	95	5	9	6.7	11008	PASS
173	174	0.00	2	0.5	795	PASS
174	95	50	100	91.6	150179	PASS
175	174	5	9	7.7	11583	PASS
176	174	95	101	98.0	147147	PASS
177	176	5	9	6.8	10063	PASS