

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY081023\
 Data File : VY015041.D
 Acq On : 10 Aug 2023 20:34
 Operator : SY/MD
 Sample : 03955-13
 Misc : 3.82g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 WC-26

Quant Time: Aug 11 01:58:35 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y080723S.M
 Quant Title : SW846 8260
 QLast Update : Tue Aug 08 07:44:56 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.789	168	219970	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.691	114	374147	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.489	117	368591	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.422	152	189448	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.143	65	137446	51.553	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	103.100%
35) Dibromofluoromethane	7.716	113	118314	49.450	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	98.900%
50) Toluene-d8	10.179	98	440118	48.329	ug/l	0.00
Spiked Amount	50.000	Range	58 - 134	Recovery	=	96.660%
62) 4-Bromofluorobenzene	12.483	95	174610	54.099	ug/l	0.00
Spiked Amount	50.000	Range	30 - 143	Recovery	=	108.200%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY081023\
Data File : VY015041.D
Acq On : 10 Aug 2023 20:34
Operator : SY/MD
Sample : 03955-13
Misc : 3.82g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
WC-26

Quant Time: Aug 11 01:58:35 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y080723S.M
Quant Title : SW846 8260
QLast Update : Tue Aug 08 07:44:56 2023
Response via : Initial Calibration




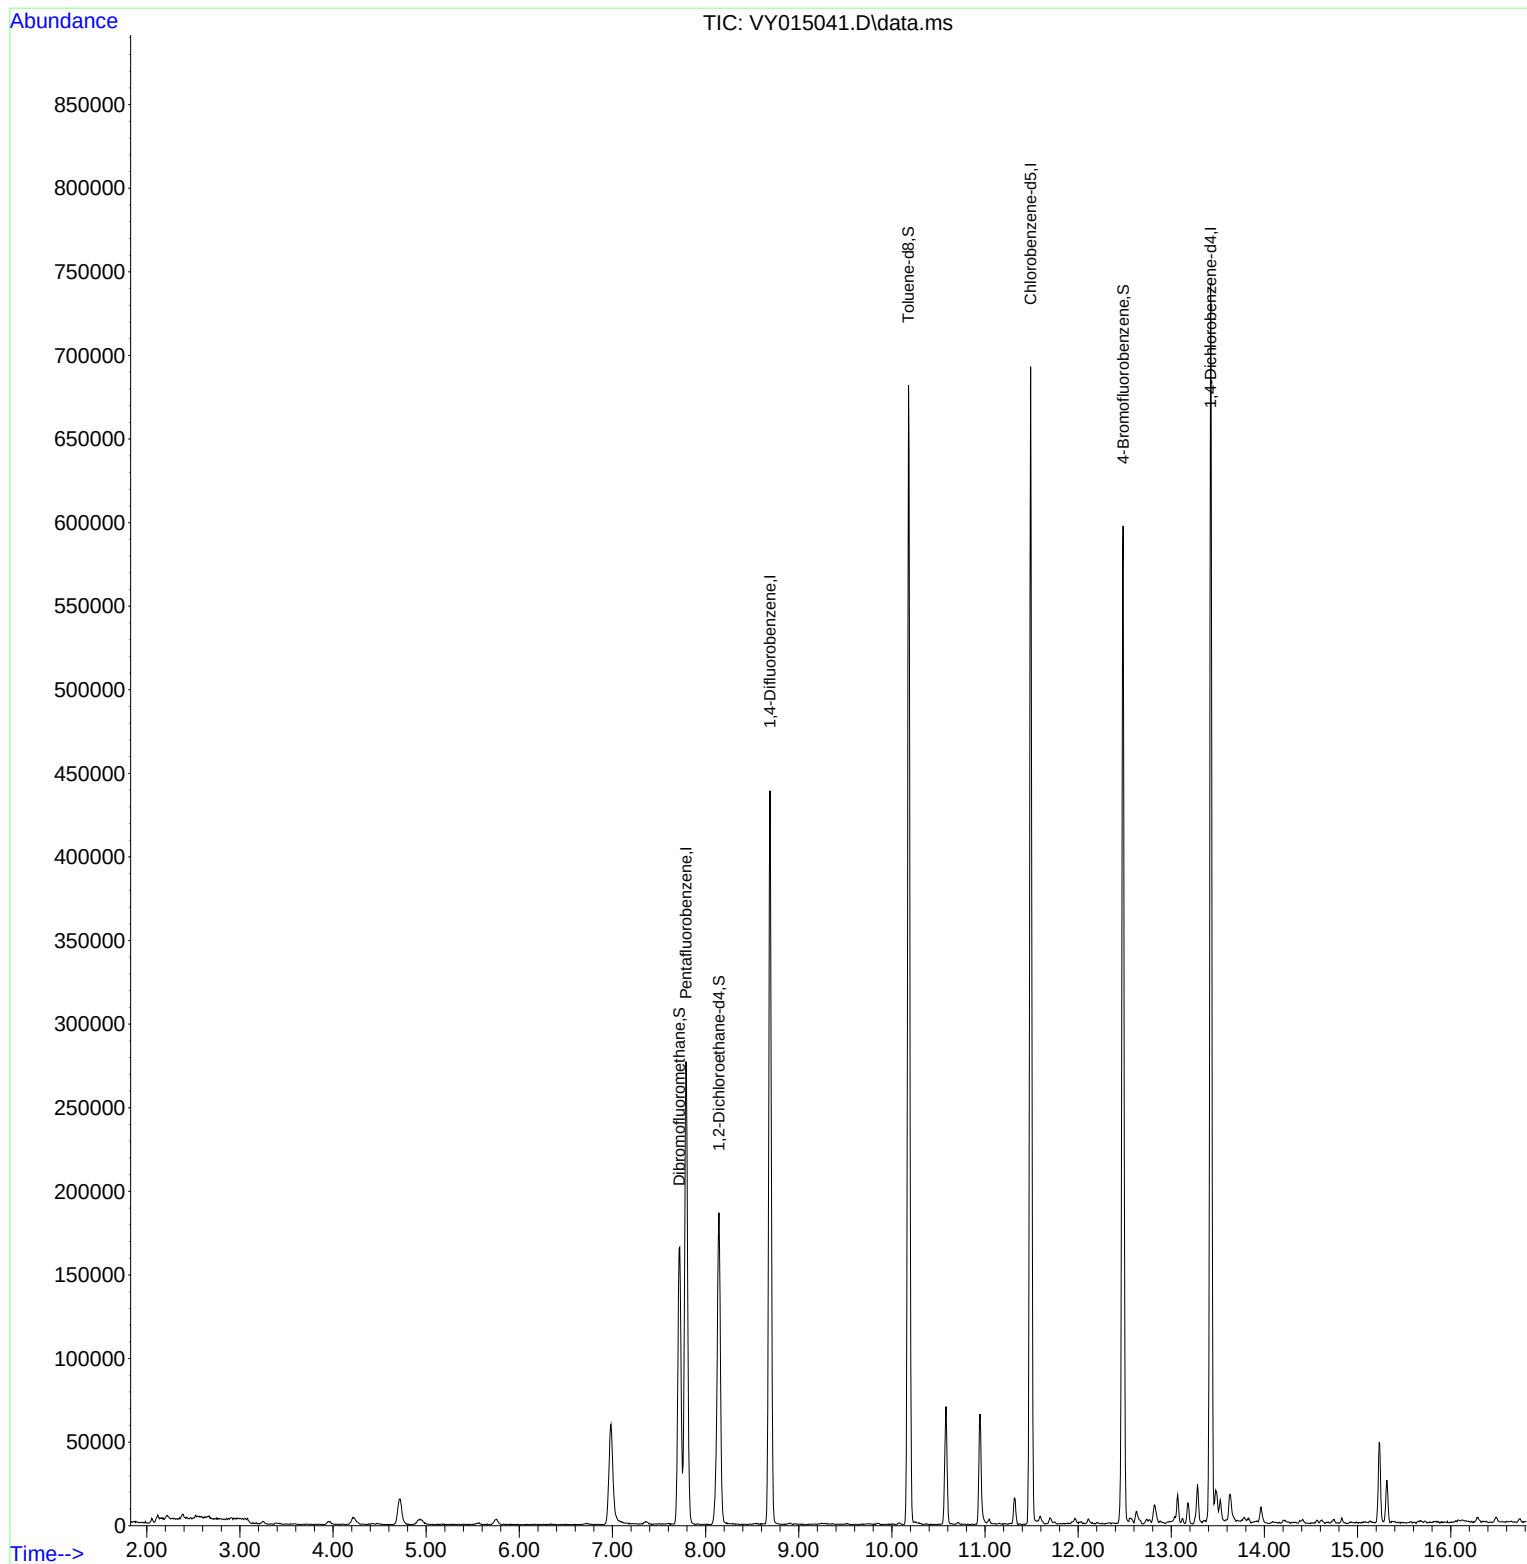


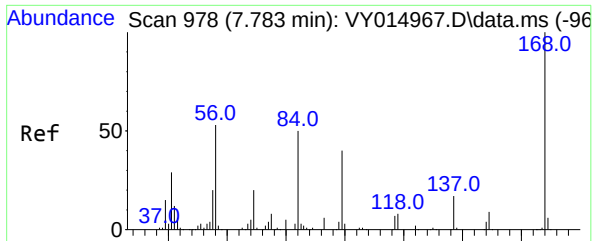

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.789 min Scan# 91
Delta R.T. 0.006 min
Lab File: VY015041.D
Acq: 10 Aug 2023 20:34




Instrument :
MSVOA_Y
ClientSampleId :
WC-26


Tgt Ion:168 Resp: 219970
Ion Ratio Lower Upper
168 100
99 53.9 43.4 65.0

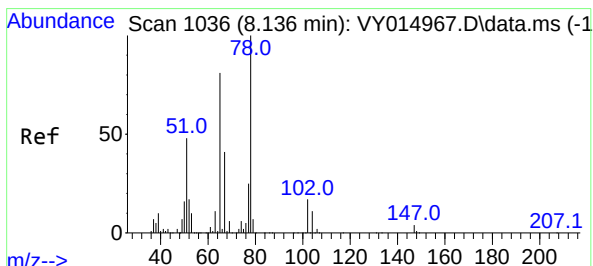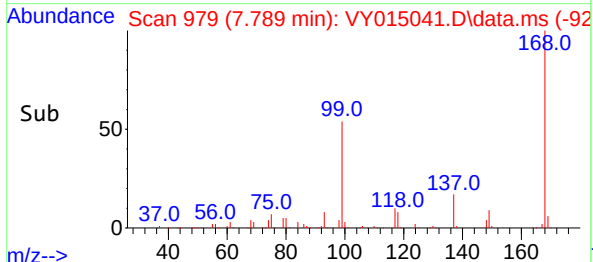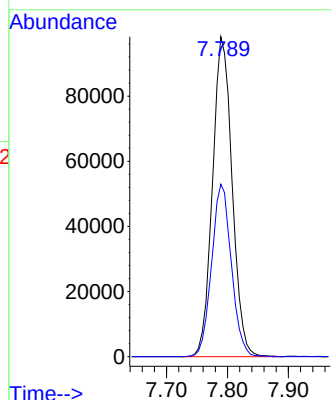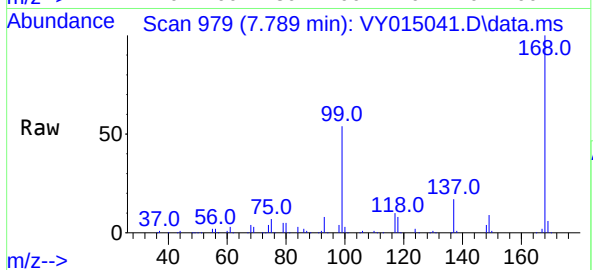

#33
1,2-Dichloroethane-d4
Concen: 51.553 ug/l
RT: 8.143 min Scan# 1037
Delta R.T. 0.006 min
Lab File: VY015041.D
Acq: 10 Aug 2023 20:34

Tgt Ion: 65 Resp: 137446
Ion Ratio Lower Upper
65 100
67 52.5 0.0 101.8

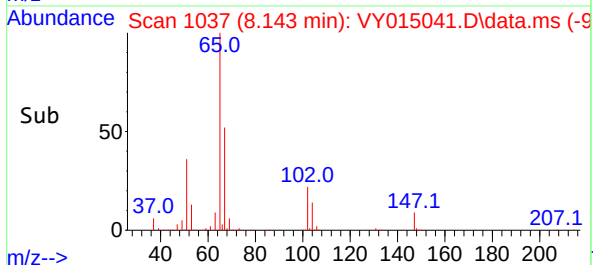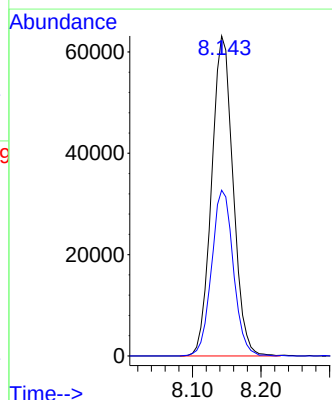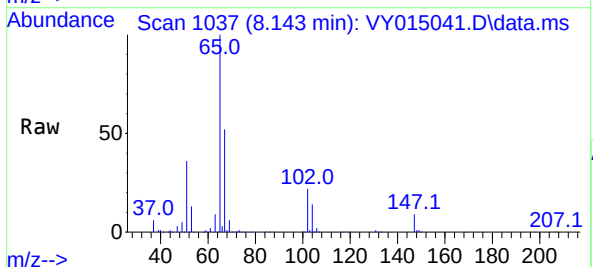

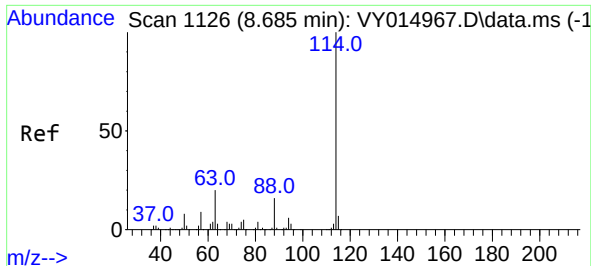

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.691 min Scan# 1126

Delta R.T. 0.006 min

Lab File: VY015041.D

Acq: 10 Aug 2023 20:34

Instrument :

MSVOA_Y

ClientSampleId :

WC-26





Tgt Ion:114 Resp: 374147

Ion Ratio Lower Upper

114 100

63 18.7 0.0 42.4

88 15.2 0.0 30.6

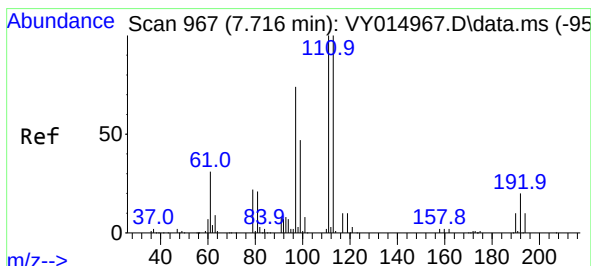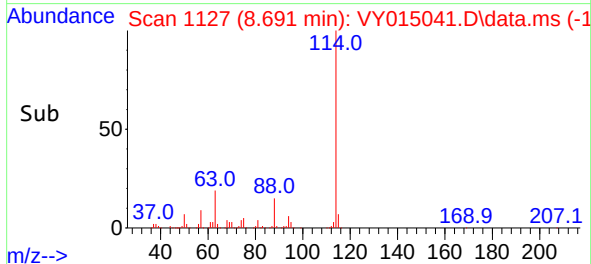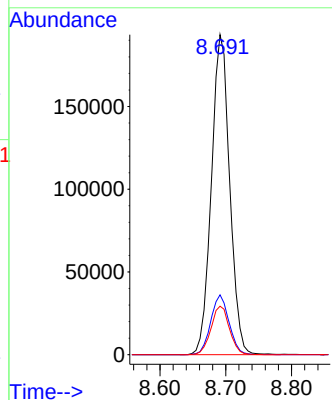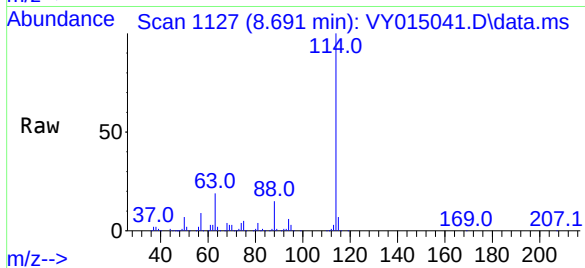

#35

Dibromofluoromethane

Concen: 49.450 ug/l

RT: 7.716 min Scan# 967

Delta R.T. 0.000 min

Lab File: VY015041.D

Acq: 10 Aug 2023 20:34




Tgt Ion:113 Resp: 118314


Ion Ratio Lower Upper

113 100

111 102.3 81.3 121.9

192 20.4 16.9 25.3


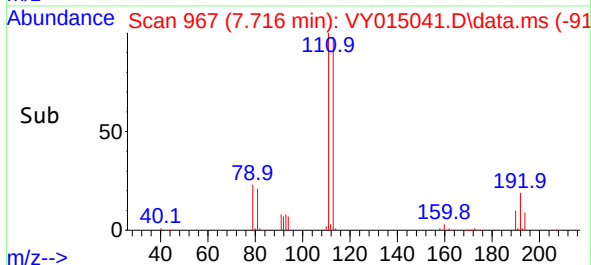
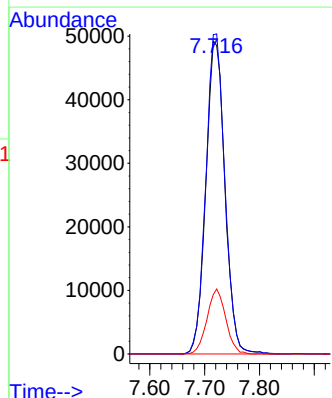
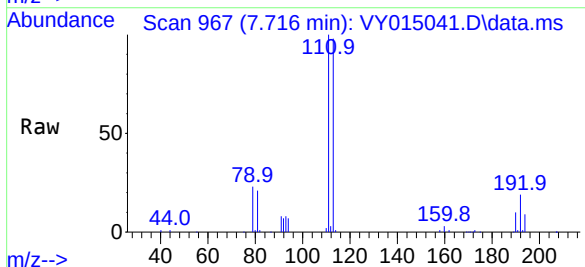


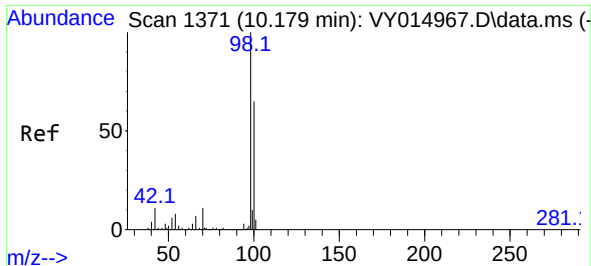

#50
Toluene-d8
Concen: 48.329 ug/l
RT: 10.179 min Scan# 11
Delta R.T. 0.000 min
Lab File: VY015041.D
Acq: 10 Aug 2023 20:34




Instrument :
MSVOA_Y
ClientSampleId :
WC-26


Tgt Ion: 98 Resp: 440118
Ion Ratio Lower Upper
98 100
100 65.7 50.1 75.1

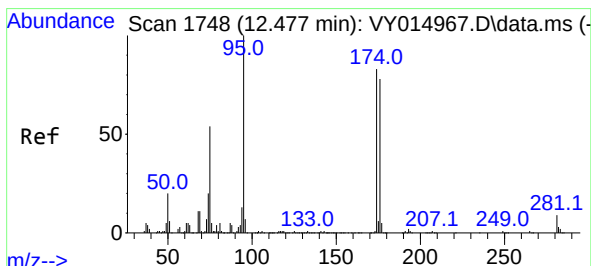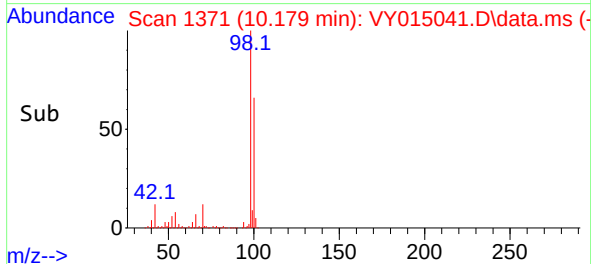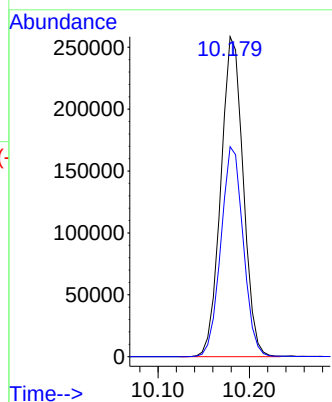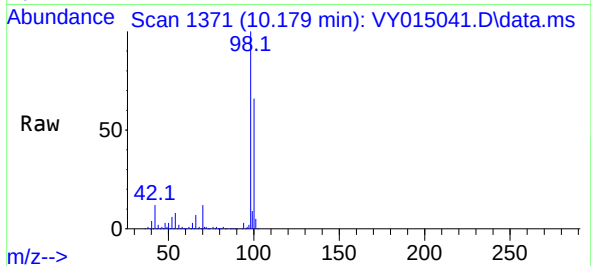

#62
4-Bromofluorobenzene
Concen: 54.099 ug/l
RT: 12.483 min Scan# 1749
Delta R.T. 0.006 min
Lab File: VY015041.D
Acq: 10 Aug 2023 20:34

Tgt Ion: 95 Resp: 174610
Ion Ratio Lower Upper
95 100
174 84.8 0.0 178.2
176 82.6 0.0 173.8


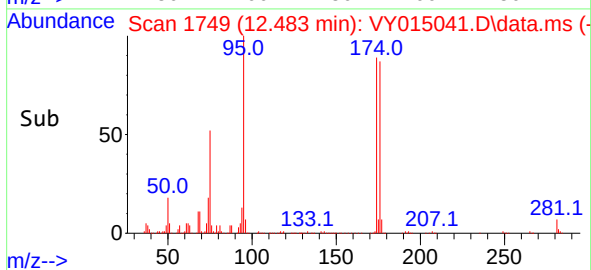
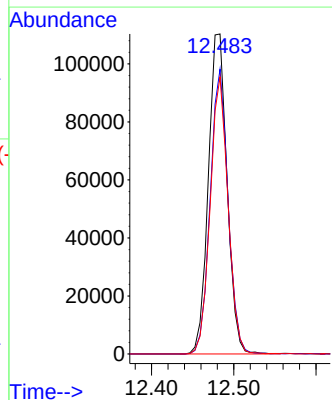
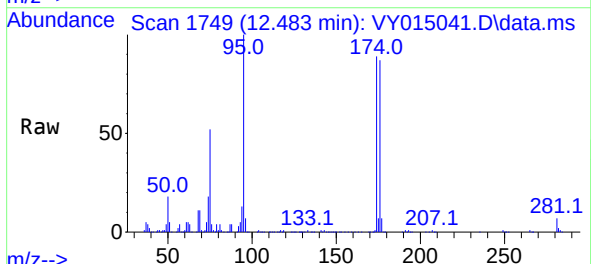


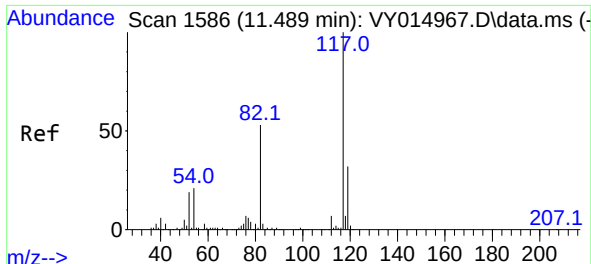

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.489 min Scan# 117
Delta R.T. 0.000 min
Lab File: VY015041.D
Acq: 10 Aug 2023 20:34

Instrument :
MSVOA_Y
ClientSampleId :
WC-26

Tgt Ion:117 Resp: 368591
Ion Ratio Lower Upper
117 100
82 53.6 43.4 65.0
119 32.5 26.3 39.5

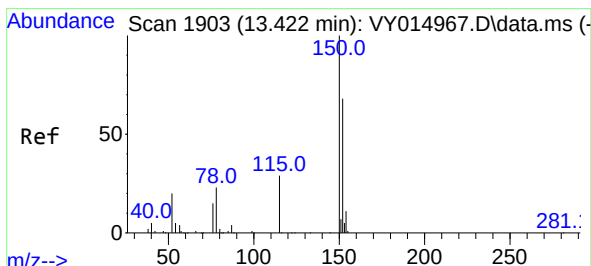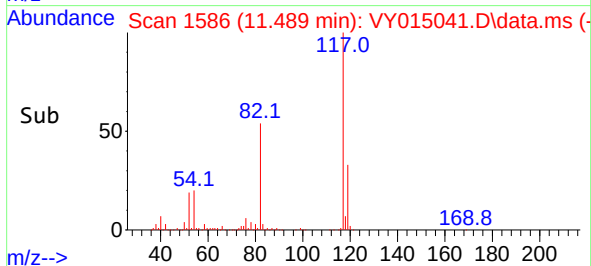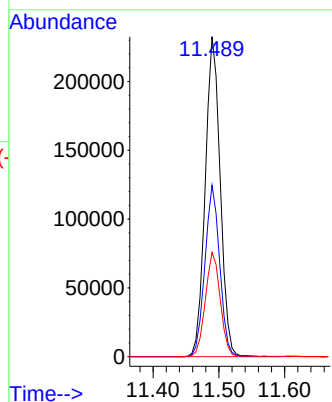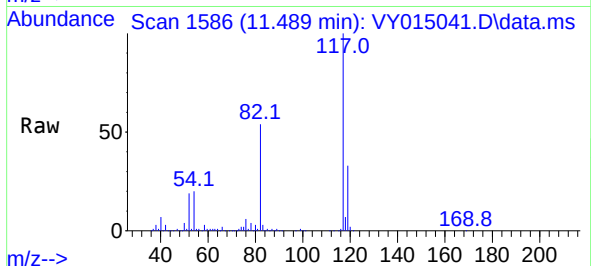

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.422 min Scan# 1903
Delta R.T. 0.000 min
Lab File: VY015041.D
Acq: 10 Aug 2023 20:34

Tgt Ion:152 Resp: 189448
Ion Ratio Lower Upper
152 100
115 58.2 28.8 86.5
150 156.5 0.0 348.8

