
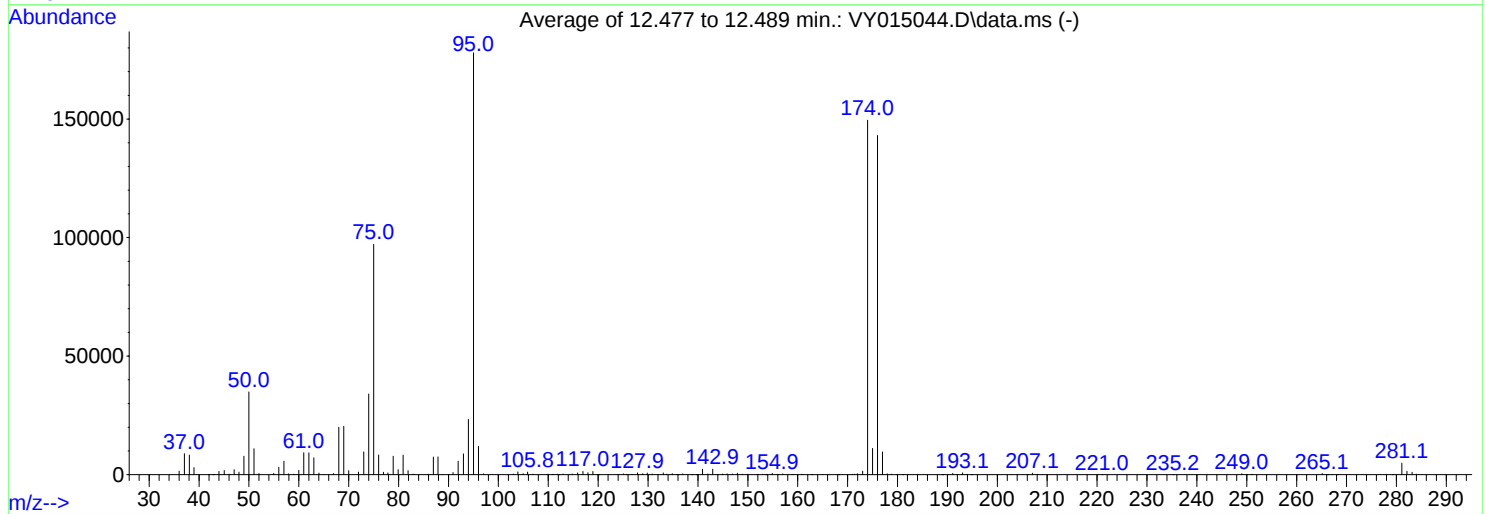


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY081123\
Data File : VY015044.D
Acq On : 11 Aug 2023 08:27
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y080723S.M
Title : SW846 8260
Last Update : Tue Aug 08 07:44:56 2023

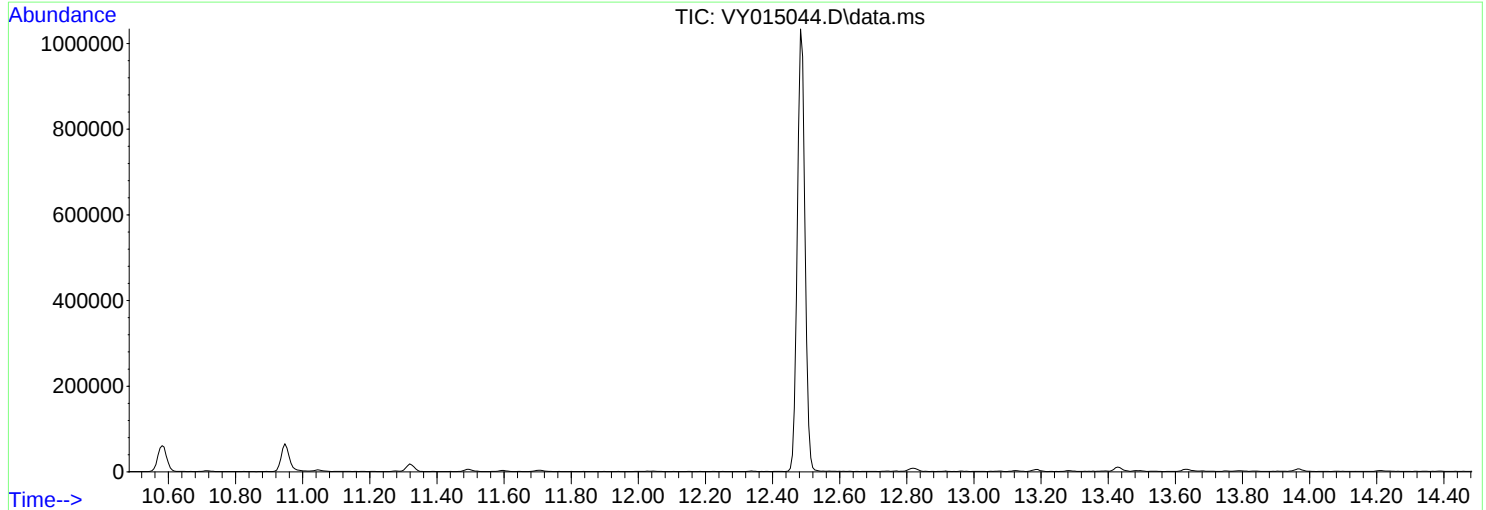

AutoFind: Scans 1748, 1749, 1750; Background Corrected with Scan 1739

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.6	34931	PASS
75	95	30	60	54.6	97155	PASS
95	95	100	100	100.0	177941	PASS
96	95	5	9	6.7	11891	PASS
173	174	0.00	2	1.0	1464	PASS
174	95	50	100	84.0	149501	PASS
175	174	5	9	7.4	11052	PASS
176	174	95	101	95.7	143112	PASS
177	176	5	9	6.7	9576	PASS