
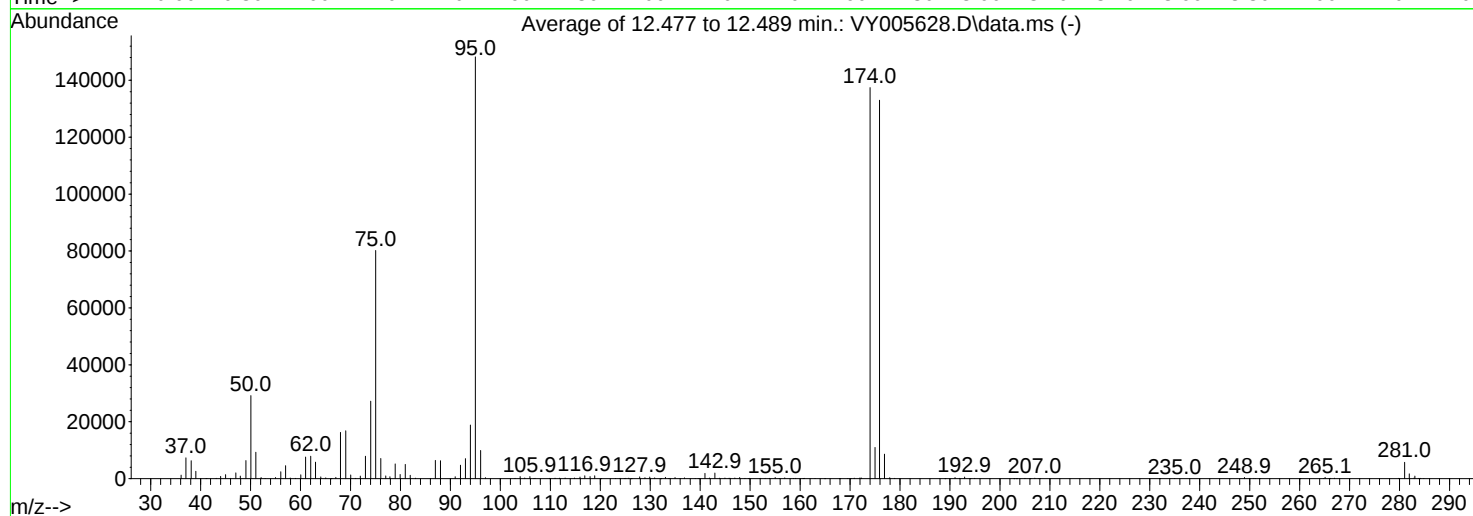


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY081321\
 Data File : VY005628.D
 Acq On : 13 Aug 2021 12:28
 Operator : SY/MD
 Sample : BFB
 Misc : 5.00G/5ML/MSVOA_Y/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y080221S.M
 Title : SW846 8260
 Last Update : Tue Aug 03 04:52:05 2021

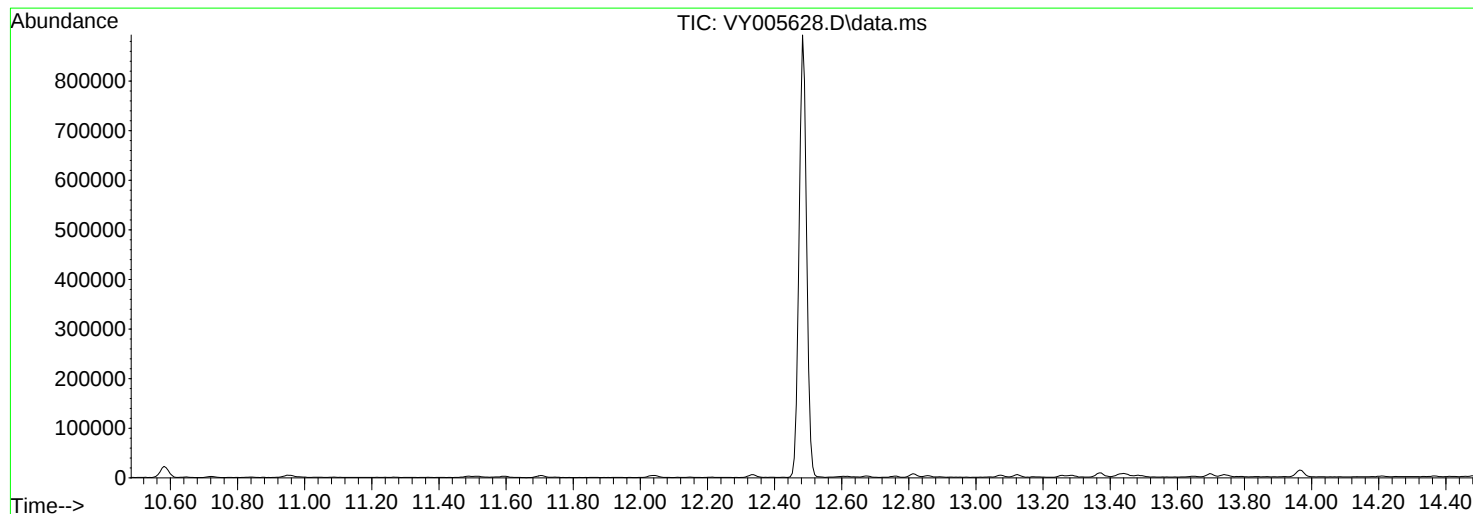

AutoFind: Scans 1748, 1749, 1750; Background Corrected with Scan 1740

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.7	29192	PASS
75	95	30	60	54.1	80179	PASS
95	95	100	100	100.0	148245	PASS
96	95	5	9	6.7	9887	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	92.7	137461	PASS
175	174	5	9	8.0	10977	PASS
176	174	95	101	96.8	133011	PASS
177	176	5	9	6.5	8595	PASS