

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY081422\
 Data File : VY010023.D
 Acq On : 15 Aug 2022 01:18
 Operator : KP/MD
 Sample : N4046-15
 Misc : 6.48g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 BEACONPOINT-BACKFILL-08

Quant Time: Aug 15 06:24:18 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y081222S.M
 Quant Title : SW846 8260
 QLast Update : Sat Aug 13 02:54:57 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	7.783	168	71430	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.685	114	138908	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.490	117	138642	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.422	152	63737	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.136	65	39934	55.113	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	110.220%
35) Dibromofluoromethane	7.710	113	39878	46.906	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	93.820%
50) Toluene-d8	10.179	98	142731	43.815	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	=	87.640%
62) 4-Bromofluorobenzene	12.477	95	49092	41.132	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	=	82.260%
Target Compounds						
					Qvalue	
18) Methyl Acetate	4.472	43	23	Below Cal	#	52
20) Methylene Chloride	4.710	84	3282	Below Cal	#	82
36) 1,1-Dichloropropene	7.783	75	5265	4.159	ug/l #	48
38) Carbon Tetrachloride	7.783	117	7157	5.665	ug/l #	17
76) 1,2,3-Trichloropropane	12.477	75	22622	30.714	ug/l #	100
81) trans-1,4-Dichloro-2-b...	12.477	75	22622	66.766	ug/l #	13


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY081422\
Data File : VY010023.D
Acq On : 15 Aug 2022 01:18
Operator : KP/MD
Sample : N4046-15
Misc : 6.48g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BEACONPOINT-BACKFILL-08

Quant Time: Aug 15 06:24:18 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y081222S.M
Quant Title : SW846 8260
QLast Update : Sat Aug 13 02:54:57 2022
Response via : Initial Calibration




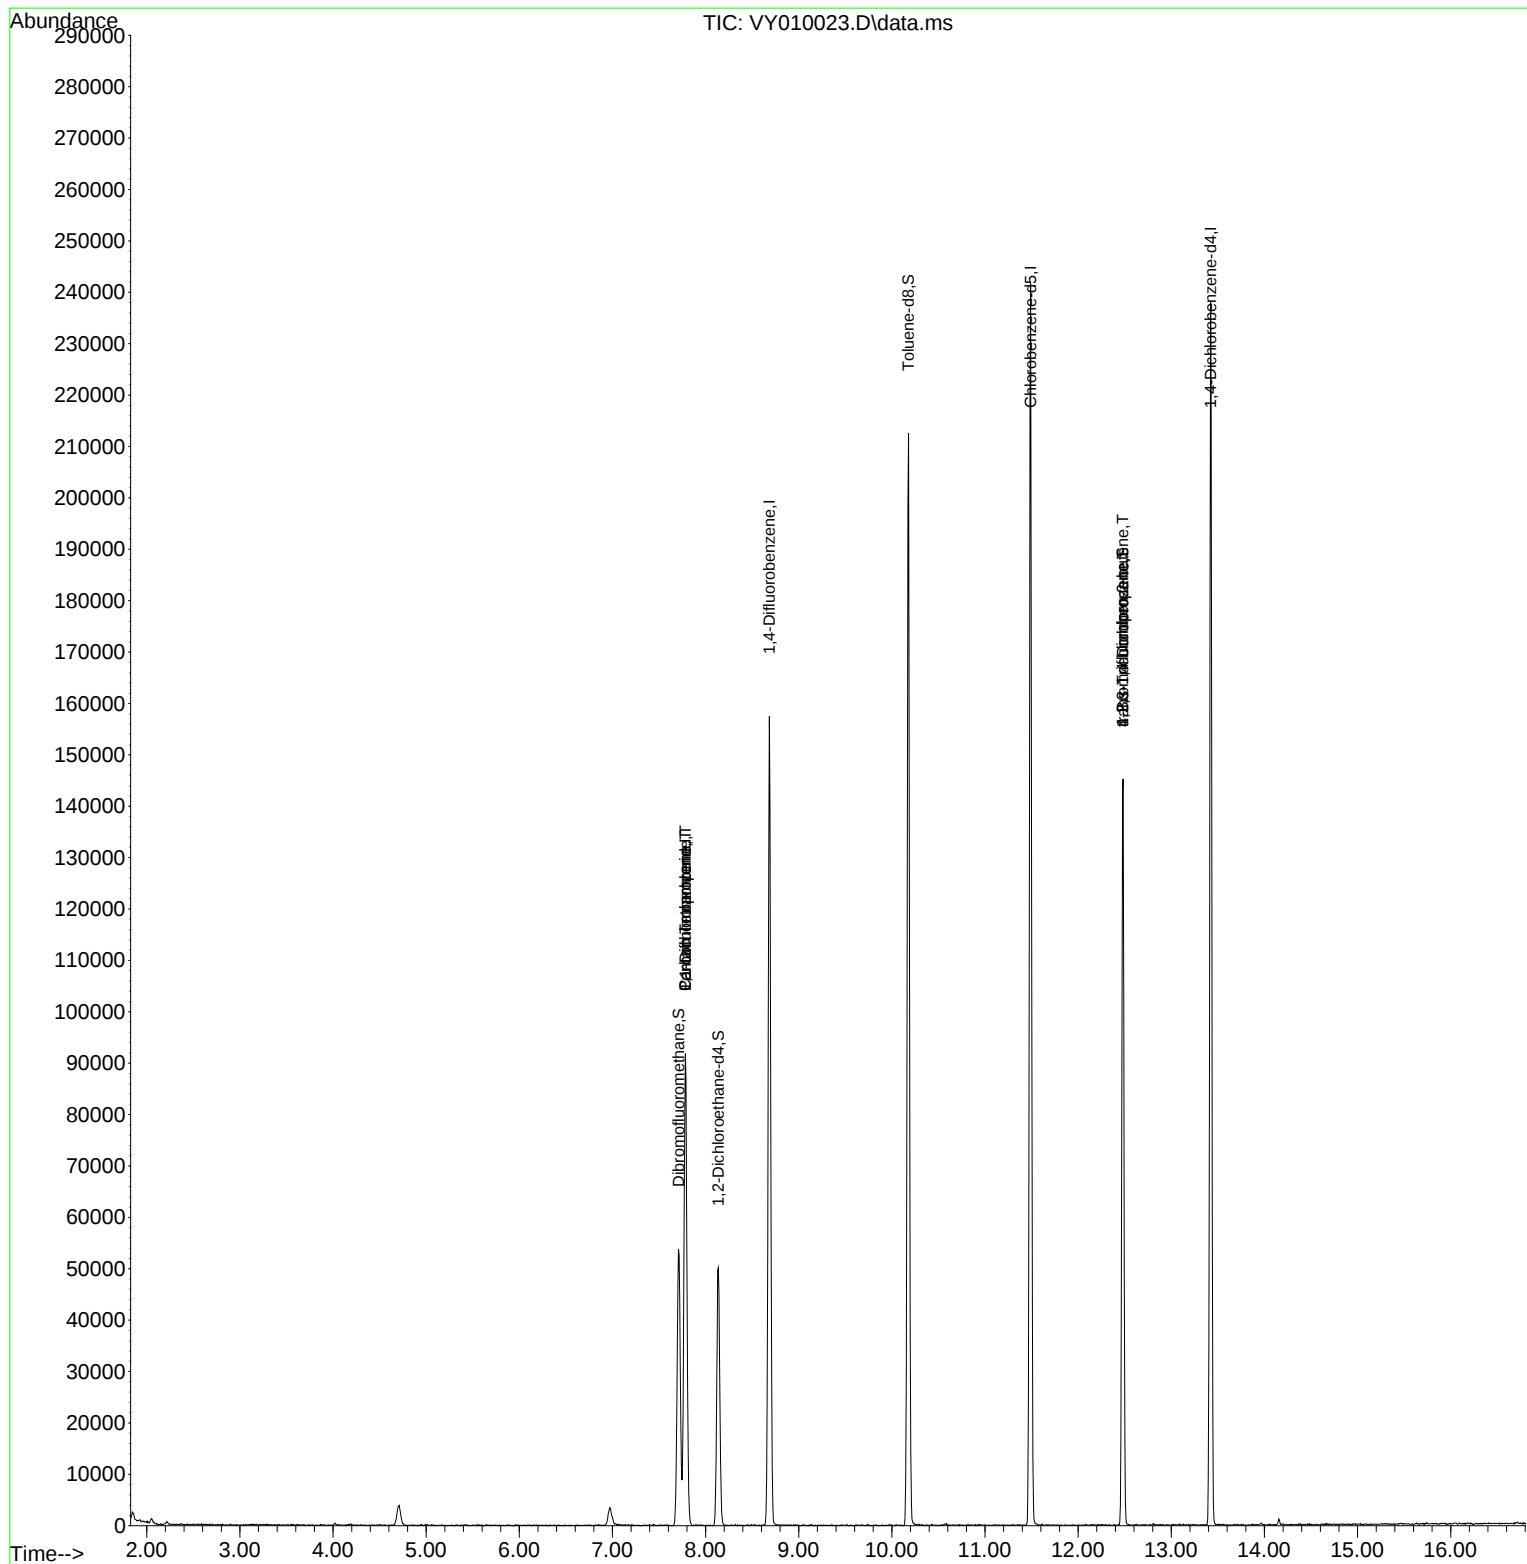


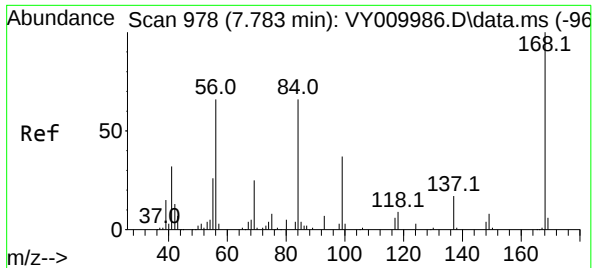

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.783 min Scan# 91
Delta R.T. -0.000 min
Lab File: VY010023.D
Acq: 15 Aug 2022 01:18




Instrument :
MSVOA_Y
ClientSampleId :
BEACONPOINT-BACKFILL-08


Tgt Ion:168 Resp: 71430
Ion Ratio Lower Upper
168 100
99 55.0 42.1 63.1

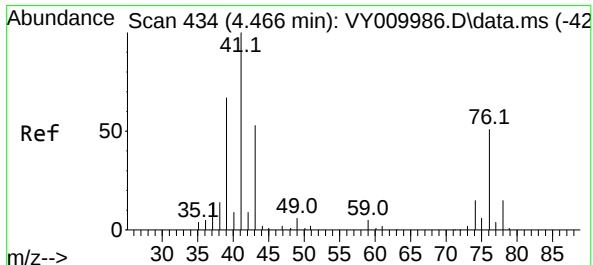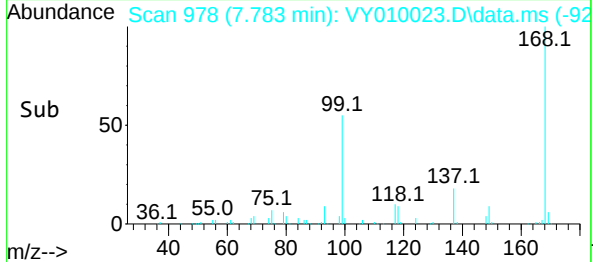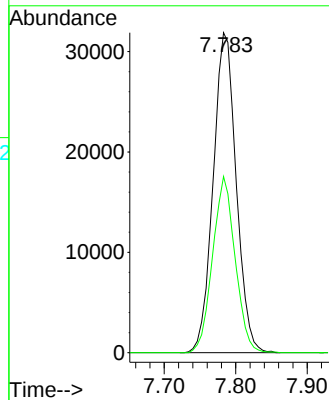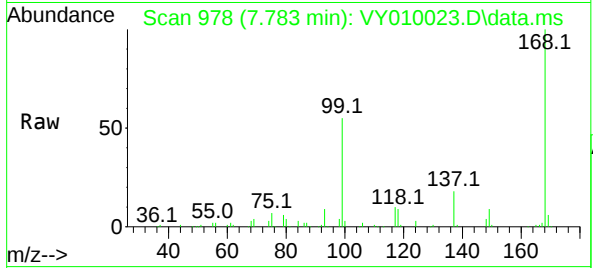

#18
Methyl Acetate
Concen: Below Cal
RT: 4.472 min Scan# 435
Delta R.T. 0.006 min
Lab File: VY010023.D
Acq: 15 Aug 2022 01:18

Tgt Ion: 43 Resp: 23
Ion Ratio Lower Upper
43 100
74 0.0 18.8 28.2#


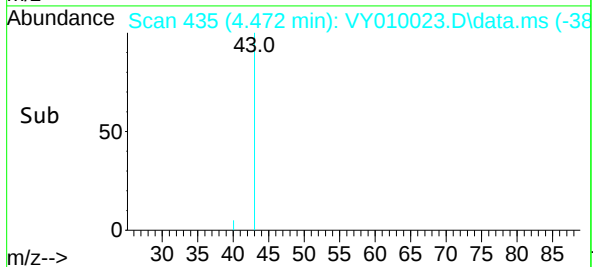
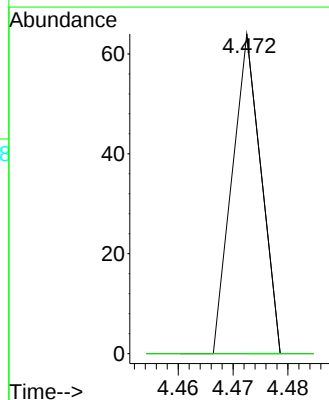
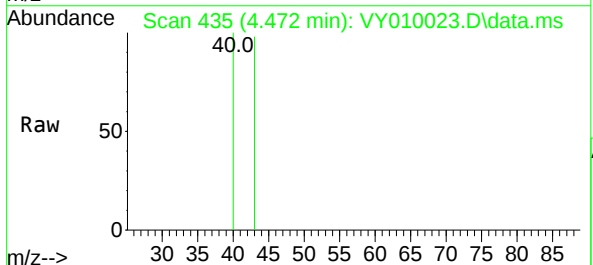


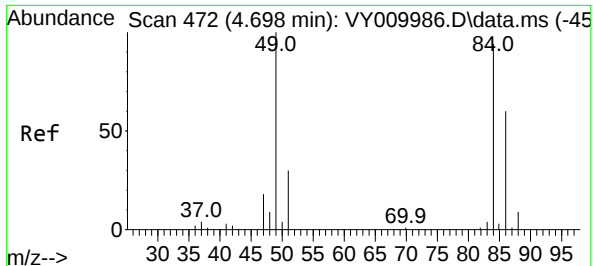

#20
Methylene Chloride
Concen: Below Cal
RT: 4.710 min Scan# 41
Delta R.T. 0.012 min
Lab File: VY010023.D
Acq: 15 Aug 2022 01:18




Instrument :
MSVOA_Y
ClientSampleId :
BEACONPOINT-BACKFILL-08


Tgt Ion: 84 Resp: 3282
Ion Ratio Lower Upper
84 100
49 92.8 98.2 147.4#
51 31.3 33.4 50.0#
86 64.1 52.3 78.5

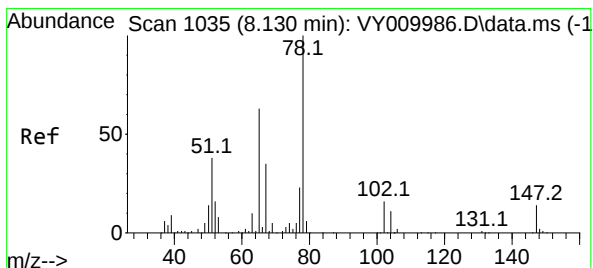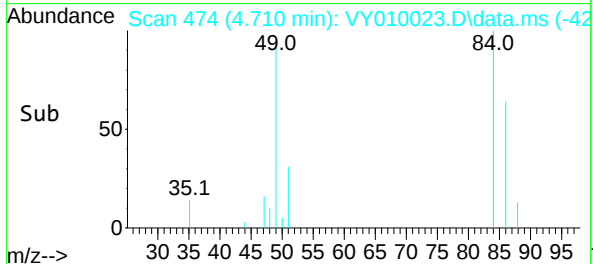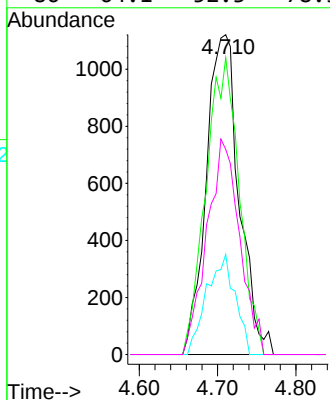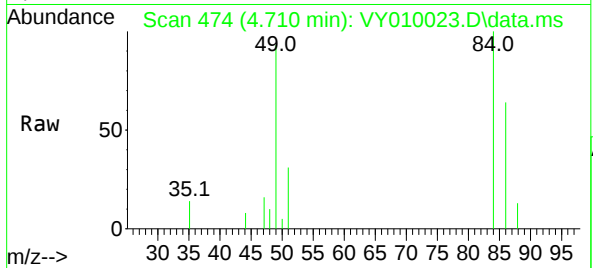

#33
1,2-Dichloroethane-d4
Concen: 55.113 ug/l
RT: 8.136 min Scan# 1036
Delta R.T. 0.006 min
Lab File: VY010023.D
Acq: 15 Aug 2022 01:18

Tgt Ion: 65 Resp: 39934
Ion Ratio Lower Upper
65 100
67 52.0 0.0 108.4


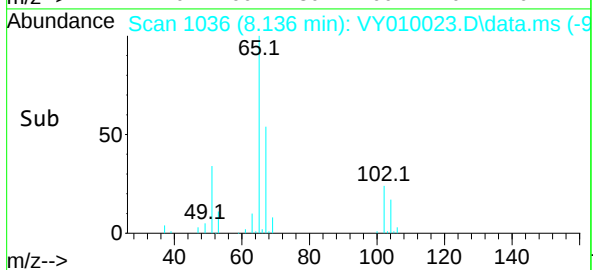
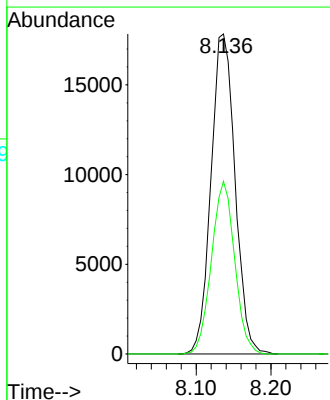
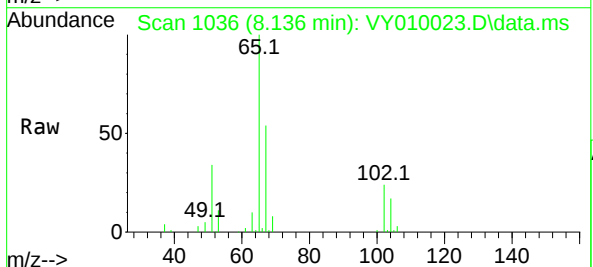


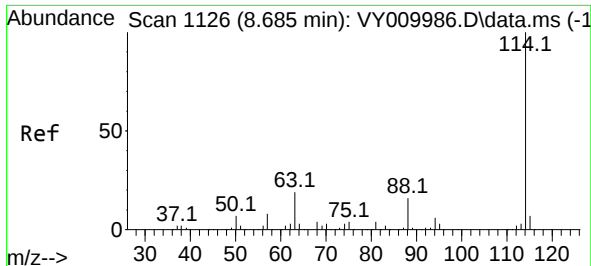

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.685 min Scan# 1126
Delta R.T. 0.000 min
Lab File: VY010023.D
Acq: 15 Aug 2022 01:18




Instrument :
MSVOA_Y
ClientSampleId :
BEACONPOINT-BACKFILL-08


Tgt Ion:114 Resp: 138908
Ion Ratio Lower Upper
114 100
63 17.8 0.0 38.0
88 14.4 0.0 30.0

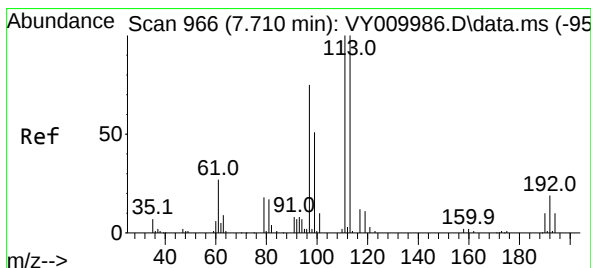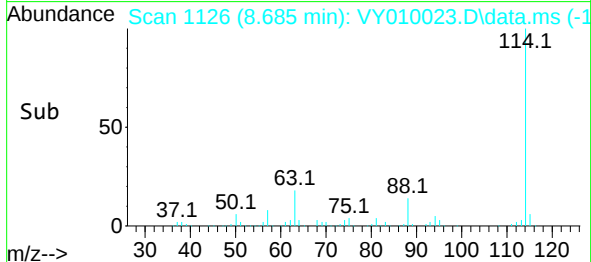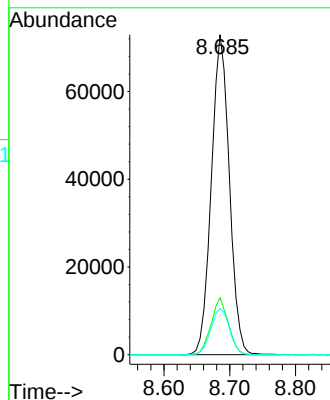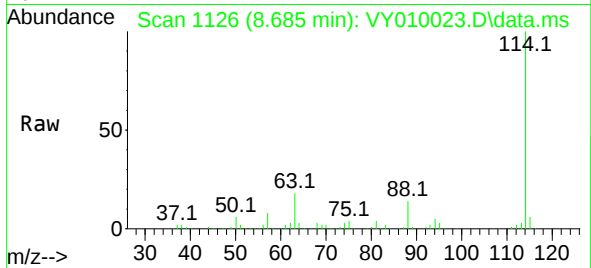

#35
Dibromofluoromethane
Concen: 46.906 ug/l
RT: 7.710 min Scan# 966
Delta R.T. 0.000 min
Lab File: VY010023.D
Acq: 15 Aug 2022 01:18

Tgt Ion:113 Resp: 39878
Ion Ratio Lower Upper
113 100
111 99.7 80.6 120.8
192 19.8 16.2 24.4


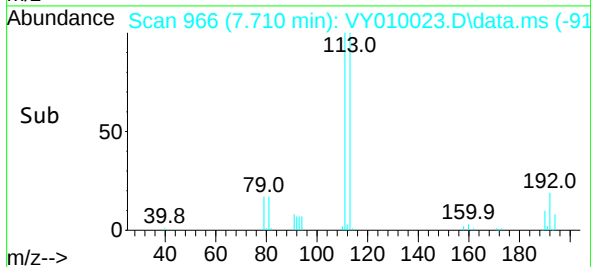
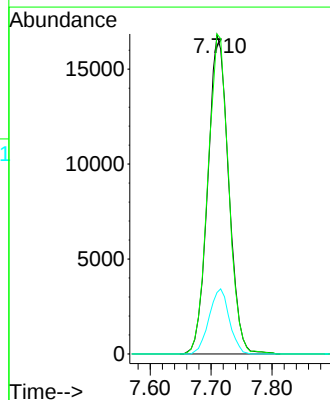
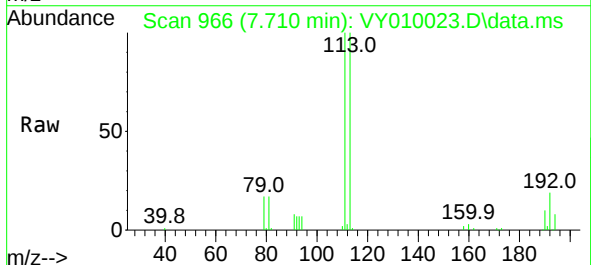


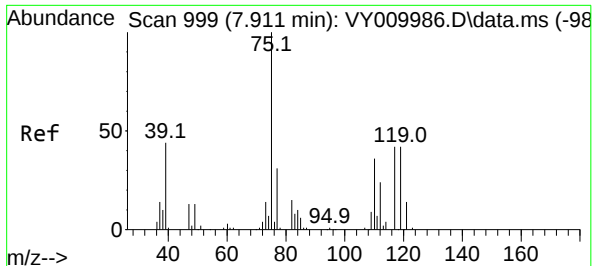

#36
1,1-Dichloropropene
Concen: 4.159 ug/l
RT: 7.783 min Scan# 91
Delta R.T. -0.128 min
Lab File: VY010023.D
Acq: 15 Aug 2022 01:18




Instrument :
MSVOA_Y
ClientSampleId :
BEACONPOINT-BACKFILL-08


Tgt Ion: 75 Resp: 5265
Ion Ratio Lower Upper
75 100
110 8.8 18.6 56.0#
77 0.0 25.0 37.4#

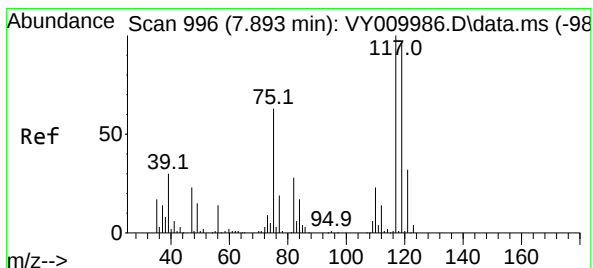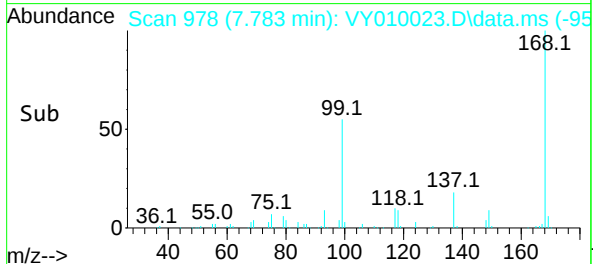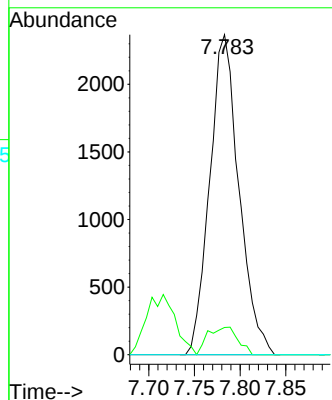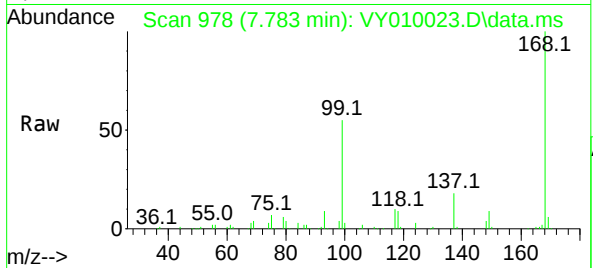

#38
Carbon Tetrachloride
Concen: 5.665 ug/l
RT: 7.783 min Scan# 978
Delta R.T. -0.110 min
Lab File: VY010023.D
Acq: 15 Aug 2022 01:18

Tgt Ion: 117 Resp: 7157
Ion Ratio Lower Upper
117 100
119 6.0 75.9 113.9#
121 0.0 24.9 37.3#


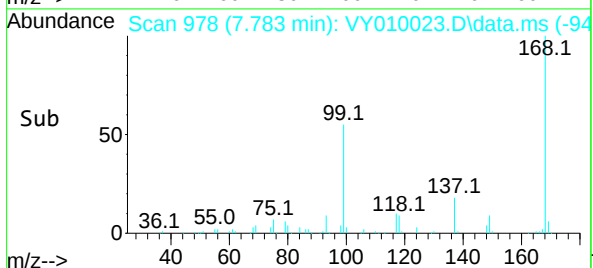
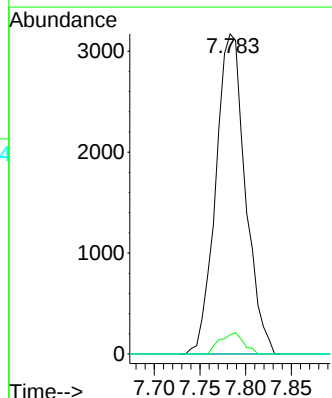
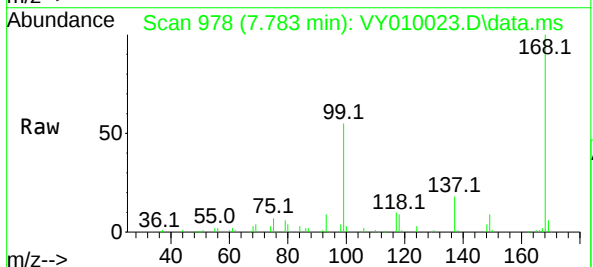


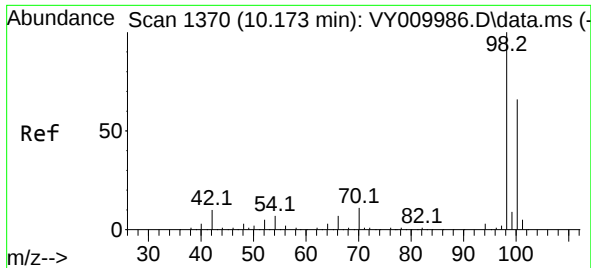

#50
Toluene-d8
Concen: 43.815 ug/l
RT: 10.179 min Scan# 11
Delta R.T. 0.006 min
Lab File: VY010023.D
Acq: 15 Aug 2022 01:18




Instrument :
MSVOA_Y
ClientSampleId :
BEACONPOINT-BACKFILL-08


Tgt Ion: 98 Resp: 142731
Ion Ratio Lower Upper
98 100
100 65.2 52.9 79.3

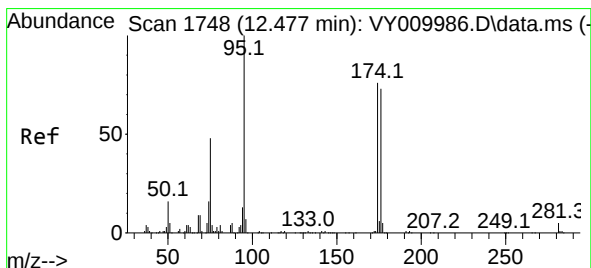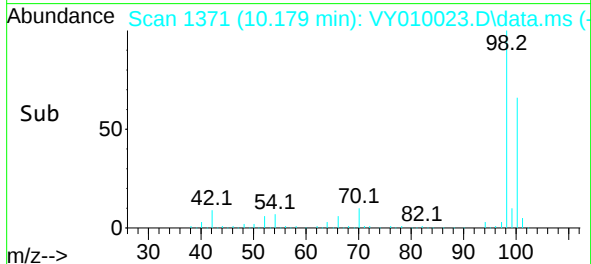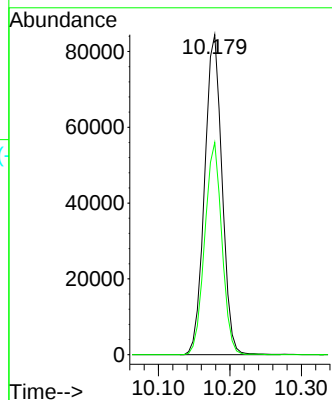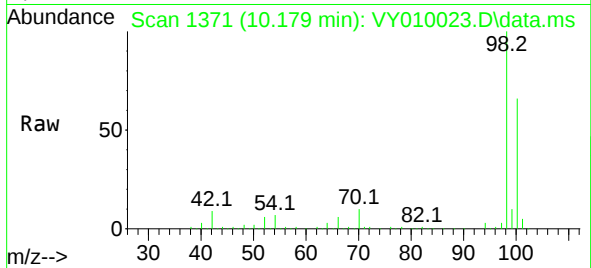

#62
4-Bromofluorobenzene
Concen: 41.132 ug/l
RT: 12.477 min Scan# 1748
Delta R.T. 0.000 min
Lab File: VY010023.D
Acq: 15 Aug 2022 01:18

Tgt Ion: 95 Resp: 49092
Ion Ratio Lower Upper
95 100
174 81.8 0.0 173.8
176 79.7 0.0 167.0


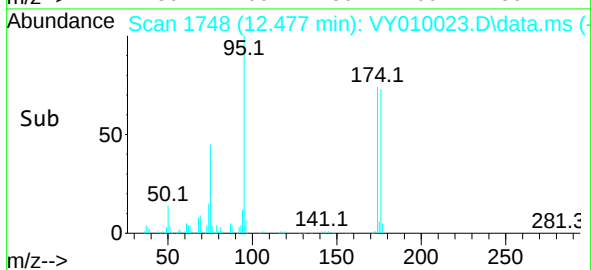
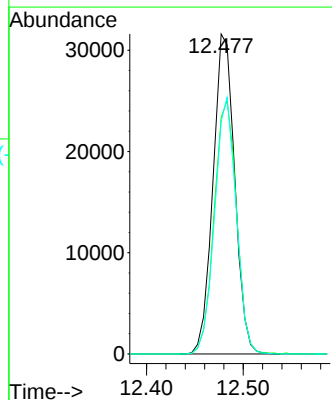
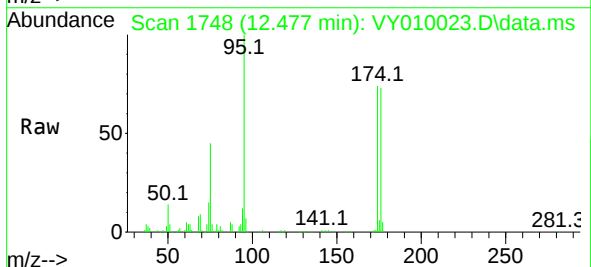


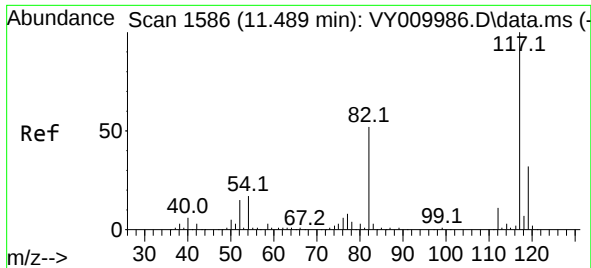

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.490 min Scan# 11
Delta R.T. 0.000 min
Lab File: VY010023.D
Acq: 15 Aug 2022 01:18




Instrument :
MSVOA_Y
ClientSampleId :
BEACONPOINT-BACKFILL-08


Tgt Ion:117 Resp: 138642
Ion Ratio Lower Upper
117 100
82 51.1 41.8 62.6
119 32.1 25.6 38.4

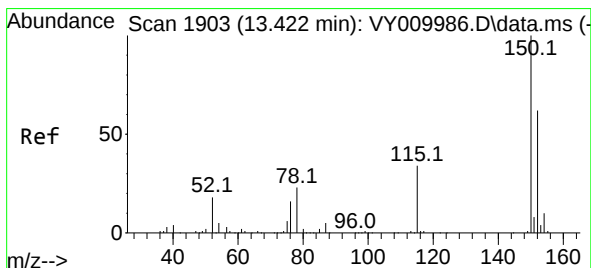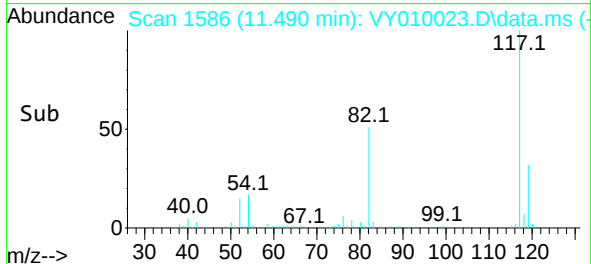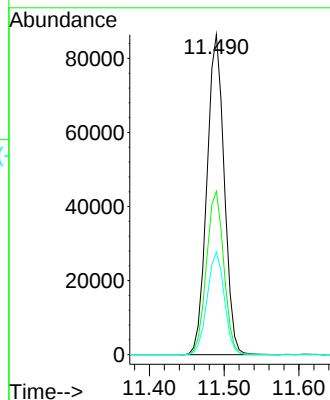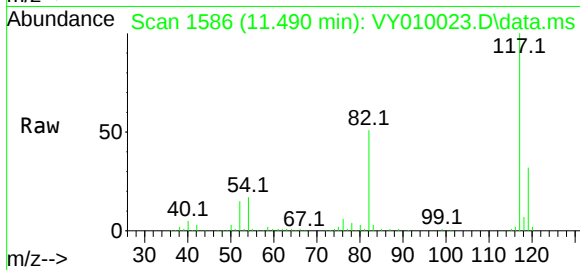

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.422 min Scan# 1903
Delta R.T. 0.000 min
Lab File: VY010023.D
Acq: 15 Aug 2022 01:18

Tgt Ion:152 Resp: 63737
Ion Ratio Lower Upper
152 100
115 58.5 28.6 85.9
150 158.3 0.0 349.8


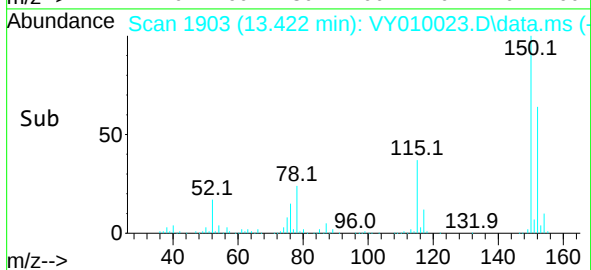
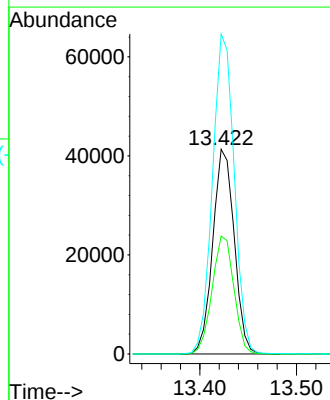
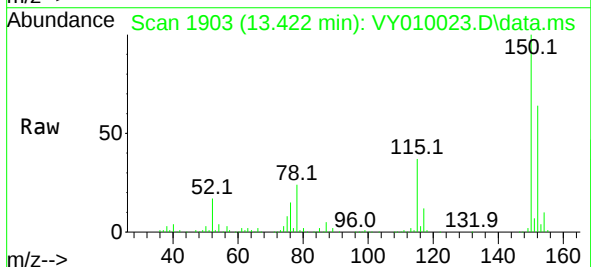


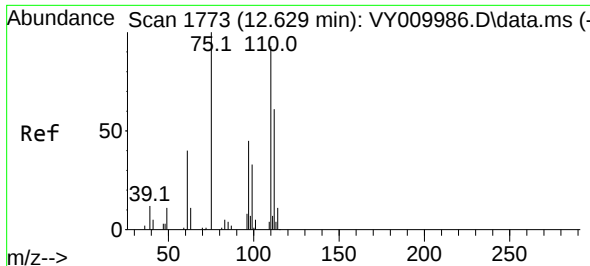

#76
1,2,3-Trichloropropane
Concen: 30.714 ug/l
RT: 12.477 min Scan# 1748
Delta R.T. -0.152 min
Lab File: VY010023.D
Acq: 15 Aug 2022 01:18

Instrument :
MSVOA_Y
ClientSampleId :
BEACONPOINT-BACKFILL-08

Tgt Ion: 75 Resp: 22622
Ion Ratio Lower Upper
75 100
77 1.3 0.0 0.0#

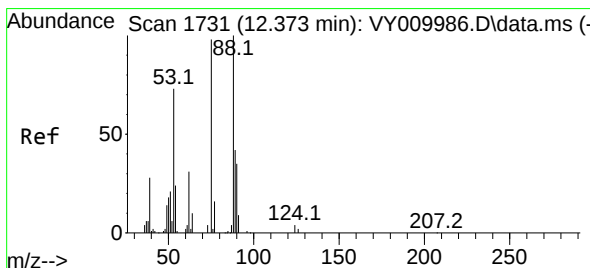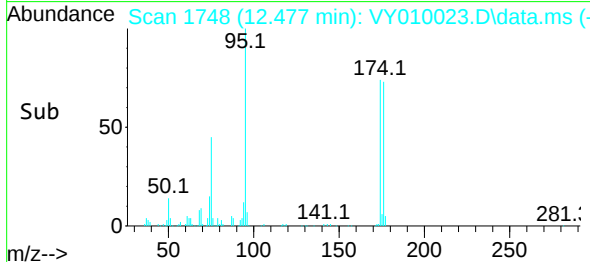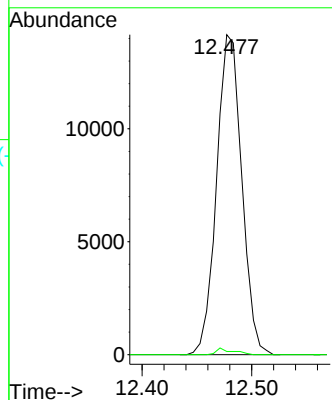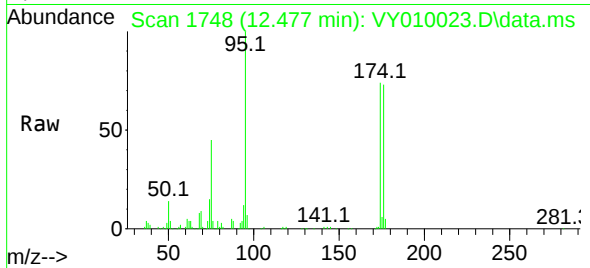

#81
trans-1,4-Dichloro-2-butene
Concen: 66.766 ug/l
RT: 12.477 min Scan# 1748
Delta R.T. 0.104 min
Lab File: VY010023.D
Acq: 15 Aug 2022 01:18

Tgt Ion: 75 Resp: 22622
Ion Ratio Lower Upper
75 100
53 0.0 71.4 107.2#
89 0.0 38.1 57.1#

