

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY081422\
 Data File : VY010003.D
 Acq On : 14 Aug 2022 17:24
 Operator : KP/MD
 Sample : VY0814SBL01
 Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 VY0814SBL01

Quant Time: Aug 15 00:39:46 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y081222S.M
 Quant Title : SW846 8260
 QLast Update : Sat Aug 13 02:54:57 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.783	168	87933	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.685	114	159417	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.489	117	143173	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.422	152	64130	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.136	65	51041	57.221	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	114.440%
35) Dibromofluoromethane	7.710	113	53859	55.200	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	110.400%
50) Toluene-d8	10.179	98	194470	52.018	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	=	104.040%
62) 4-Bromofluorobenzene	12.483	95	64360	46.987	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	=	93.980%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY081422\
Data File : VY010003.D
Acq On : 14 Aug 2022 17:24
Operator : KP/MD
Sample : VY0814SBL01
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
VY0814SBL01

Quant Time: Aug 15 00:39:46 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y081222S.M
Quant Title : SW846 8260
QLast Update : Sat Aug 13 02:54:57 2022
Response via : Initial Calibration




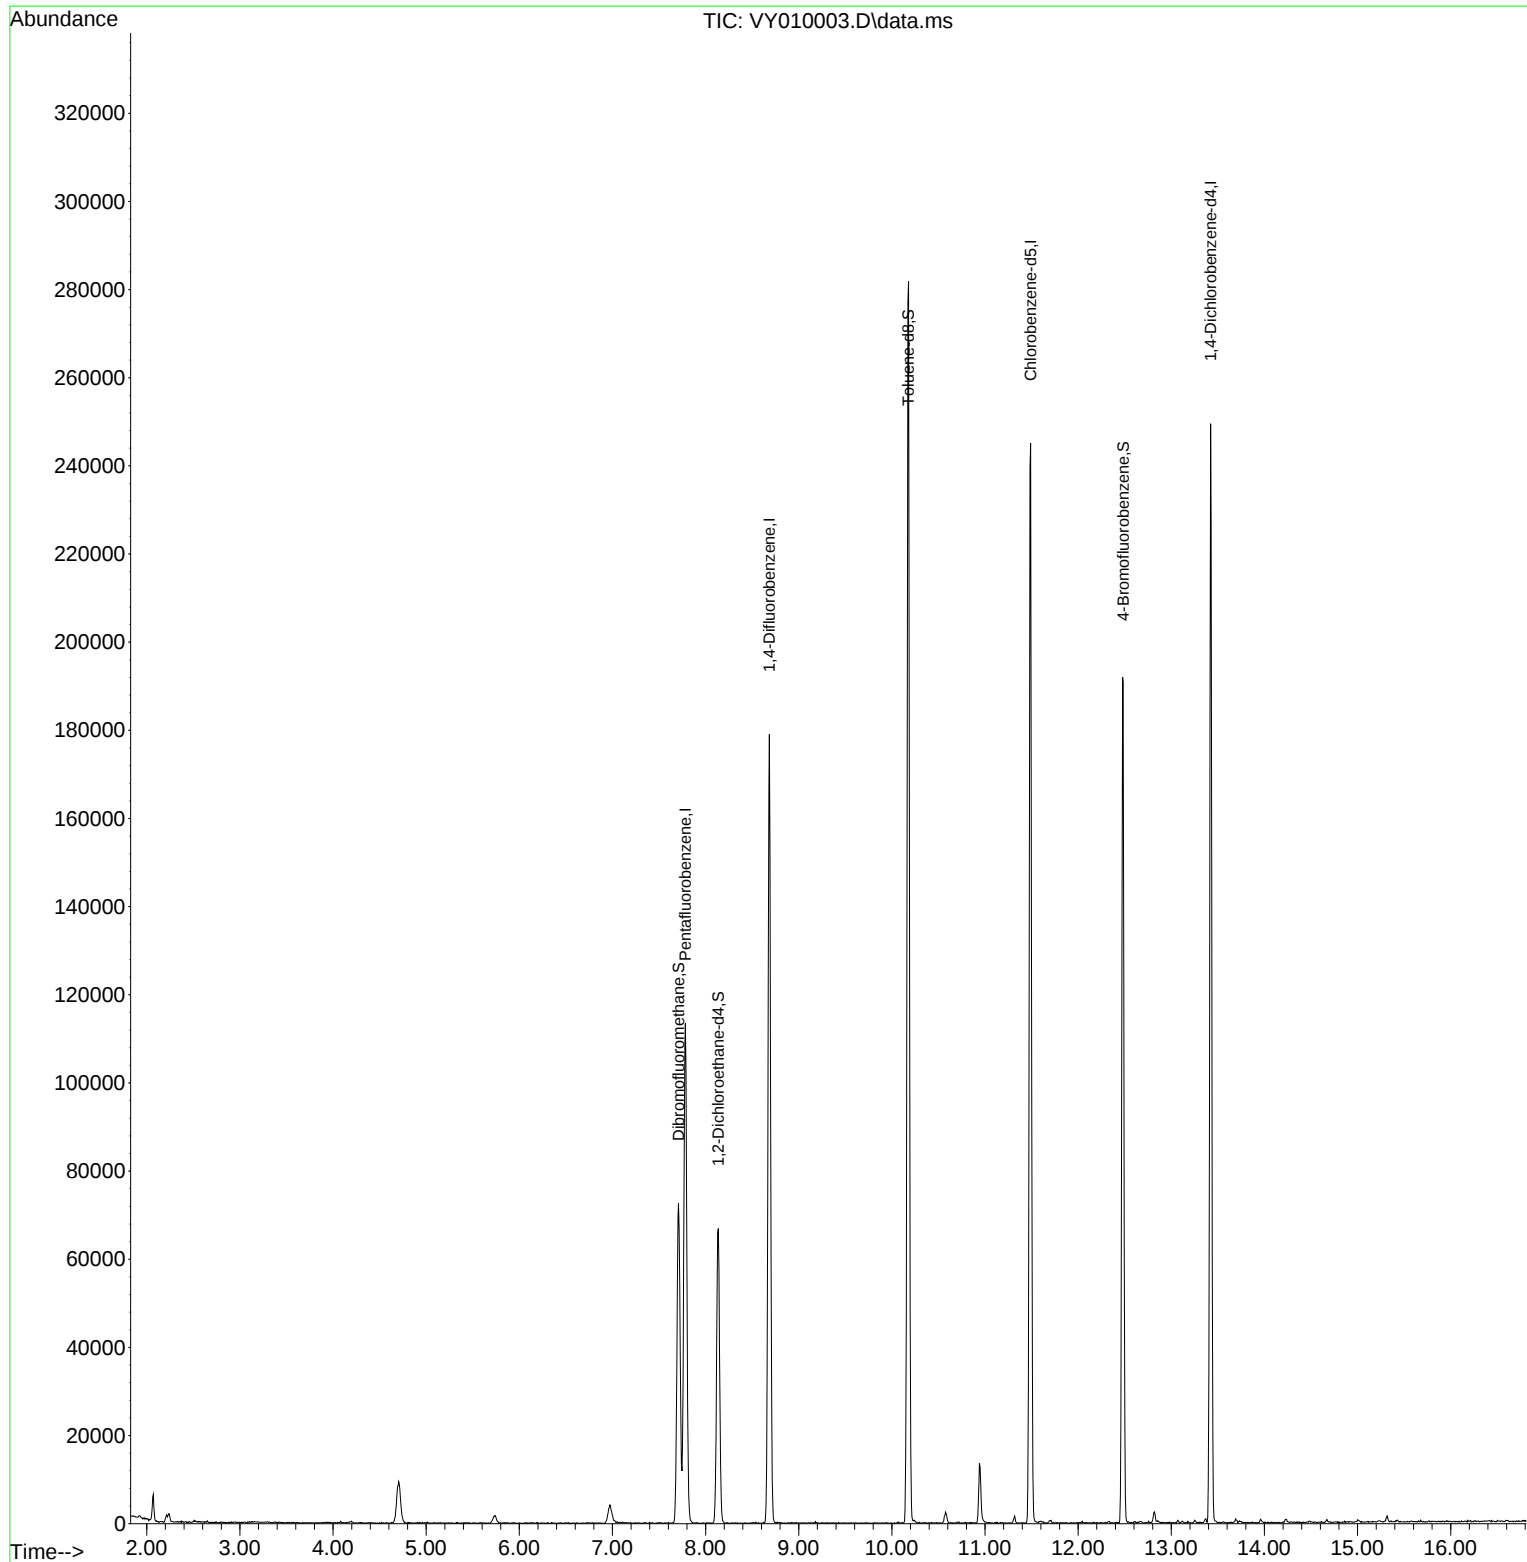


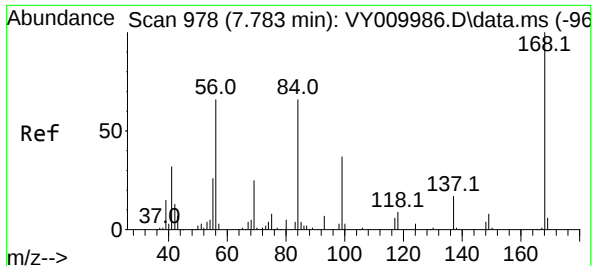

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.783 min Scan# 91
Delta R.T. -0.000 min
Lab File: VY010003.D
Acq: 14 Aug 2022 17:24




Instrument :
MSVOA_Y
ClientSampleId :
VY0814SBL01


Tgt Ion:168 Resp: 87933
Ion Ratio Lower Upper
168 100
99 55.6 42.1 63.1

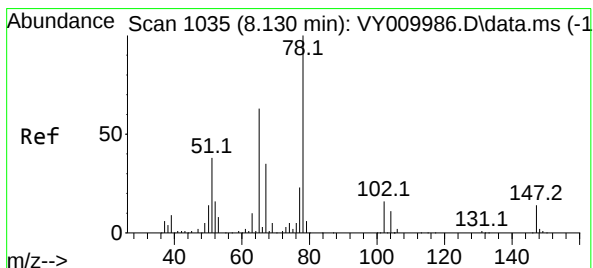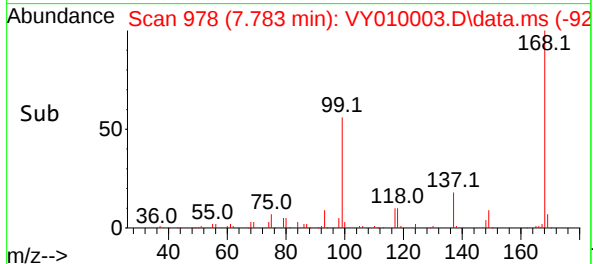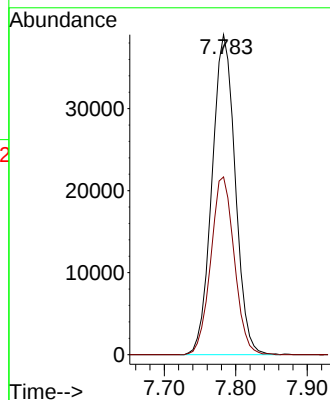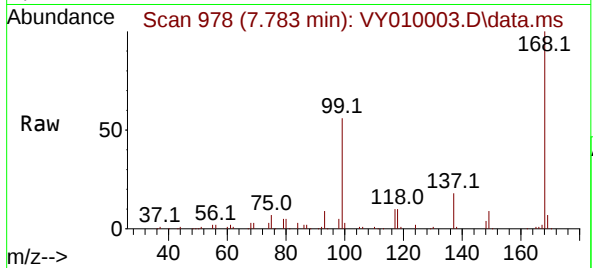

#33
1,2-Dichloroethane-d4
Concen: 57.221 ug/l
RT: 8.136 min Scan# 1036
Delta R.T. 0.006 min
Lab File: VY010003.D
Acq: 14 Aug 2022 17:24

Tgt Ion: 65 Resp: 51041
Ion Ratio Lower Upper
65 100
67 54.1 0.0 108.4


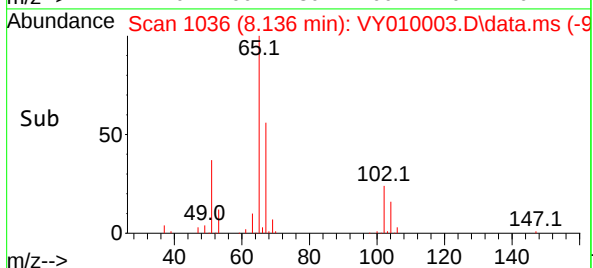
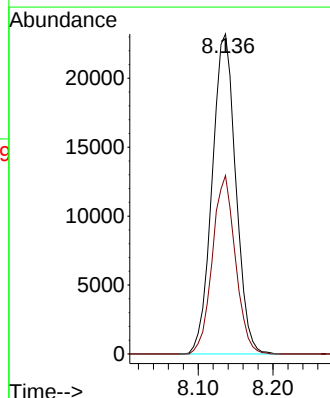
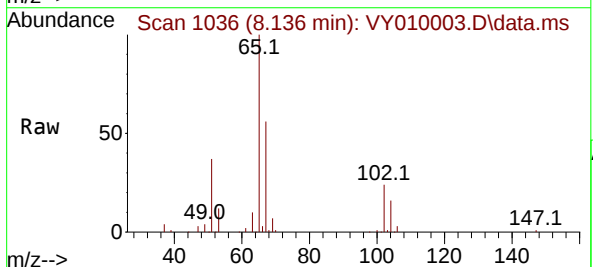


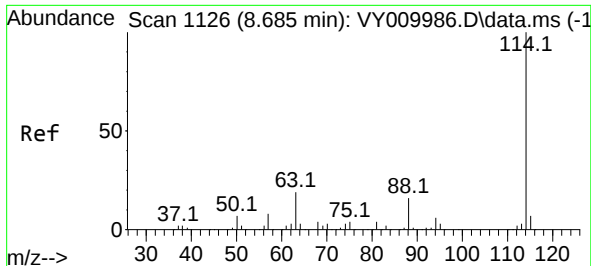

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.685 min Scan# 1126
Delta R.T. 0.000 min
Lab File: VY010003.D
Acq: 14 Aug 2022 17:24




Instrument :
MSVOA_Y
ClientSampleId :
VY0814SBL01


Tgt Ion:114 Resp: 159417
Ion Ratio Lower Upper
114 100
63 17.4 0.0 38.0
88 14.8 0.0 30.0

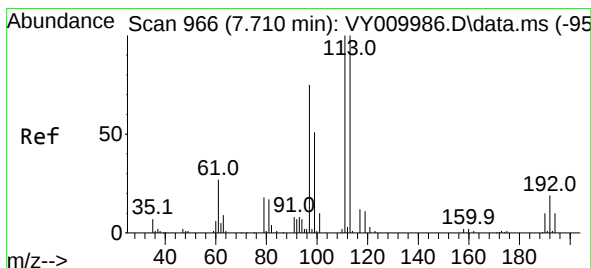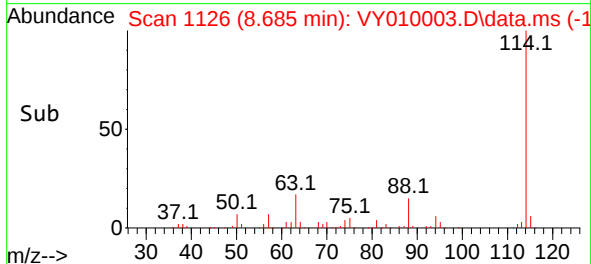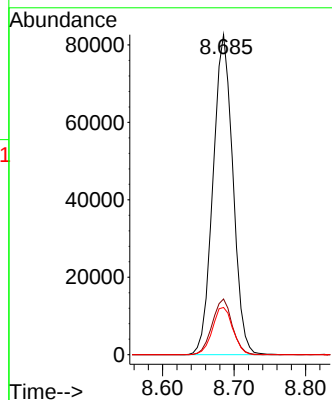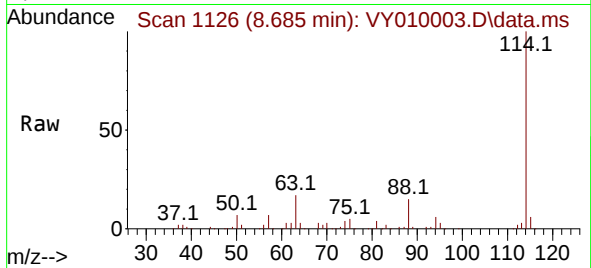

#35
Dibromofluoromethane
Concen: 55.200 ug/l
RT: 7.710 min Scan# 966
Delta R.T. 0.000 min
Lab File: VY010003.D
Acq: 14 Aug 2022 17:24

Tgt Ion:113 Resp: 53859
Ion Ratio Lower Upper
113 100
111 101.6 80.6 120.8
192 19.2 16.2 24.4


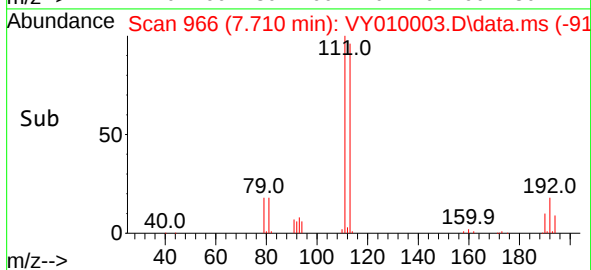
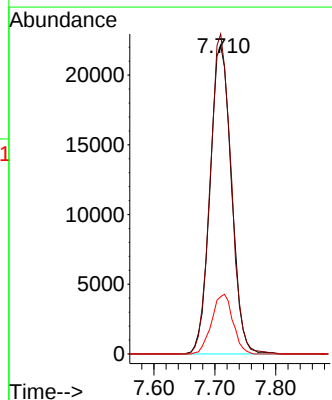
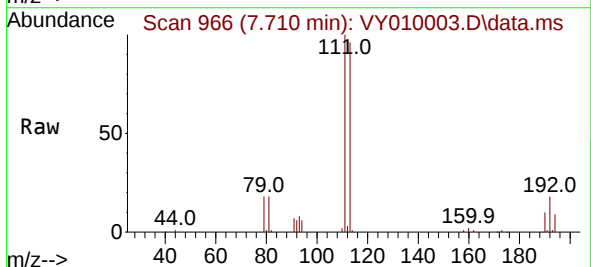


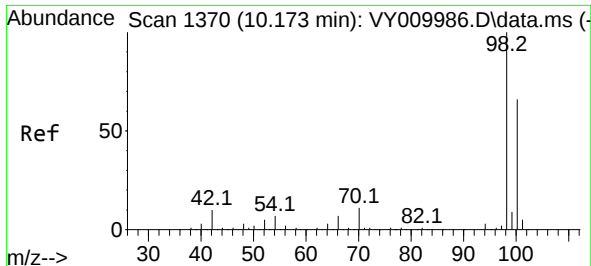

#50
Toluene-d8
Concen: 52.018 ug/l
RT: 10.179 min Scan# 11
Delta R.T. 0.006 min
Lab File: VY010003.D
Acq: 14 Aug 2022 17:24




Instrument :
MSVOA_Y
ClientSampleId :
VY0814SBL01


Tgt Ion: 98 Resp: 194470
Ion Ratio Lower Upper
98 100
100 65.0 52.9 79.3

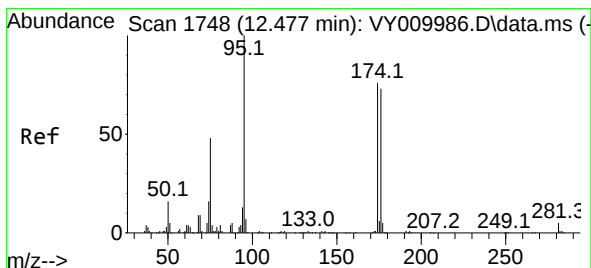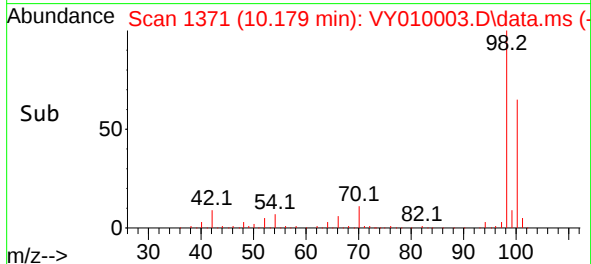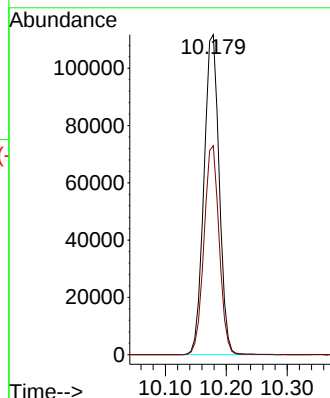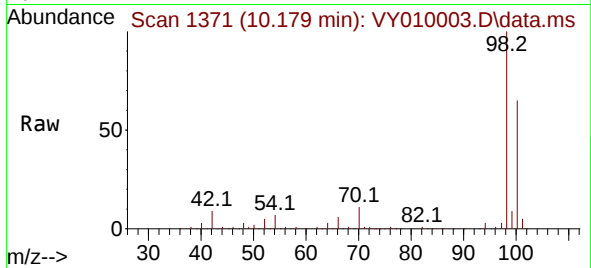

#62
4-Bromofluorobenzene
Concen: 46.987 ug/l
RT: 12.483 min Scan# 1749
Delta R.T. 0.006 min
Lab File: VY010003.D
Acq: 14 Aug 2022 17:24

Tgt Ion: 95 Resp: 64360
Ion Ratio Lower Upper
95 100
174 80.0 0.0 173.8
176 75.9 0.0 167.0


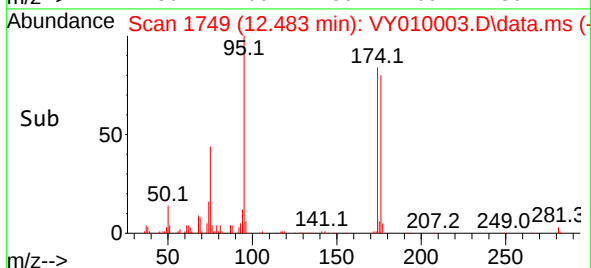
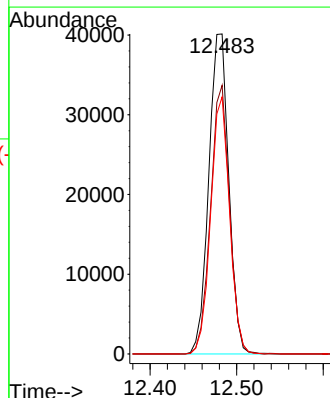
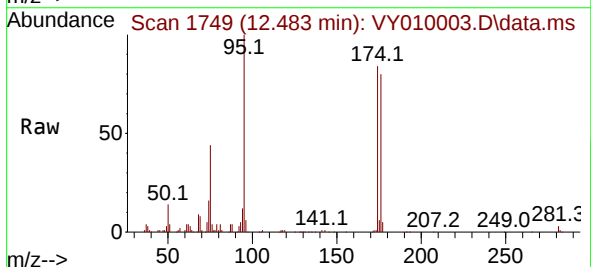


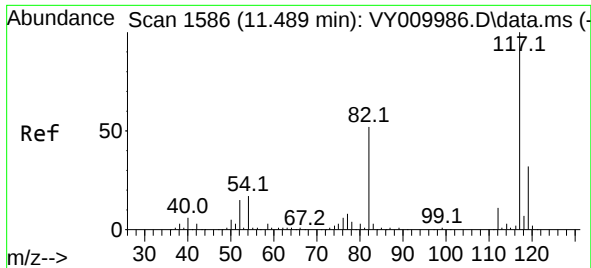

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.489 min Scan# 117
Delta R.T. 0.000 min
Lab File: VY010003.D
Acq: 14 Aug 2022 17:24

Instrument :
MSVOA_Y
ClientSampleId :
VY0814SBL01

Tgt Ion:117 Resp: 143173
Ion Ratio Lower Upper
117 100
82 51.7 41.8 62.6
119 33.1 25.6 38.4

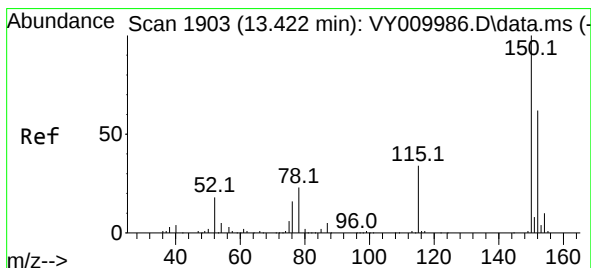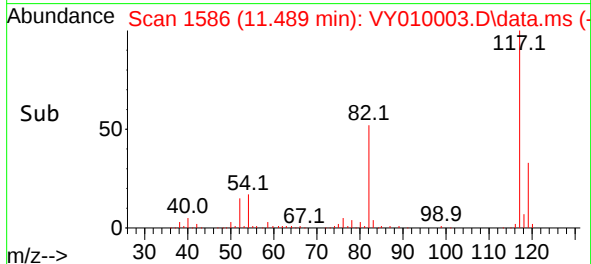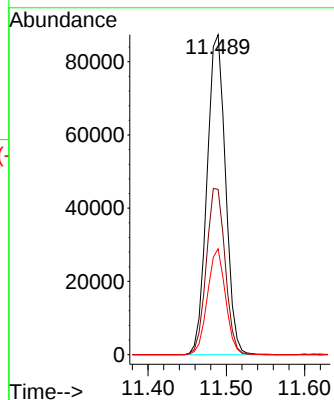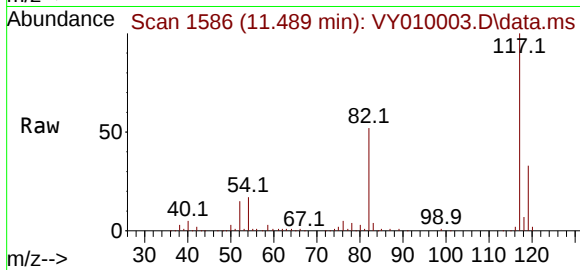

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.422 min Scan# 1903
Delta R.T. 0.000 min
Lab File: VY010003.D
Acq: 14 Aug 2022 17:24

Tgt Ion:152 Resp: 64130
Ion Ratio Lower Upper
152 100
115 59.7 28.6 85.9
150 160.3 0.0 349.8

