


Methylene Chloride

Response Ratio

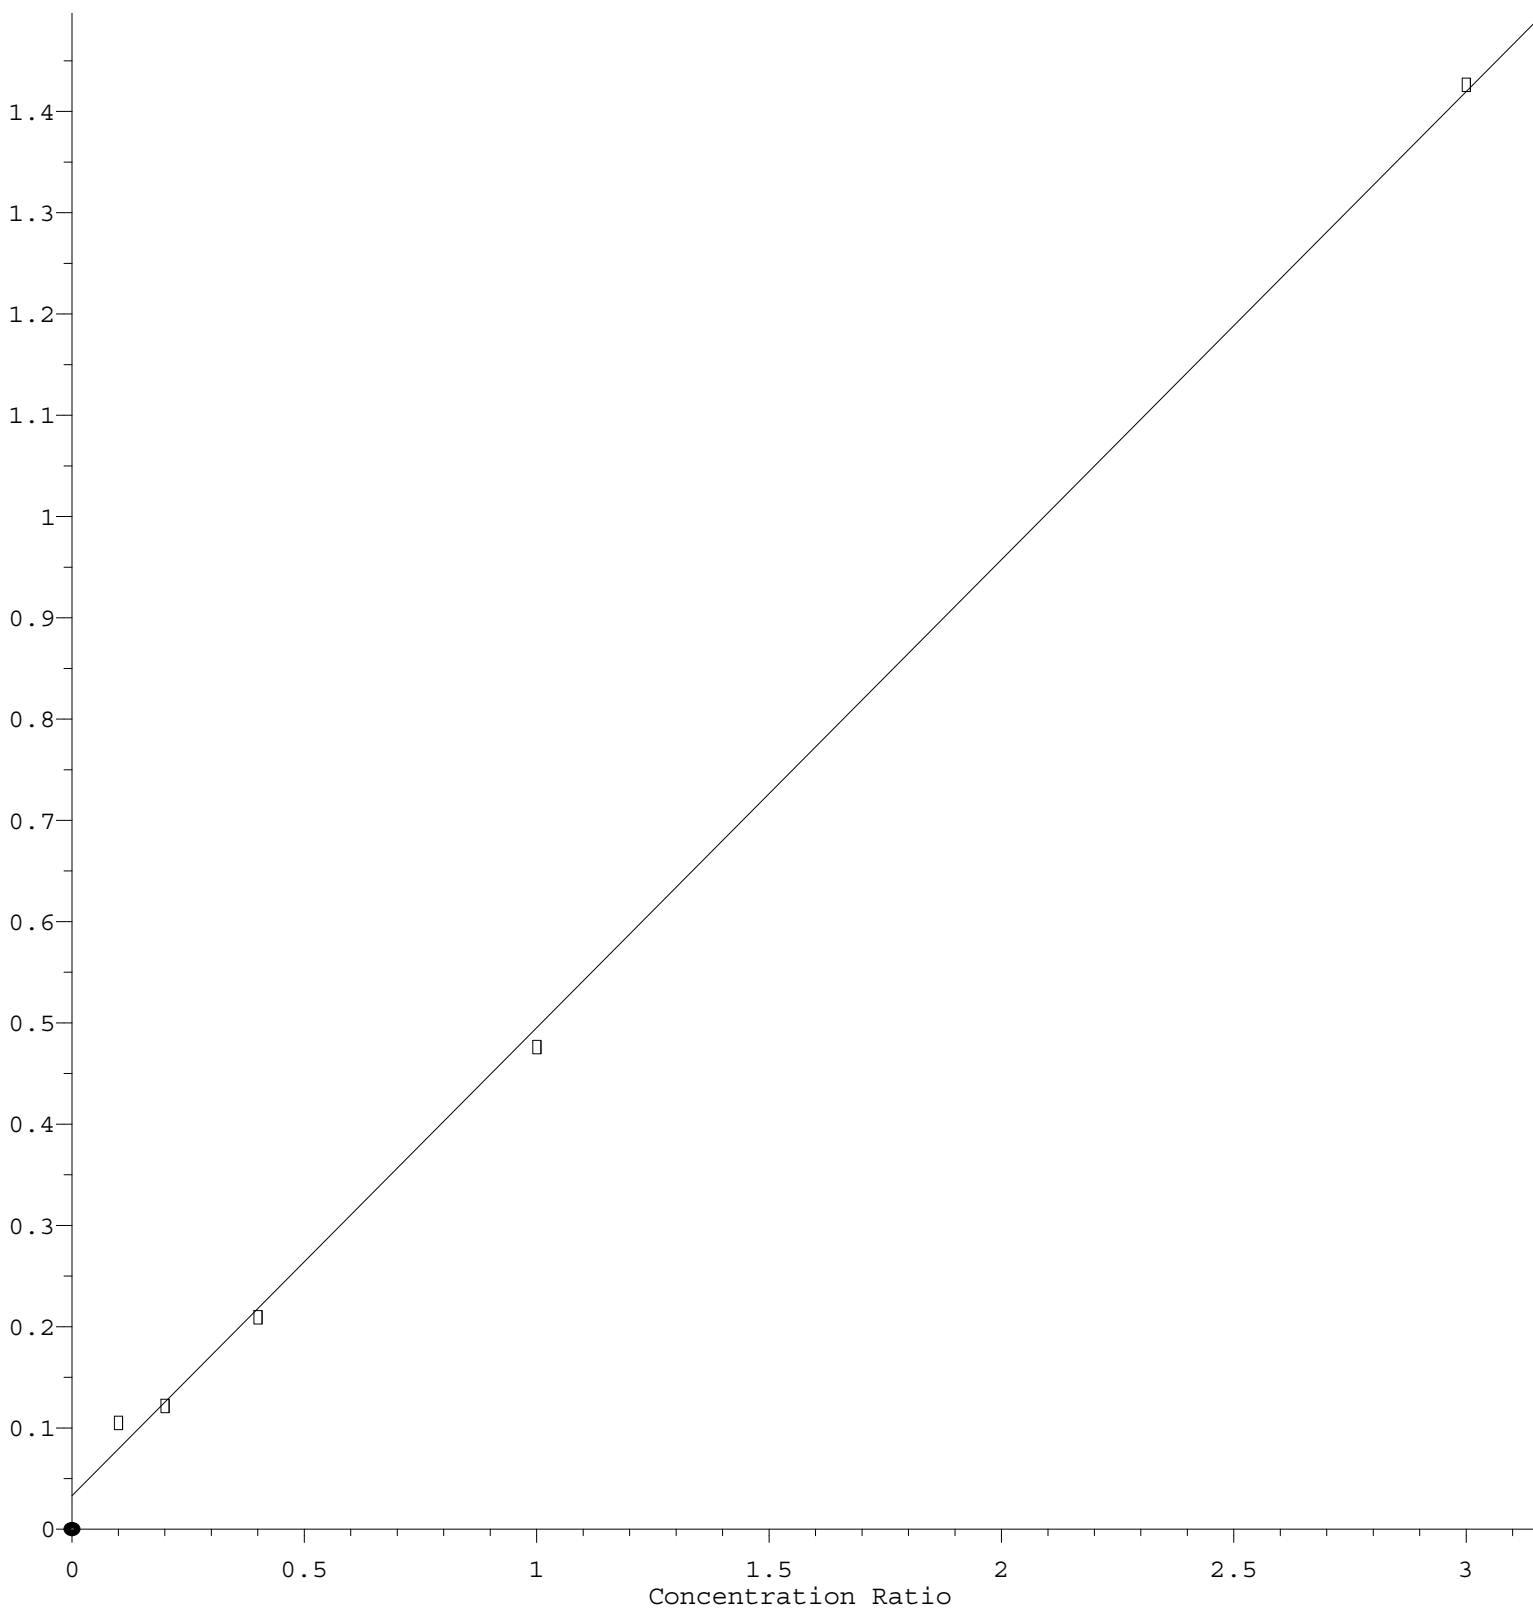

$$\text{Response} = 4.619\text{e-}001 * \text{Amt} + 3.340\text{e-}002$$


Coef of Det (r^2) = 0.999060 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA Y\methods\82Y081522S.M

Calibration Table Last Updated: Tue Aug 16 07:01:08 2022

N-amyl acetate

Response Ratio

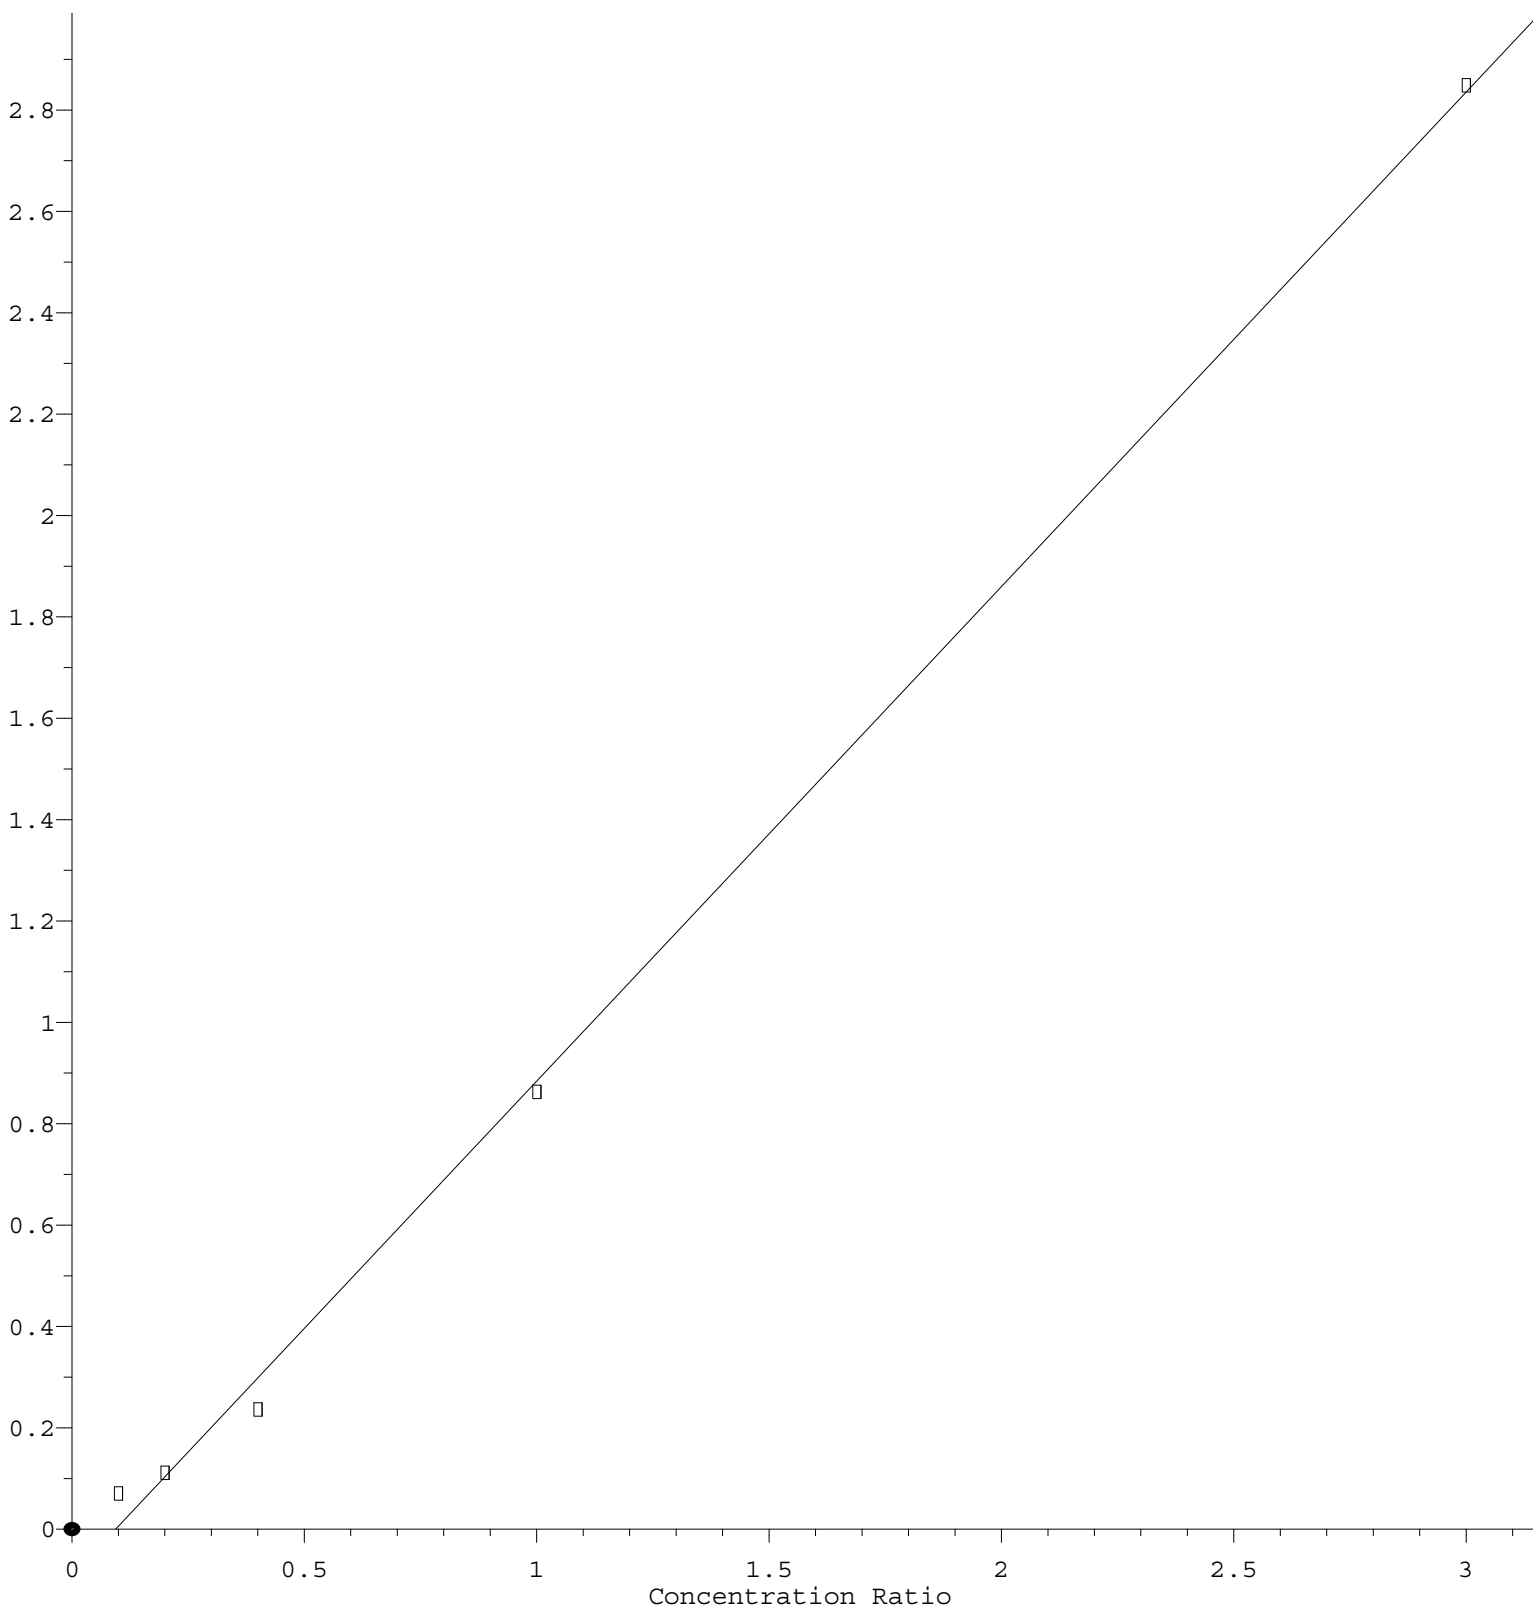

$$\text{Response} = 9.757\text{e-}001 * \text{Amt} - 9.138\text{e-}002$$


Coef of Det (r^2) = 0.998417 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA Y\methods\82Y081522S.M

Calibration Table Last Updated: Tue Aug 16 07:01:08 2022

Acetone

Response Ratio

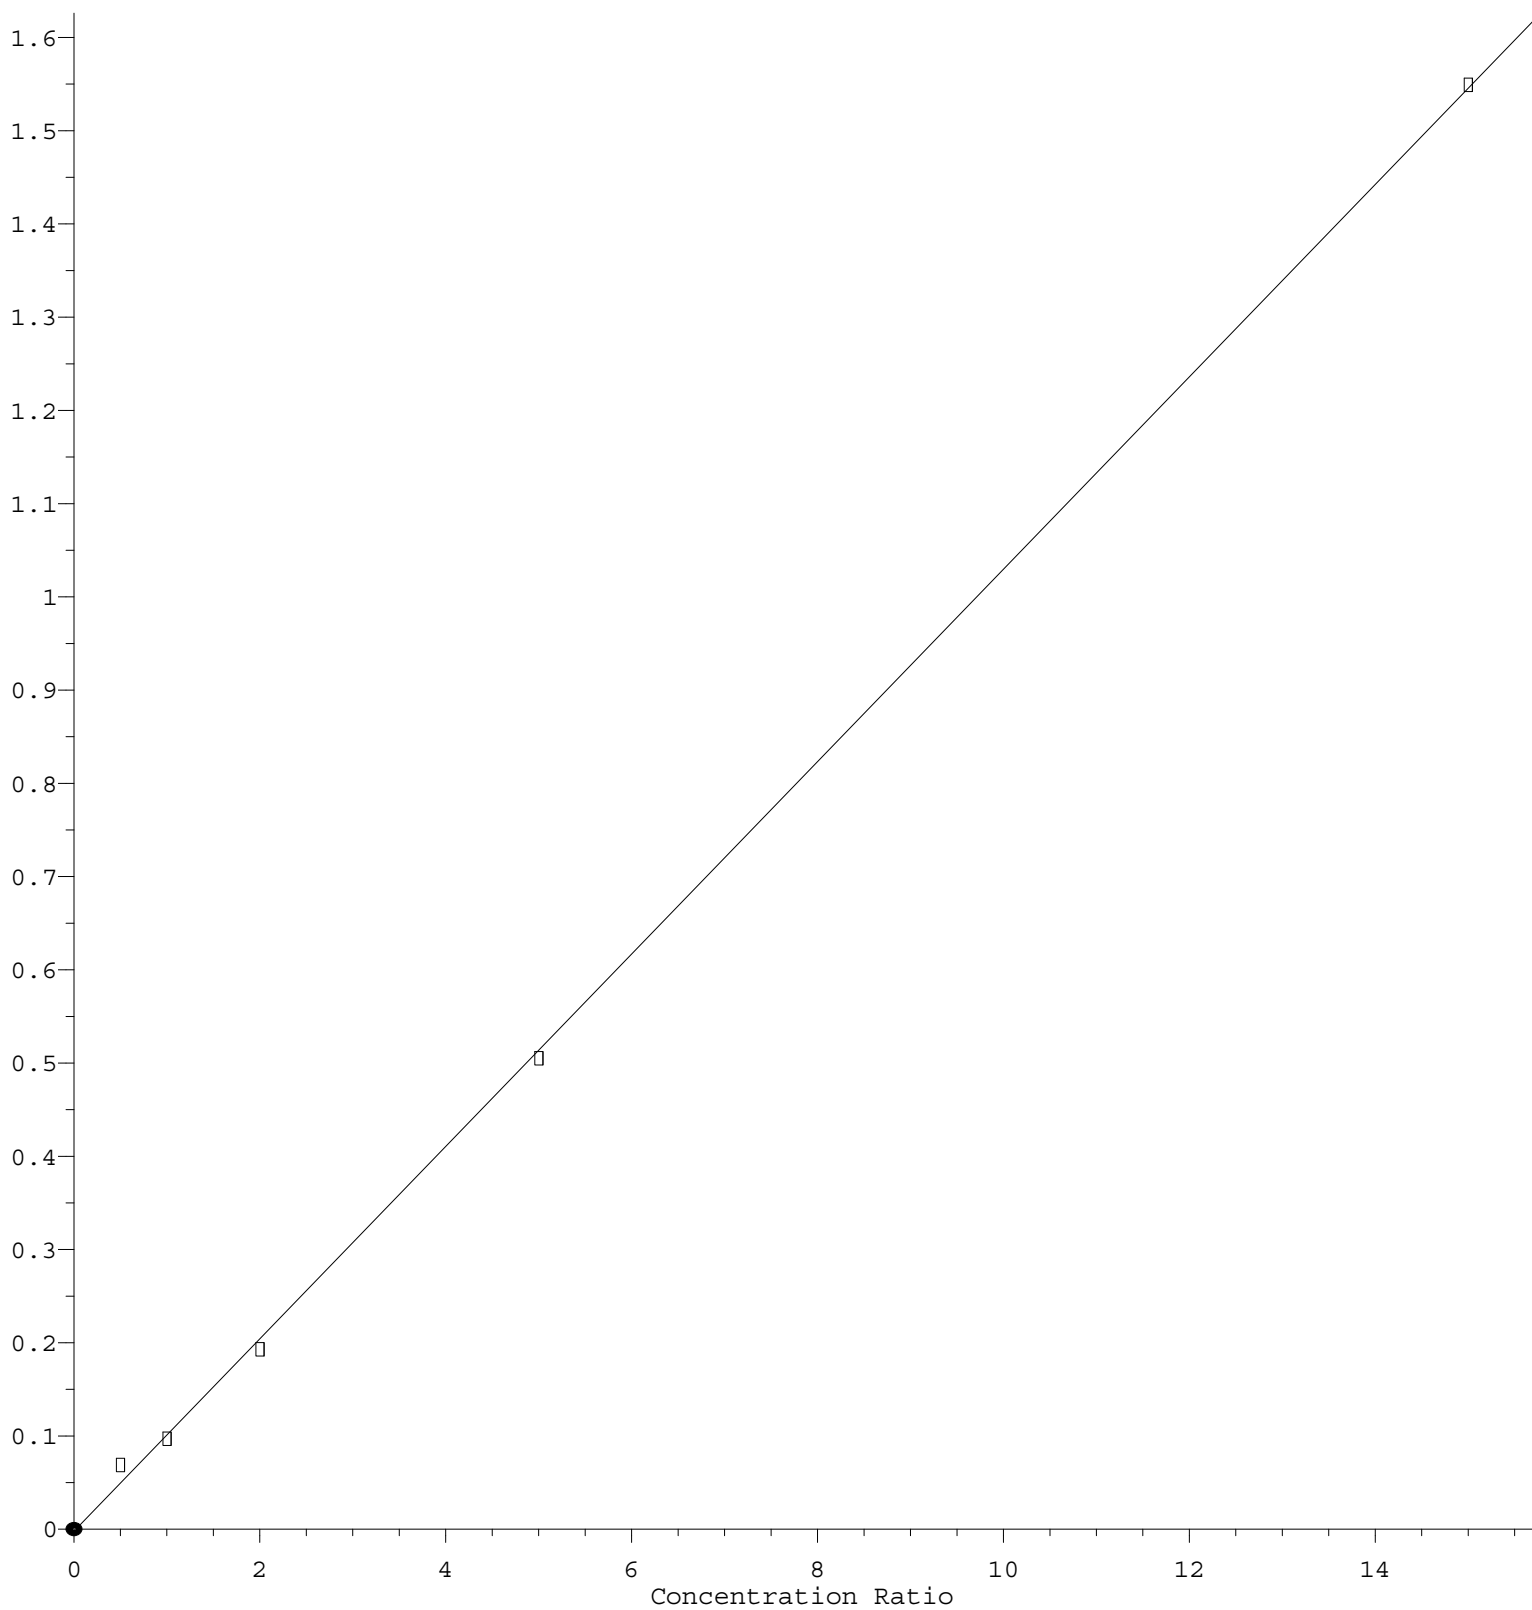

$$\text{Response} = 1.032\text{e-}001 * \text{Amt} - 2.299\text{e-}003$$


Coef of Det (r^2) = 0.999605 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA Y\methods\82Y081522S.M

Calibration Table Last Updated: Tue Aug 30 15:49:11 2022

2-Hexanone

Response Ratio

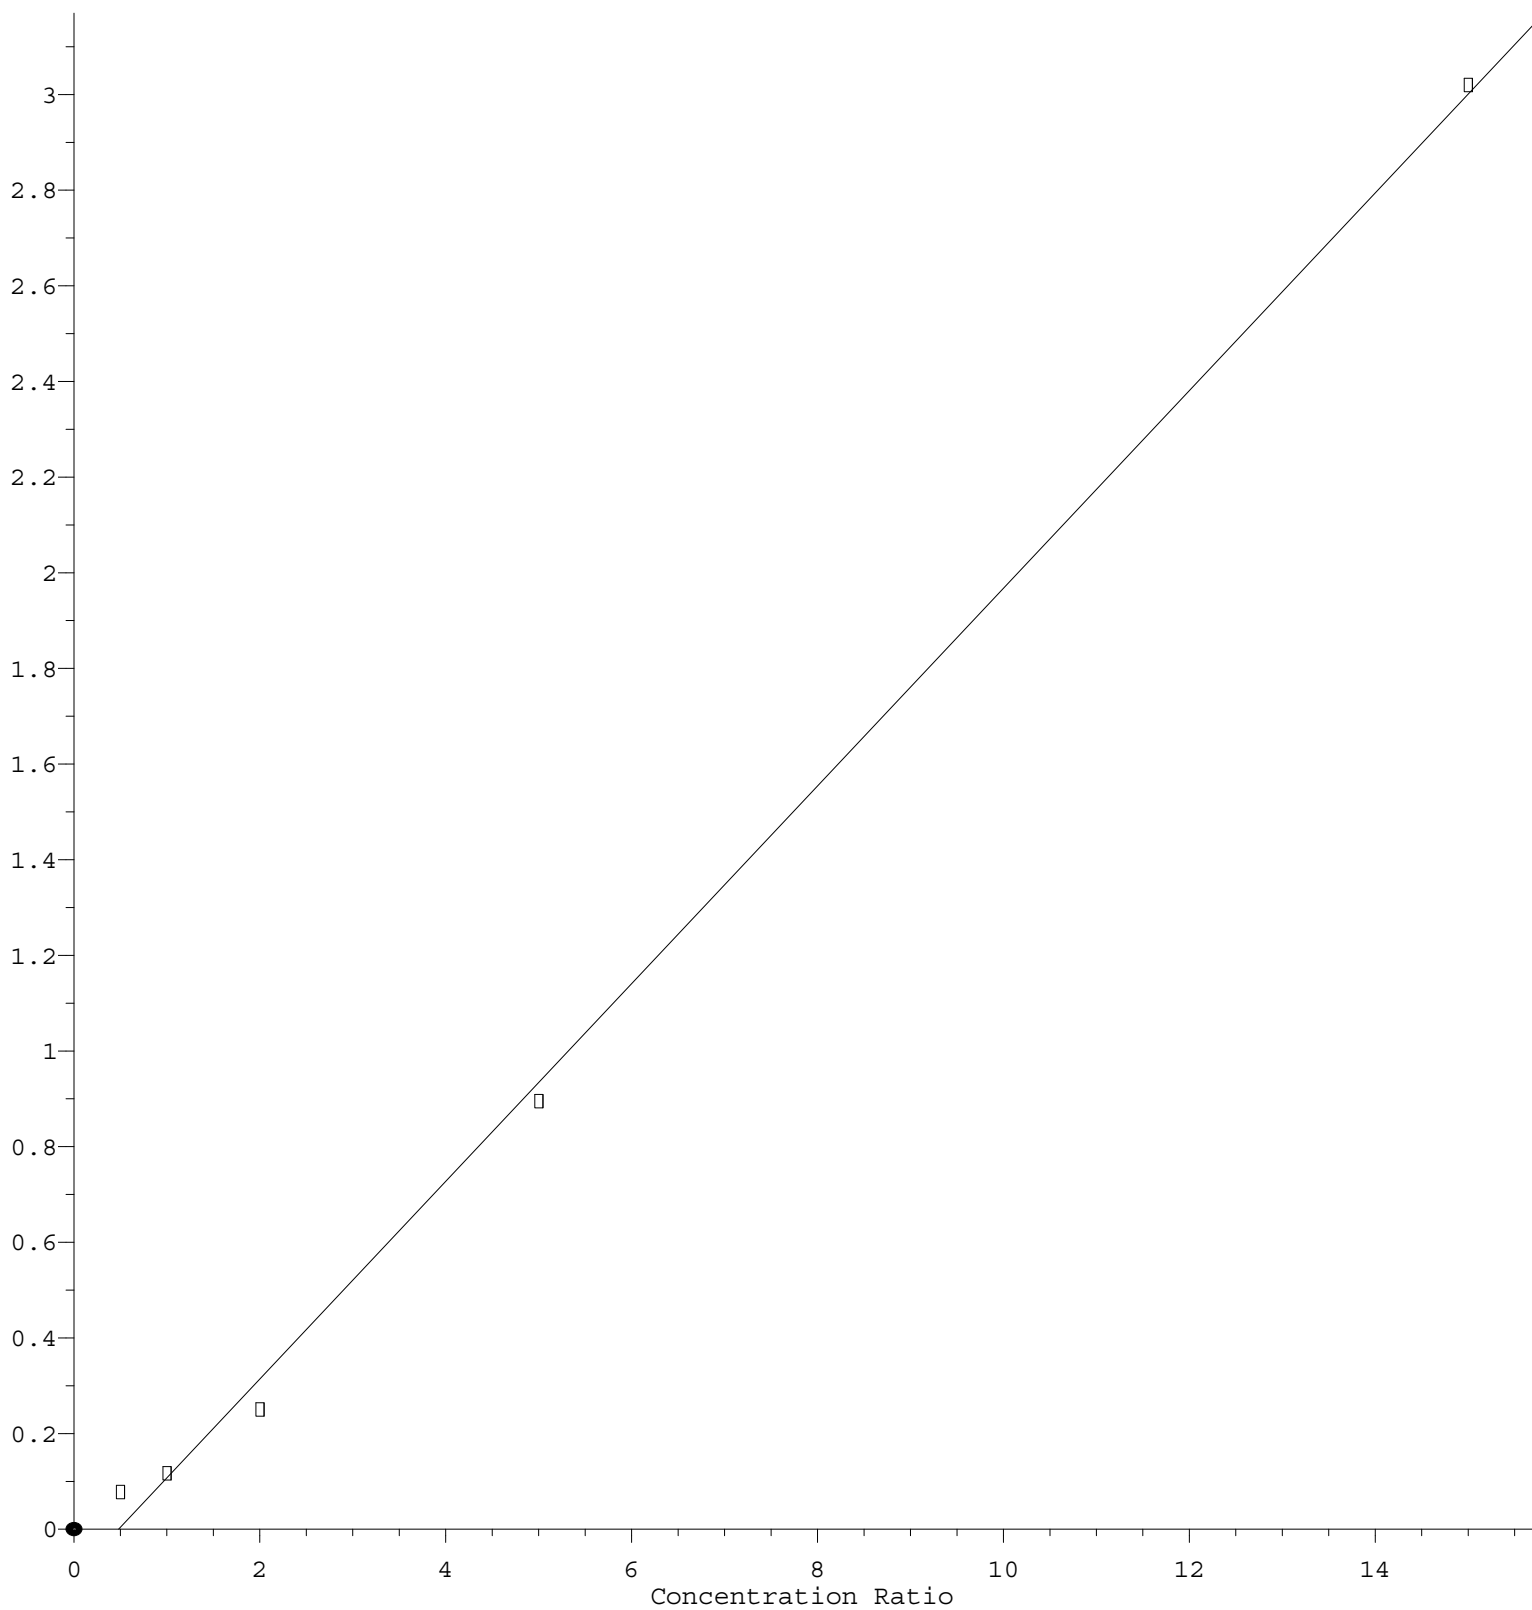

$$\text{Response} = 2.068\text{e-}001 * \text{Amt} - 9.990\text{e-}002$$

Coef of Det (r^2) = 0.998153 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA Y\methods\82Y081522S.M

Calibration Table Last Updated: Tue Aug 16 07:01:08 2022