
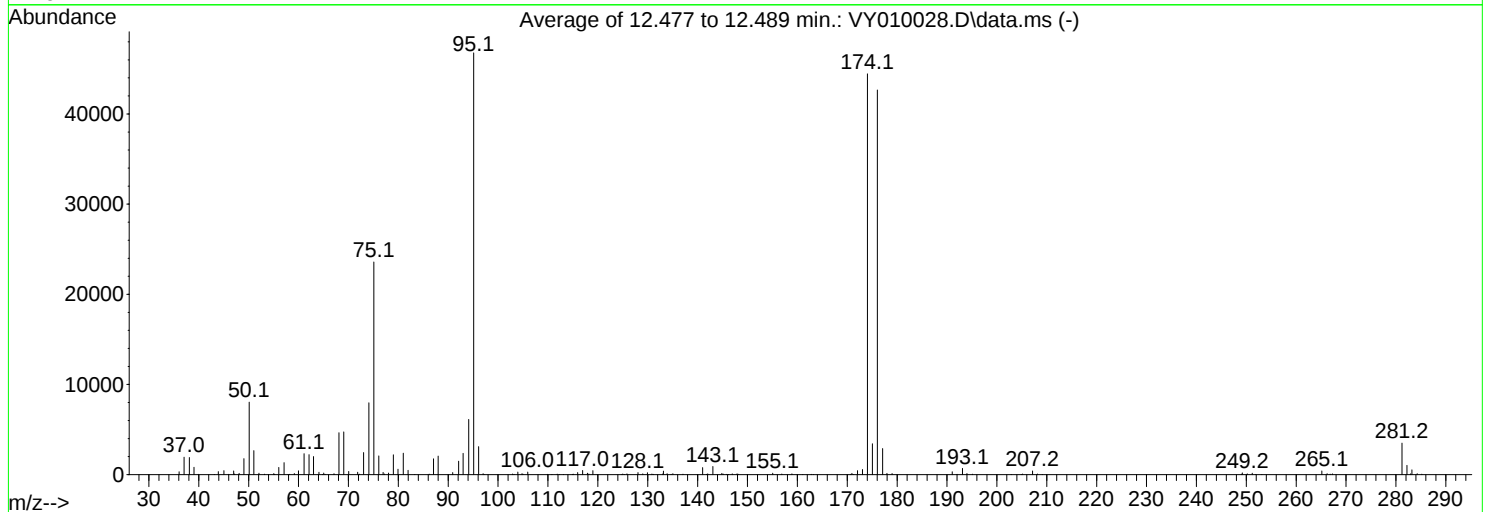


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY081522\
 Data File : VY010028.D
 Acq On : 15 Aug 2022 14:23
 Operator : KP/MD
 Sample : BFB
 Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y081522S.M
 Title : SW846 8260
 Last Update : Tue Aug 16 07:01:08 2022

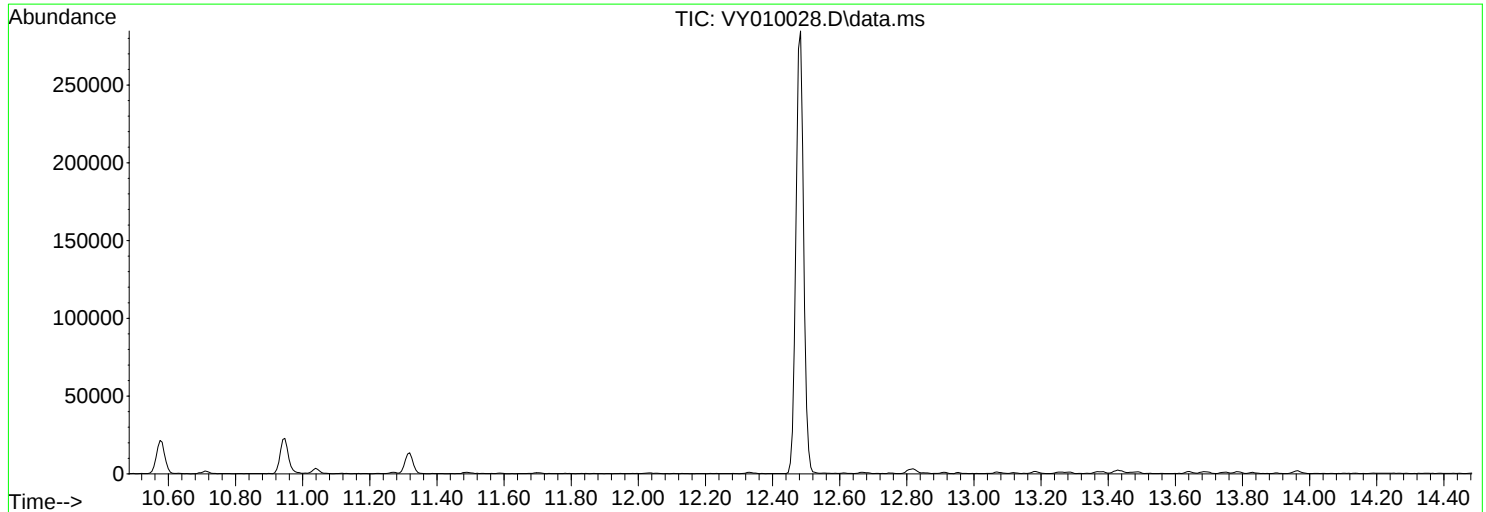

AutoFind: Scans 1748, 1749, 1750; Background Corrected with Scan 1740

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.2	8033	PASS
75	95	30	60	50.4	23592	PASS
95	95	100	100	100.0	46779	PASS
96	95	5	9	6.6	3102	PASS
173	174	0.00	2	1.3	574	PASS
174	95	50	100	95.0	44459	PASS
175	174	5	9	7.7	3432	PASS
176	174	95	101	96.0	42661	PASS
177	176	5	9	6.8	2890	PASS