
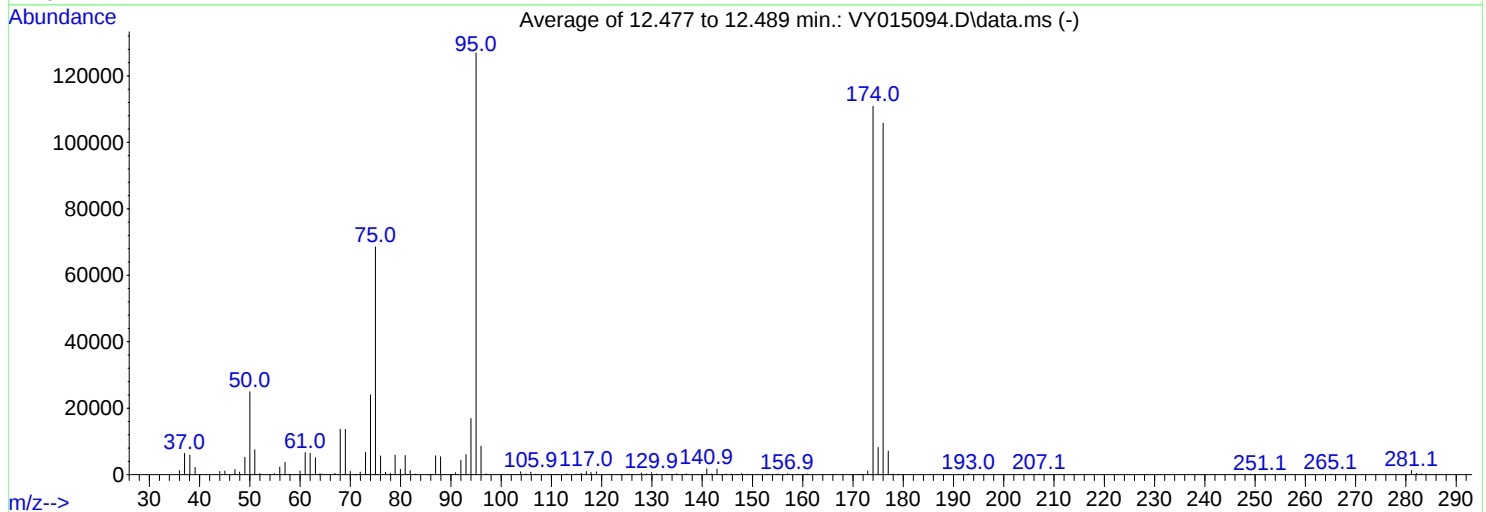


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY081523\
 Data File : VY015094.D
 Acq On : 15 Aug 2023 08:53
 Operator : SY/MD
 Sample : BFB
 Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y081423S.M
 Title : SW846 8260
 Last Update : Mon Aug 14 12:43:26 2023

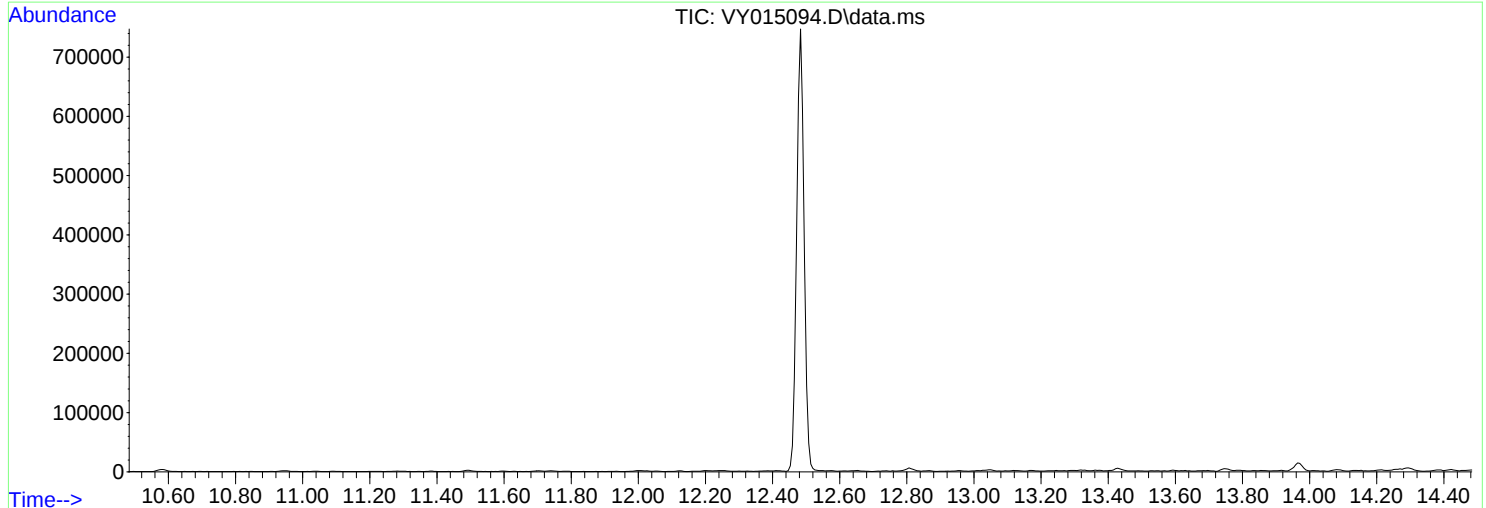

AutoFind: Scans 1748, 1749, 1750; Background Corrected with Scan 1737

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.6	24941	PASS
75	95	30	60	54.0	68520	PASS
95	95	100	100	100.0	126941	PASS
96	95	5	9	6.7	8561	PASS
173	174	0.00	2	1.0	1103	PASS
174	95	50	100	87.3	110864	PASS
175	174	5	9	7.4	8195	PASS
176	174	95	101	95.4	105805	PASS
177	176	5	9	6.7	7102	PASS