

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY081621\
 Data File : VY005661.D
 Acq On : 16 Aug 2021 11:39
 Operator : SY/MD
 Sample : M3407-28
 Misc : 10.2G/5ML/MSVOA_Y/SOIL
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 29S

Quant Time: Aug 17 05:17:51 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y080221S.M
 Quant Title : SW846 8260
 QLast Update : Tue Aug 03 04:52:05 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.795	168	185678	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.697	114	309011	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.490	117	304759	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.428	152	146619	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.149	65	119607	63.637	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	127.280%
35) Dibromofluoromethane	7.728	113	94378	54.551	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	109.100%
50) Toluene-d8	10.185	98	393512	54.234	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	=	108.460%
62) 4-Bromofluorobenzene	12.483	95	130694	54.393	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	=	108.780%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY081621\
Data File : VY005661.D
Acq On : 16 Aug 2021 11:39
Operator : SY/MD
Sample : M3407-28
Misc : 10.2G/5ML/MSVOA_Y/SOIL
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
29S

Quant Time: Aug 17 05:17:51 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y080221S.M
Quant Title : SW846 8260
QLast Update : Tue Aug 03 04:52:05 2021
Response via : Initial Calibration




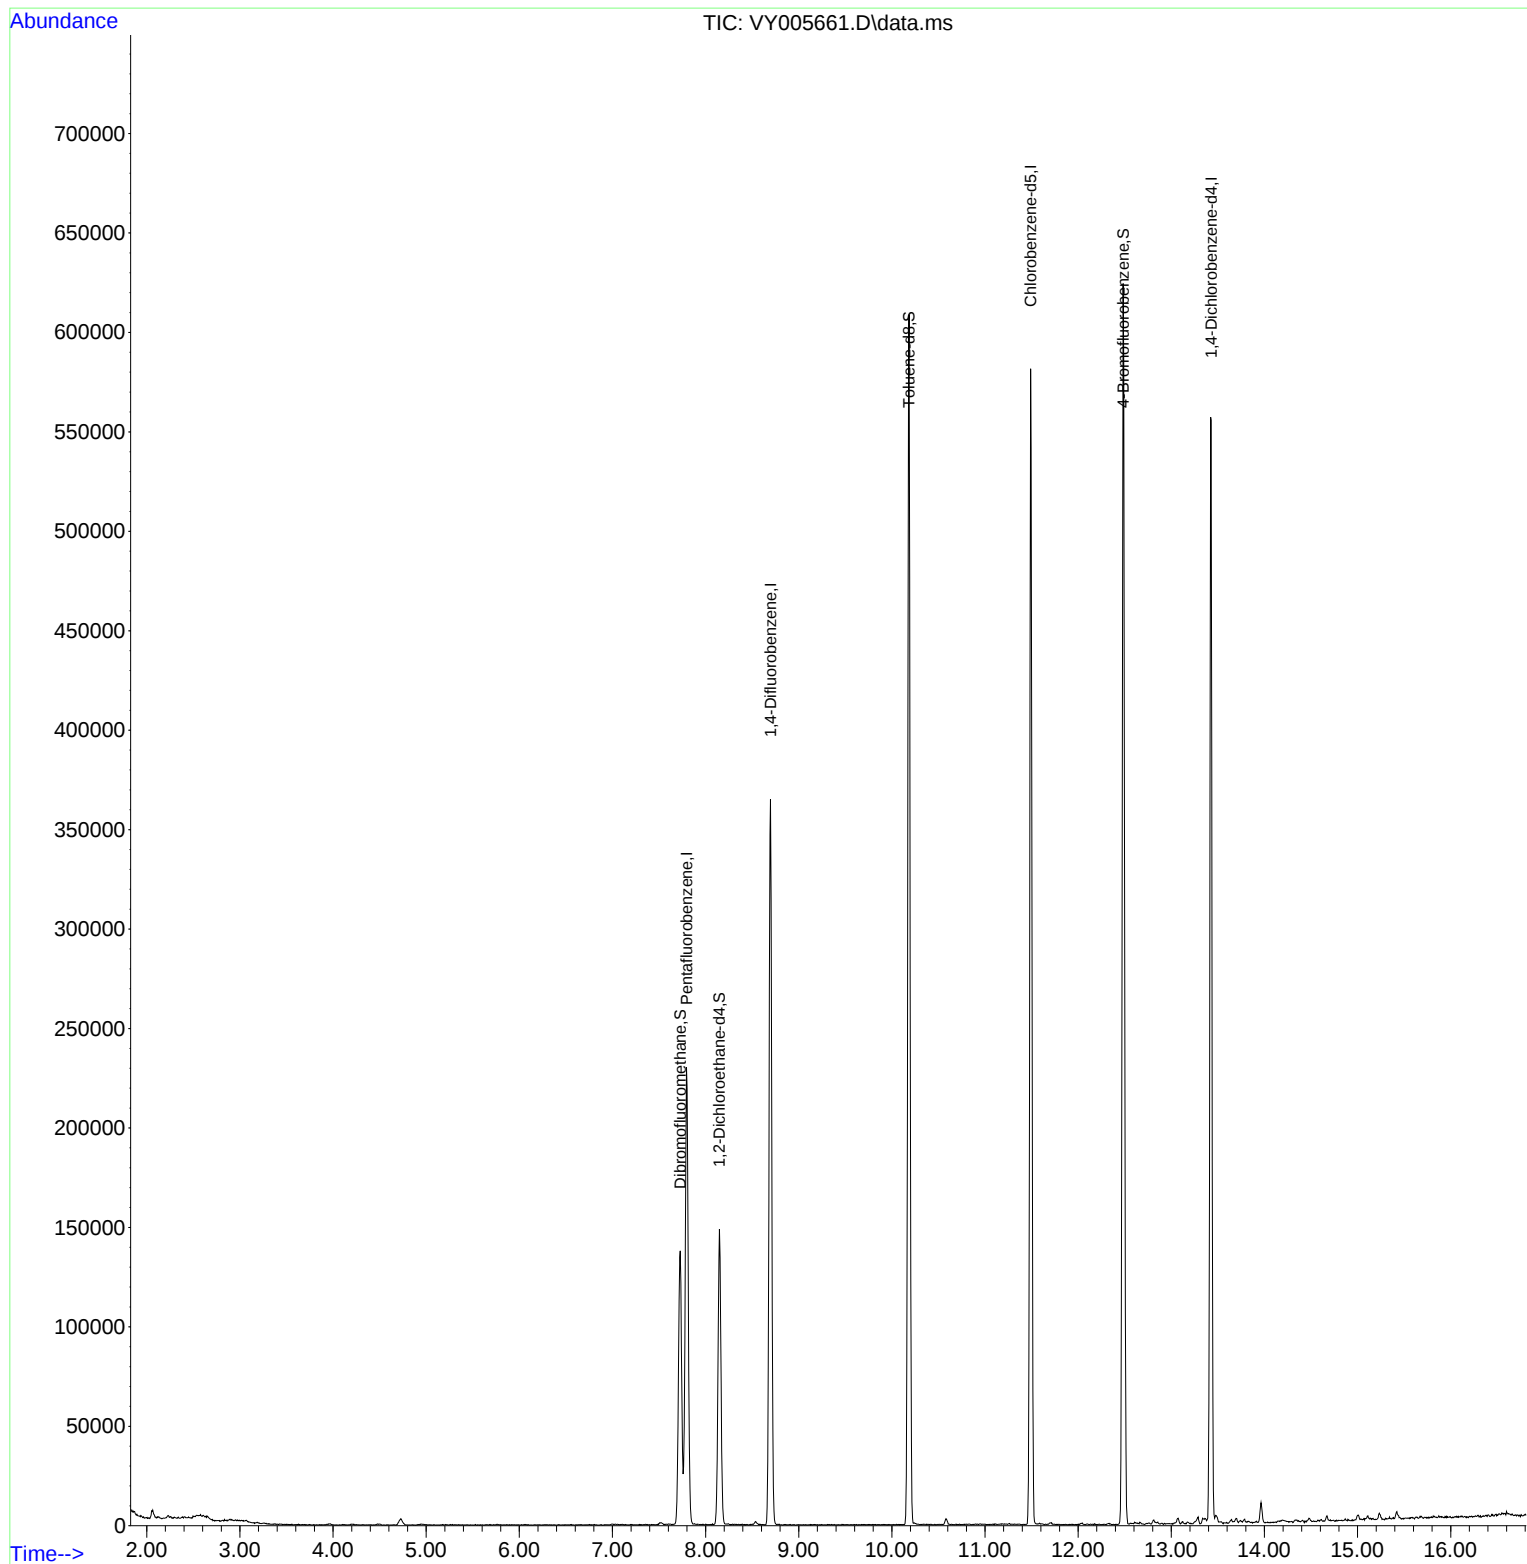


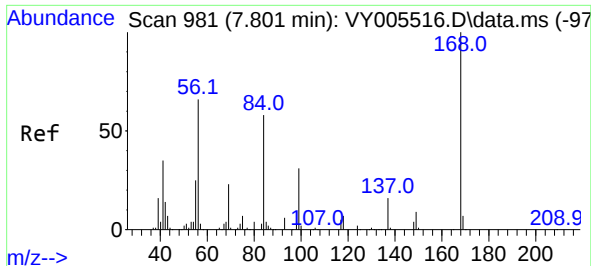

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.795 min Scan# 980
Delta R.T. -0.006 min
Lab File: VY005661.D
Acq: 16 Aug 2021 11:39




Instrument :
MSVOA_Y
ClientSampleId :
29S


Tgt Ion:168 Resp: 185678
Ion Ratio Lower Upper
168 100
99 52.2 38.9 58.3

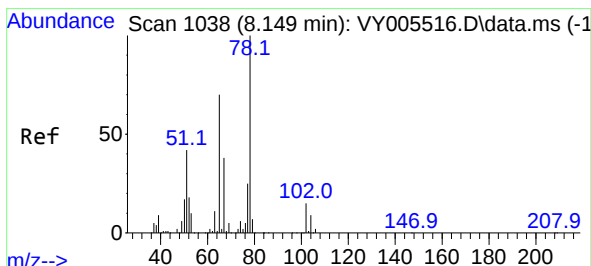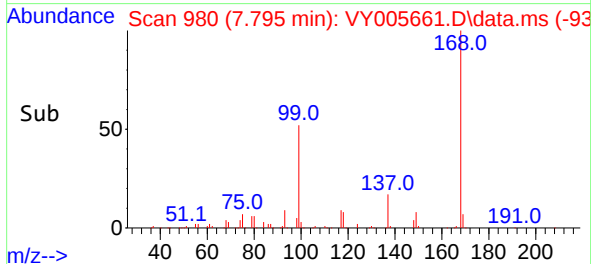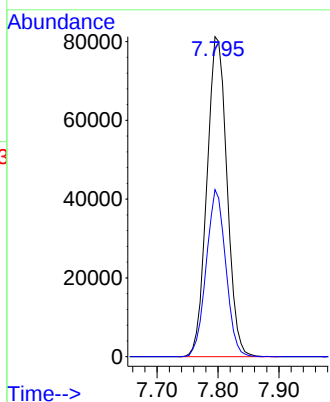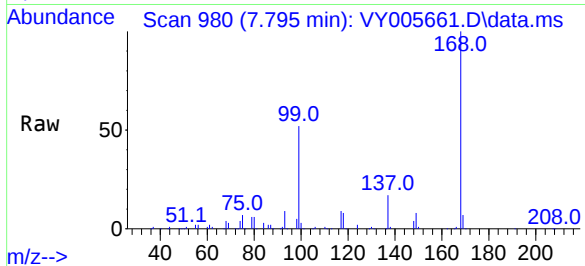

#33
1,2-Dichloroethane-d4
Concen: 63.637 ug/l
RT: 8.149 min Scan# 1038
Delta R.T. -0.000 min
Lab File: VY005661.D
Acq: 16 Aug 2021 11:39

Tgt Ion: 65 Resp: 119607
Ion Ratio Lower Upper
65 100
67 51.1 0.0 103.4


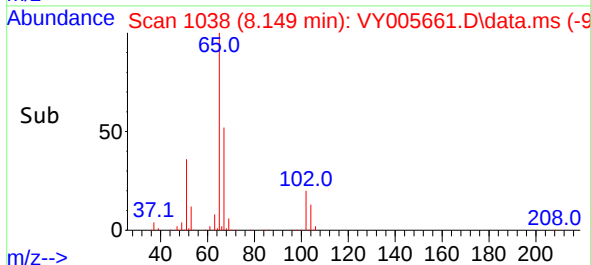
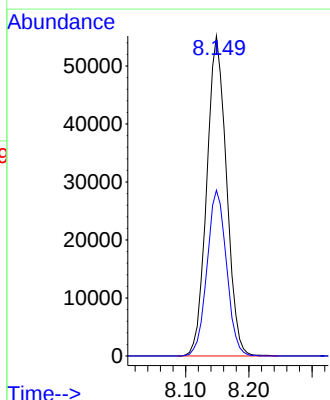
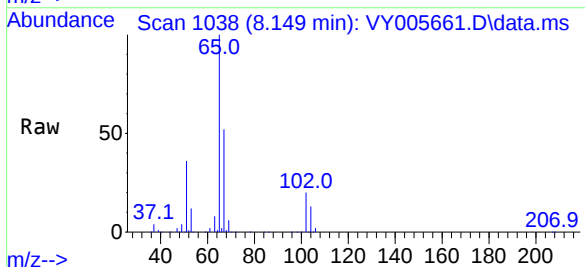


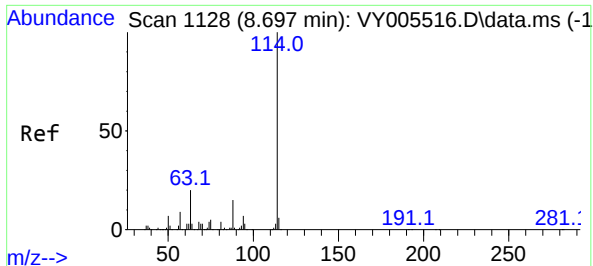

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.697 min Scan# 1128
Delta R.T. -0.000 min
Lab File: VY005661.D
Acq: 16 Aug 2021 11:39




Instrument :
MSVOA_Y
ClientSampleId :
29S


Tgt Ion:	114	Resp:	309011
Ion Ratio	Lower	Upper	
114	100		
63	20.1	0.0	39.2
88	15.0	0.0	30.8

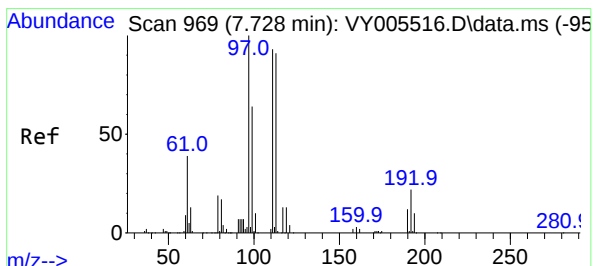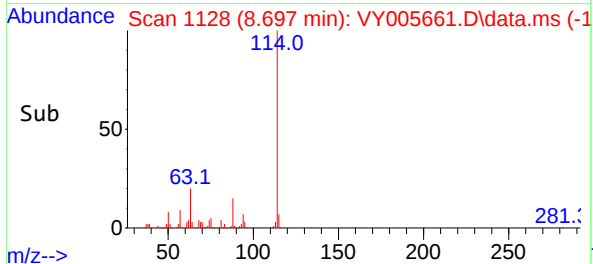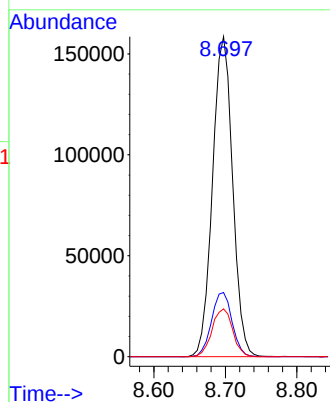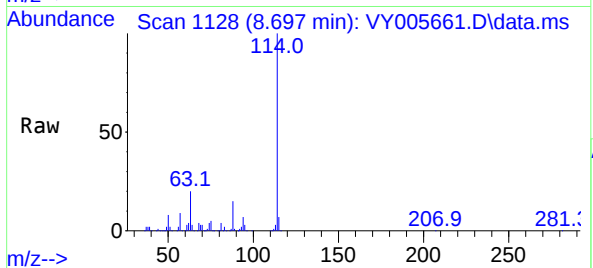

#35
Dibromofluoromethane
Concen: 54.551 ug/l
RT: 7.728 min Scan# 969
Delta R.T. -0.000 min
Lab File: VY005661.D
Acq: 16 Aug 2021 11:39

Tgt Ion:	113	Resp:	94378
Ion Ratio	Lower	Upper	
113	100		
111	101.4	81.9	122.9
192	23.5	19.2	28.8


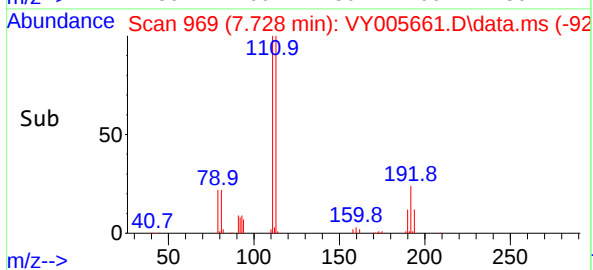
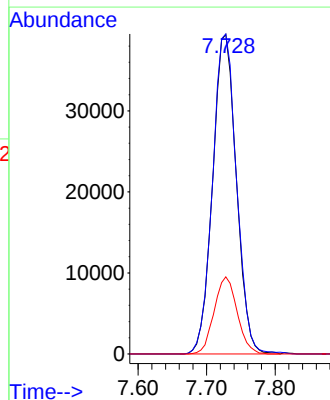
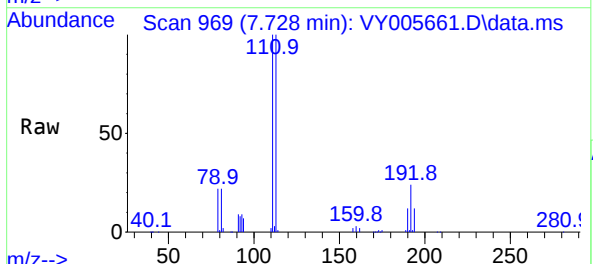


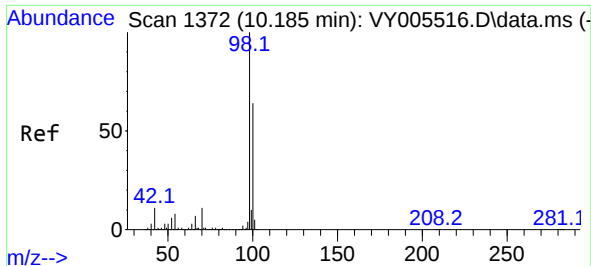

#50
Toluene-d8
Concen: 54.234 ug/l
RT: 10.185 min Scan# 1372
Delta R.T. -0.000 min
Lab File: VY005661.D
Acq: 16 Aug 2021 11:39




Instrument :
MSVOA_Y
ClientSampled :
29S


Tgt Ion: 98 Resp: 393512
Ion Ratio Lower Upper
98 100
100 62.9 51.3 76.9

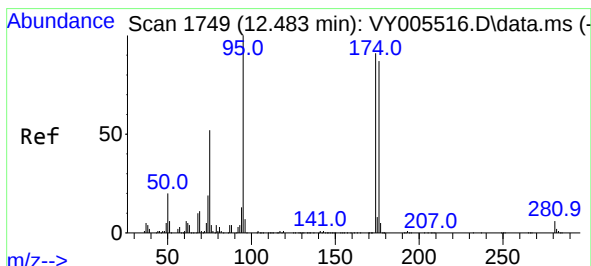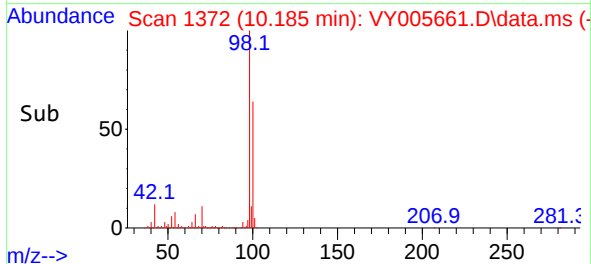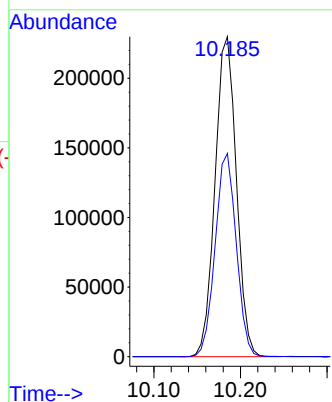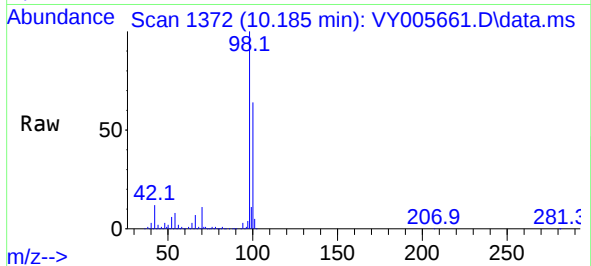

#62
4-Bromofluorobenzene
Concen: 54.393 ug/l
RT: 12.483 min Scan# 1749
Delta R.T. -0.000 min
Lab File: VY005661.D
Acq: 16 Aug 2021 11:39

Tgt Ion: 95 Resp: 130694
Ion Ratio Lower Upper
95 100
174 97.8 0.0 191.4
176 95.4 0.0 183.6


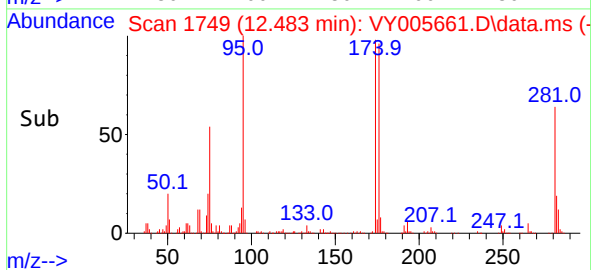
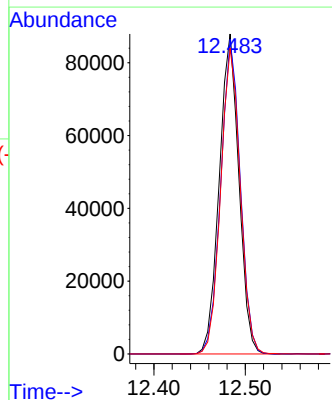
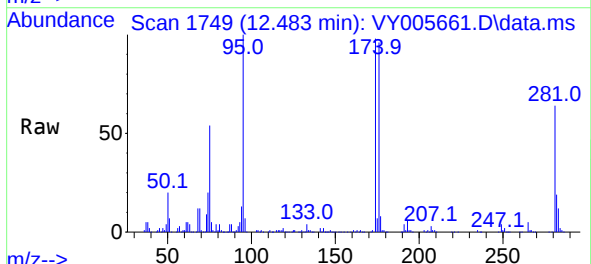


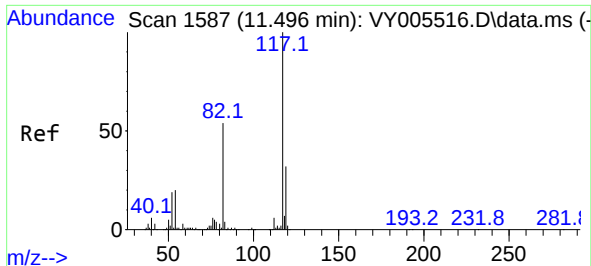

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.490 min Scan# 1586
Delta R.T. -0.006 min
Lab File: VY005661.D
Acq: 16 Aug 2021 11:39

Instrument :
MSVOA_Y
ClientSampled :
29S

Tgt Ion:117 Resp: 304759
Ion Ratio Lower Upper
117 100
82 56.3 43.5 65.3
119 32.1 25.5 38.3

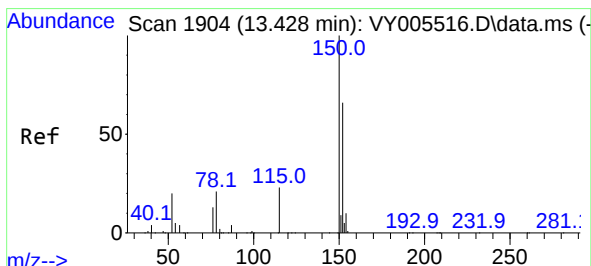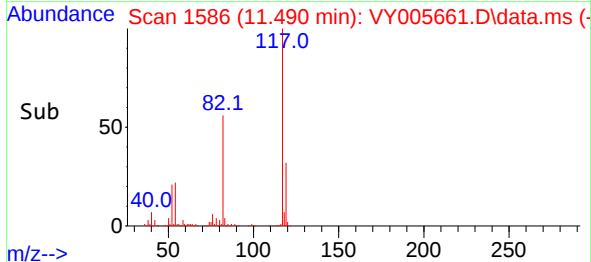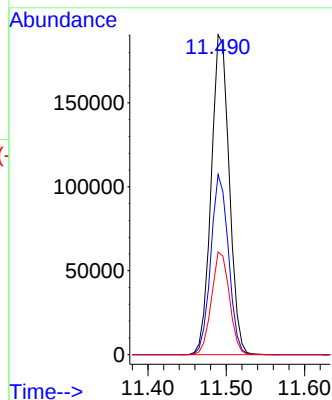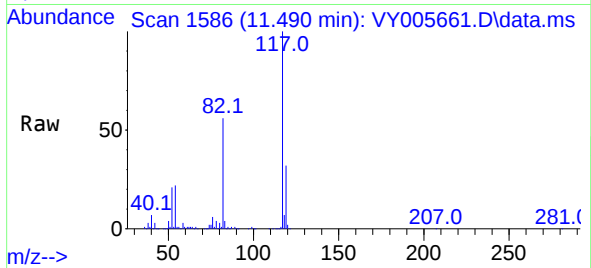

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.428 min Scan# 1904
Delta R.T. -0.000 min
Lab File: VY005661.D
Acq: 16 Aug 2021 11:39

Tgt Ion:152 Resp: 146619
Ion Ratio Lower Upper
152 100
115 53.9 27.3 81.9
150 156.1 0.0 350.2

