


Data Path : Z:\voasrv\HPCHEM1\MSVOA\_Y\Data\VY081622\  
Data File : VY010037.D  
Acq On : 16 Aug 2022 08:20  
Operator : KP/MD  
Sample : BFB  
Misc : 5.00g/5.0mL/MSVOA\_Y/SOIL  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
MSVOA\_Y  
ClientSampleId :  
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA\_Y\methods\82Y081522S.M  
Title : SW846 8260  
Last Update : Wed Aug 17 05:12:02 2022

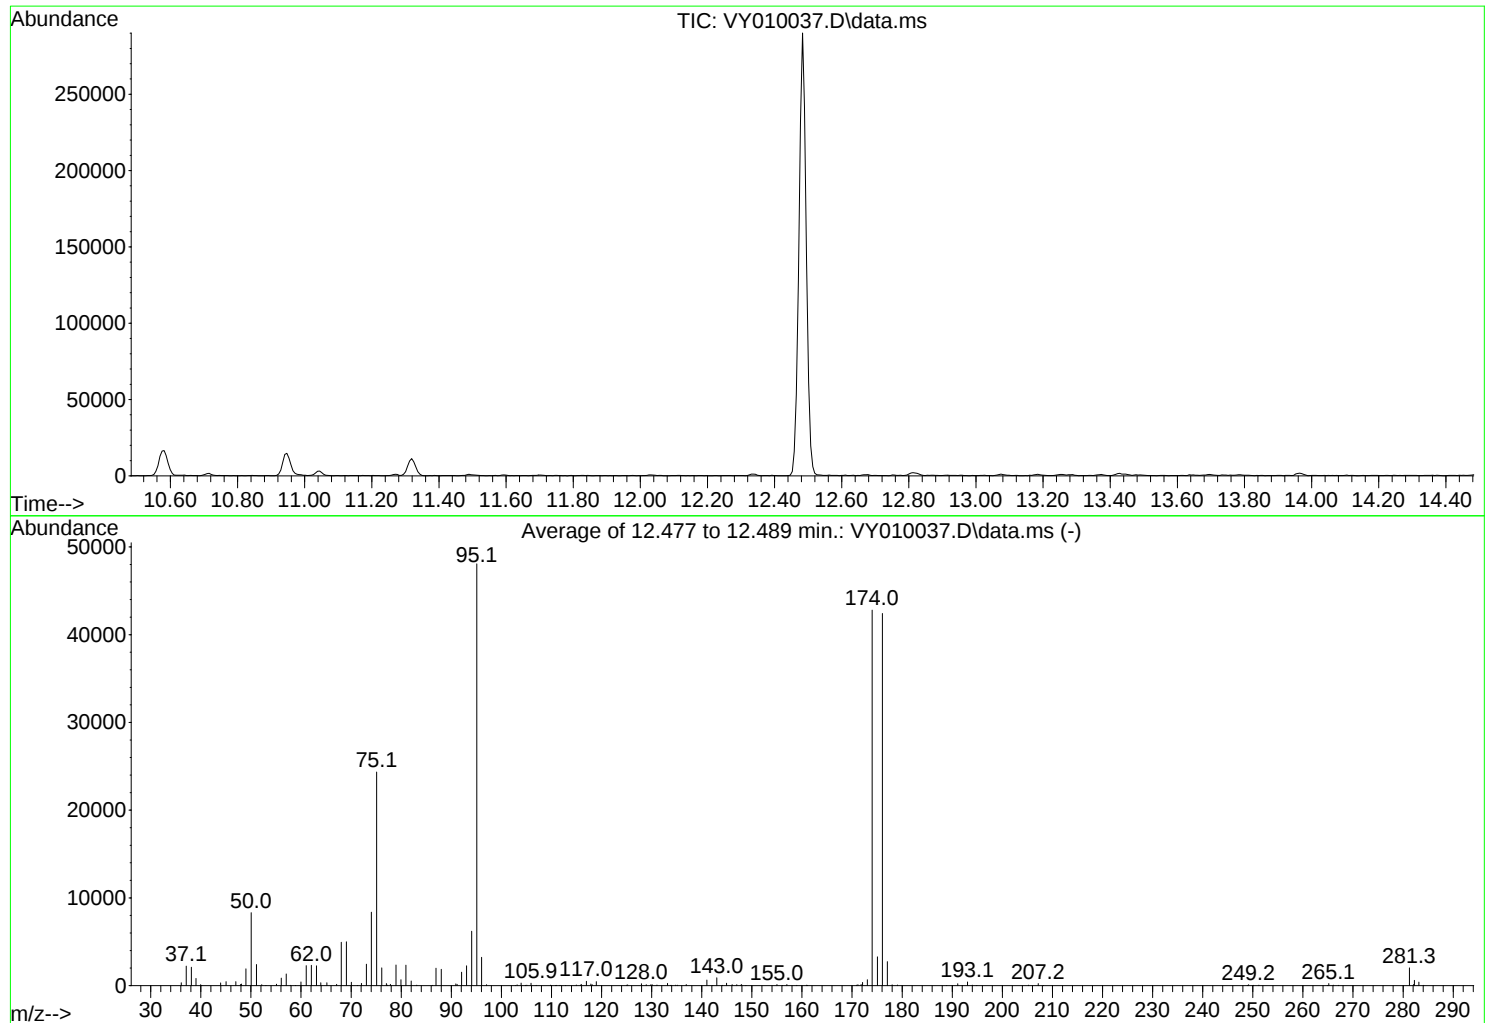

AutoFind: Scans 1748, 1749, 1750; Background Corrected with Scan 1740

| Target | Rel. to | Lower  | Upper  | Rel.  | Raw   | Result    |
|--------|---------|--------|--------|-------|-------|-----------|
| Mass   | Mass    | Limit% | Limit% | Abn%  | Abn   | Pass/Fail |
| 50     | 95      | 15     | 40     | 17.3  | 8325  | PASS      |
| 75     | 95      | 30     | 60     | 50.6  | 24341 | PASS      |
| 95     | 95      | 100    | 100    | 100.0 | 48072 | PASS      |
| 96     | 95      | 5      | 9      | 6.7   | 3237  | PASS      |
| 173    | 174     | 0.00   | 2      | 1.6   | 668   | PASS      |
| 174    | 95      | 50     | 100    | 89.0  | 42803 | PASS      |
| 175    | 174     | 5      | 9      | 7.7   | 3275  | PASS      |
| 176    | 174     | 95     | 101    | 99.1  | 42411 | PASS      |
| 177    | 176     | 5      | 9      | 6.5   | 2736  | PASS      |