
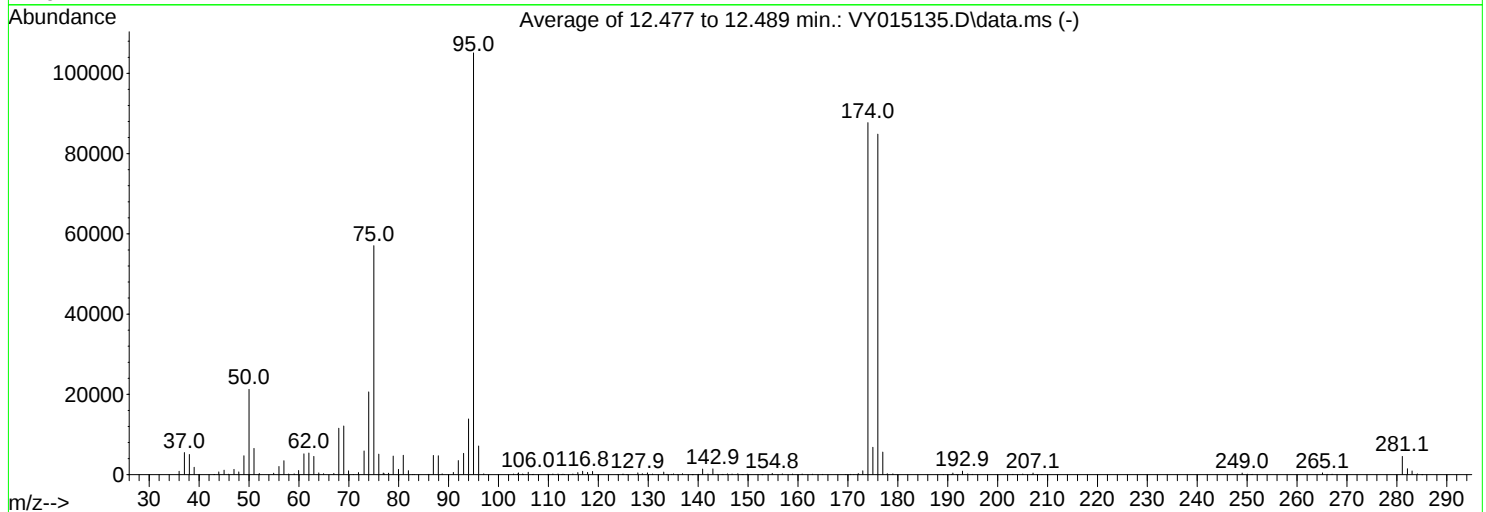


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY081623\
Data File : VY015135.D
Acq On : 16 Aug 2023 08:42
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y081423S.M
Title : SW846 8260
Last Update : Mon Aug 14 12:43:26 2023

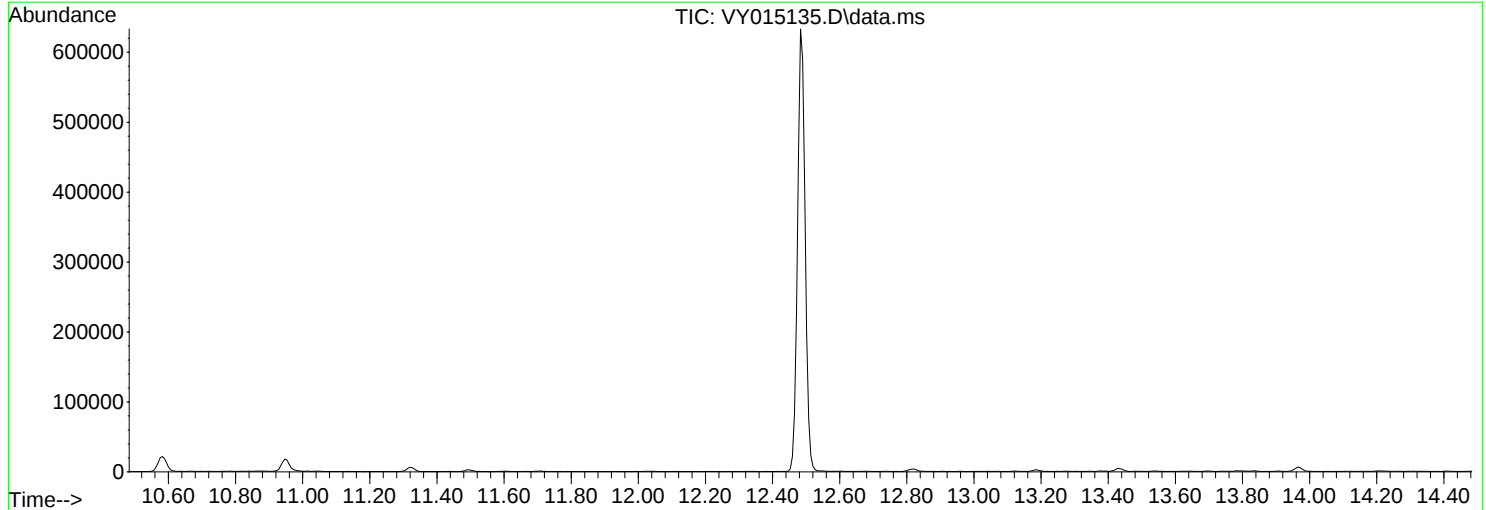

AutoFind: Scans 1748, 1749, 1750; Background Corrected with Scan 1740

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.2	21275	PASS
75	95	30	60	54.3	57053	PASS
95	95	100	100	100.0	105109	PASS
96	95	5	9	6.8	7127	PASS
173	174	0.00	2	1.1	960	PASS
174	95	50	100	83.5	87715	PASS
175	174	5	9	7.8	6829	PASS
176	174	95	101	96.8	84867	PASS
177	176	5	9	6.6	5624	PASS