


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY081624\
Data File : VY019079.D
Acq On : 16 Aug 2024 08:09
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y081524S.M
Title : SW846 8260
Last Update : Fri Aug 16 05:10:30 2024

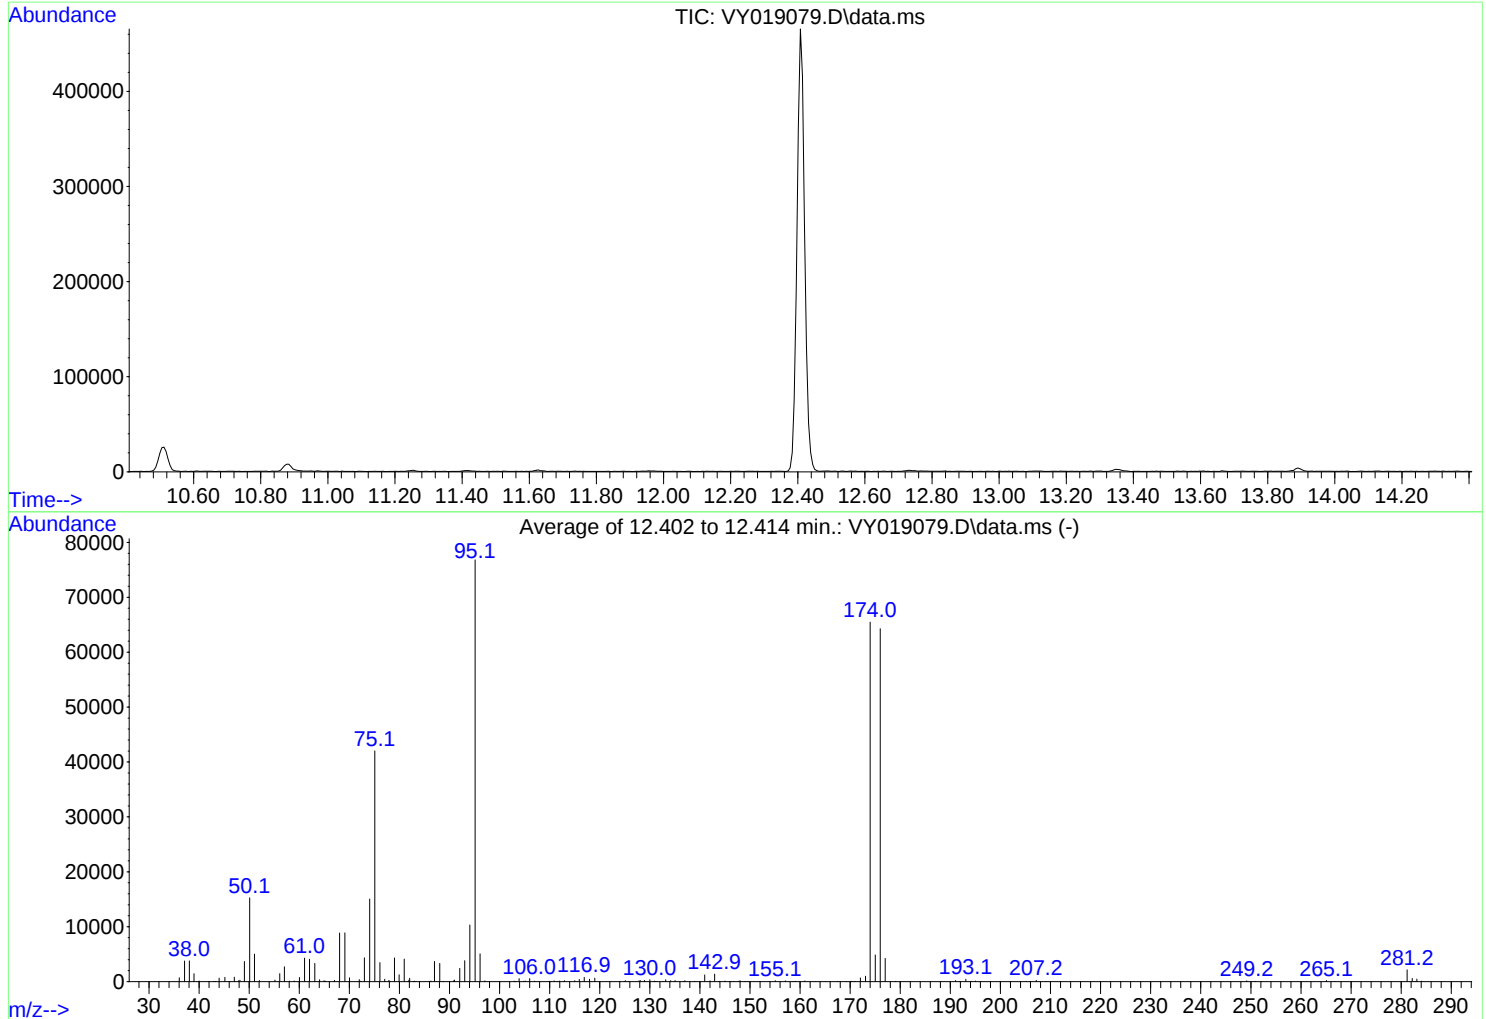

AutoFind: Scans 1752, 1753, 1754; Background Corrected with Scan 1744

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	19.9	15266	PASS
75	95	30	60	54.7	42029	PASS
95	95	100	100	100.0	76816	PASS
96	95	5	9	6.6	5071	PASS
173	174	0.00	2	1.5	990	PASS
174	95	50	100	85.2	65469	PASS
175	174	5	9	7.4	4863	PASS
176	174	95	101	98.2	64285	PASS
177	176	5	9	6.6	4216	PASS