

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_Y\Data\VY081722\  
 Data File : VY010079.D  
 Acq On : 17 Aug 2022 19:22  
 Operator : KP/MD  
 Sample : N4124-03  
 Misc : 12.82g/5.0mL/MSVOA\_Y/SOIL  
 ALS Vial : 26 Sample Multiplier: 1

Instrument :  
 MSVOA\_Y  
 ClientSampleId :  
 SSP3

Quant Time: Aug 18 08:23:05 2022  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_Y\methods\82Y081522S.M  
 Quant Title : SW846 8260  
 QLast Update : Wed Aug 17 05:12:02 2022  
 Response via : Initial Calibration

| Compound                   | R.T.   | QIon | Response | Conc   | Units | Dev(Min) |
|----------------------------|--------|------|----------|--------|-------|----------|
| -----                      |        |      |          |        |       |          |
| Internal Standards         |        |      |          |        |       |          |
| 1) Pentafluorobenzene      | 7.783  | 168  | 70620    | 50.000 | ug/l  | 0.00     |
| 34) 1,4-Difluorobenzene    | 8.685  | 114  | 116847   | 50.000 | ug/l  | 0.00     |
| 63) Chlorobenzene-d5       | 11.489 | 117  | 117460   | 50.000 | ug/l  | 0.00     |
| 72) 1,4-Dichlorobenzene-d4 | 13.422 | 152  | 56712    | 50.000 | ug/l  | 0.00     |

|                             |        |       |          |          |      |          |
|-----------------------------|--------|-------|----------|----------|------|----------|
| System Monitoring Compounds |        |       |          |          |      |          |
| 33) 1,2-Dichloroethane-d4   | 8.136  | 65    | 43233    | 61.227   | ug/l | 0.00     |
| Spiked Amount               | 50.000 | Range | 50 - 163 | Recovery | =    | 122.460% |
| 35) Dibromofluoromethane    | 7.710  | 113   | 40567    | 53.536   | ug/l | 0.00     |
| Spiked Amount               | 50.000 | Range | 54 - 147 | Recovery | =    | 107.080% |
| 50) Toluene-d8              | 10.179 | 98    | 133436   | 47.596   | ug/l | 0.00     |
| Spiked Amount               | 50.000 | Range | 49 - 140 | Recovery | =    | 95.200%  |
| 62) 4-Bromofluorobenzene    | 12.483 | 95    | 46475    | 47.198   | ug/l | 0.00     |
| Spiked Amount               | 50.000 | Range | 25 - 144 | Recovery | =    | 94.400%  |


| Target Compounds | Qvalue |
|------------------|--------|
| -----            |        |


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_Y\Data\VY081722\  
Data File : VY010079.D  
Acq On : 17 Aug 2022 19:22  
Operator : KP/MD  
Sample : N4124-03  
Misc : 12.82g/5.0mL/MSVOA\_Y/SOIL  
ALS Vial : 26 Sample Multiplier: 1

Instrument :  
MSVOA\_Y  
ClientSampleId :  
SSP3

Quant Time: Aug 18 08:23:05 2022  
Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_Y\methods\82Y081522S.M  
Quant Title : SW846 8260  
QLast Update : Wed Aug 17 05:12:02 2022  
Response via : Initial Calibration




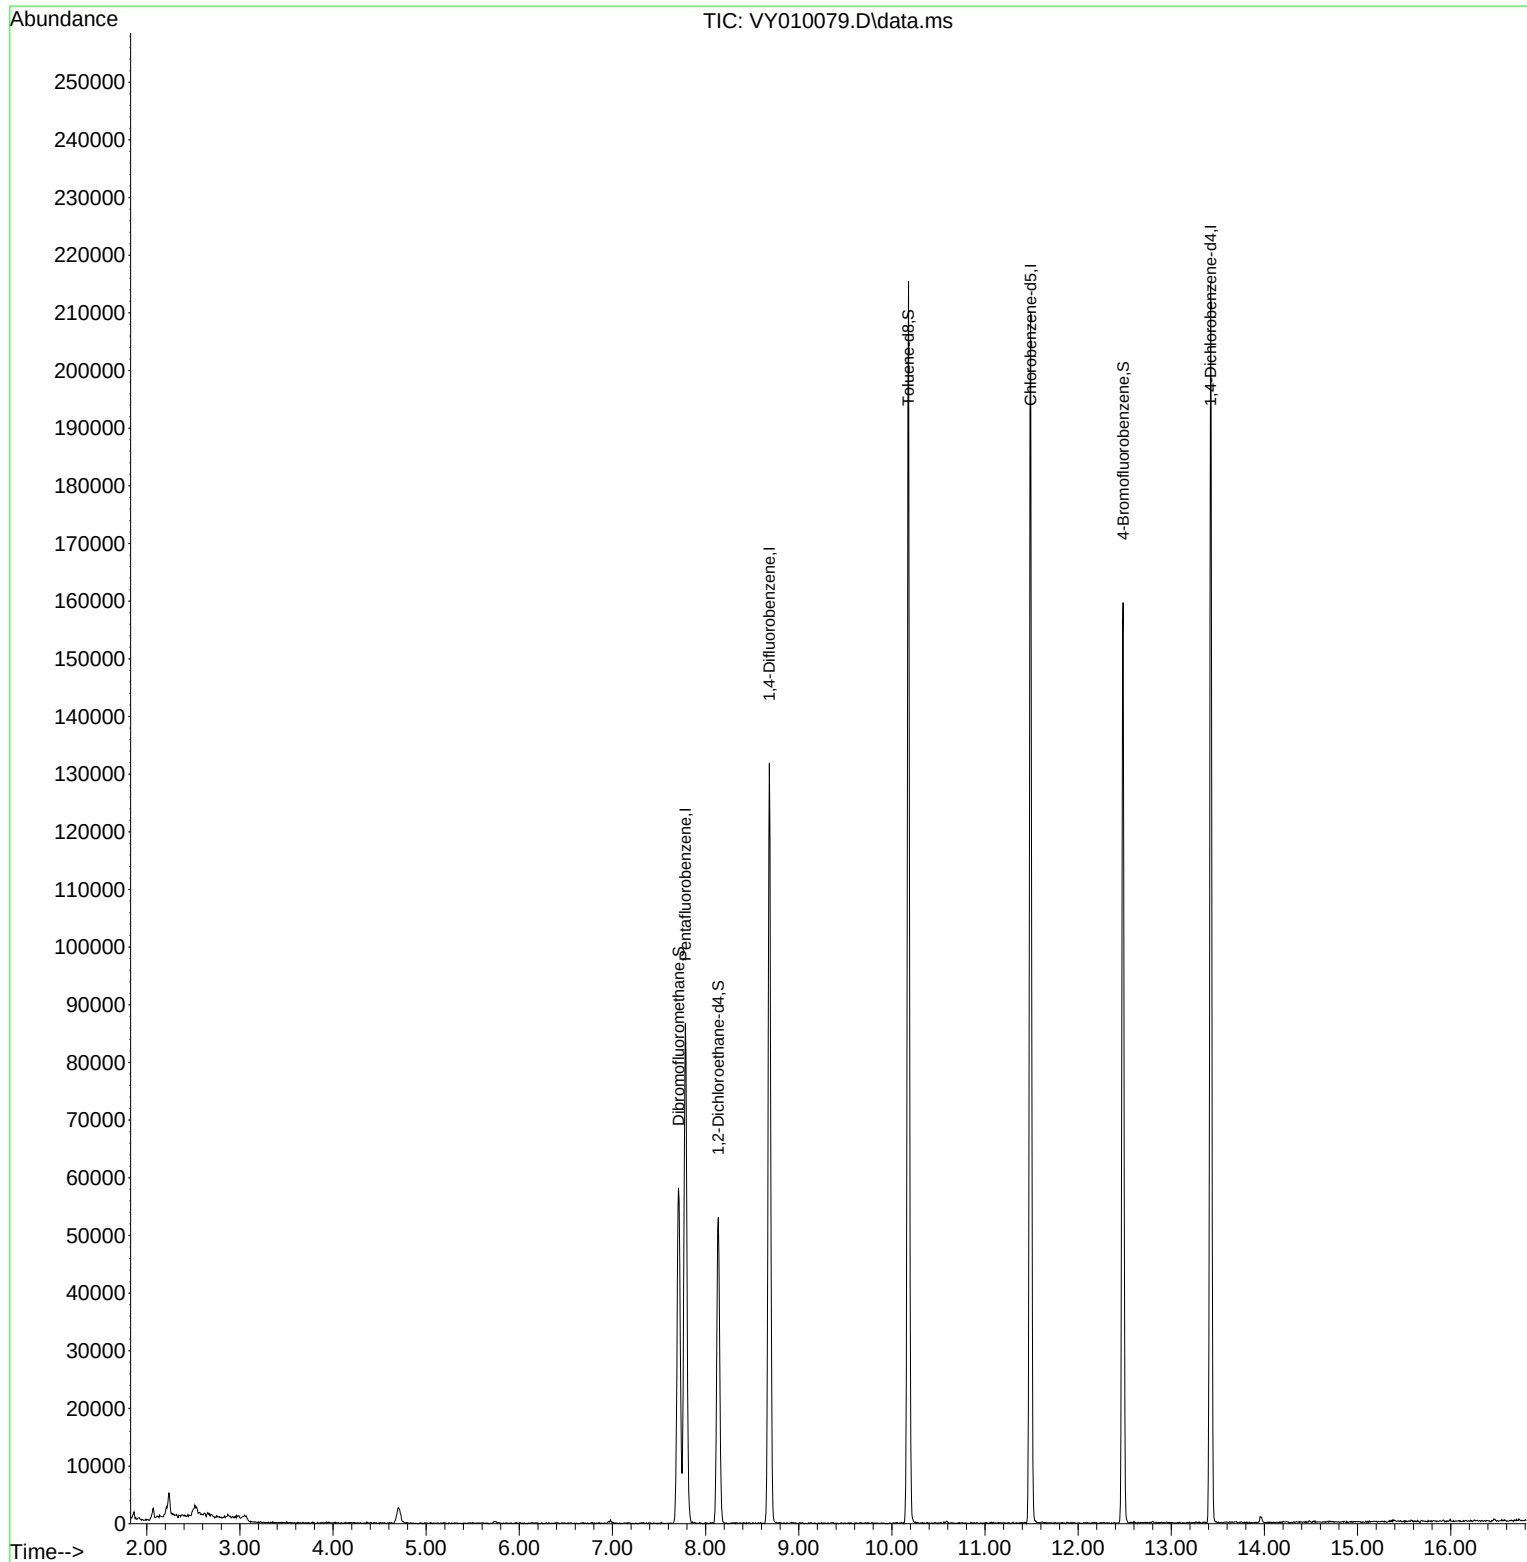


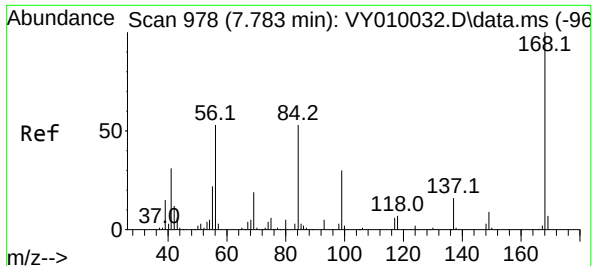

#1  
Pentafluorobenzene  
Concen: 50.000 ug/l  
RT: 7.783 min Scan# 91  
Delta R.T. -0.000 min  
Lab File: VY010079.D  
Acq: 17 Aug 2022 19:22




Instrument :  
MSVOA\_Y  
ClientSampleId :  
SSP3


Tgt Ion:168 Resp: 70620  
Ion Ratio Lower Upper  
168 100  
99 47.7 37.7 56.5

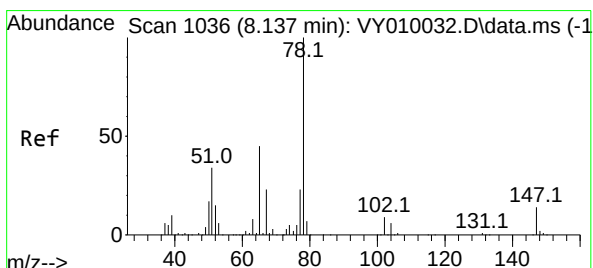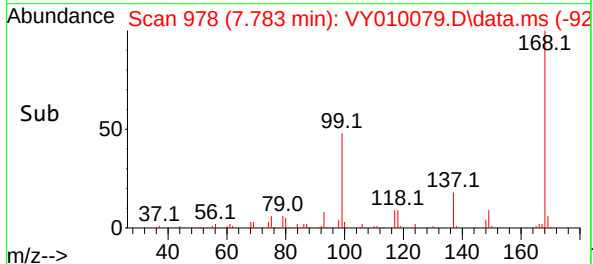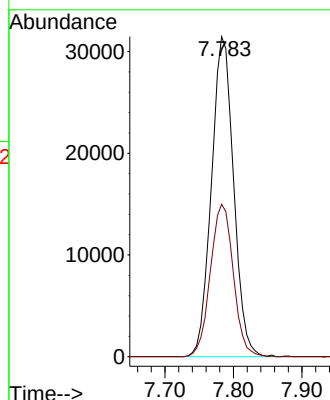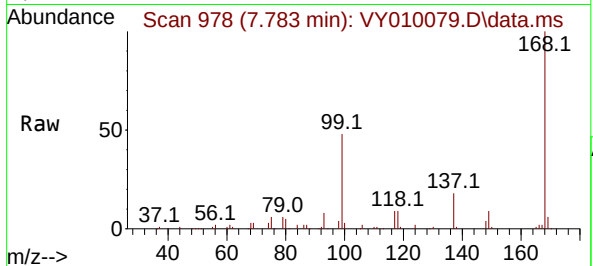

#33  
1,2-Dichloroethane-d4  
Concen: 61.227 ug/l  
RT: 8.136 min Scan# 1036  
Delta R.T. -0.001 min  
Lab File: VY010079.D  
Acq: 17 Aug 2022 19:22

Tgt Ion: 65 Resp: 43233  
Ion Ratio Lower Upper  
65 100  
67 49.8 0.0 104.4

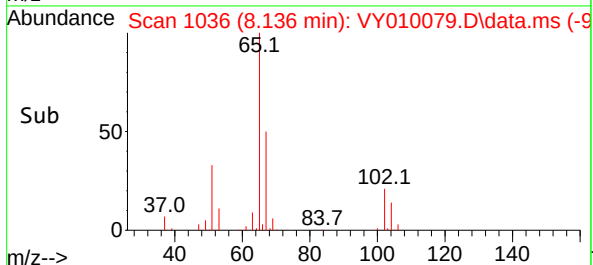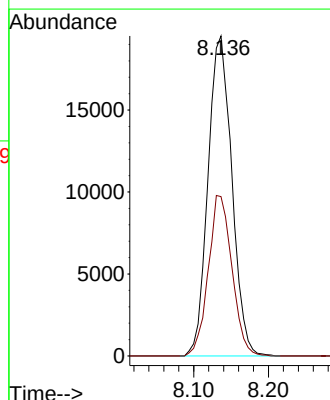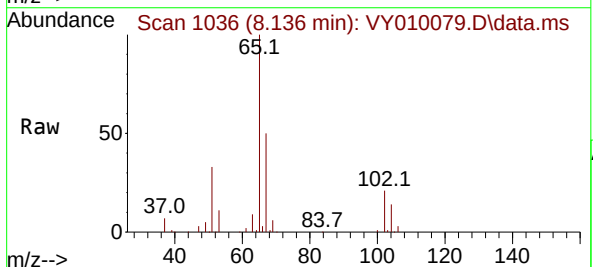

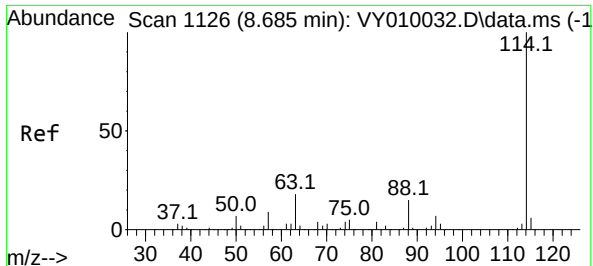

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.685 min Scan# 1126

Delta R.T. 0.000 min

Lab File: VY010079.D

Acq: 17 Aug 2022 19:22

Instrument :

MSVOA\_Y

ClientSampleId :

SSP3





Tgt Ion:114 Resp: 116847

Ion Ratio Lower Upper

114 100

63 16.9 0.0 35.2

88 14.4 0.0 30.2

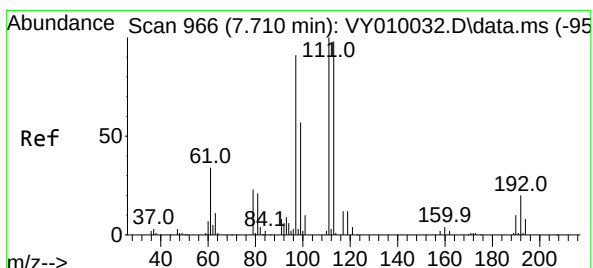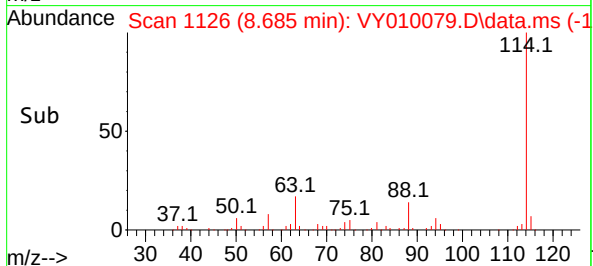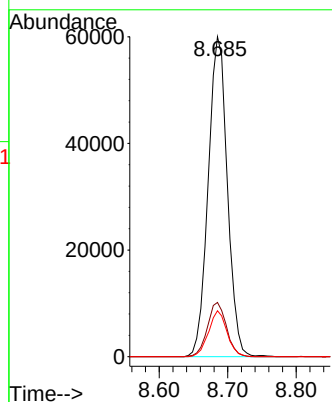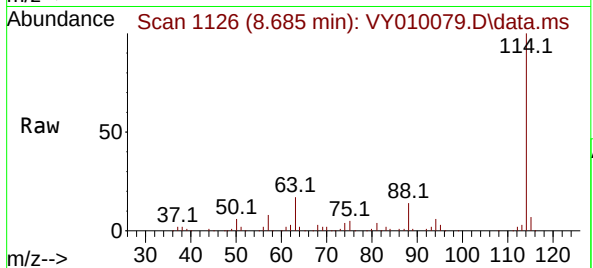

#35

Dibromofluoromethane

Concen: 53.536 ug/l

RT: 7.710 min Scan# 966

Delta R.T. -0.000 min

Lab File: VY010079.D

Acq: 17 Aug 2022 19:22




Tgt Ion:113 Resp: 40567


Ion Ratio Lower Upper

113 100

111 103.1 82.7 124.1

192 22.5 17.2 25.8


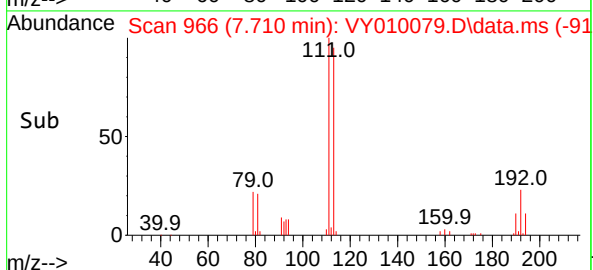
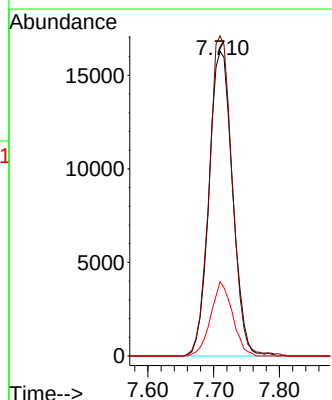
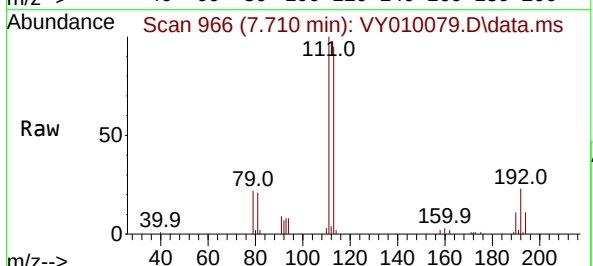


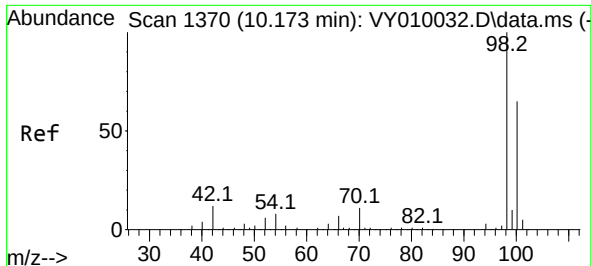

#50  
Toluene-d8  
Concen: 47.596 ug/l  
RT: 10.179 min Scan# 1370  
Delta R.T. 0.006 min  
Lab File: VY010079.D  
Acq: 17 Aug 2022 19:22




Instrument :  
MSVOA\_Y  
ClientSampleId :  
SSP3


Tgt Ion: 98 Resp: 133436  
Ion Ratio Lower Upper  
98 100  
100 66.6 52.1 78.1

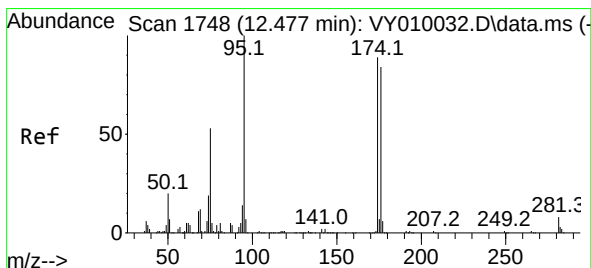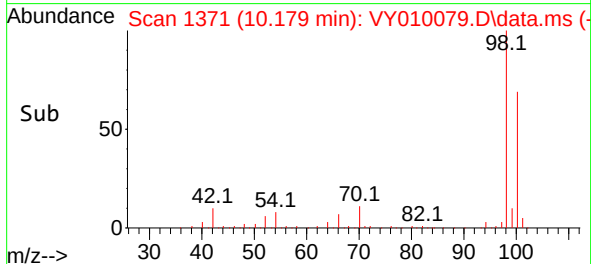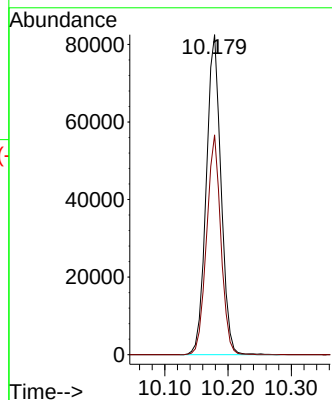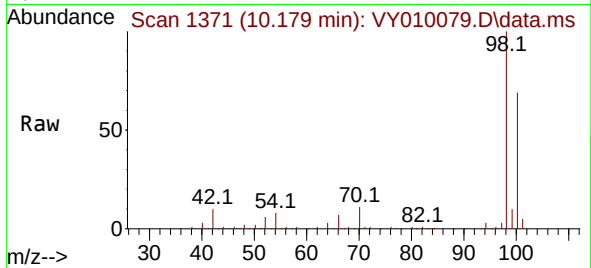

#62  
4-Bromofluorobenzene  
Concen: 47.198 ug/l  
RT: 12.483 min Scan# 1749  
Delta R.T. 0.006 min  
Lab File: VY010079.D  
Acq: 17 Aug 2022 19:22


Tgt Ion: 95 Resp: 46475  
Ion Ratio Lower Upper  
95 100  
174 97.3 0.0 184.2  
176 92.2 0.0 178.4

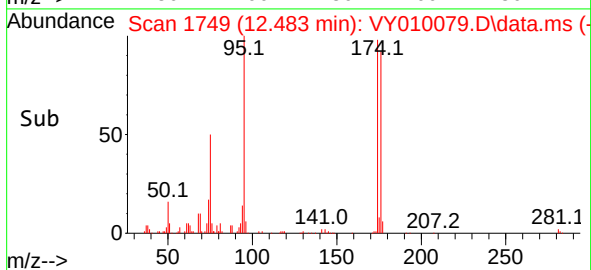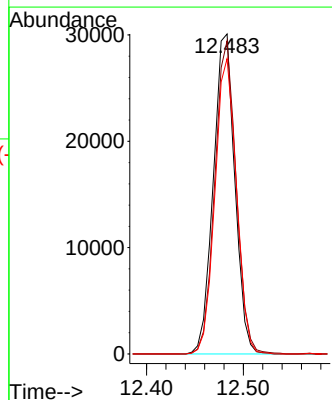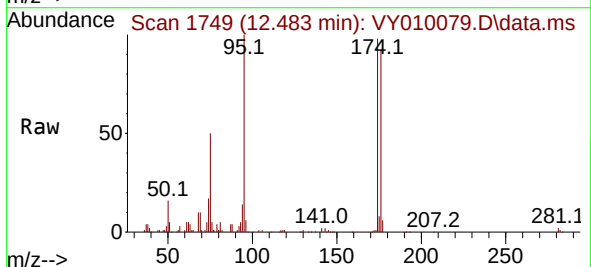



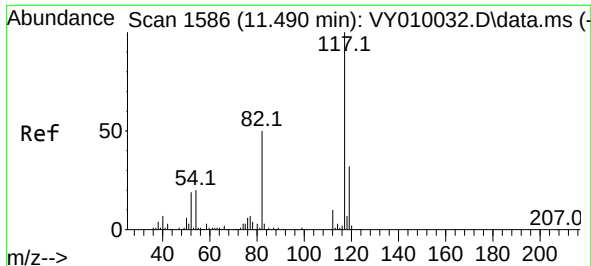


#63  
Chlorobenzene-d5  
Concen: 50.000 ug/l  
RT: 11.489 min Scan# 117460  
Delta R.T. -0.001 min  
Lab File: VY010079.D  
Acq: 17 Aug 2022 19:22

Instrument :  
MSVOA\_Y  
ClientSampleId :  
SSP3

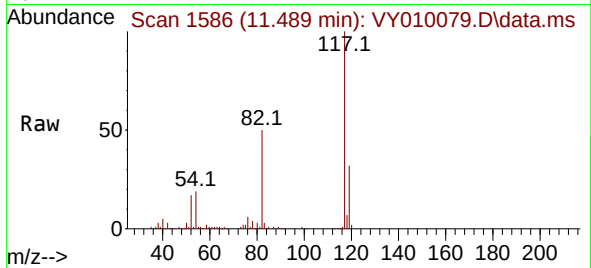

Tgt Ion:117 Resp: 117460  
Ion Ratio Lower Upper  
117 100  
82 49.8 39.8 59.6  
119 32.4 25.6 38.4

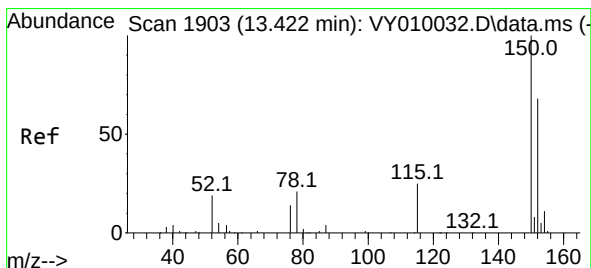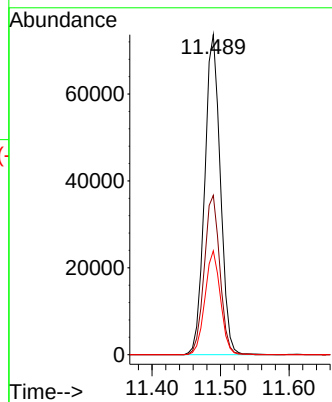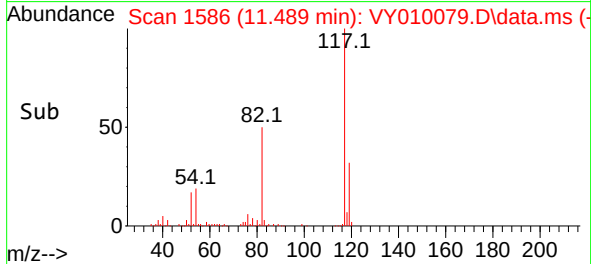

#72  
1,4-Dichlorobenzene-d4  
Concen: 50.000 ug/l  
RT: 13.422 min Scan# 1903  
Delta R.T. 0.000 min  
Lab File: VY010079.D  
Acq: 17 Aug 2022 19:22

Tgt Ion:152 Resp: 56712  
Ion Ratio Lower Upper  
152 100  
115 55.1 28.1 84.3  
150 159.5 0.0 346.6

