
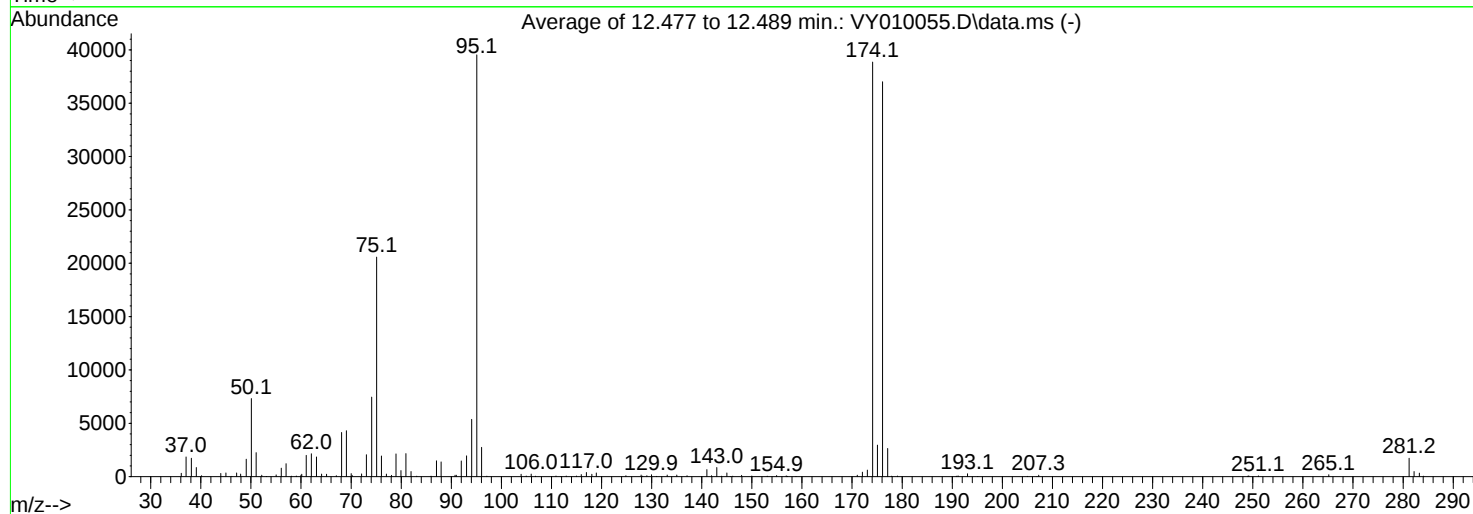


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY081722\
Data File : VY010055.D
Acq On : 17 Aug 2022 08:53
Operator : KP/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y081522S.M
Title : SW846 8260
Last Update : Wed Aug 17 05:12:02 2022

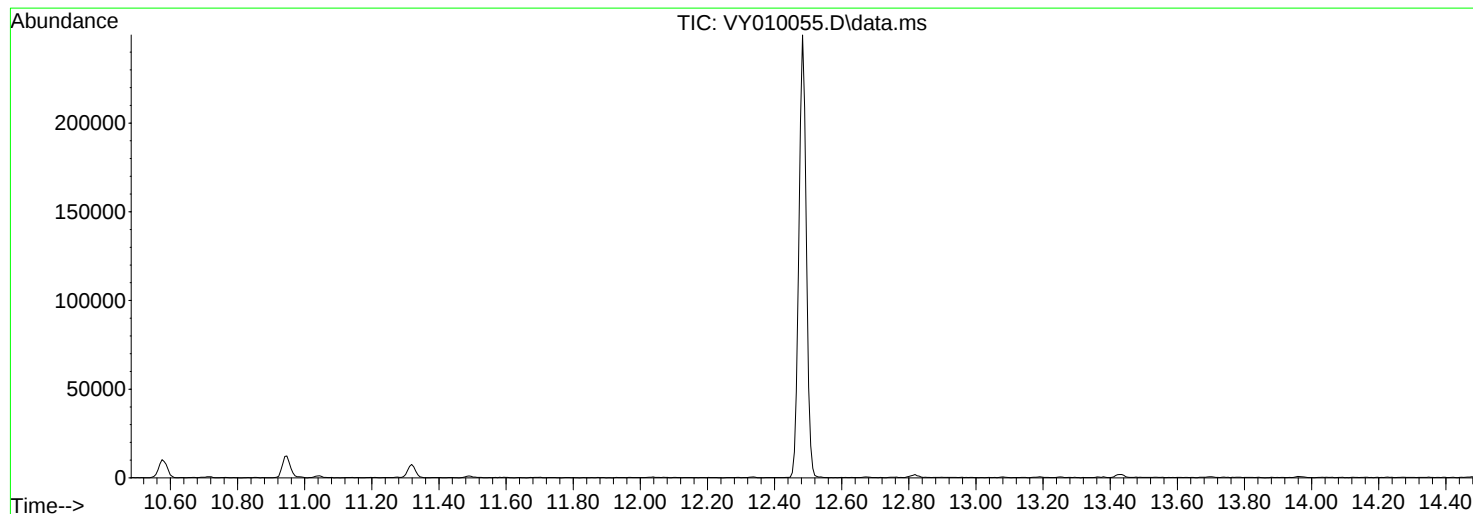

AutoFind: Scans 1748, 1749, 1750; Background Corrected with Scan 1740

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.5	7313	PASS
75	95	30	60	52.0	20568	PASS
95	95	100	100	100.0	39531	PASS
96	95	5	9	7.0	2751	PASS
173	174	0.00	2	1.6	615	PASS
174	95	50	100	98.3	38848	PASS
175	174	5	9	7.6	2949	PASS
176	174	95	101	95.3	37005	PASS
177	176	5	9	7.1	2642	PASS