

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY081823\
 Data File : VY015185.D
 Acq On : 18 Aug 2023 10:47
 Operator : SY/MD
 Sample : VY0818SBL01
 Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 VY0818SBL01

Quant Time: Aug 18 23:05:02 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y081423S.M
 Quant Title : SW846 8260
 QLast Update : Mon Aug 14 12:43:26 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	7.789	168	123071	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.691	114	218606	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.490	117	219380	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.428	152	107538	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.137	65	82736	56.003	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	112.000%
35) Dibromofluoromethane	7.716	113	70432	50.081	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	100.160%
50) Toluene-d8	10.179	98	264714	50.563	ug/l	0.00
Spiked Amount	50.000	Range	58 - 134	Recovery	=	101.120%
62) 4-Bromofluorobenzene	12.483	95	98021	51.261	ug/l	0.00
Spiked Amount	50.000	Range	30 - 143	Recovery	=	102.520%
Target Compounds						
20) Methylene Chloride	4.710	84	12007	6.629	ug/l	Qvalue 85


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY081823\
Data File : VY015185.D
Acq On : 18 Aug 2023 10:47
Operator : SY/MD
Sample : VY0818SBL01
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
VY0818SBL01

Quant Time: Aug 18 23:05:02 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y081423S.M
Quant Title : SW846 8260
QLast Update : Mon Aug 14 12:43:26 2023
Response via : Initial Calibration




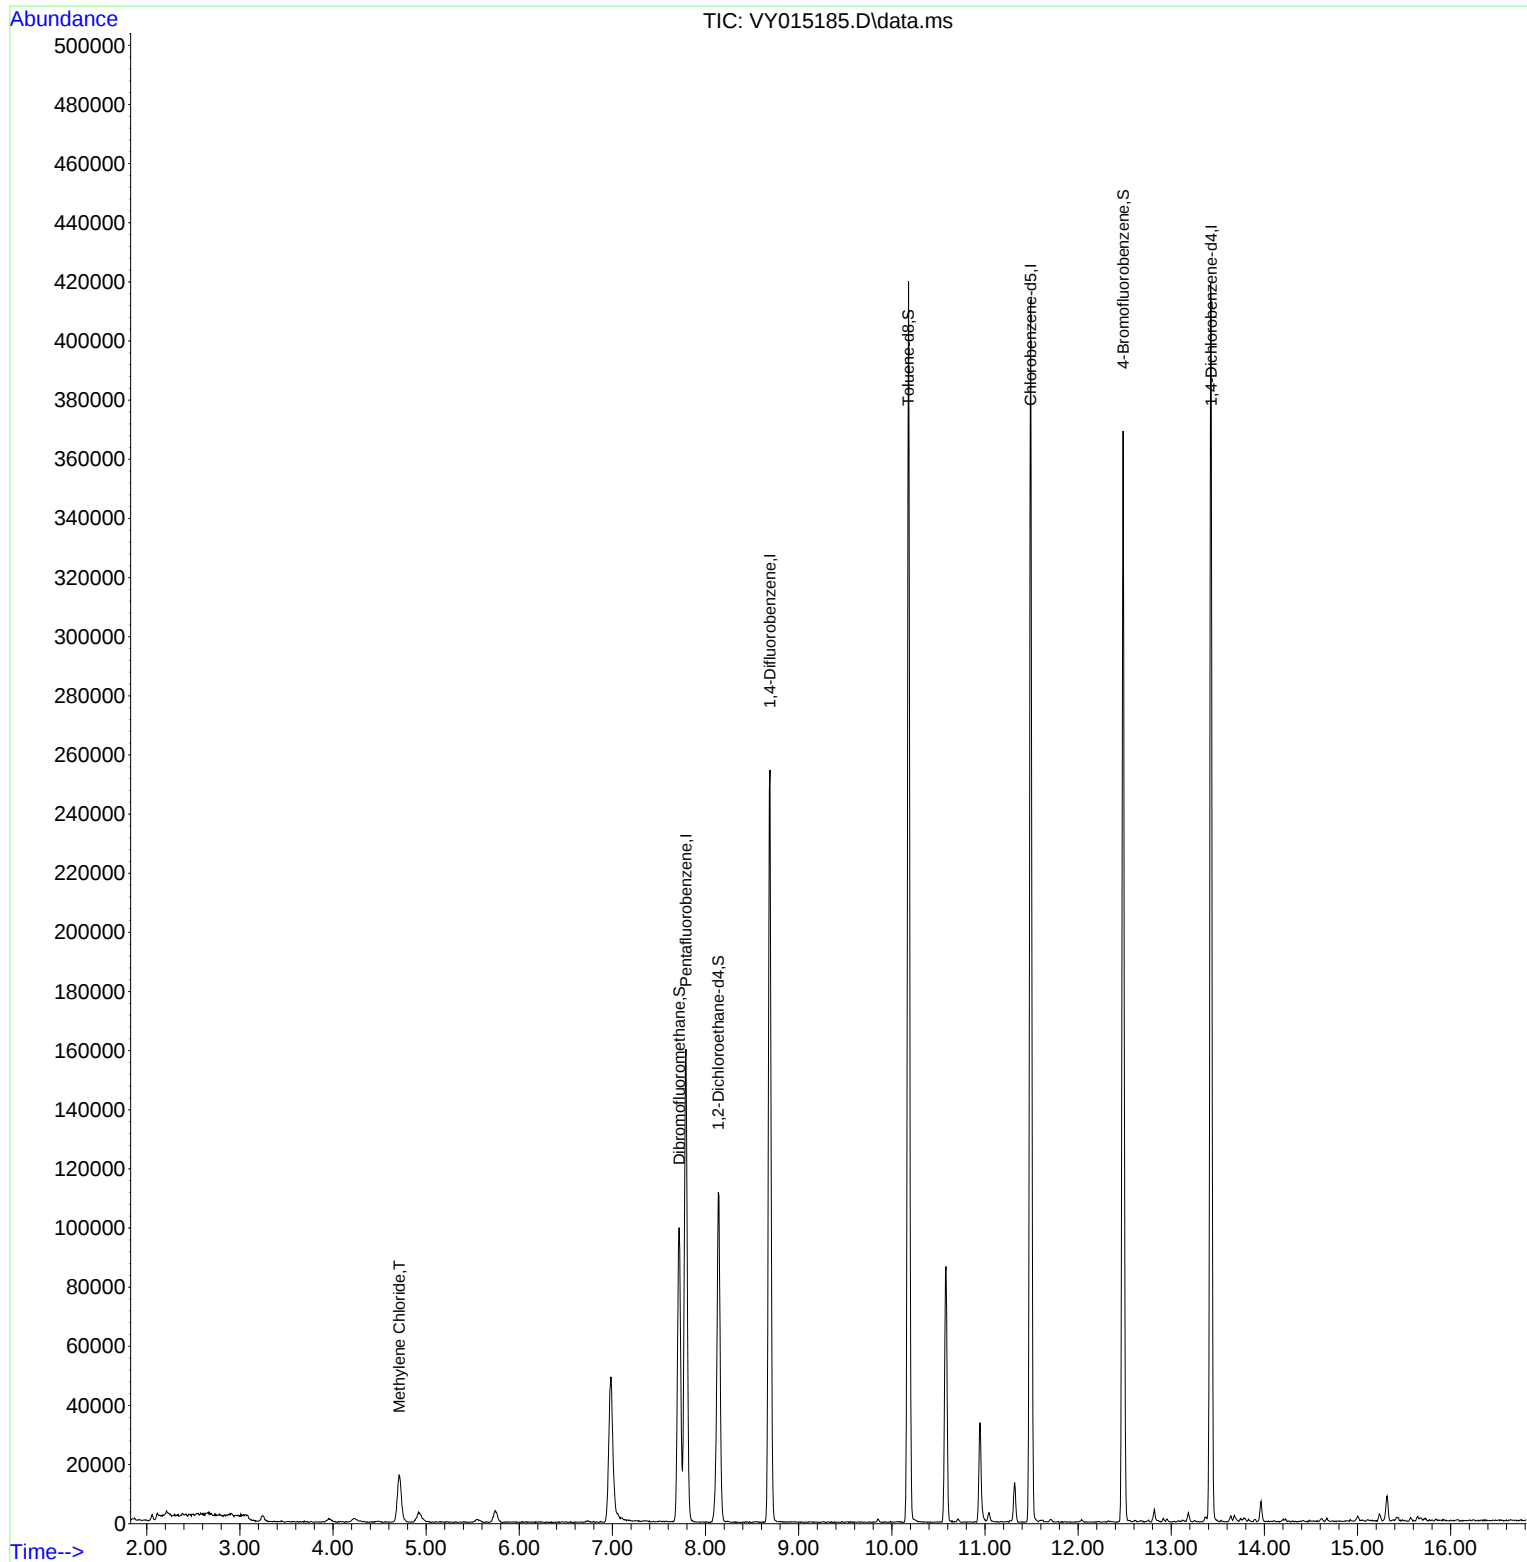


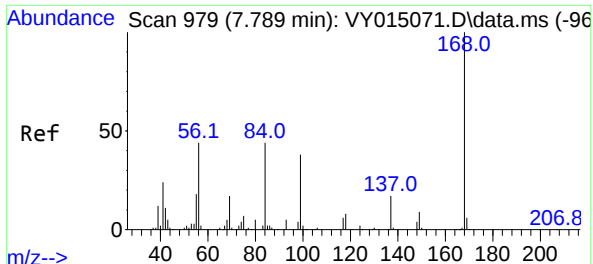

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.789 min Scan# 91
Delta R.T. 0.006 min
Lab File: VY015185.D
Acq: 18 Aug 2023 10:47




Instrument :
MSVOA_Y
ClientSampleId :
VY0818SBL01


Tgt Ion:168 Resp: 123071
Ion Ratio Lower Upper
168 100
99 51.7 43.4 65.0

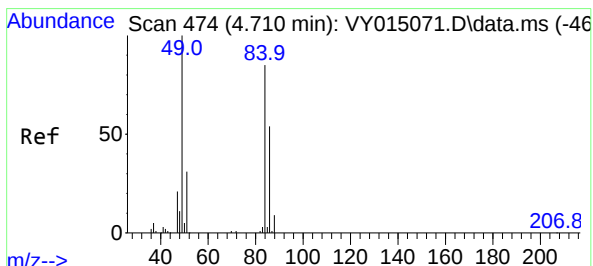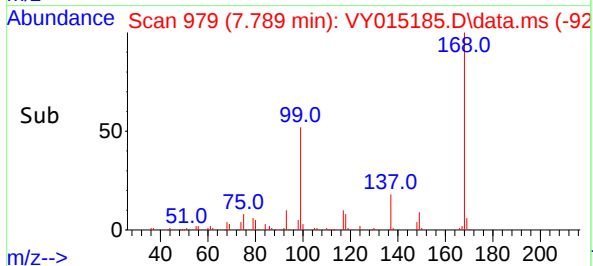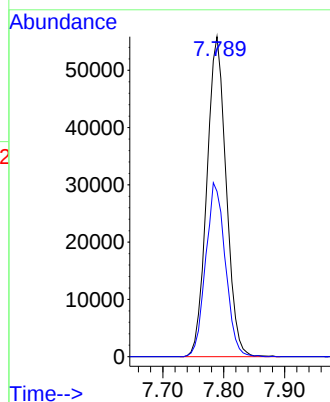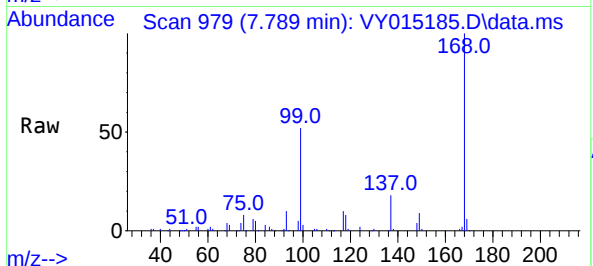

#20
Methylene Chloride
Concen: 6.629 ug/l
RT: 4.710 min Scan# 474
Delta R.T. 0.000 min
Lab File: VY015185.D
Acq: 18 Aug 2023 10:47

Tgt Ion: 84 Resp: 12007
Ion Ratio Lower Upper
84 100
49 110.2 106.9 160.3
51 35.6 33.2 49.8
86 58.4 51.0 76.6

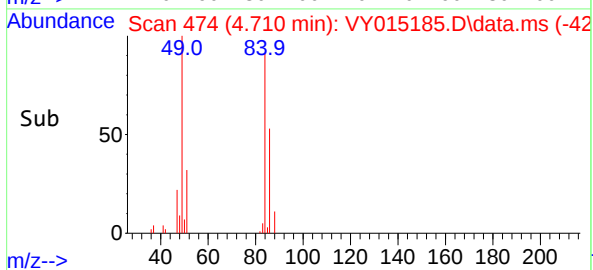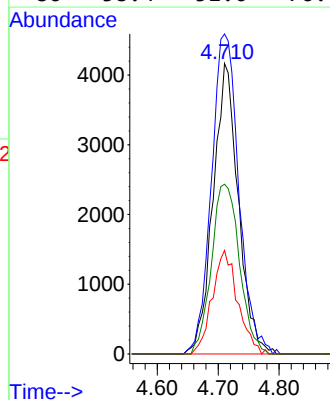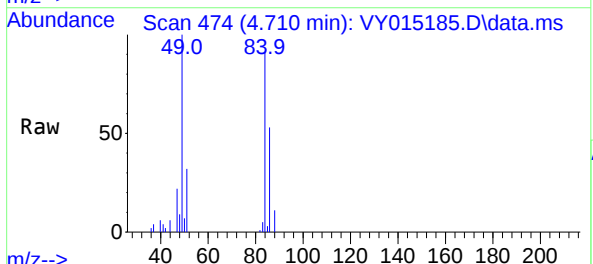

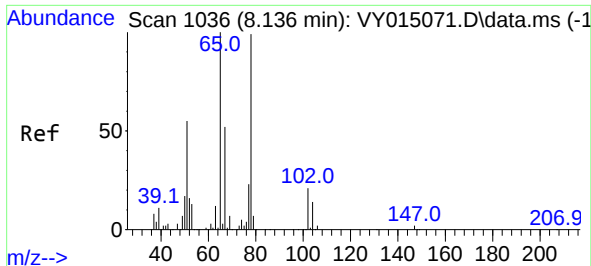

#33

1,2-Dichloroethane-d4

Concen: 56.003 ug/l

RT: 8.137 min Scan# 1036

Delta R.T. 0.000 min

Lab File: VY015185.D

Acq: 18 Aug 2023 10:47

Instrument :

MSVOA_Y

ClientSampleId :





VY0818SBL01

Tgt Ion: 65 Resp: 82736

Ion Ratio Lower Upper

65 100

67 52.9 0.0 101.8

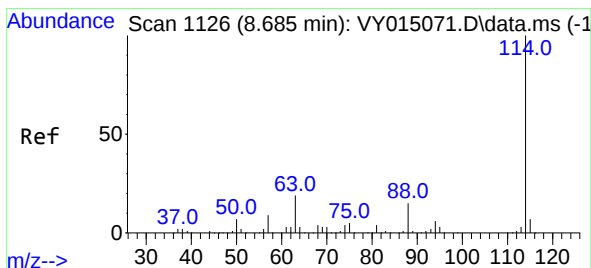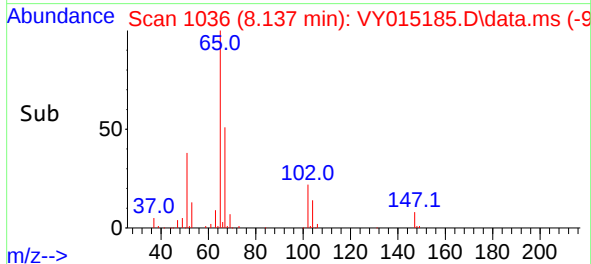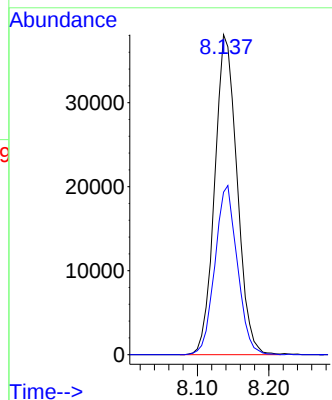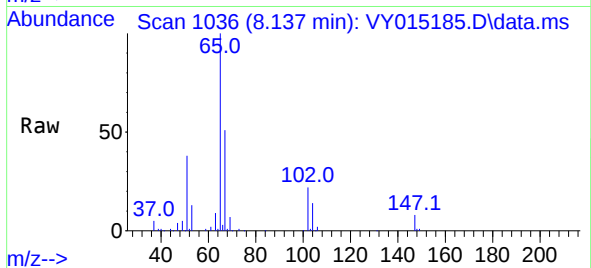

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.691 min Scan# 1127

Delta R.T. 0.006 min

Lab File: VY015185.D

Acq: 18 Aug 2023 10:47




Tgt Ion: 114 Resp: 218606

Ion Ratio Lower Upper

114 100

63 19.5 0.0 42.4

88 15.4 0.0 30.6


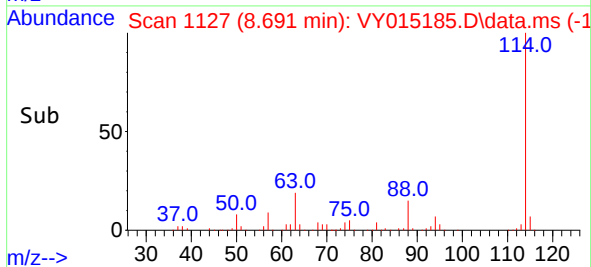
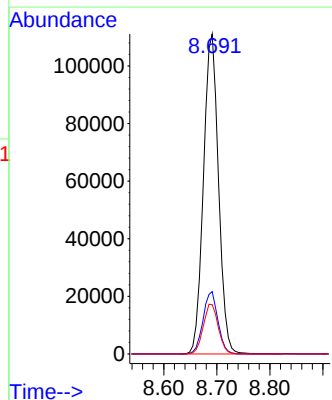
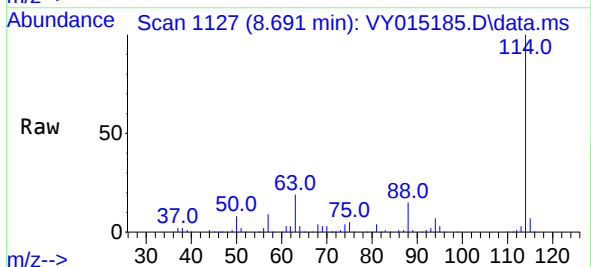




#35
Dibromofluoromethane
Concen: 50.081 ug/l
RT: 7.716 min Scan# 967
Delta R.T. 0.000 min
Lab File: VY015185.D
Acq: 18 Aug 2023 10:47




Instrument :
MSVOA_Y
ClientSampleId :
VY0818SBL01

Tgt Ion:113 Resp: 70432
Ion Ratio Lower Upper
113 100
111 102.6 81.3 121.9
192 19.4 16.9 25.3

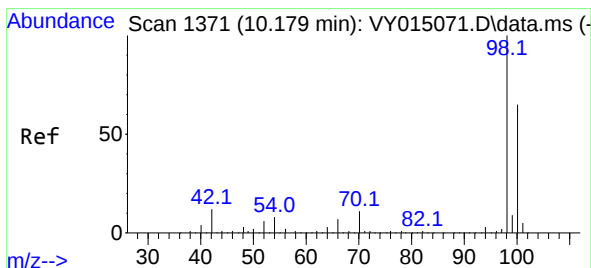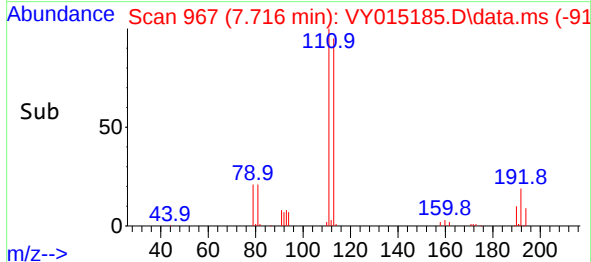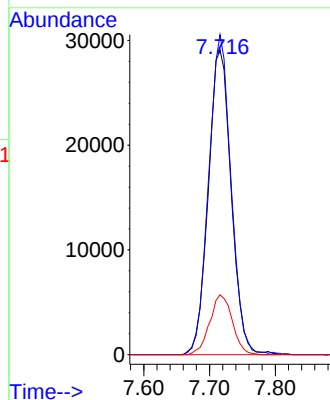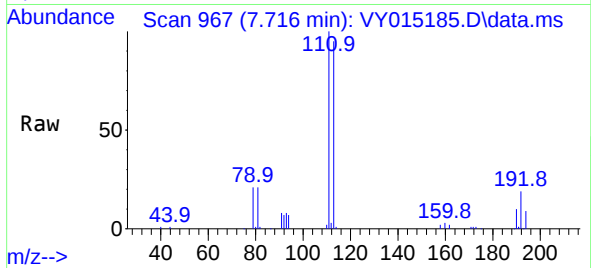

#50
Toluene-d8
Concen: 50.563 ug/l
RT: 10.179 min Scan# 1371
Delta R.T. 0.000 min
Lab File: VY015185.D
Acq: 18 Aug 2023 10:47

Tgt Ion: 98 Resp: 264714
Ion Ratio Lower Upper
98 100
100 65.1 50.1 75.1


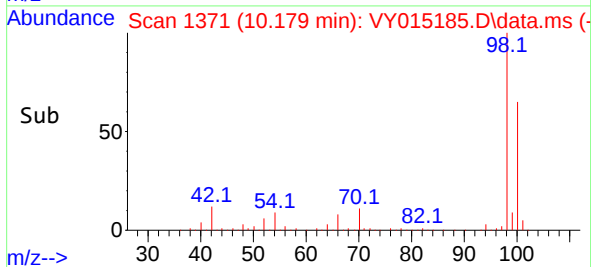
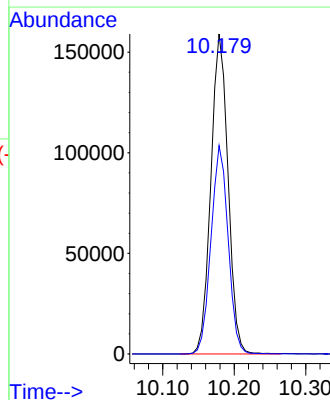
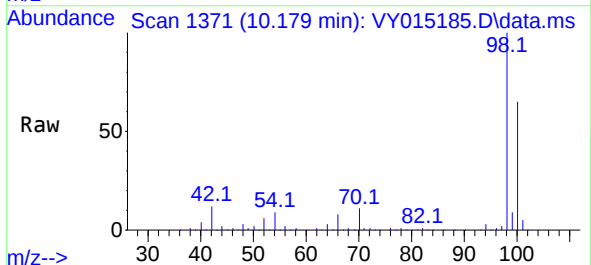




#62
4-Bromofluorobenzene
Concen: 51.261 ug/l
RT: 12.483 min Scan# 1749
Delta R.T. 0.006 min
Lab File: VY015185.D
Acq: 18 Aug 2023 10:47




Instrument :
MSVOA_Y
ClientSampleId :
VY0818SBL01


Tgt Ion: 95 Resp: 98021
Ion Ratio Lower Upper
95 100
174 85.1 0.0 178.2
176 81.8 0.0 173.8

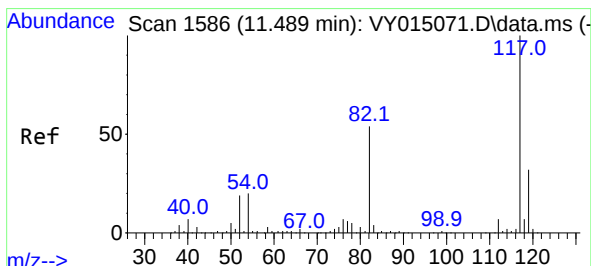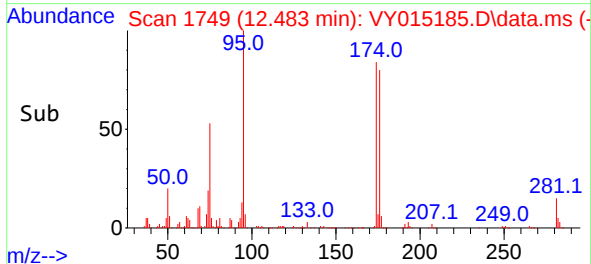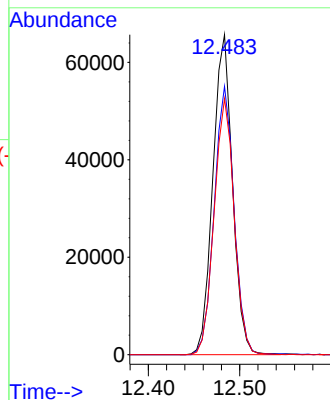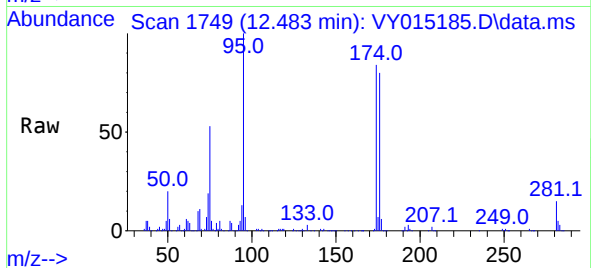

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.490 min Scan# 1586
Delta R.T. 0.000 min
Lab File: VY015185.D
Acq: 18 Aug 2023 10:47

Tgt Ion: 117 Resp: 219380
Ion Ratio Lower Upper
117 100
82 53.3 43.4 65.0
119 31.6 26.3 39.5

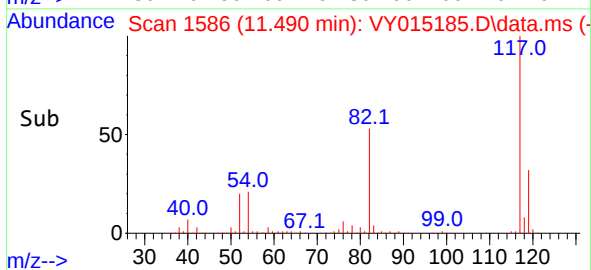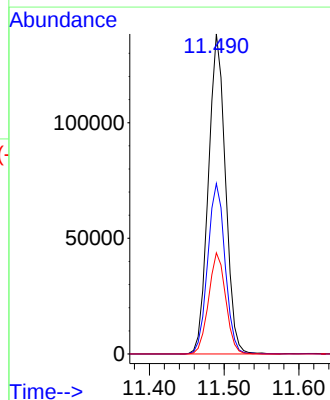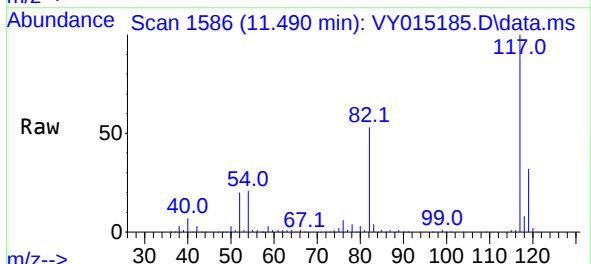

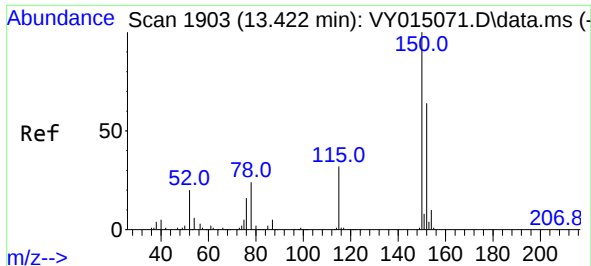

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.428 min Scan# 1904
Delta R.T. 0.006 min
Lab File: VY015185.D
Acq: 18 Aug 2023 10:47

Instrument :
MSVOA_Y
ClientSampleId :
VY0818SBL01

Tgt Ion:152 Resp: 107538
Ion Ratio Lower Upper
152 100
115 58.9 28.8 86.5
150 159.1 0.0 348.8

