

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY081922\
 Data File : VY010102.D
 Acq On : 19 Aug 2022 14:40
 Operator : KP/MD
 Sample : VY0819SBL01
 Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 VY0819SBL01

Quant Time: Aug 22 02:39:38 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y081922S.M
 Quant Title : SW846 8260
 QLast Update : Mon Aug 22 02:37:07 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.783	168	255424	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.685	114	424535	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.489	117	372378	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.422	152	174198	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.130	65	110578	52.853	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	105.700%
35) Dibromofluoromethane	7.710	113	122001	51.000	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	102.000%
50) Toluene-d8	10.172	98	421942	47.072	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	=	94.140%
62) 4-Bromofluorobenzene	12.477	95	144628	45.159	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	=	90.320%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY081922\
Data File : VY010102.D
Acq On : 19 Aug 2022 14:40
Operator : KP/MD
Sample : VY0819SBL01
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
VY0819SBL01

Quant Time: Aug 22 02:39:38 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y081922S.M
Quant Title : SW846 8260
QLast Update : Mon Aug 22 02:37:07 2022
Response via : Initial Calibration




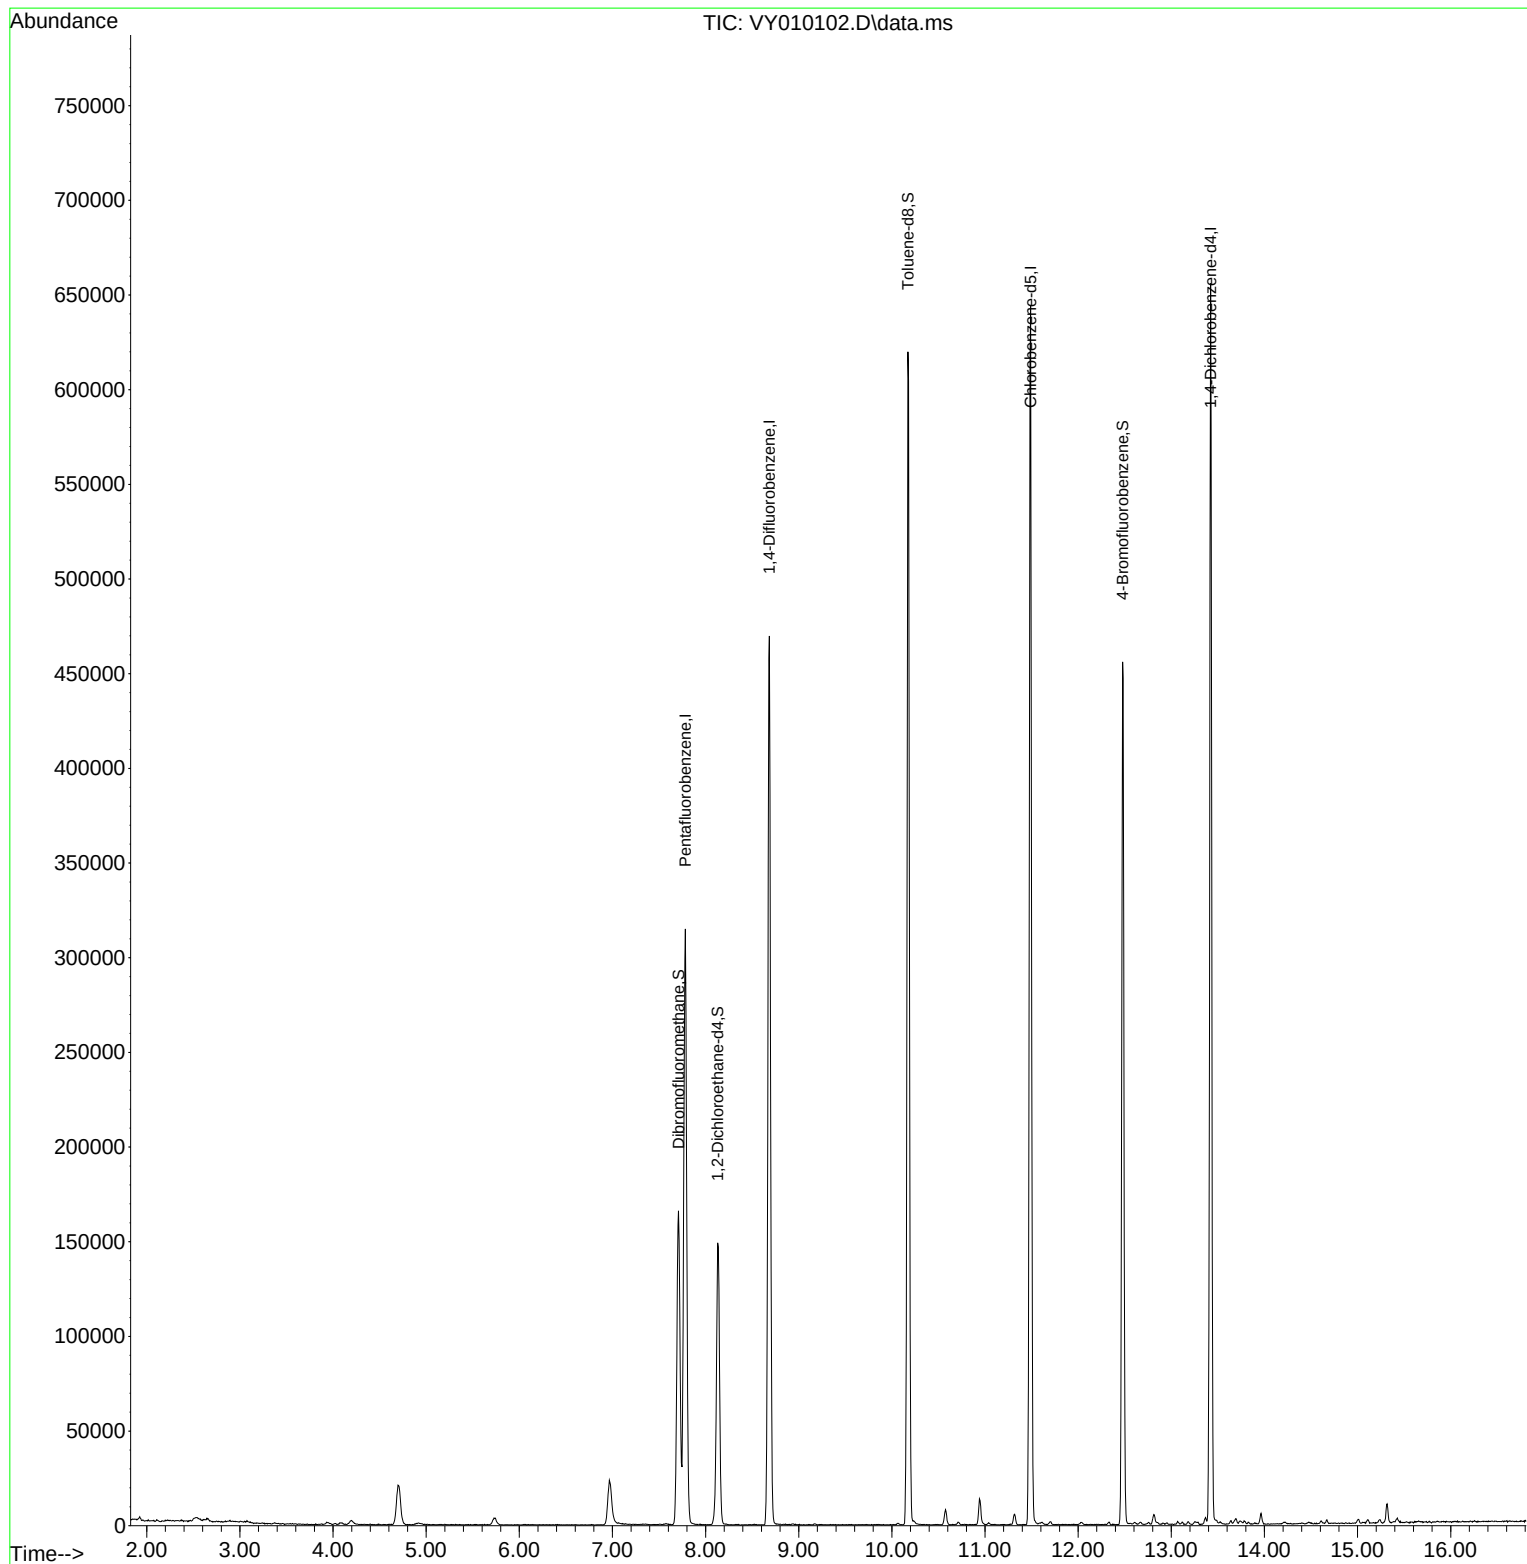


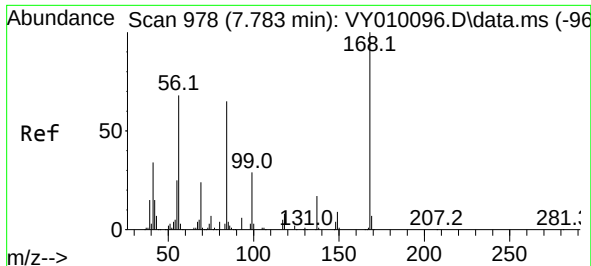

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.783 min Scan# 91
Delta R.T. -0.000 min
Lab File: VY010102.D
Acq: 19 Aug 2022 14:40




Instrument :
MSVOA_Y
ClientSampleId :
VY0819SBL01


Tgt Ion:168 Resp: 255424
Ion Ratio Lower Upper
168 100
99 48.1 40.7 61.1

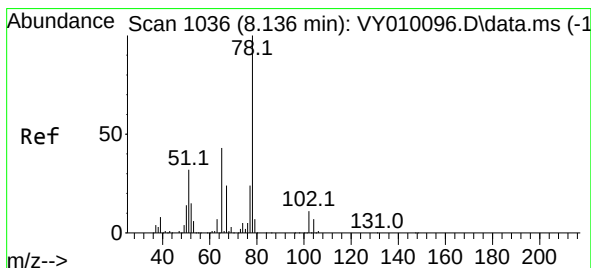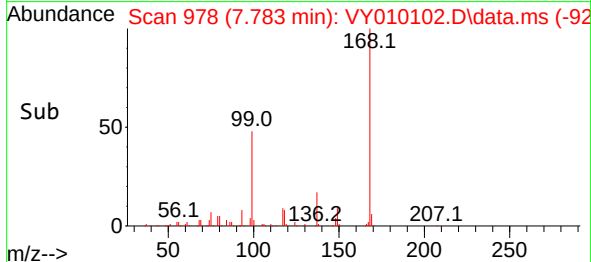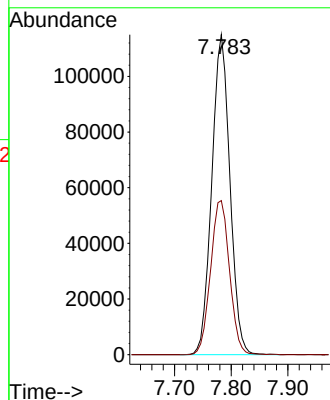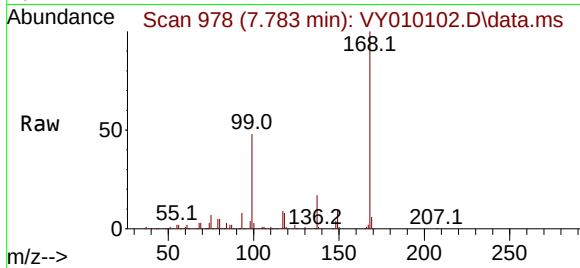

#33
1,2-Dichloroethane-d4
Concen: 52.853 ug/l
RT: 8.130 min Scan# 1035
Delta R.T. -0.006 min
Lab File: VY010102.D
Acq: 19 Aug 2022 14:40

Tgt Ion: 65 Resp: 110578
Ion Ratio Lower Upper
65 100
67 55.0 0.0 110.6

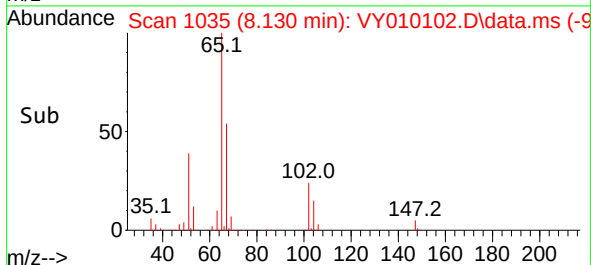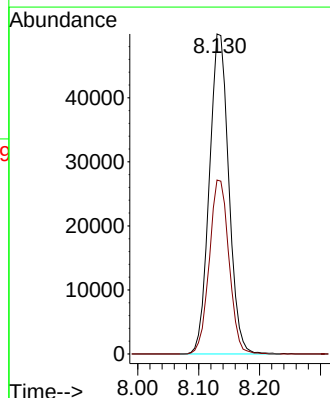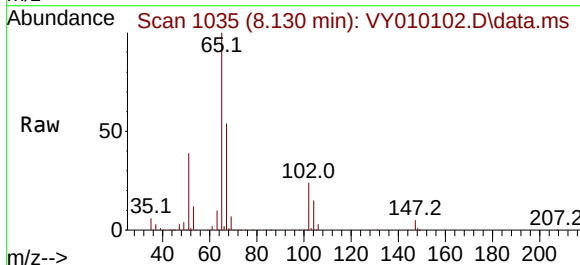

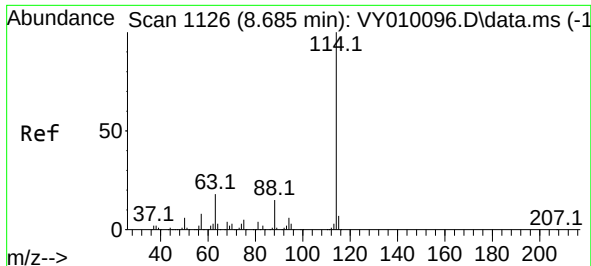

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.685 min Scan# 1126

Delta R.T. -0.000 min

Lab File: VY010102.D

Acq: 19 Aug 2022 14:40

Instrument :

MSVOA_Y

ClientSampleId :

VY0819SBL01





Tgt Ion:114 Resp: 424535

Ion Ratio Lower Upper

114 100

63 17.9 0.0 35.6

88 14.7 0.0 29.6

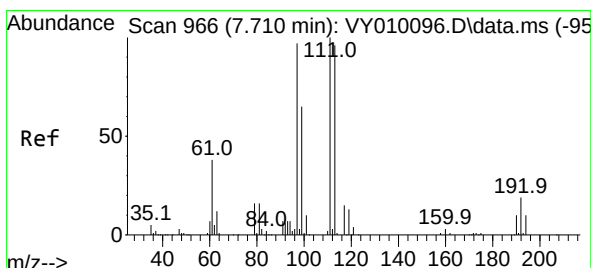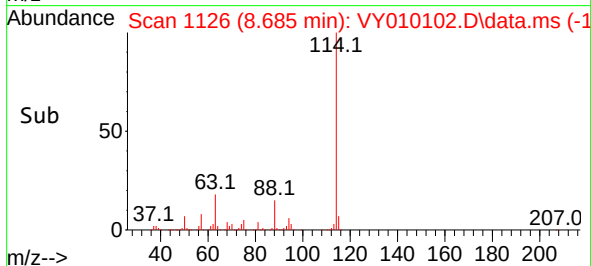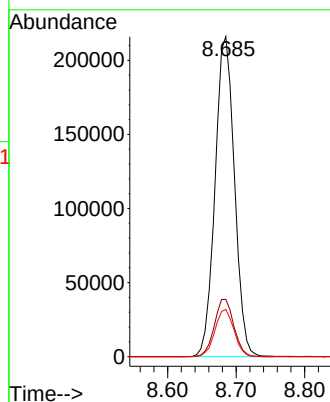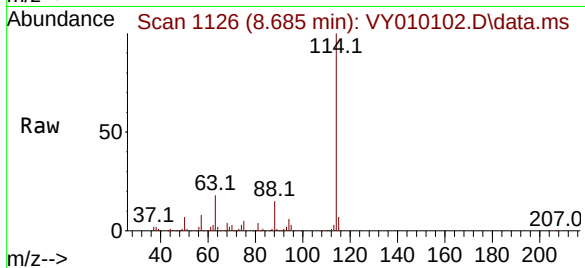

#35

Dibromofluoromethane

Concen: 51.000 ug/l

RT: 7.710 min Scan# 966

Delta R.T. -0.000 min

Lab File: VY010102.D

Acq: 19 Aug 2022 14:40




Tgt Ion:113 Resp: 122001


Ion Ratio Lower Upper

113 100

111 103.7 82.8 124.2

192 20.4 16.3 24.5


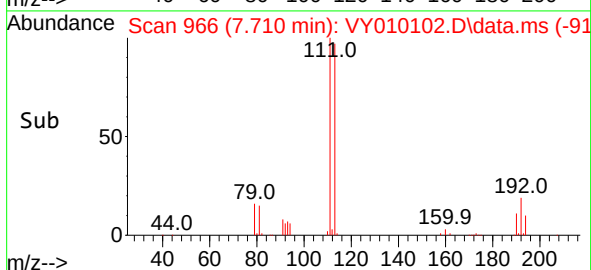
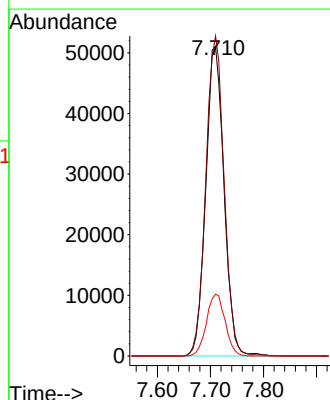
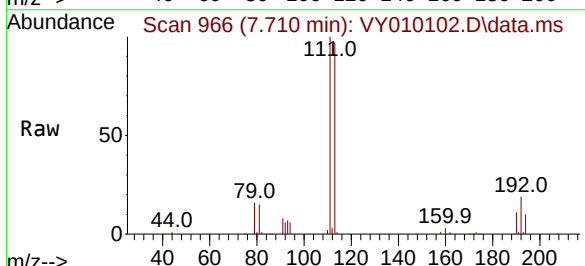


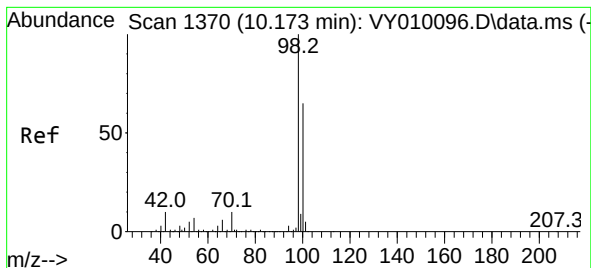

#50
Toluene-d8
Concen: 47.072 ug/l
RT: 10.172 min Scan# 1370
Delta R.T. -0.001 min
Lab File: VY010102.D
Acq: 19 Aug 2022 14:40




Instrument :
MSVOA_Y
ClientSampleId :
VY0819SBL01


Tgt Ion: 98 Resp: 421942
Ion Ratio Lower Upper
98 100
100 64.7 51.9 77.9

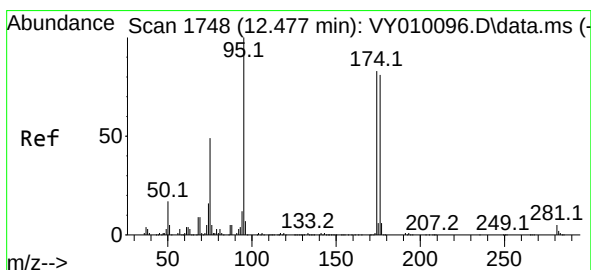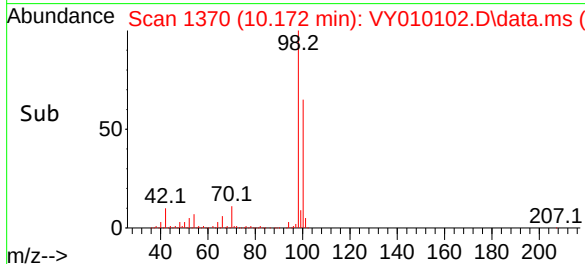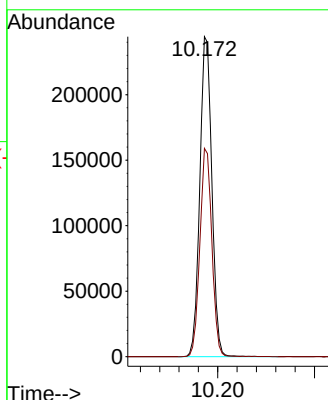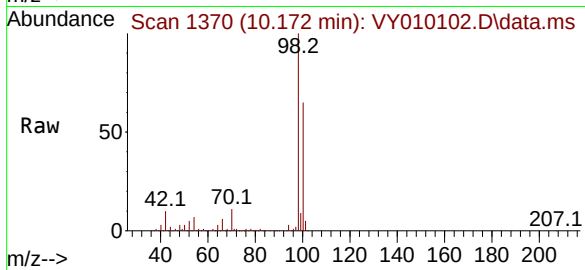

#62
4-Bromofluorobenzene
Concen: 45.159 ug/l
RT: 12.477 min Scan# 1748
Delta R.T. -0.000 min
Lab File: VY010102.D
Acq: 19 Aug 2022 14:40

Tgt Ion: 95 Resp: 144628
Ion Ratio Lower Upper
95 100
174 88.1 0.0 173.8
176 84.1 0.0 167.2


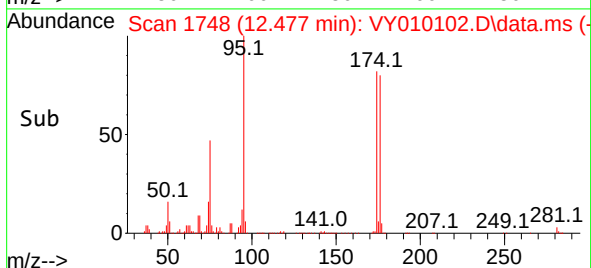
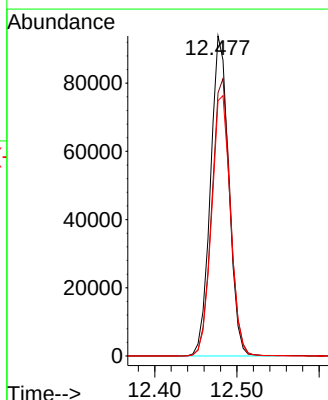
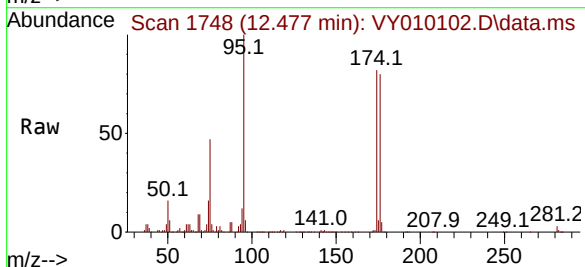


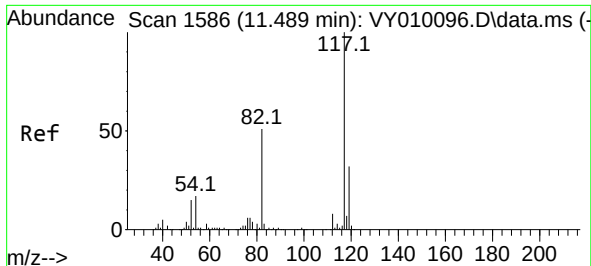

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.489 min Scan# 117
Delta R.T. -0.000 min
Lab File: VY010102.D
Acq: 19 Aug 2022 14:40

Instrument :
MSVOA_Y
ClientSampleId :
VY0819SBL01

Tgt Ion:117 Resp: 372378
Ion Ratio Lower Upper
117 100
82 50.8 40.6 61.0
119 32.6 25.8 38.8

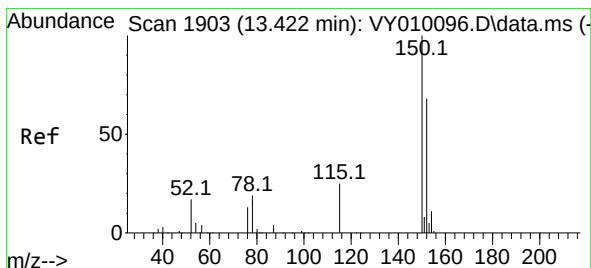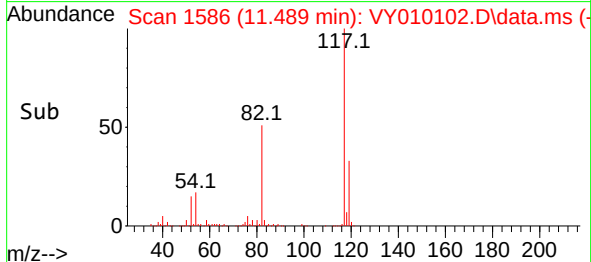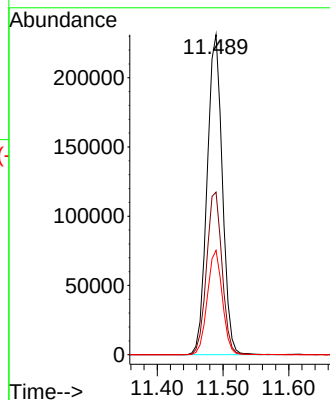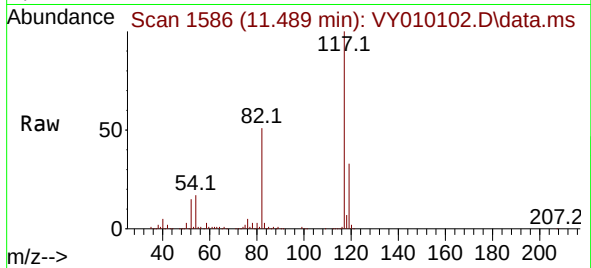

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.422 min Scan# 1903
Delta R.T. -0.000 min
Lab File: VY010102.D
Acq: 19 Aug 2022 14:40

Tgt Ion:152 Resp: 174198
Ion Ratio Lower Upper
152 100
115 55.8 28.1 84.2
150 157.7 0.0 346.2

