

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY081922\
 Data File : VY010123.D
 Acq On : 20 Aug 2022 00:05
 Operator : KP/MD
 Sample : N4219-01
 Misc : 5.34g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 PX-1

Quant Time: Aug 22 02:49:46 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y081922S.M
 Quant Title : SW846 8260
 QLast Update : Mon Aug 22 02:37:07 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.783	168	166255	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.685	114	319190	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.489	117	318698	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.422	152	155878	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.136	65	90859	66.721	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	133.440%
35) Dibromofluoromethane	7.710	113	89266	49.631	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	99.260%
50) Toluene-d8	10.179	98	330083	48.978	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	=	97.960%
62) 4-Bromofluorobenzene	12.477	95	115523	47.976	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	=	95.960%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY081922\
Data File : VY010123.D
Acq On : 20 Aug 2022 00:05
Operator : KP/MD
Sample : N4219-01
Misc : 5.34g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
PX-1

Quant Time: Aug 22 02:49:46 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y081922S.M
Quant Title : SW846 8260
QLast Update : Mon Aug 22 02:37:07 2022
Response via : Initial Calibration




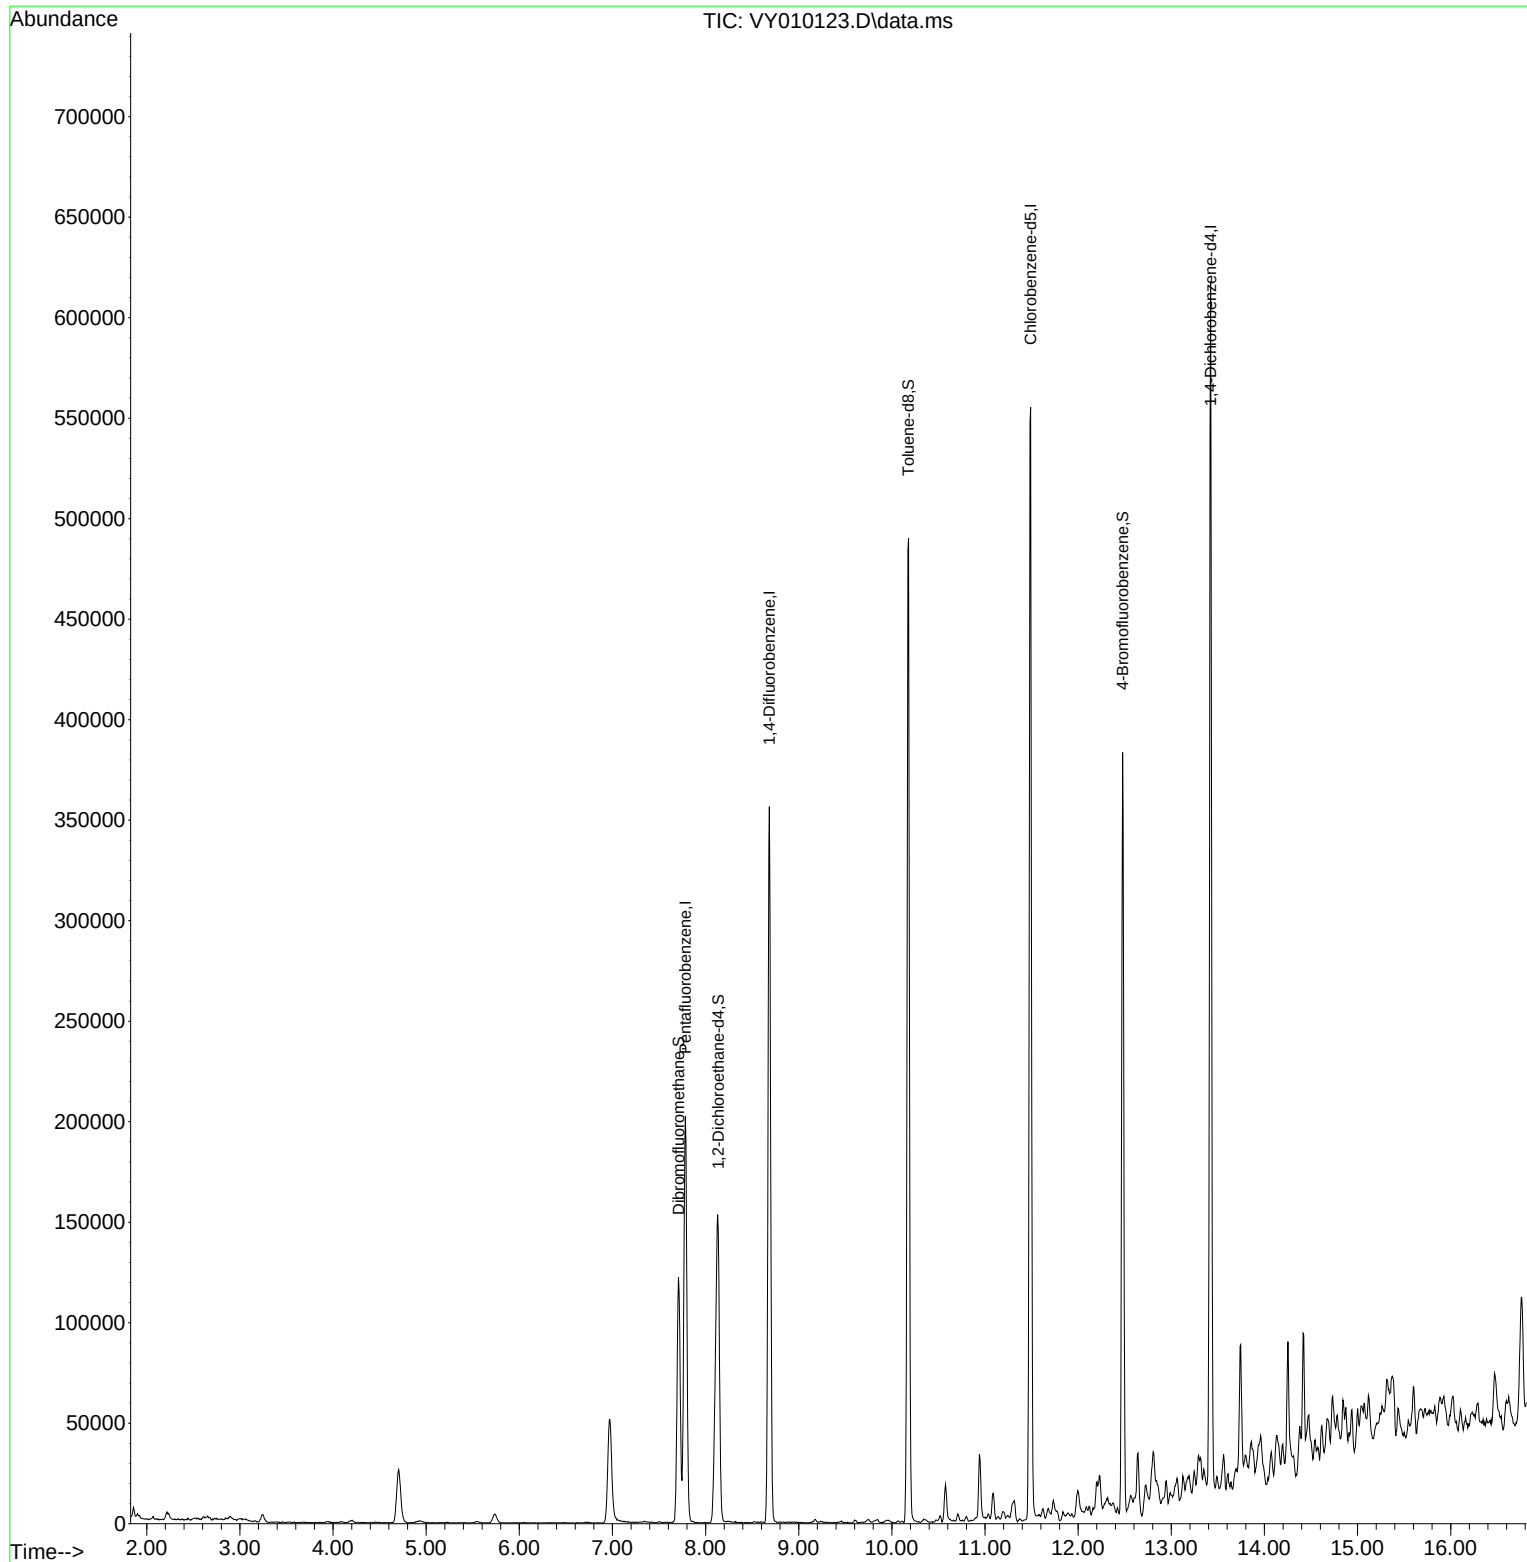


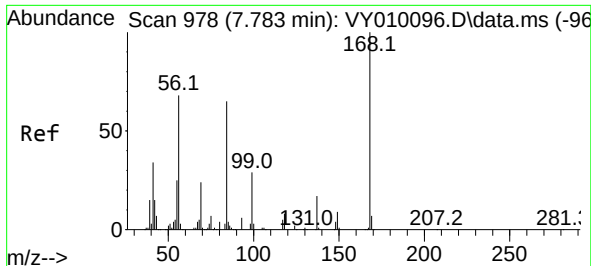

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.783 min Scan# 91
Delta R.T. -0.000 min
Lab File: VY010123.D
Acq: 20 Aug 2022 00:05




Instrument :
MSVOA_Y
ClientSampleId :
PX-1


Tgt Ion:168 Resp: 166255
Ion Ratio Lower Upper
168 100
99 51.0 40.7 61.1

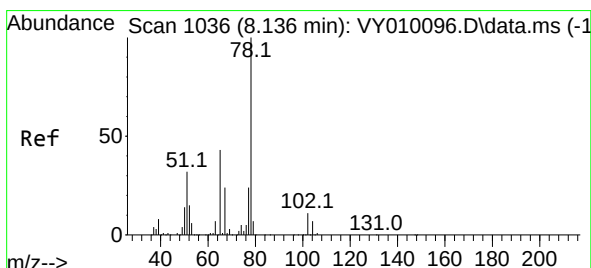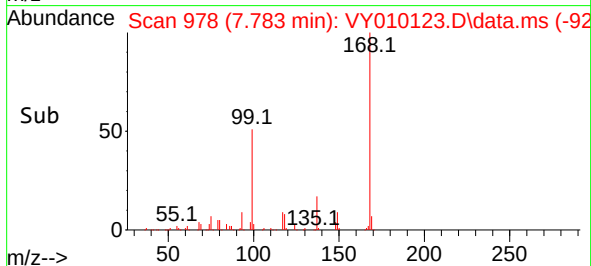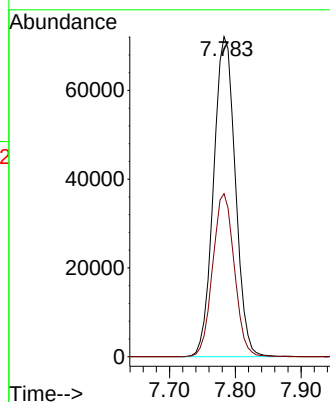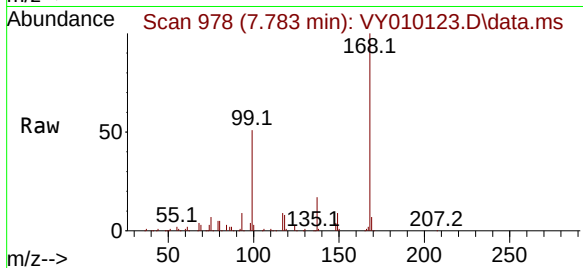

#33
1,2-Dichloroethane-d4
Concen: 66.721 ug/l
RT: 8.136 min Scan# 1036
Delta R.T. 0.000 min
Lab File: VY010123.D
Acq: 20 Aug 2022 00:05

Tgt Ion: 65 Resp: 90859
Ion Ratio Lower Upper
65 100
67 55.9 0.0 110.6


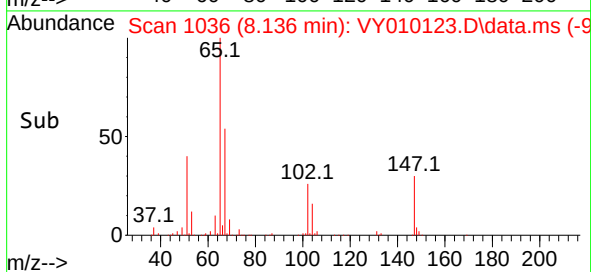
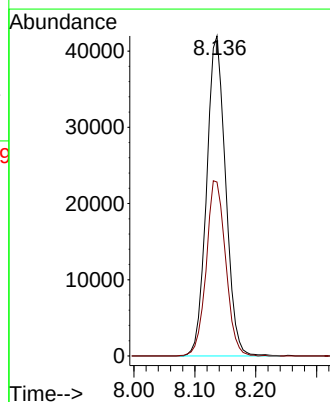
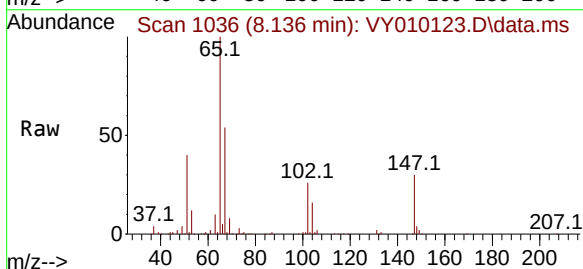


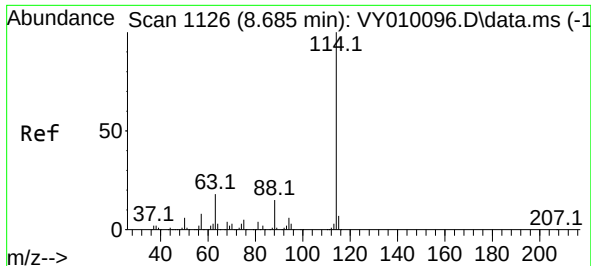

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.685 min Scan# 1126
Delta R.T. 0.000 min
Lab File: VY010123.D
Acq: 20 Aug 2022 00:05




Instrument :
MSVOA_Y
ClientSampleId :
PX-1


Tgt Ion:114 Resp: 319190
Ion Ratio Lower Upper
114 100
63 17.7 0.0 35.6
88 14.5 0.0 29.6

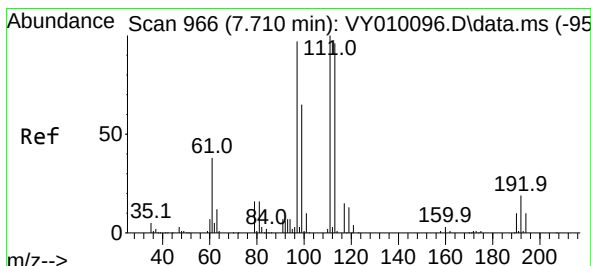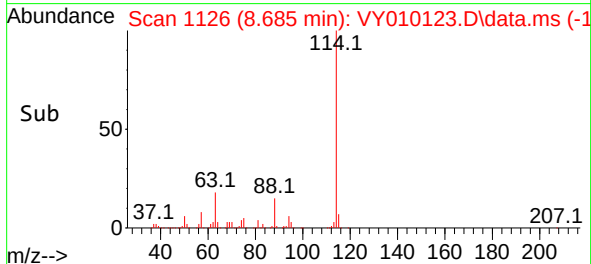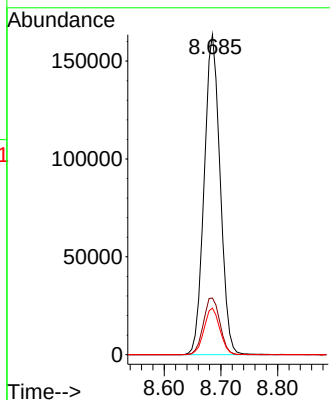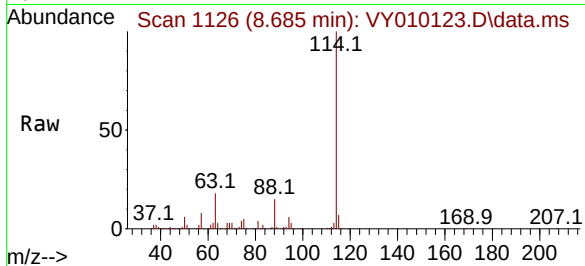

#35
Dibromofluoromethane
Concen: 49.631 ug/l
RT: 7.710 min Scan# 966
Delta R.T. -0.000 min
Lab File: VY010123.D
Acq: 20 Aug 2022 00:05

Tgt Ion:113 Resp: 89266
Ion Ratio Lower Upper
113 100
111 101.9 82.8 124.2
192 20.0 16.3 24.5


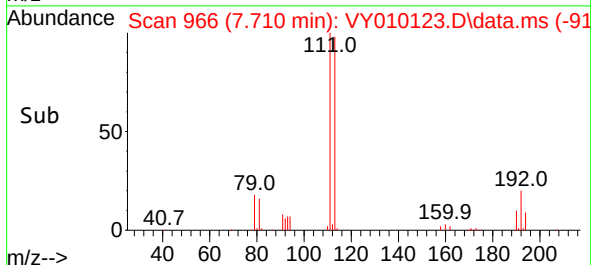
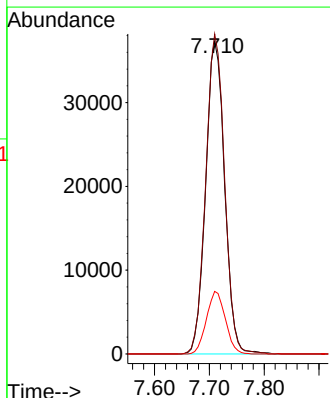
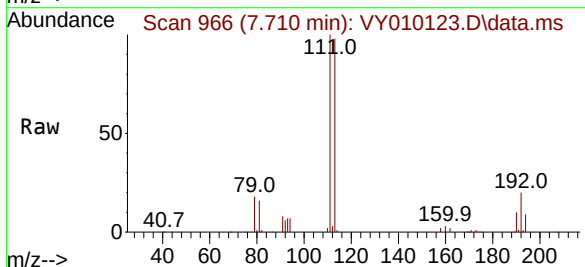


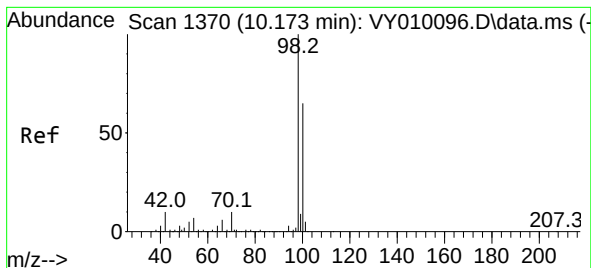

#50
Toluene-d8
Concen: 48.978 ug/l
RT: 10.179 min Scan# 11
Delta R.T. 0.006 min
Lab File: VY010123.D
Acq: 20 Aug 2022 00:05




Instrument :
MSVOA_Y
ClientSampleId :
PX-1


Tgt Ion: 98 Resp: 330083
Ion Ratio Lower Upper
98 100
100 64.2 51.9 77.9

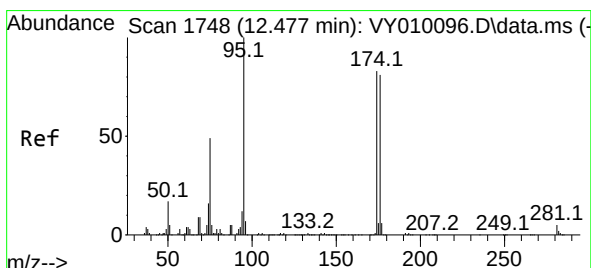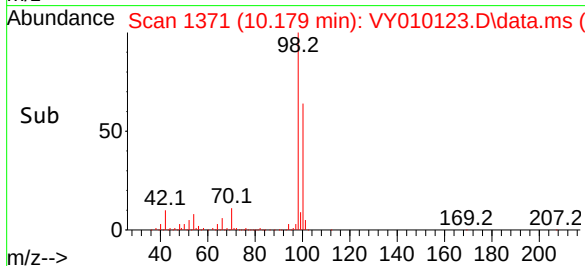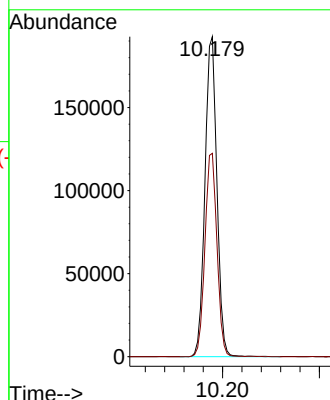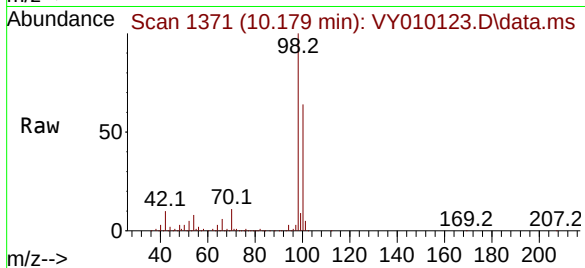

#62
4-Bromofluorobenzene
Concen: 47.976 ug/l
RT: 12.477 min Scan# 1748
Delta R.T. 0.000 min
Lab File: VY010123.D
Acq: 20 Aug 2022 00:05

Tgt Ion: 95 Resp: 115523
Ion Ratio Lower Upper
95 100
174 87.7 0.0 173.8
176 83.8 0.0 167.2


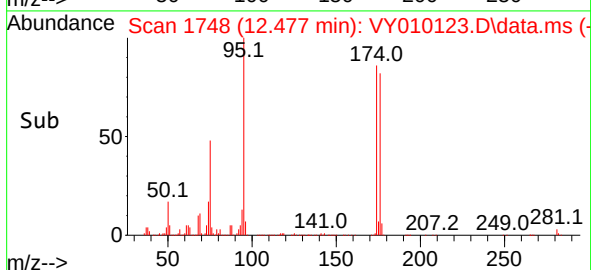
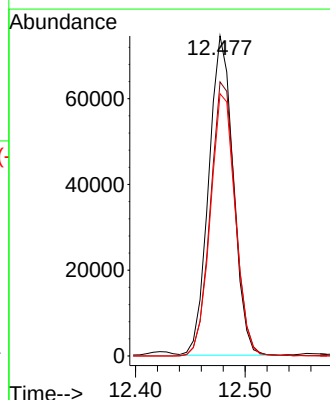
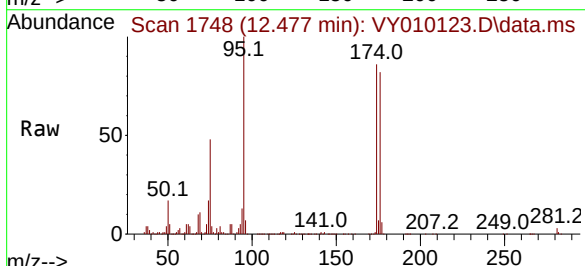


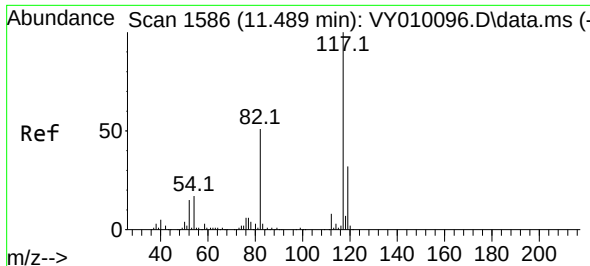

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.489 min Scan# 117
Delta R.T. 0.000 min
Lab File: VY010123.D
Acq: 20 Aug 2022 00:05

Instrument :
MSVOA_Y
ClientSampleId :
PX-1

Tgt Ion:117 Resp: 318698
Ion Ratio Lower Upper
117 100
82 51.1 40.6 61.0
119 31.6 25.8 38.8

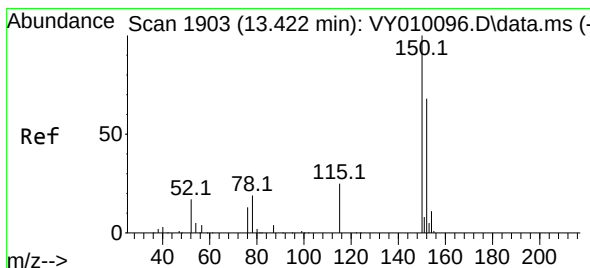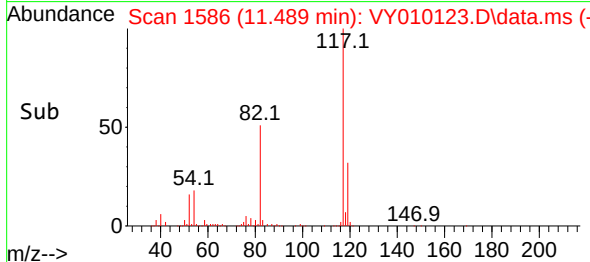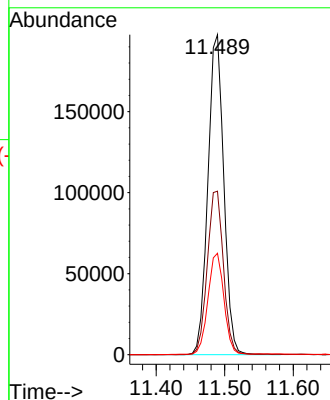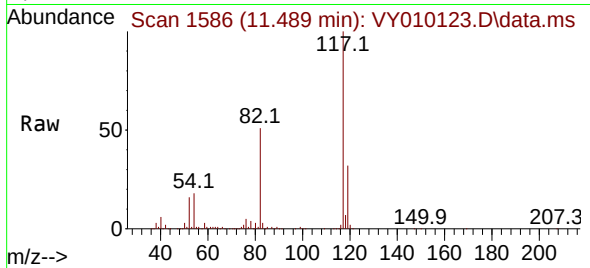

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.422 min Scan# 1903
Delta R.T. 0.000 min
Lab File: VY010123.D
Acq: 20 Aug 2022 00:05

Tgt Ion:152 Resp: 155878
Ion Ratio Lower Upper
152 100
115 56.9 28.1 84.2
150 158.7 0.0 346.2

