

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY082021\
 Data File : VY005801.D
 Acq On : 20 Aug 2021 18:24
 Operator : SY/MD
 Sample : M3451-04
 Misc : 4.26G/5ML/MSVOA_Y/SOIL
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 TP-5-10-COMP

Quant Time: Aug 23 01:09:58 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y080221S.M
 Quant Title : SW846 8260
 QLast Update : Tue Aug 03 04:52:05 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.801	168	184352	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.697	114	315695	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.496	117	327621	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.428	152	159203	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.149	65	121519	65.119	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	130.240%
35) Dibromofluoromethane	7.728	113	97387	55.099	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	110.200%
50) Toluene-d8	10.185	98	408021	55.043	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	=	110.080%
62) 4-Bromofluorobenzene	12.483	95	139824	56.961	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	=	113.920%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY082021\
Data File : VY005801.D
Acq On : 20 Aug 2021 18:24
Operator : SY/MD
Sample : M3451-04
Misc : 4.26G/5ML/MSVOA_Y/SOIL
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
TP-5-10-COMP

Quant Time: Aug 23 01:09:58 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y080221S.M
Quant Title : SW846 8260
QLast Update : Tue Aug 03 04:52:05 2021
Response via : Initial Calibration




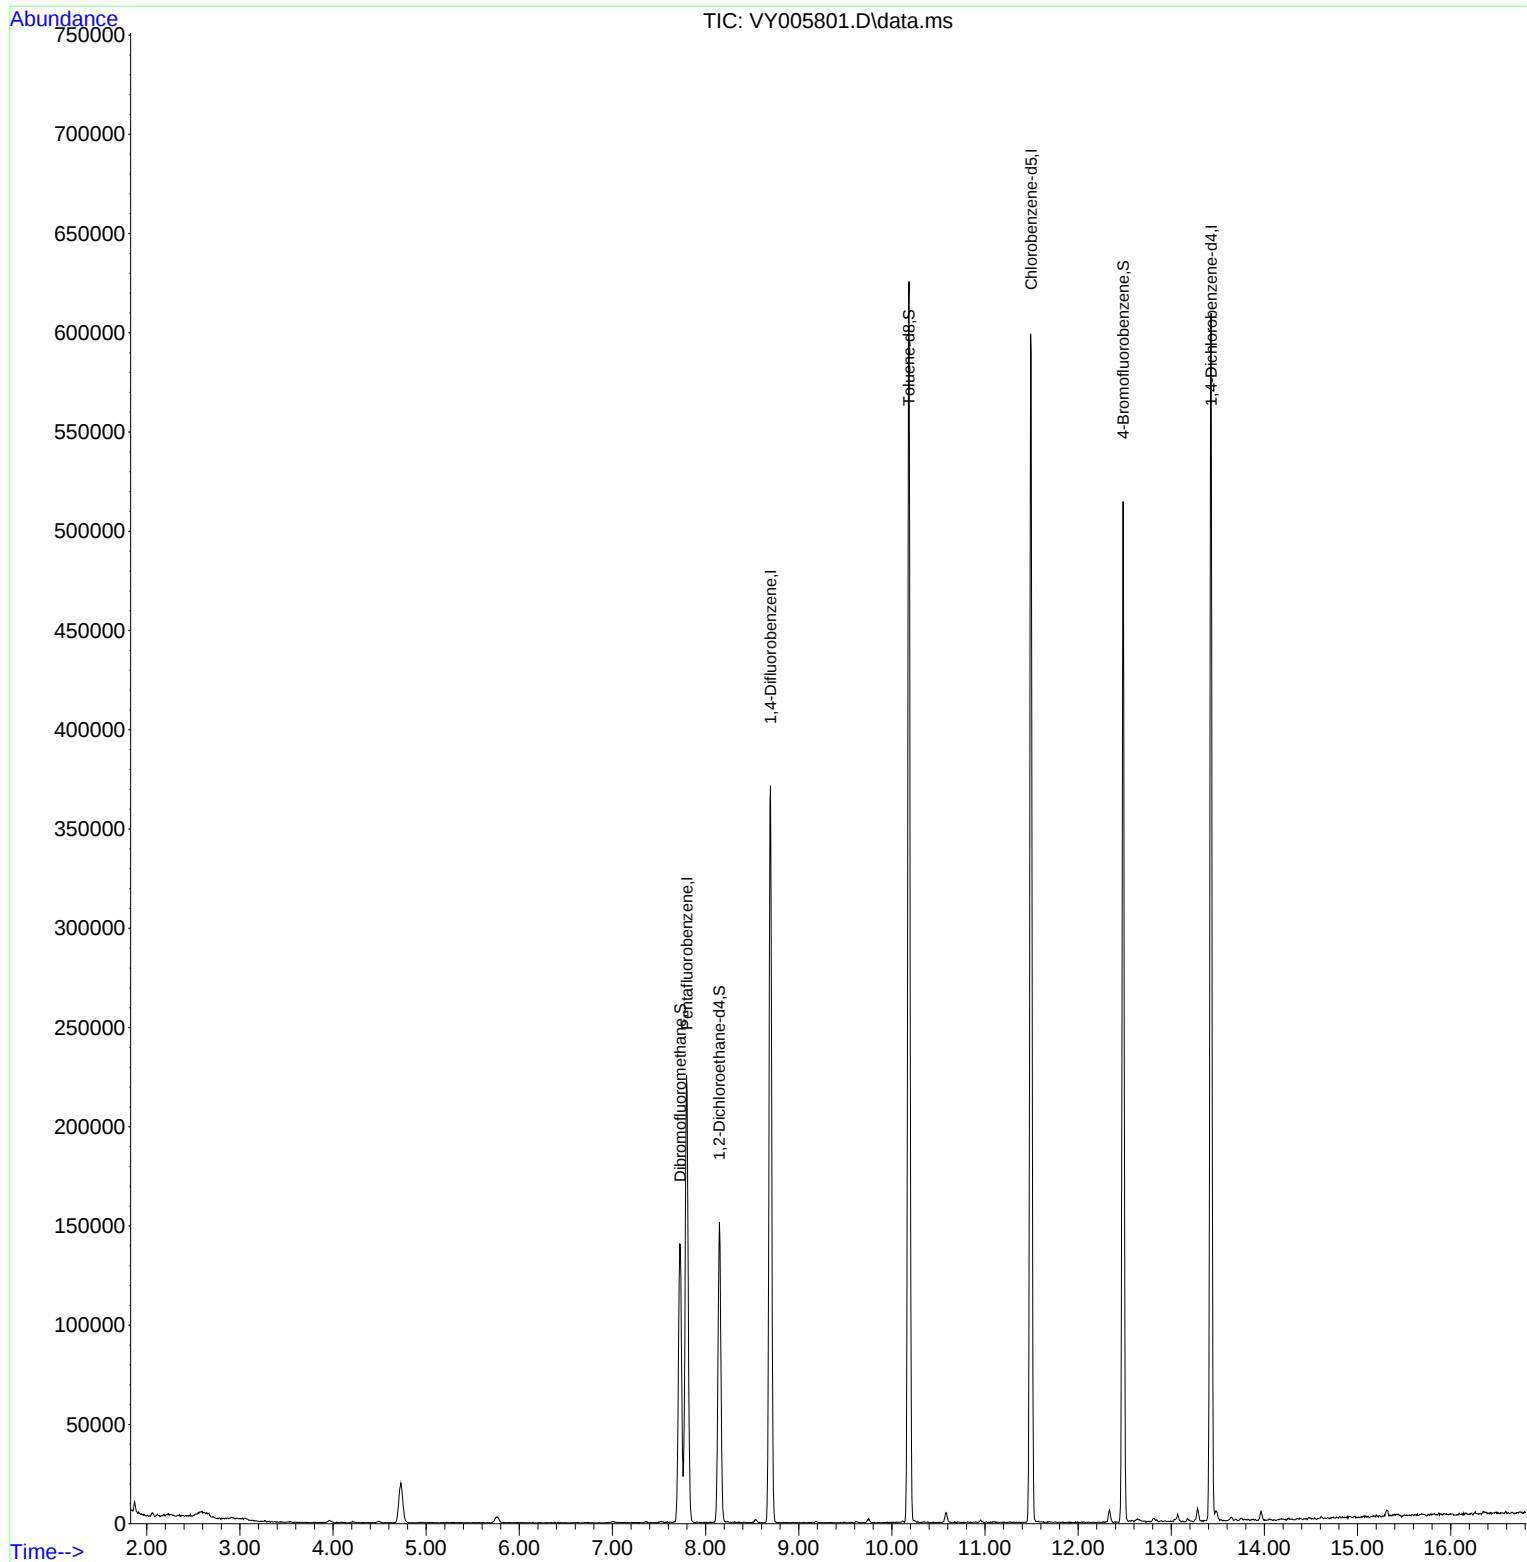


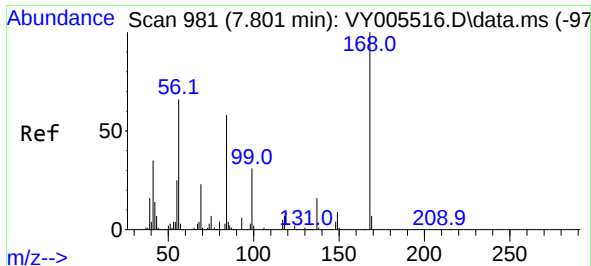

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.801 min Scan# 981
Delta R.T. 0.000 min
Lab File: VY005801.D
Acq: 20 Aug 2021 18:24




Instrument :
MSVOA_Y
ClientSampleId :
TP-5-10-COMP


Tgt Ion:168 Resp: 184352
Ion Ratio Lower Upper
168 100
99 49.5 38.9 58.3

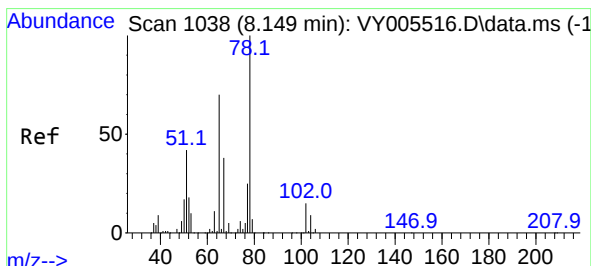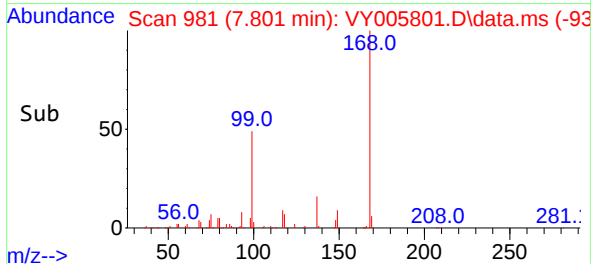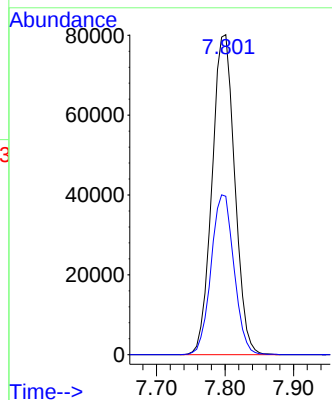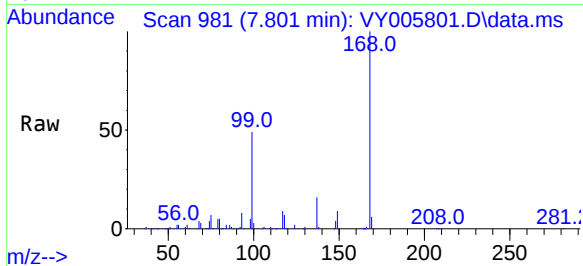

#33
1,2-Dichloroethane-d4
Concen: 65.119 ug/l
RT: 8.149 min Scan# 1038
Delta R.T. -0.000 min
Lab File: VY005801.D
Acq: 20 Aug 2021 18:24

Tgt Ion: 65 Resp: 121519
Ion Ratio Lower Upper
65 100
67 50.4 0.0 103.4


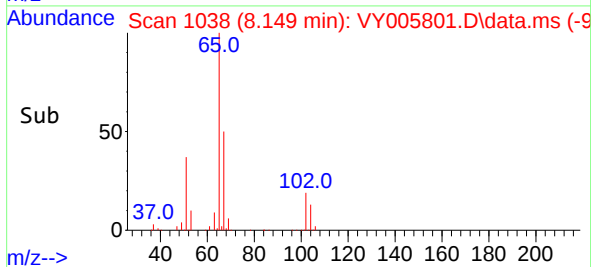
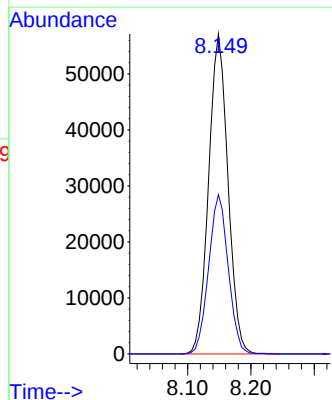
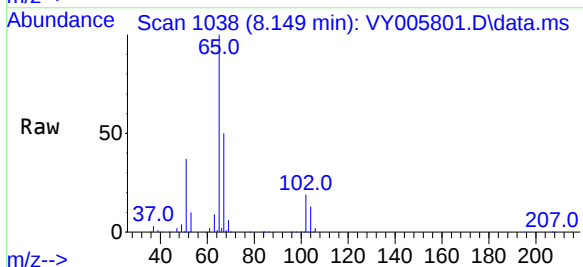


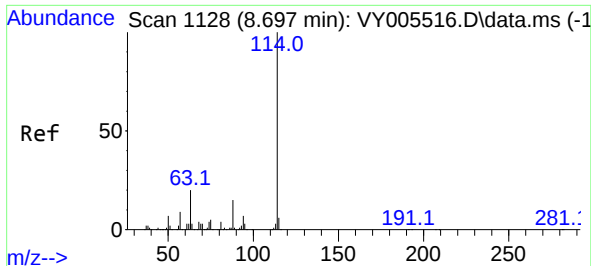

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.697 min Scan# 1128
Delta R.T. -0.000 min
Lab File: VY005801.D
Acq: 20 Aug 2021 18:24




Instrument :
MSVOA_Y
ClientSampleId :
TP-5-10-COMP


Tgt Ion:	114	Resp:	315695
Ion	Ratio	Lower	Upper
114	100		
63	19.7	0.0	39.2
88	14.8	0.0	30.8

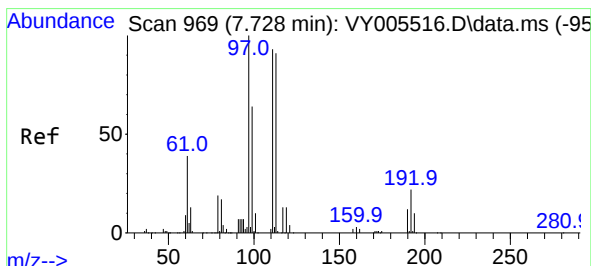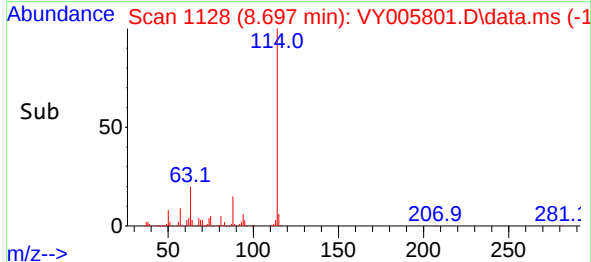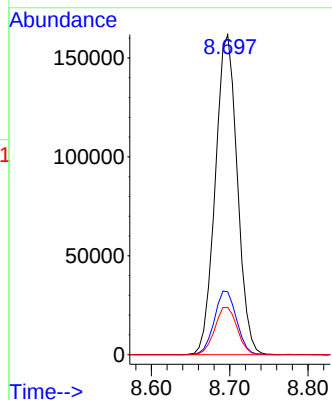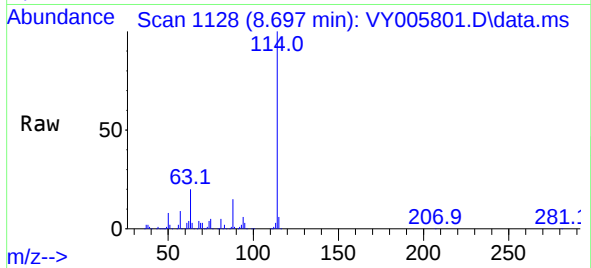

#35
Dibromofluoromethane
Concen: 55.099 ug/l
RT: 7.728 min Scan# 969
Delta R.T. -0.000 min
Lab File: VY005801.D
Acq: 20 Aug 2021 18:24

Tgt Ion:	113	Resp:	97387
Ion	Ratio	Lower	Upper
113	100		
111	101.5	81.9	122.9
192	23.4	19.2	28.8


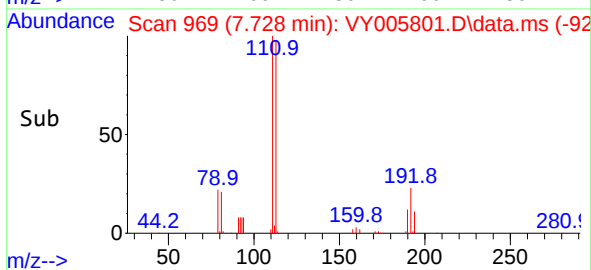
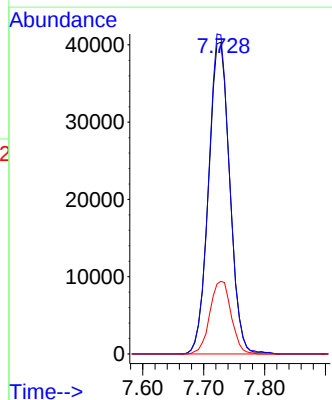
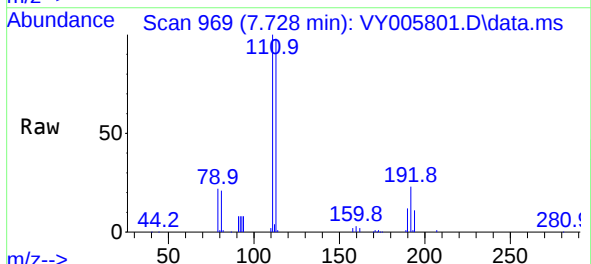


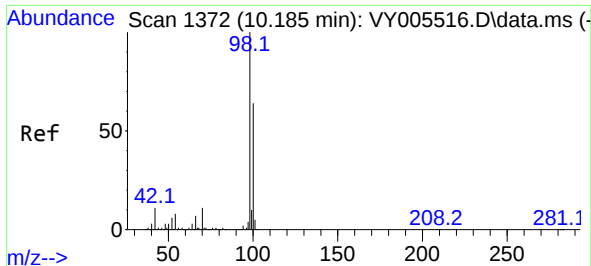

#50
Toluene-d8
Concen: 55.043 ug/l
RT: 10.185 min Scan# 1372
Delta R.T. -0.000 min
Lab File: VY005801.D
Acq: 20 Aug 2021 18:24




Instrument :
MSVOA_Y
ClientSampleId :
TP-5-10-COMP


Tgt Ion: 98 Resp: 408021
Ion Ratio Lower Upper
98 100
100 62.8 51.3 76.9

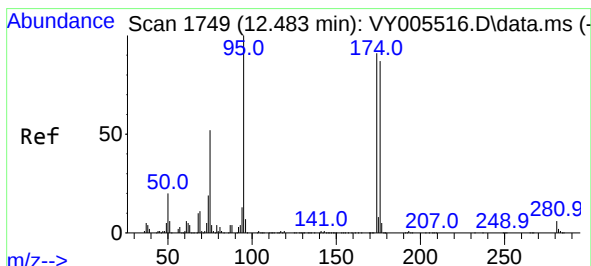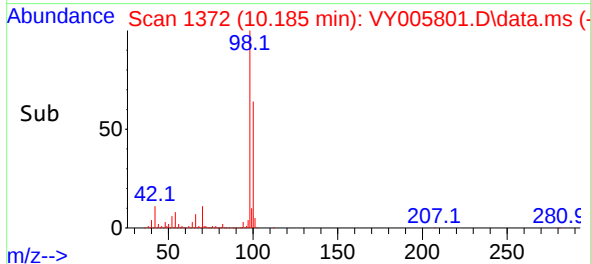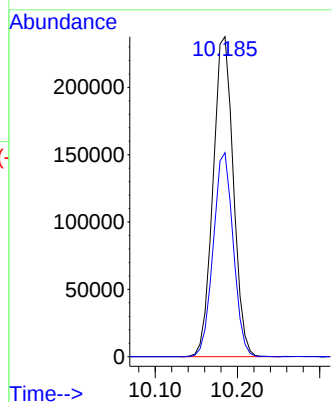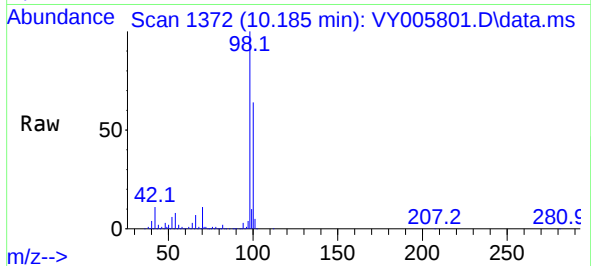

#62
4-Bromofluorobenzene
Concen: 56.961 ug/l
RT: 12.483 min Scan# 1749
Delta R.T. -0.000 min
Lab File: VY005801.D
Acq: 20 Aug 2021 18:24

Tgt Ion: 95 Resp: 139824
Ion Ratio Lower Upper
95 100
174 96.0 0.0 191.4
176 94.2 0.0 183.6


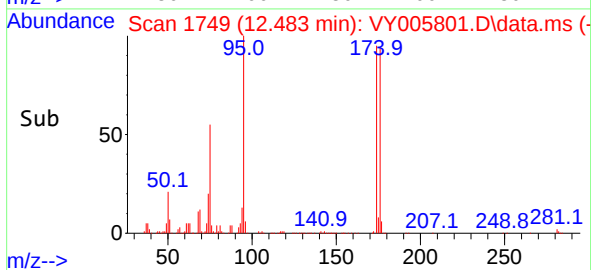
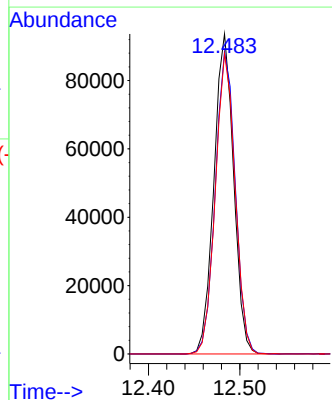
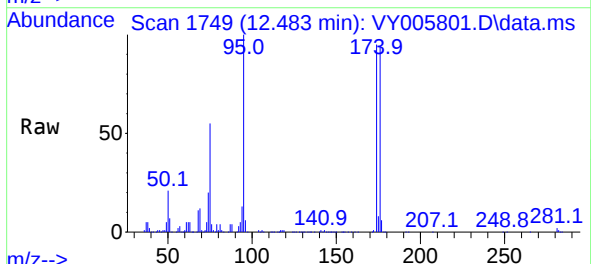


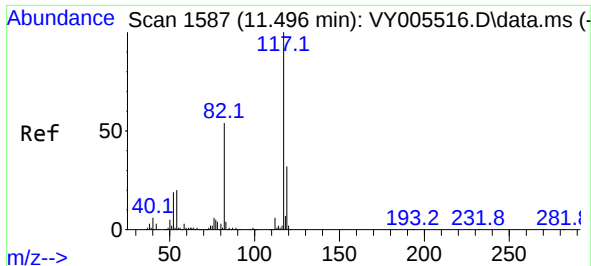

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.496 min Scan# 1587
Delta R.T. -0.000 min
Lab File: VY005801.D
Acq: 20 Aug 2021 18:24

Instrument :
MSVOA_Y
ClientSampleId :
TP-5-10-COMP

Tgt Ion:117 Resp: 327621
Ion Ratio Lower Upper
117 100
82 53.9 43.5 65.3
119 32.9 25.5 38.3

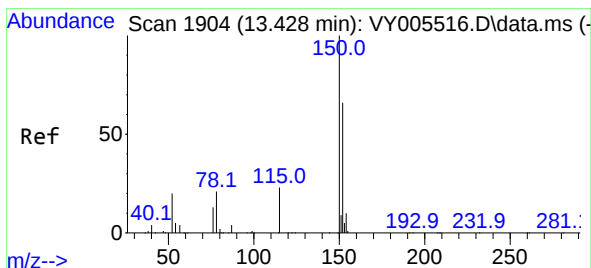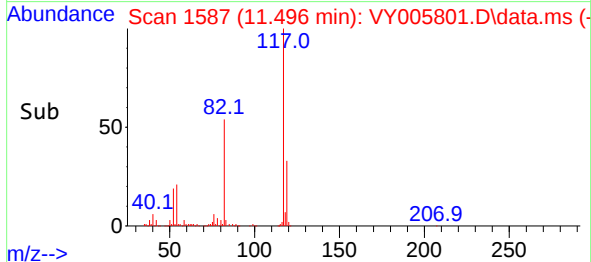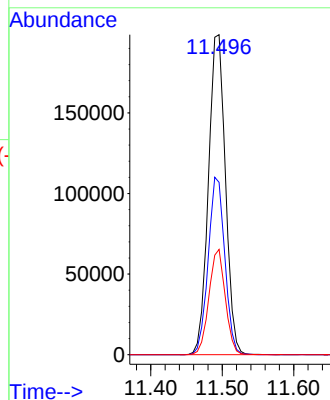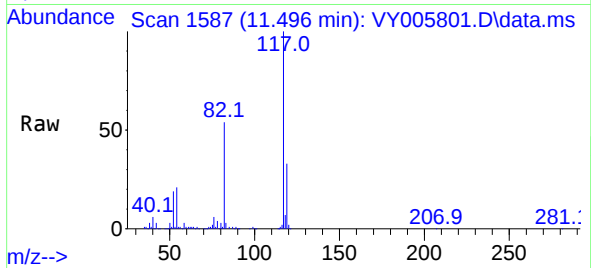

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.428 min Scan# 1904
Delta R.T. -0.000 min
Lab File: VY005801.D
Acq: 20 Aug 2021 18:24

Tgt Ion:152 Resp: 159203
Ion Ratio Lower Upper
152 100
115 54.0 27.3 81.9
150 157.4 0.0 350.2

