


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY082021\
 Data File : VY005783.D
 Acq On : 20 Aug 2021 09:45
 Operator : SY/MD
 Sample : BFB
 Misc : 5.00G/5ML/MSVOA_Y/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y080221S.M
 Title : SW846 8260
 Last Update : Tue Aug 03 04:52:05 2021

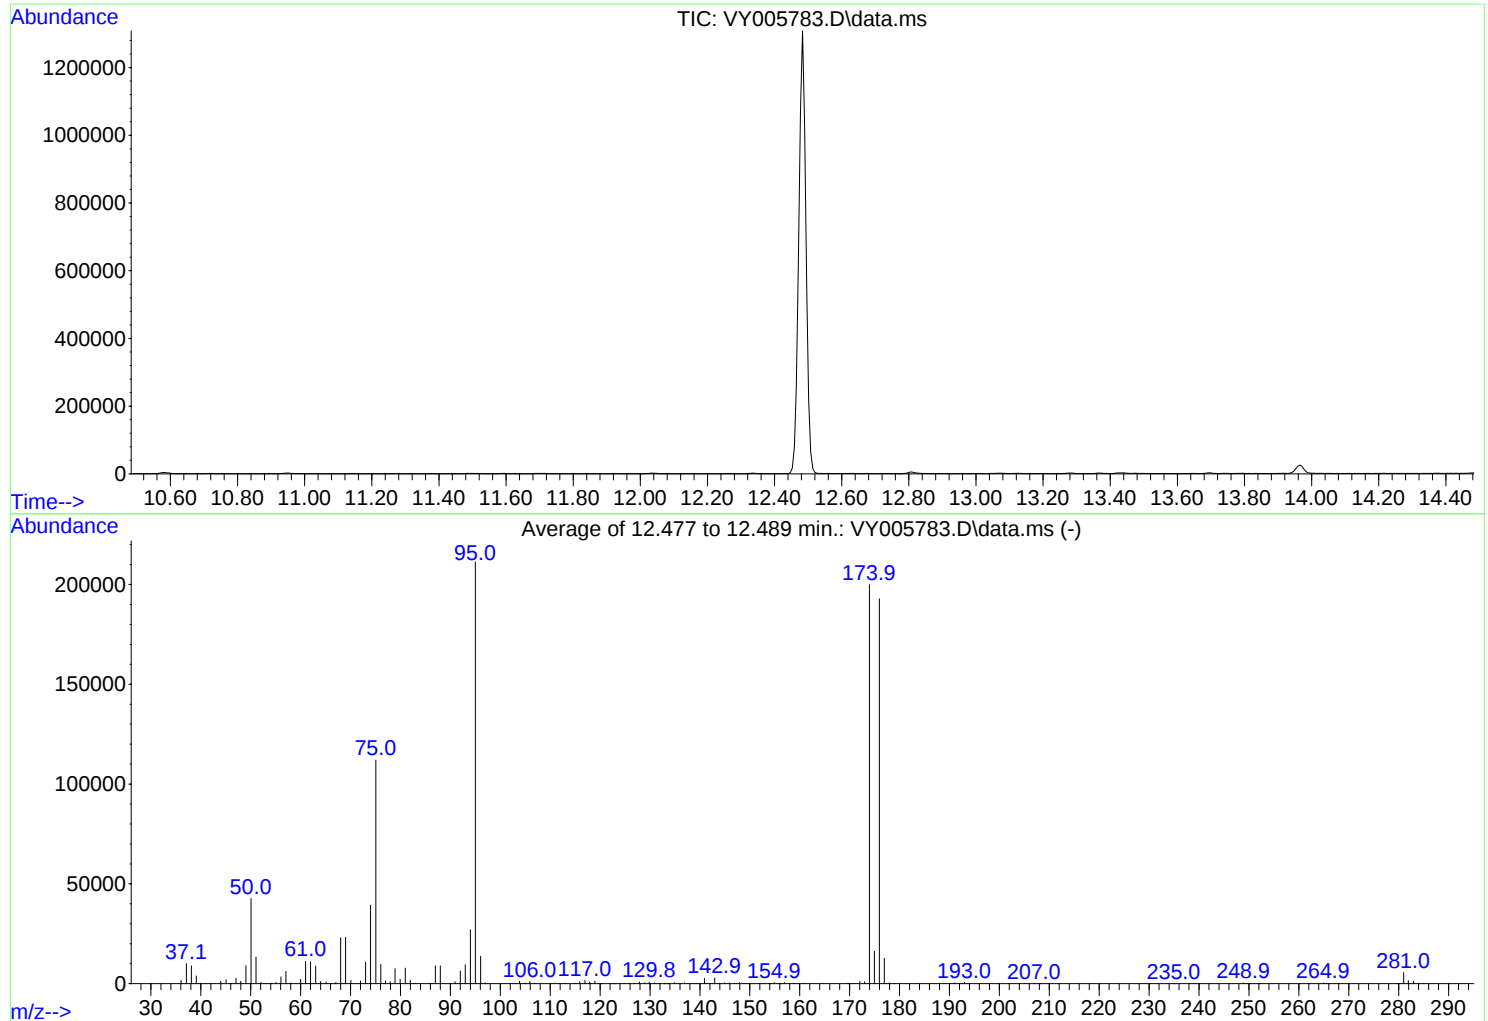

AutoFind: Scans 1748, 1749, 1750; Background Corrected with Scan 1739

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.2	42685	PASS
75	95	30	60	53.0	112035	PASS
95	95	100	100	100.0	211349	PASS
96	95	5	9	6.5	13720	PASS
173	174	0.00	2	0.5	980	PASS
174	95	50	100	94.6	199851	PASS
175	174	5	9	8.1	16160	PASS
176	174	95	101	96.5	192811	PASS
177	176	5	9	6.6	12657	PASS