

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY082224\
 Data File : VY019212.D
 Acq On : 22 Aug 2024 11:52
 Operator : SY/MD
 Sample : VY0822SBL01
 Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 VY0822SBL01

Quant Time: Aug 23 01:49:26 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y081524S.M
 Quant Title : SW846 8260
 QLast Update : Fri Aug 16 05:10:30 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.701	168	98791	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.609	114	175566	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.420	117	153759	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.352	152	55761	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.055	65	49487	49.972	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	99.940%
35) Dibromofluoromethane	7.628	113	55227	48.109	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	96.220%
50) Toluene-d8	10.103	98	194308	47.035	ug/l	0.00
Spiked Amount	50.000	Range	58 - 134	Recovery	=	94.080%
62) 4-Bromofluorobenzene	12.408	95	58505	41.543	ug/l	0.00
Spiked Amount	50.000	Range	29 - 146	Recovery	=	83.080%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY082224\
Data File : VY019212.D
Acq On : 22 Aug 2024 11:52
Operator : SY/MD
Sample : VY0822SBL01
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
VY0822SBL01

Quant Time: Aug 23 01:49:26 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y081524S.M
Quant Title : SW846 8260
QLast Update : Fri Aug 16 05:10:30 2024
Response via : Initial Calibration




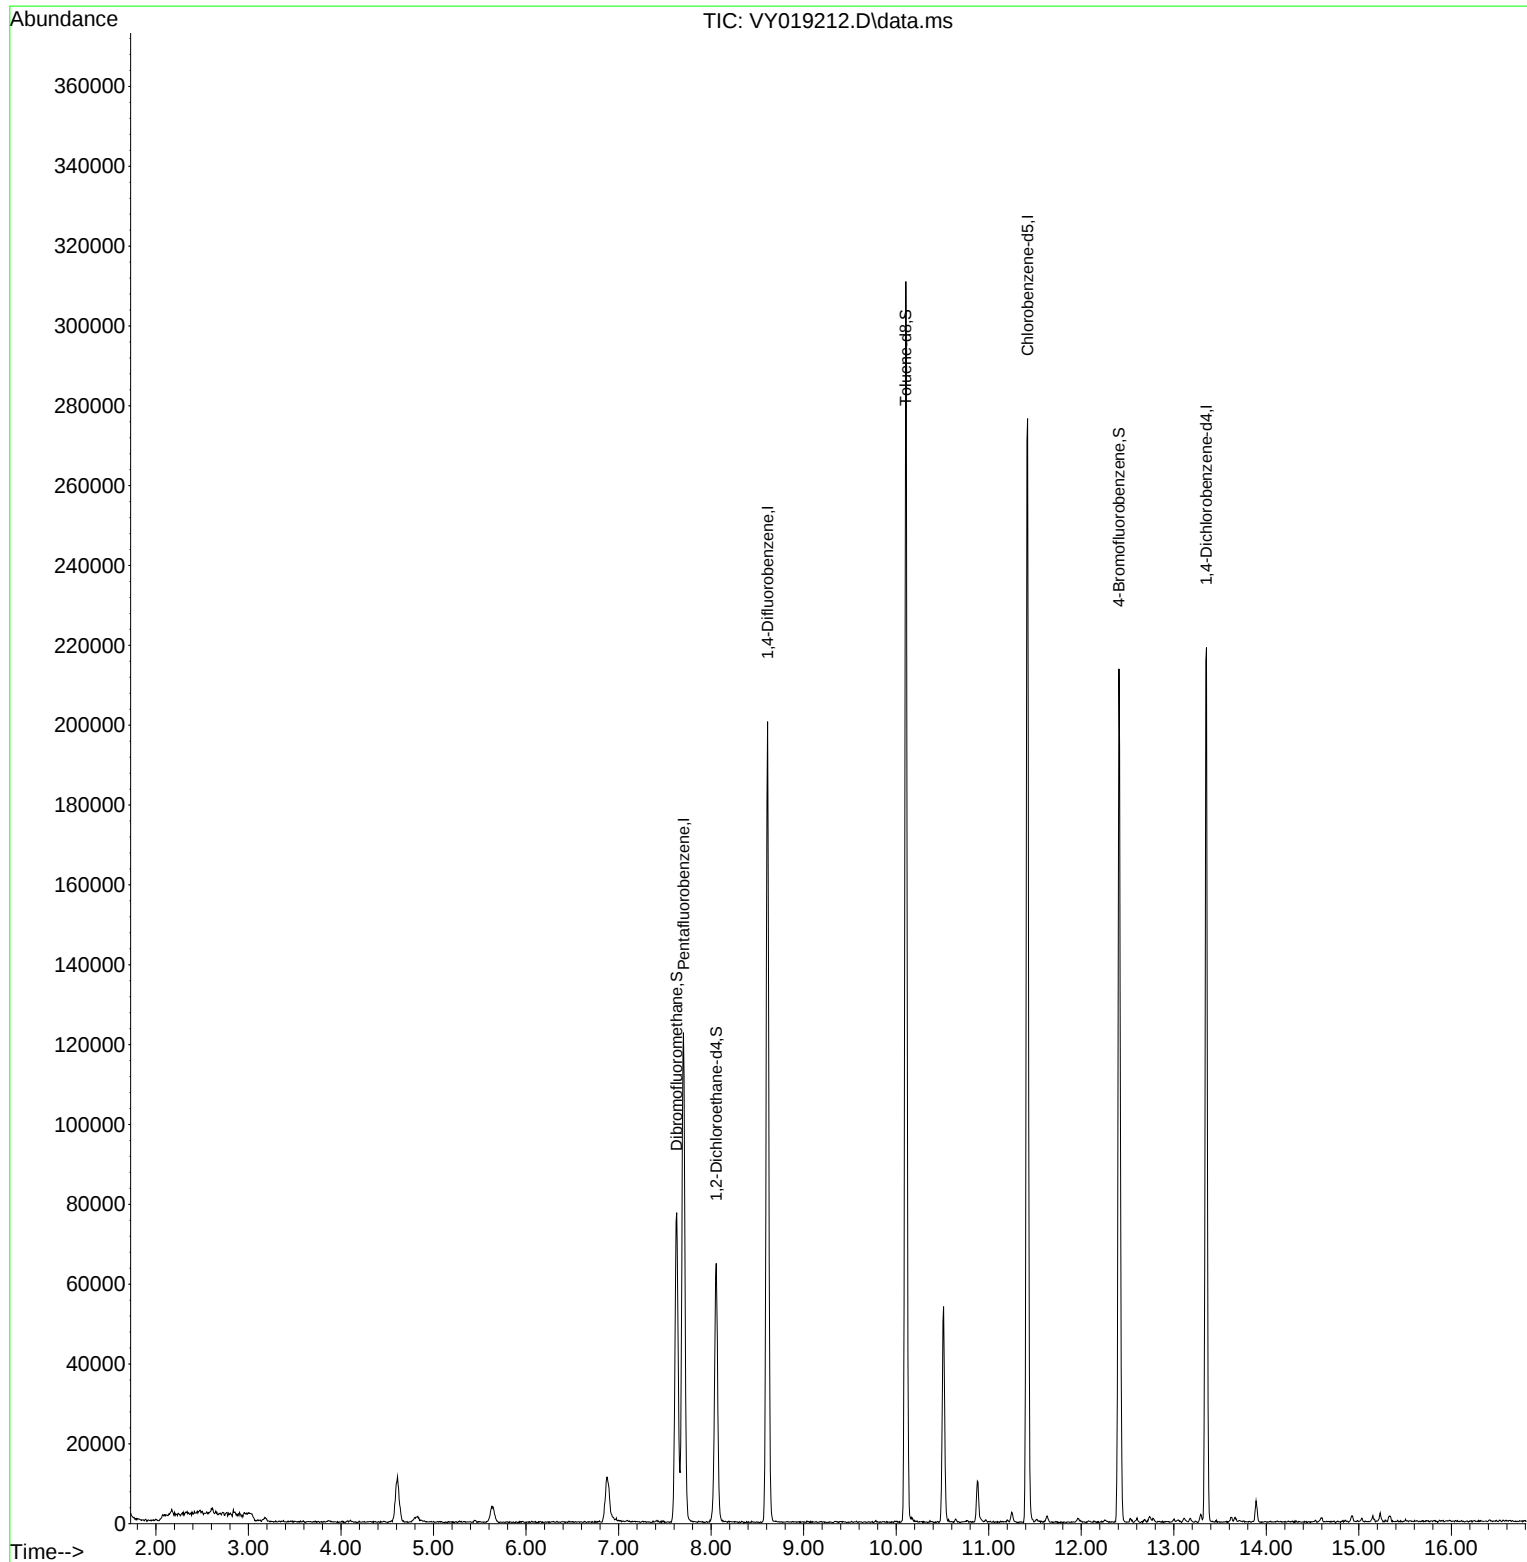


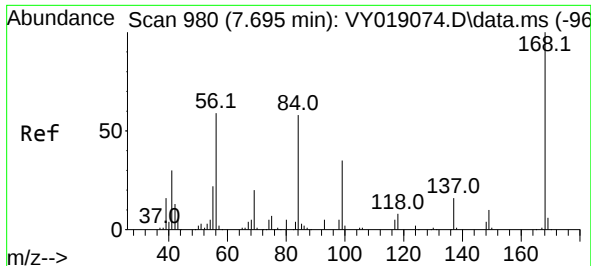

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.701 min Scan# 981
Delta R.T. 0.006 min
Lab File: VY019212.D
Acq: 22 Aug 2024 11:52




Instrument :
MSVOA_Y
ClientSampleId :
VY0822SBL01


Tgt Ion:168 Resp: 98791
Ion Ratio Lower Upper
168 100
99 50.1 39.1 58.7

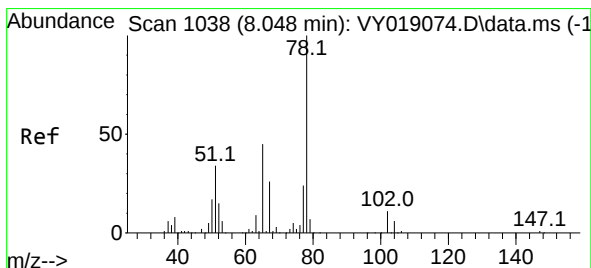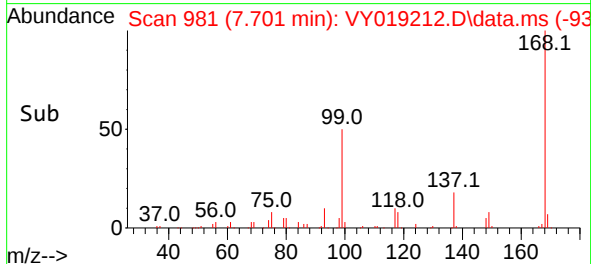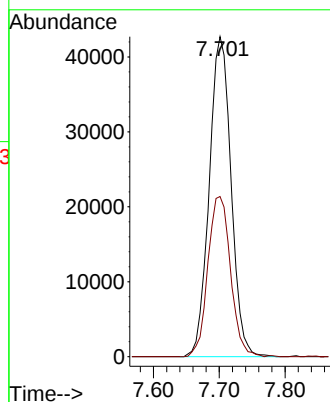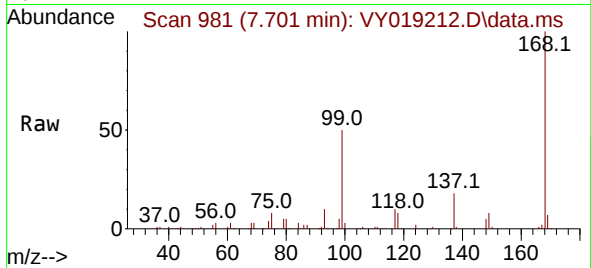

#33
1,2-Dichloroethane-d4
Concen: 49.972 ug/l
RT: 8.055 min Scan# 1039
Delta R.T. 0.006 min
Lab File: VY019212.D
Acq: 22 Aug 2024 11:52

Tgt Ion: 65 Resp: 49487
Ion Ratio Lower Upper
65 100
67 50.4 0.0 109.6

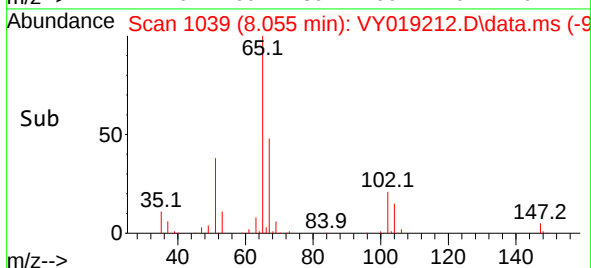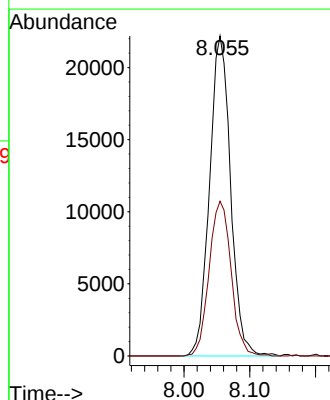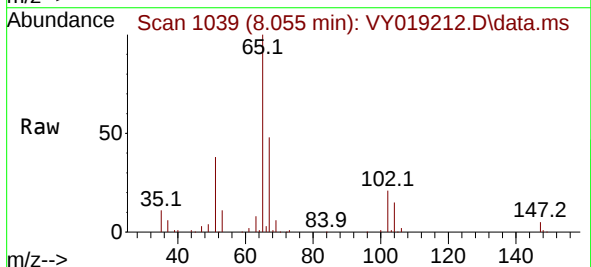

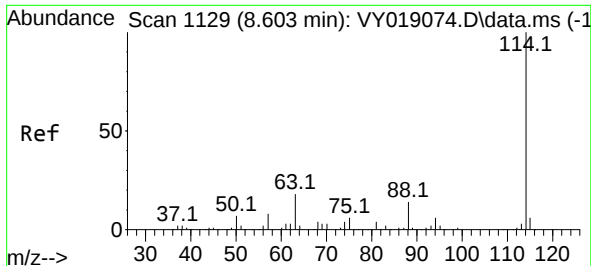

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.609 min Scan# 1129

Delta R.T. 0.006 min

Lab File: VY019212.D

Acq: 22 Aug 2024 11:52

Instrument :

MSVOA_Y

ClientSampleId :

VY0822SBL01





Tgt Ion:114 Resp: 175566

Ion Ratio Lower Upper

114 100

63 17.4 0.0 35.0

88 14.2 0.0 27.2

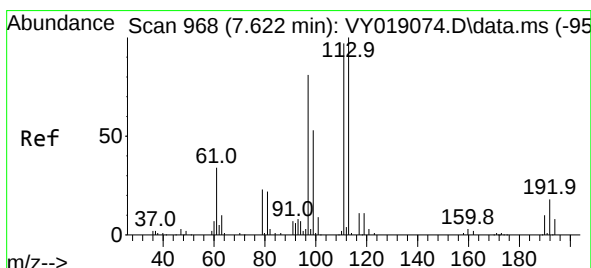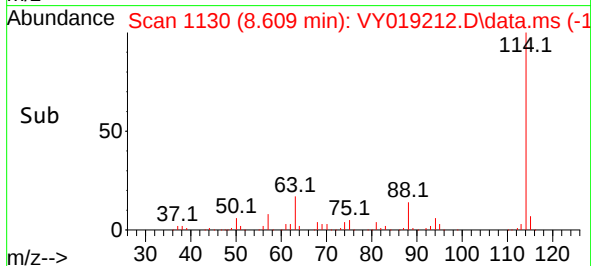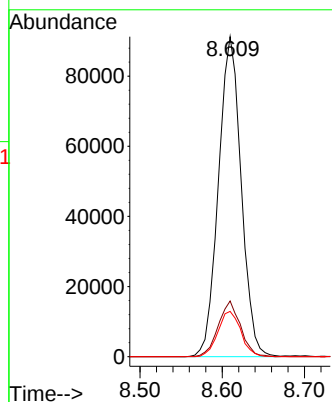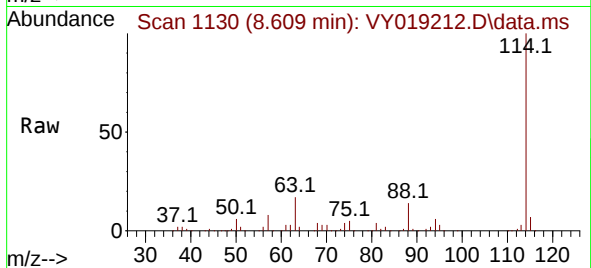

#35

Dibromofluoromethane

Concen: 48.109 ug/l

RT: 7.628 min Scan# 969

Delta R.T. 0.006 min

Lab File: VY019212.D

Acq: 22 Aug 2024 11:52




Tgt Ion:113 Resp: 55227


Ion Ratio Lower Upper

113 100

111 101.8 82.2 123.4

192 19.4 15.9 23.9


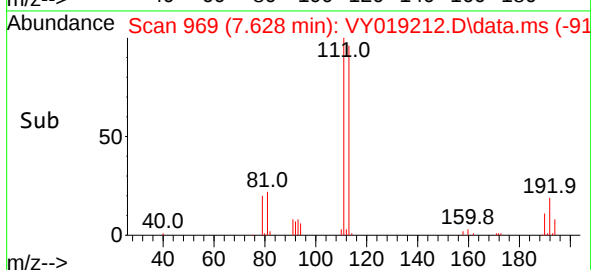
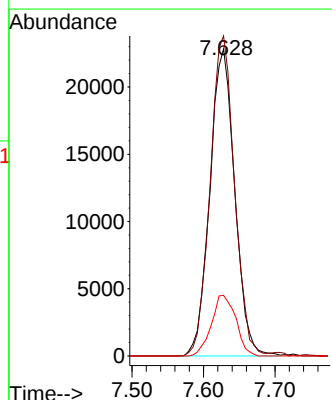
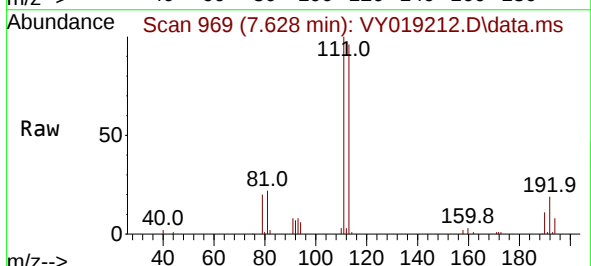


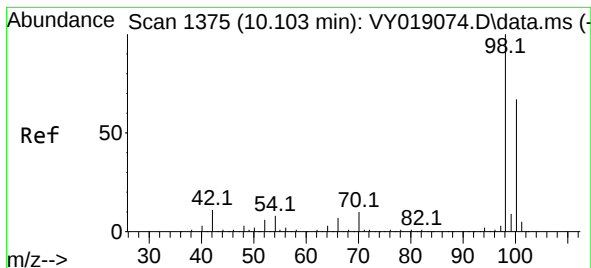

#50
Toluene-d8
Concen: 47.035 ug/l
RT: 10.103 min Scan# 11
Delta R.T. 0.000 min
Lab File: VY019212.D
Acq: 22 Aug 2024 11:52




Instrument :
MSVOA_Y
ClientSampleId :
VY0822SBL01


Tgt Ion: 98 Resp: 194308
Ion Ratio Lower Upper
98 100
100 67.9 52.0 78.0

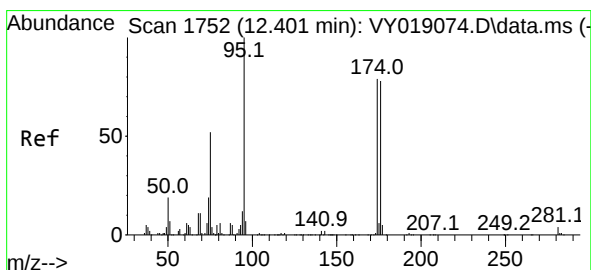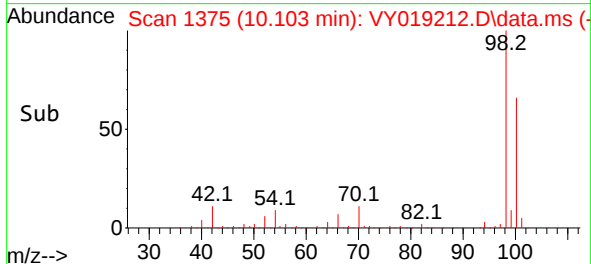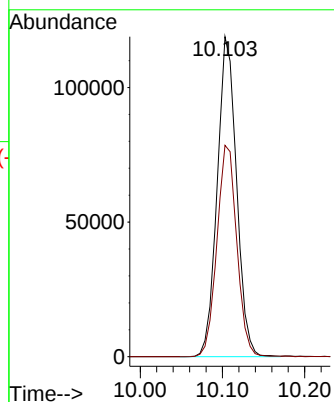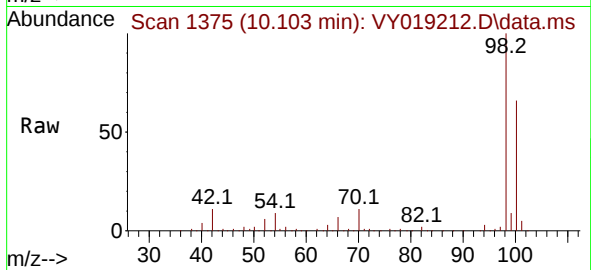

#62
4-Bromofluorobenzene
Concen: 41.543 ug/l
RT: 12.408 min Scan# 1753
Delta R.T. 0.006 min
Lab File: VY019212.D
Acq: 22 Aug 2024 11:52

Tgt Ion: 95 Resp: 58505
Ion Ratio Lower Upper
95 100
174 89.9 0.0 175.6
176 84.9 0.0 171.4

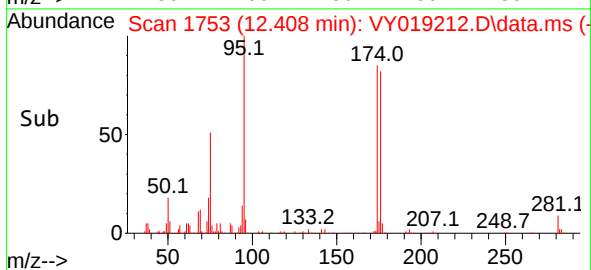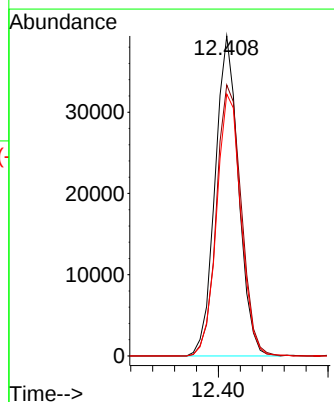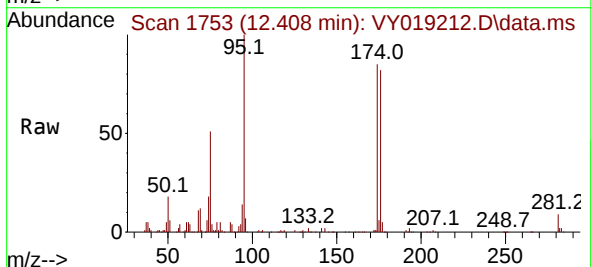

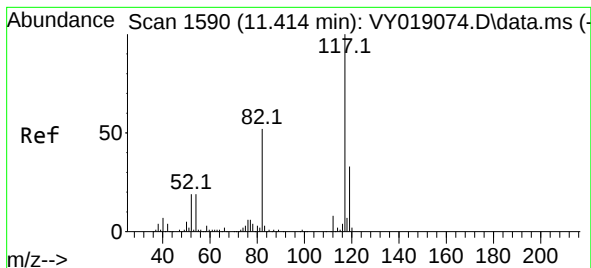

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.420 min Scan# 11

Delta R.T. 0.006 min

Lab File: VY019212.D

Acq: 22 Aug 2024 11:52

Instrument :

MSVOA_Y

ClientSampleId :

VY0822SBL01





Tgt Ion:117 Resp: 153759

Ion Ratio Lower Upper

117 100

82 50.0 42.4 63.6

119 31.8 25.9 38.9

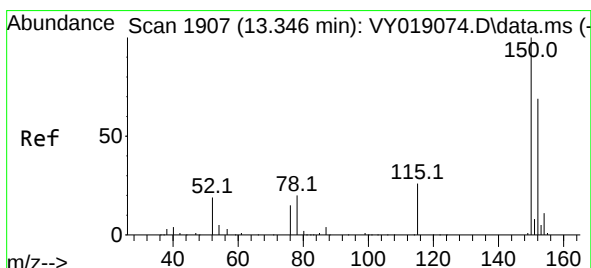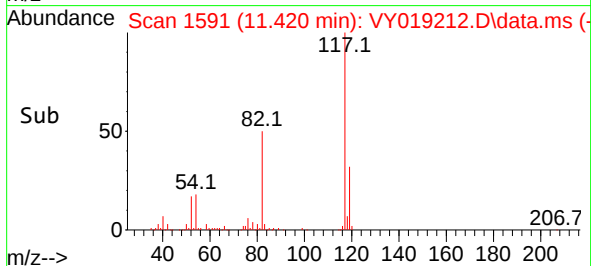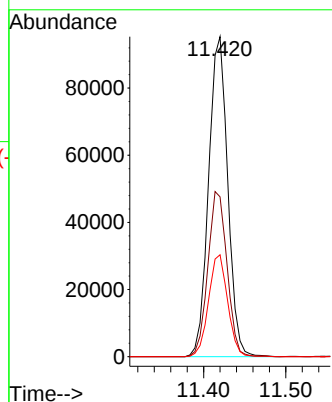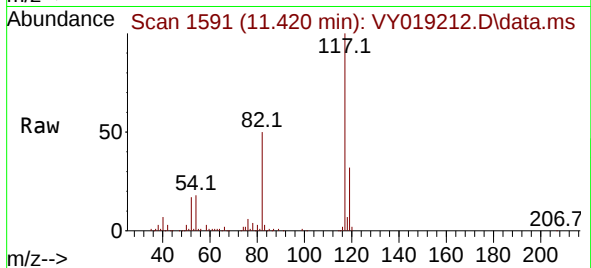

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.352 min Scan# 1908

Delta R.T. 0.006 min

Lab File: VY019212.D

Acq: 22 Aug 2024 11:52

Tgt Ion:152 Resp: 55761

Ion Ratio Lower Upper

152 100

115 57.2 28.2 84.7

150 158.9 0.0 345.6

