

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY082224\
 Data File : VY019231.D
 Acq On : 22 Aug 2024 19:35
 Operator : SY/MD
 Sample : P3694-01
 Misc : 5.10g/5.0mL/MSVOA_Y/SOIL/A
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 Kingsland-Driveway

Quant Time: Aug 23 01:57:18 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y081524S.M
 Quant Title : SW846 8260
 QLast Update : Fri Aug 16 05:10:30 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.701	168	75118	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.603	114	153637	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.414	117	135975	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.346	152	50825	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.055	65	40103	53.258	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	106.520%
35) Dibromofluoromethane	7.622	113	42887	42.692	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	85.380%
50) Toluene-d8	10.103	98	170875	47.267	ug/l	0.00
Spiked Amount	50.000	Range	58 - 134	Recovery	=	94.540%
62) 4-Bromofluorobenzene	12.408	95	51052	41.425	ug/l	0.00
Spiked Amount	50.000	Range	29 - 146	Recovery	=	82.860%


Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY082224\
Data File : VY019231.D
Acq On : 22 Aug 2024 19:35
Operator : SY/MD
Sample : P3694-01
Misc : 5.10g/5.0mL/MSVOA_Y/SOIL/A
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
Kingsland-Driveway

Quant Time: Aug 23 01:57:18 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y081524S.M
Quant Title : SW846 8260
QLast Update : Fri Aug 16 05:10:30 2024
Response via : Initial Calibration



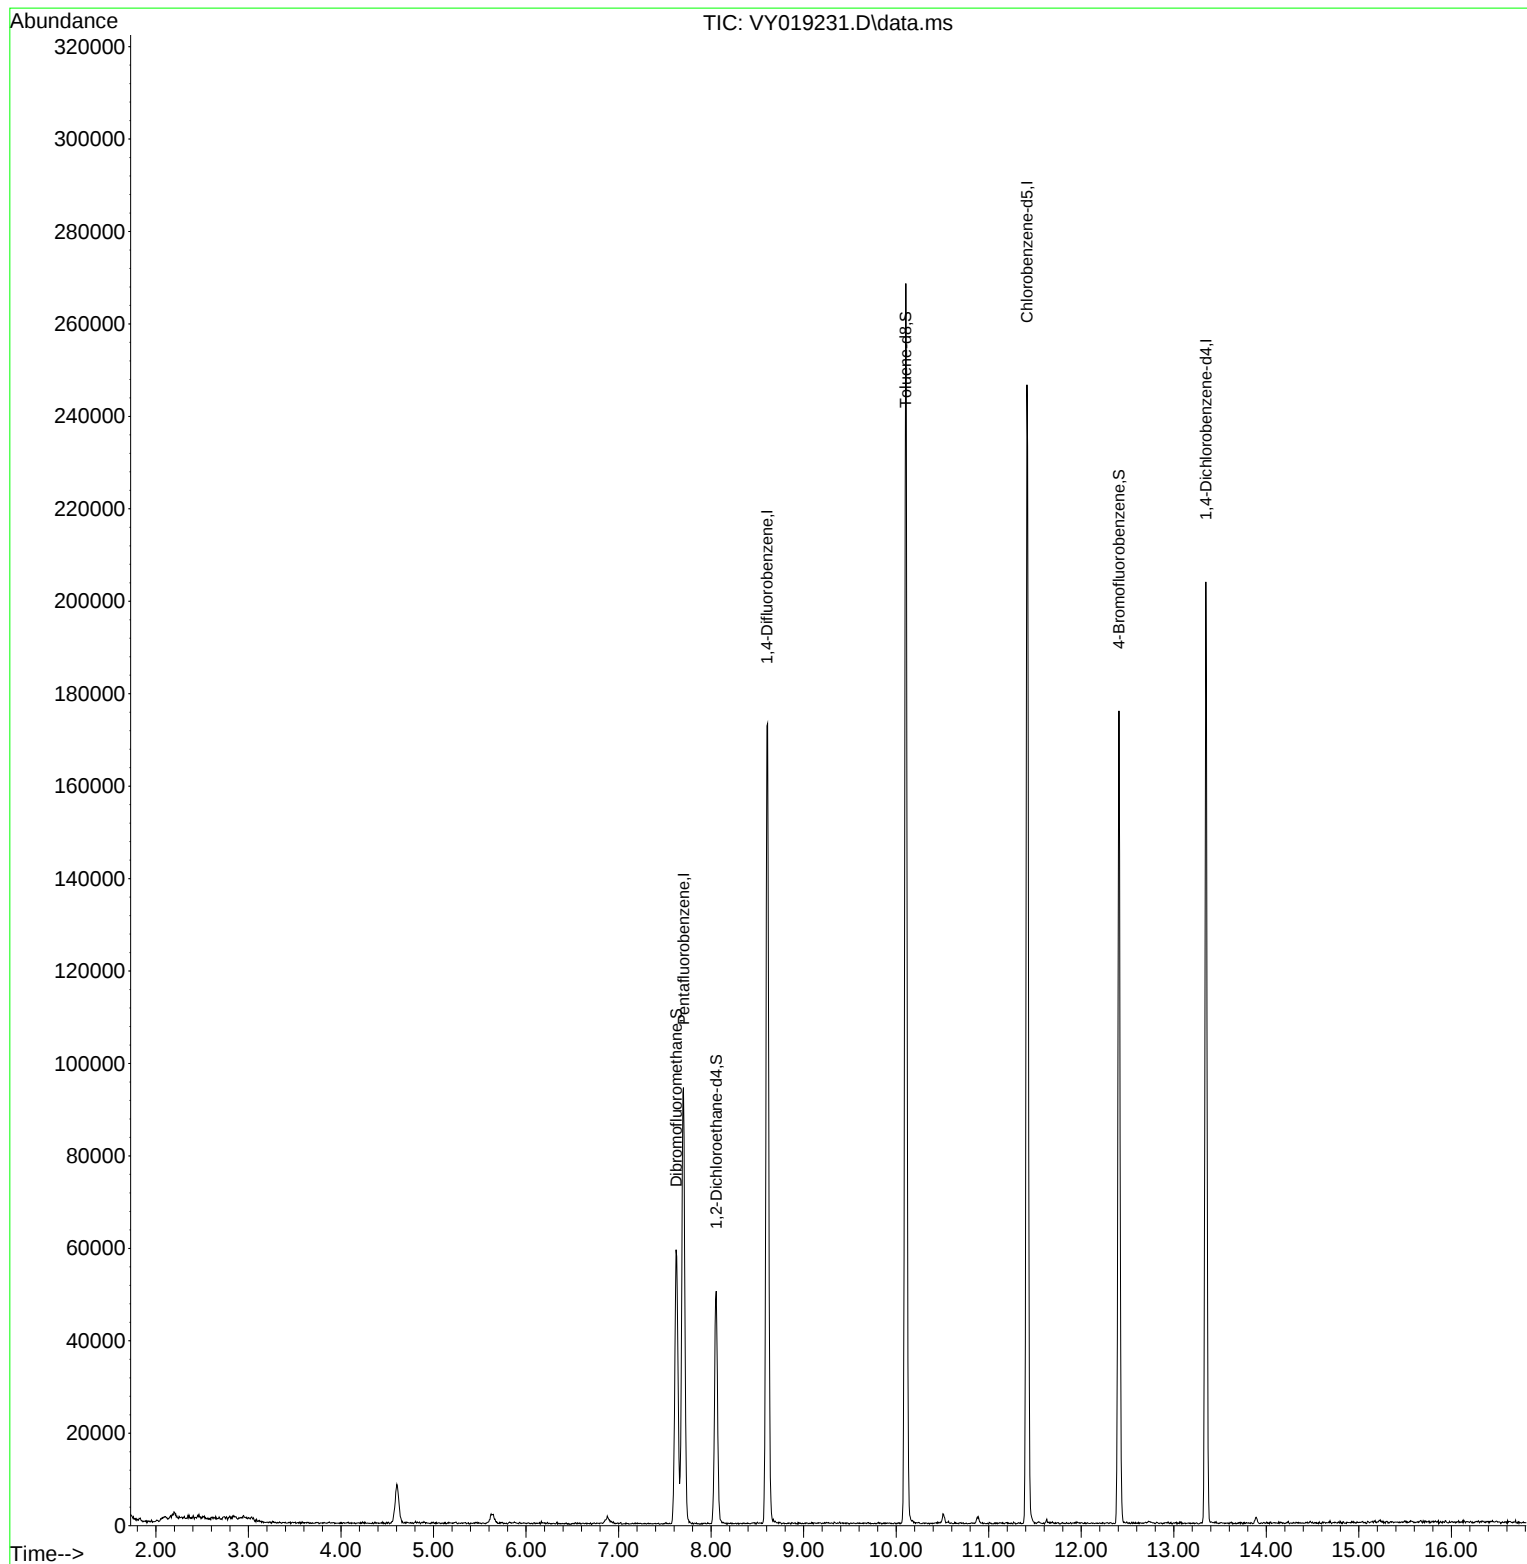




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.701 min Scan# 91
Delta R.T. 0.006 min
Lab File: VY019231.D
Acq: 22 Aug 2024 19:35




Instrument :
MSVOA_Y
ClientSampleId :
Kingsland-Driveway

Tgt Ion:168 Resp: 75118
Ion Ratio Lower Upper
168 100
99 54.1 39.1 58.7

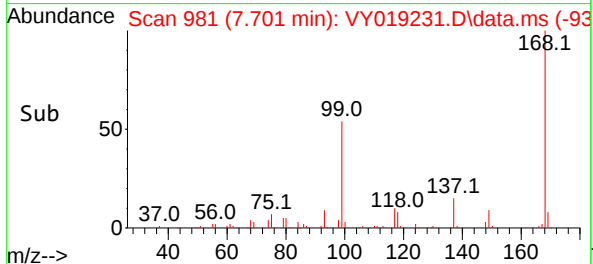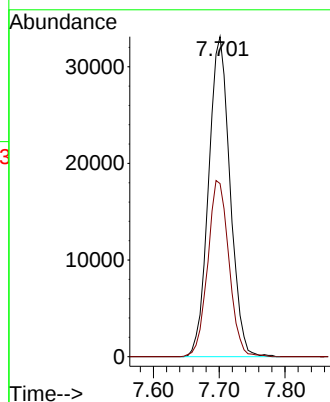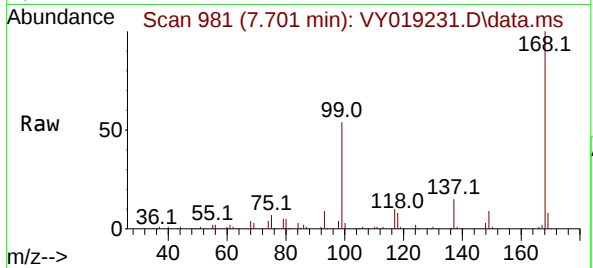

#33
1,2-Dichloroethane-d4
Concen: 53.258 ug/l
RT: 8.055 min Scan# 1039
Delta R.T. 0.006 min
Lab File: VY019231.D
Acq: 22 Aug 2024 19:35

Tgt Ion: 65 Resp: 40103
Ion Ratio Lower Upper
65 100
67 51.2 0.0 109.6

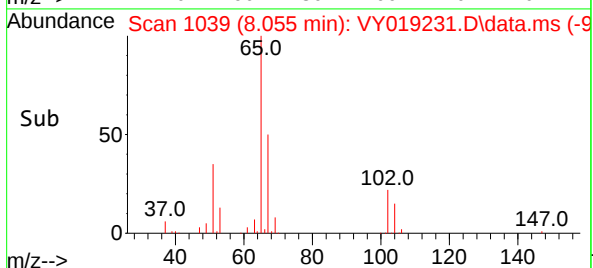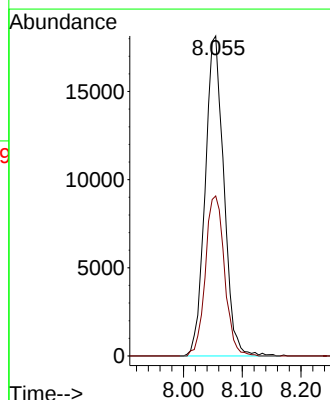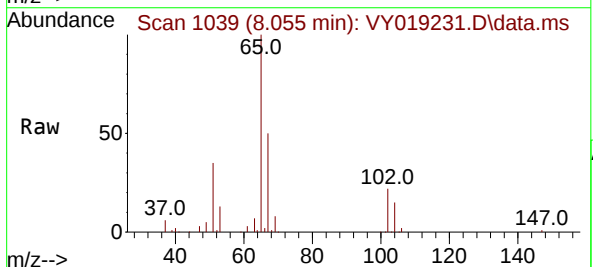



#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.603 min Scan# 1129

Delta R.T. 0.000 min

Lab File: VY019231.D

Acq: 22 Aug 2024 19:35

Instrument :

MSVOA_Y

ClientSampleId :

Kingsland-Driveway




Tgt Ion:114 Resp: 153637

Ion Ratio Lower Upper

114 100

63 18.0 0.0 35.0

88 13.9 0.0 27.2

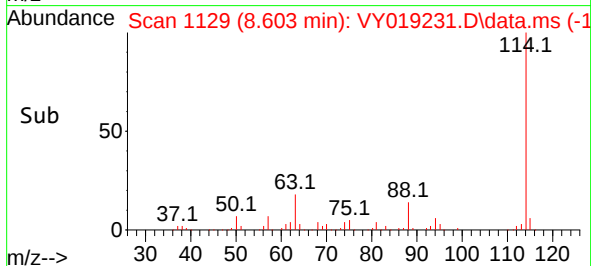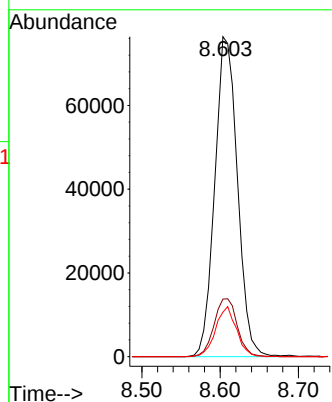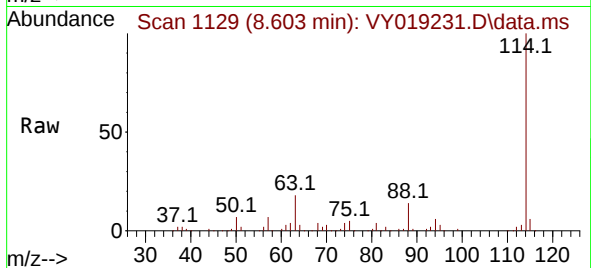

#35

Dibromofluoromethane

Concen: 42.692 ug/l

RT: 7.622 min Scan# 968

Delta R.T. 0.000 min

Lab File: VY019231.D

Acq: 22 Aug 2024 19:35




Tgt Ion:113 Resp: 42887


Ion Ratio Lower Upper

113 100

111 101.9 82.2 123.4

192 19.8 15.9 23.9

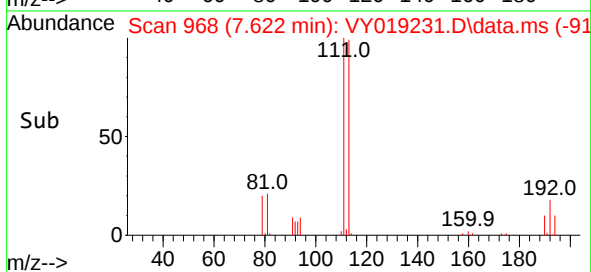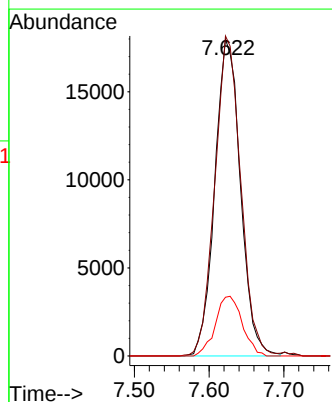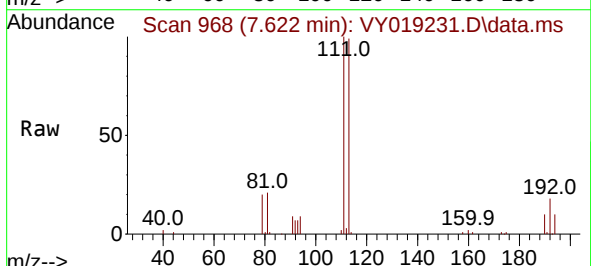

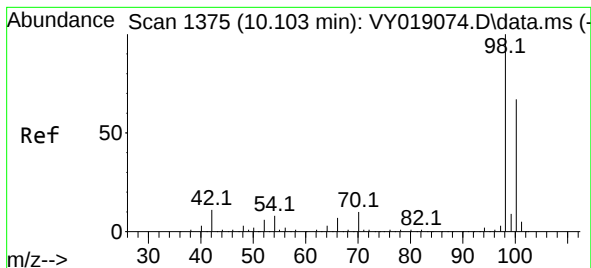

#50

Toluene-d8

Concen: 47.267 ug/l

RT: 10.103 min Scan# 11

Delta R.T. 0.000 min

Lab File: VY019231.D

Acq: 22 Aug 2024 19:35

Instrument :

MSVOA_Y

ClientSampleId :





Kingsland-Driveway

Tgt Ion: 98 Resp: 170875

Ion Ratio Lower Upper

98 100

100 67.5 52.0 78.0

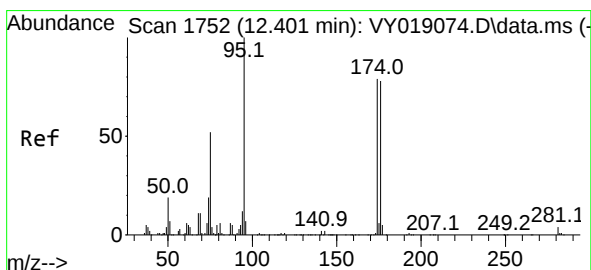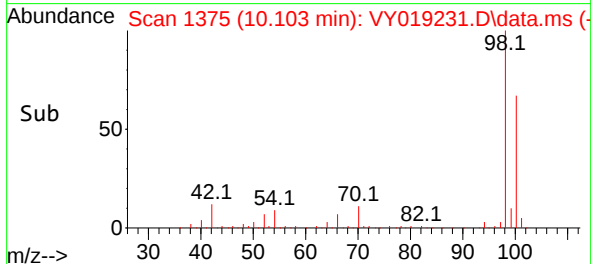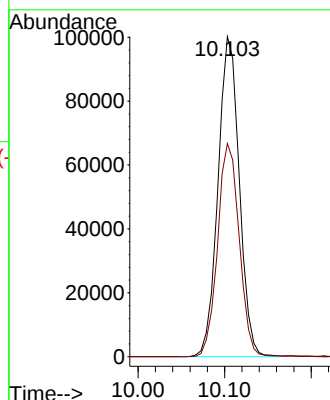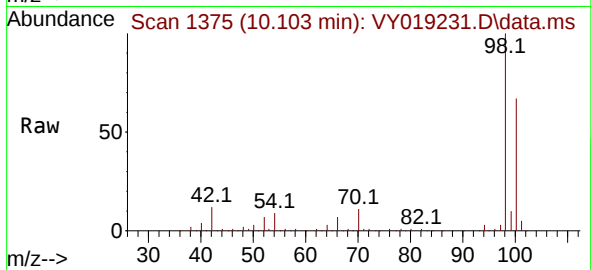

#62

4-Bromofluorobenzene

Concen: 41.425 ug/l

RT: 12.408 min Scan# 1753

Delta R.T. 0.006 min

Lab File: VY019231.D

Acq: 22 Aug 2024 19:35




Tgt Ion: 95 Resp: 51052


Ion Ratio Lower Upper

95 100

174 88.1 0.0 175.6

176 83.6 0.0 171.4


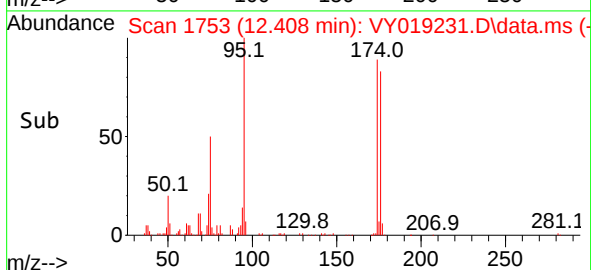
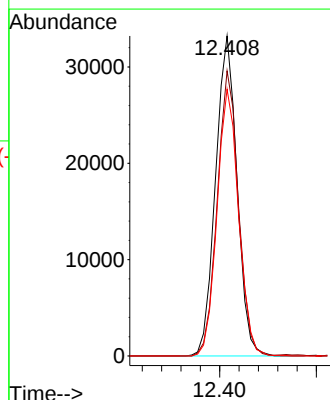
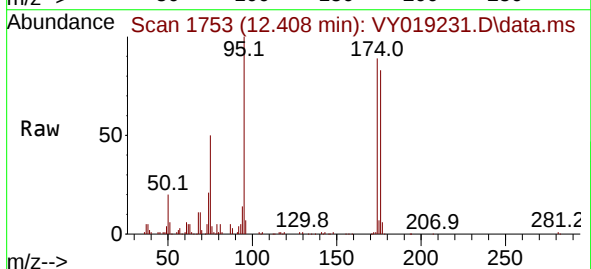


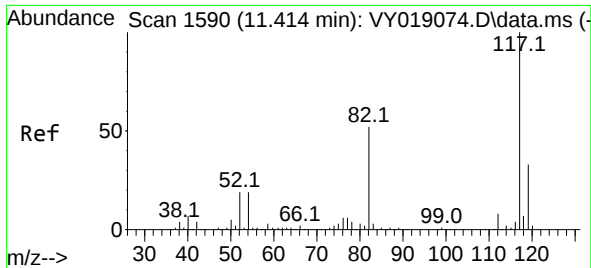

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.414 min Scan# 11
Delta R.T. 0.000 min
Lab File: VY019231.D
Acq: 22 Aug 2024 19:35

Instrument :
MSVOA_Y
ClientSampleId :
Kingsland-Driveway

Tgt Ion:117 Resp: 135975
Ion Ratio Lower Upper
117 100
82 55.4 42.4 63.6
119 33.0 25.9 38.9

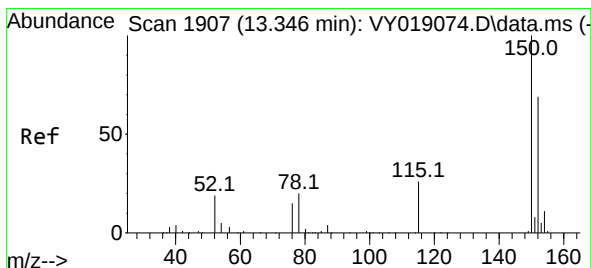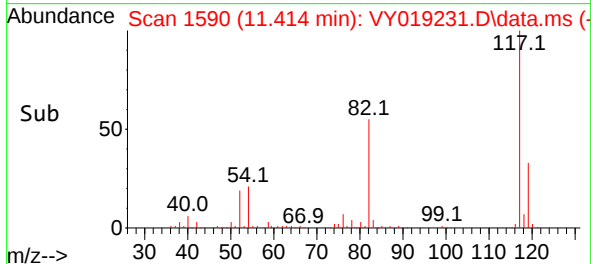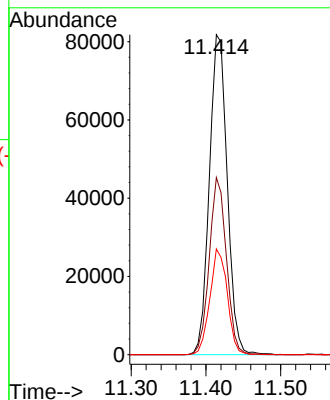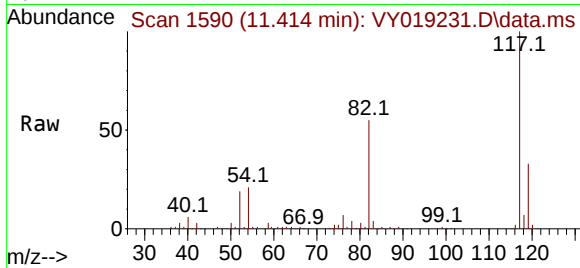

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.346 min Scan# 1907
Delta R.T. 0.000 min
Lab File: VY019231.D
Acq: 22 Aug 2024 19:35

Tgt Ion:152 Resp: 50825
Ion Ratio Lower Upper
152 100
115 57.7 28.2 84.7
150 155.7 0.0 345.6

