
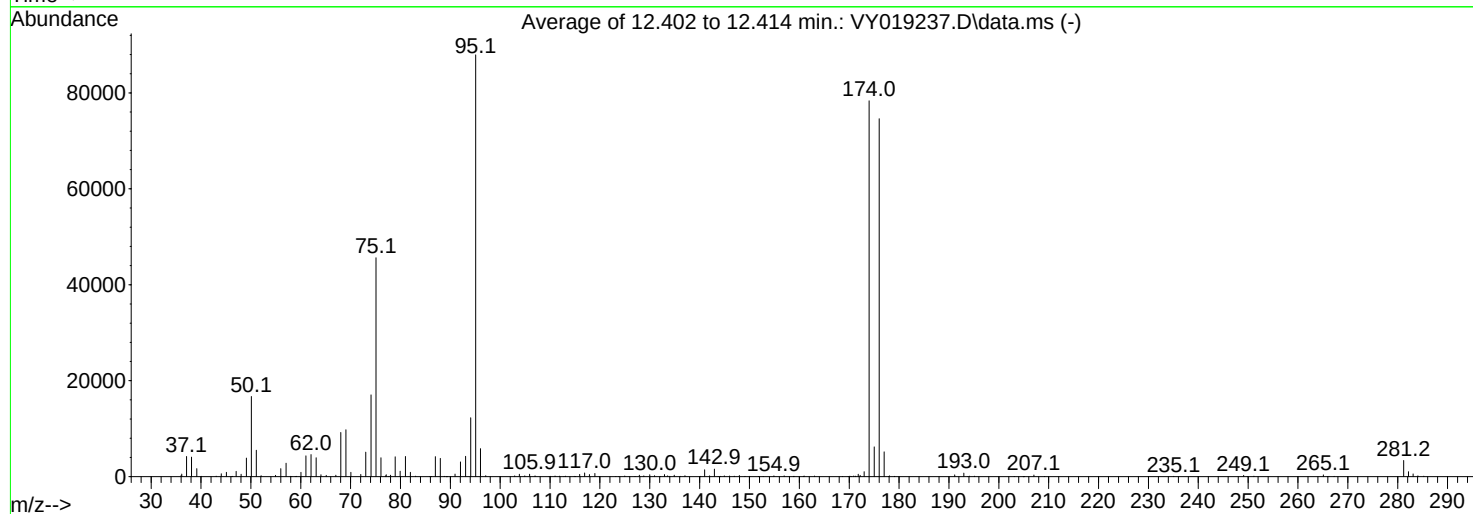


Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY082224\
Data File : VY019237.D
Acq On : 22 Aug 2024 22:43
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 31 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y081524S.M
Title : SW846 8260
Last Update : Fri Aug 16 05:10:30 2024

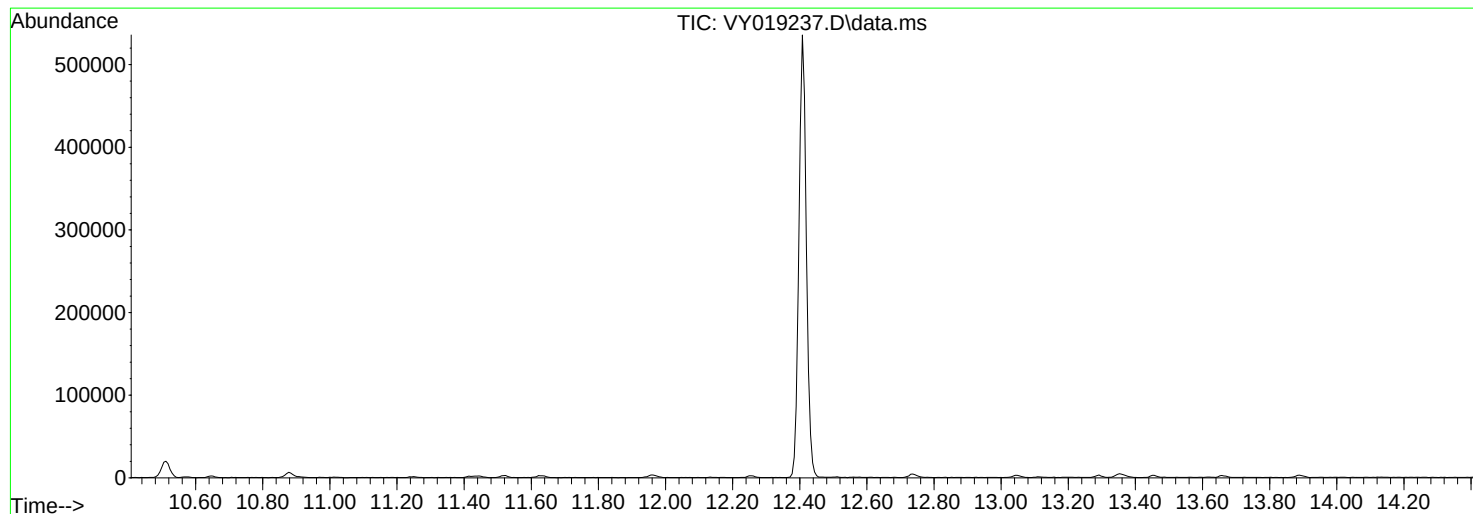

AutoFind: Scans 1752, 1753, 1754; Background Corrected with Scan 1743

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	19.0	16699	PASS
75	95	30	60	51.9	45616	PASS
95	95	100	100	100.0	87928	PASS
96	95	5	9	6.7	5850	PASS
173	174	0.00	2	1.3	1028	PASS
174	95	50	100	89.1	78365	PASS
175	174	5	9	7.9	6214	PASS
176	174	95	101	95.2	74616	PASS
177	176	5	9	6.9	5177	PASS