

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY082322\
 Data File : VY010173.D
 Acq On : 23 Aug 2022 18:21
 Operator : KP/MD
 Sample : N4272-07
 Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_Y
 ClientSampleId :
 PSC-164717

Quant Time: Aug 24 04:34:20 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y081922S.M
 Quant Title : SW846 8260
 QLast Update : Mon Aug 22 02:37:07 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.783	168	150015	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.685	114	281313	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.489	117	283993	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.422	152	130373	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.136	65	87188	70.956	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	141.920%
35) Dibromofluoromethane	7.710	113	79426	50.106	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	100.220%
50) Toluene-d8	10.179	98	290760	48.952	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	=	97.900%
62) 4-Bromofluorobenzene	12.477	95	91448	43.091	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	=	86.180%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_Y\Data\VY082322\
Data File : VY010173.D
Acq On : 23 Aug 2022 18:21
Operator : KP/MD
Sample : N4272-07
Misc : 5.00g/5.0mL/MSVOA_Y/SOIL
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_Y
ClientSampleId :
PSC-164717

Quant Time: Aug 24 04:34:20 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_Y\methods\82Y081922S.M
Quant Title : SW846 8260
QLast Update : Mon Aug 22 02:37:07 2022
Response via : Initial Calibration




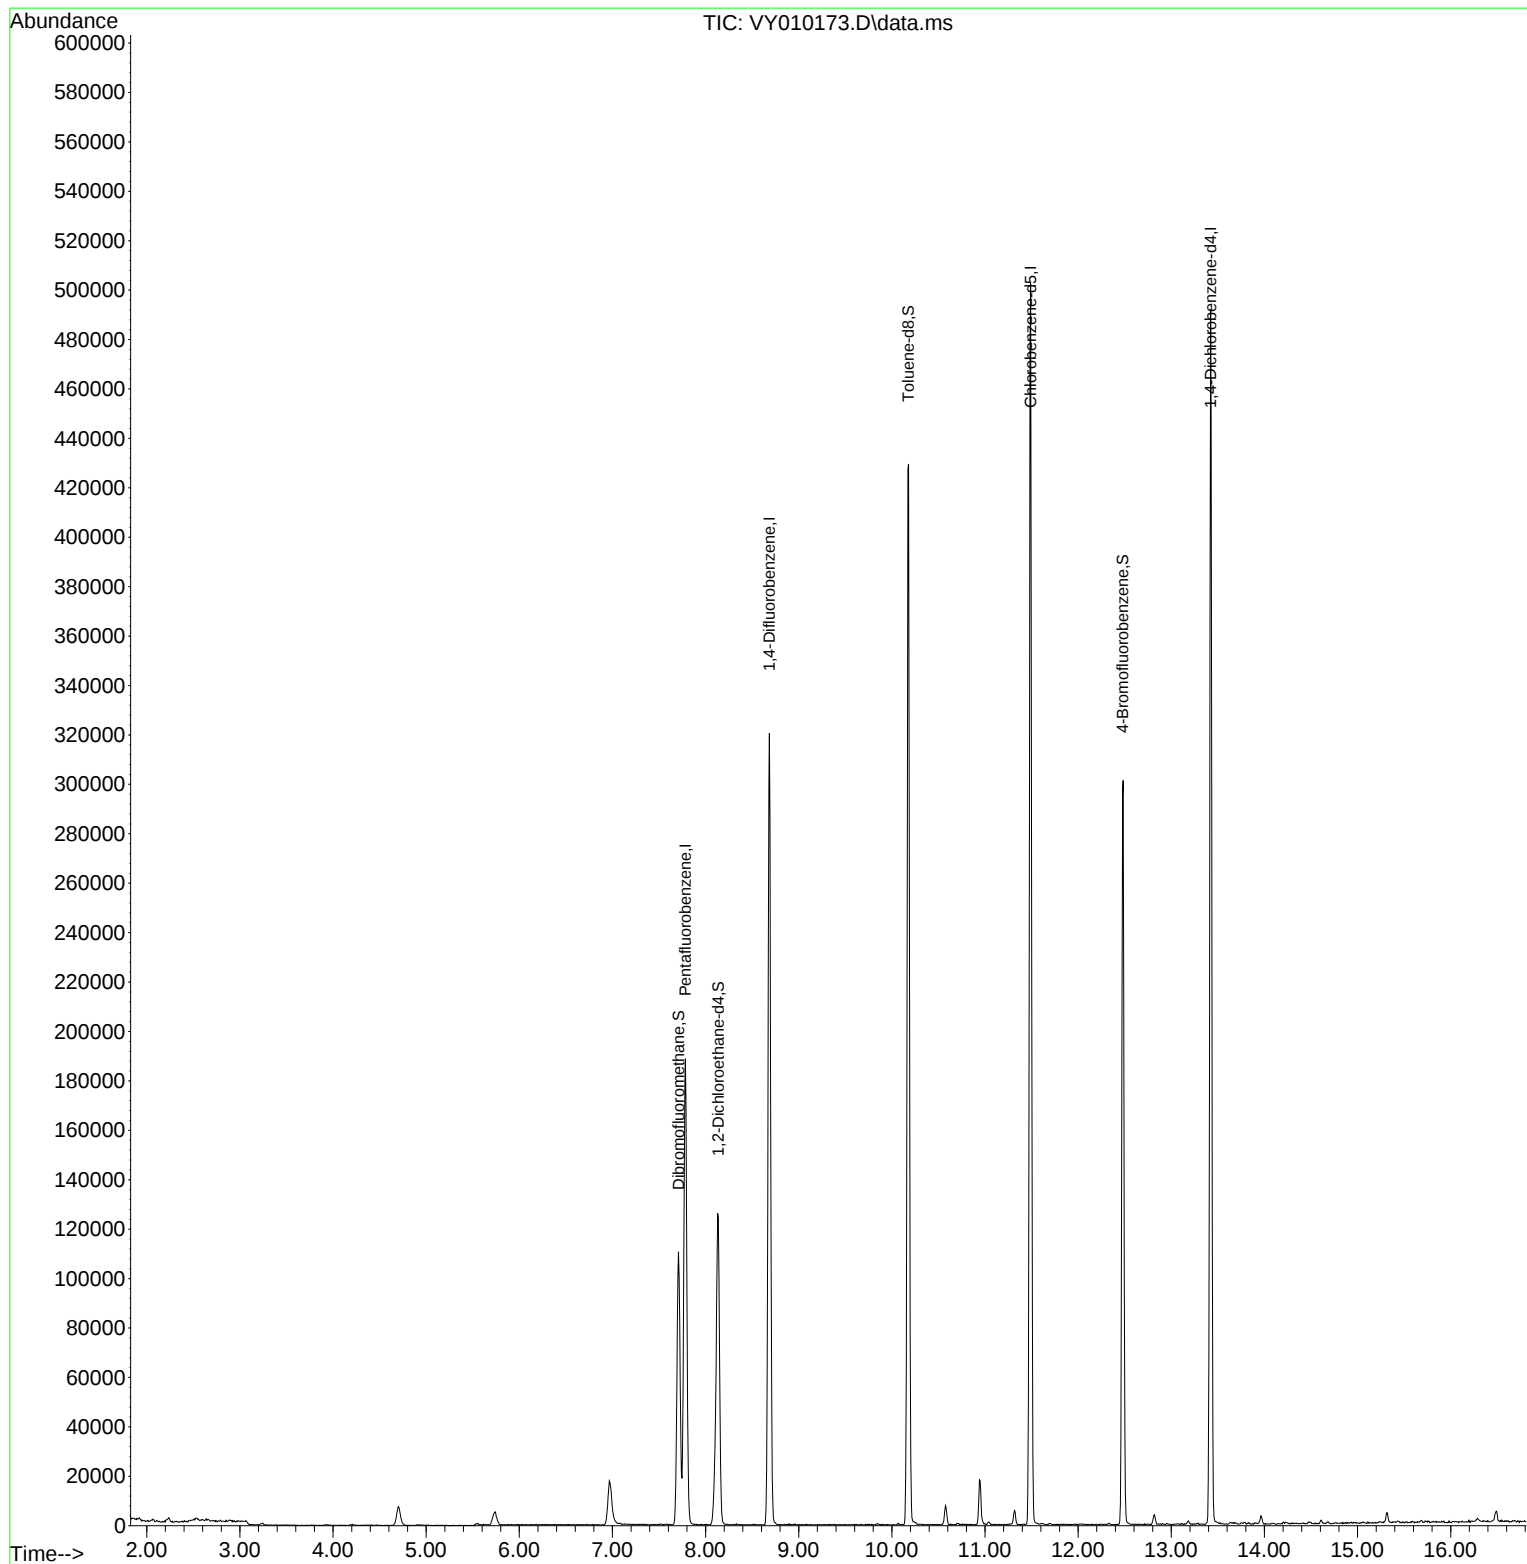


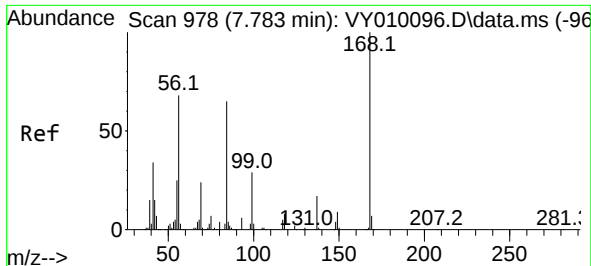

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.783 min Scan# 91
Delta R.T. -0.000 min
Lab File: VY010173.D
Acq: 23 Aug 2022 18:21




Instrument :
MSVOA_Y
ClientSampleId :
PSC-164717


Tgt Ion:168 Resp: 150015
Ion Ratio Lower Upper
168 100
99 51.8 40.7 61.1

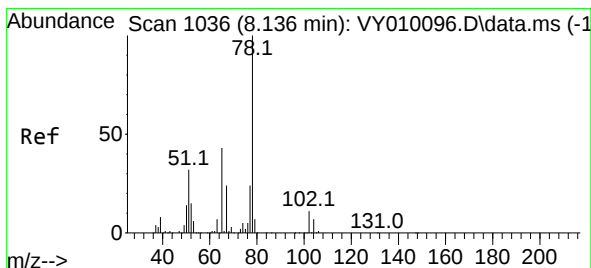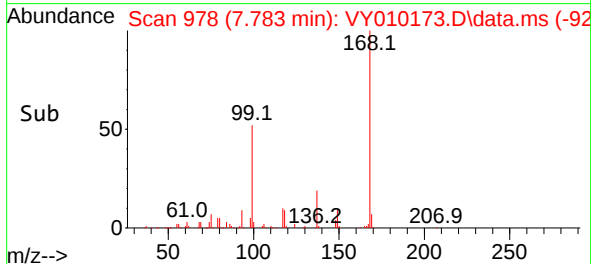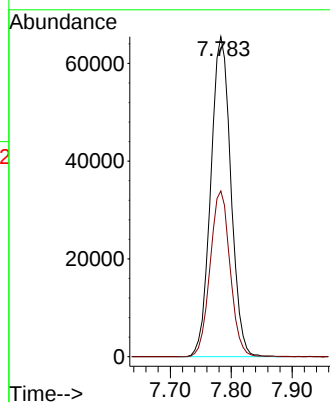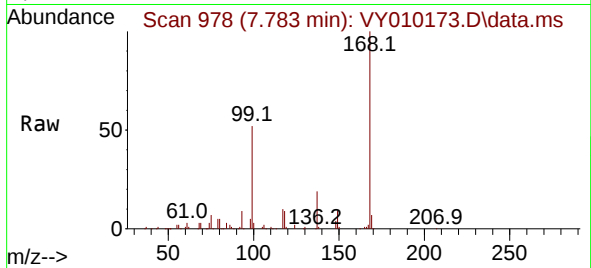

#33
1,2-Dichloroethane-d4
Concen: 70.956 ug/l
RT: 8.136 min Scan# 1036
Delta R.T. 0.000 min
Lab File: VY010173.D
Acq: 23 Aug 2022 18:21

Tgt Ion: 65 Resp: 87188
Ion Ratio Lower Upper
65 100
67 54.9 0.0 110.6

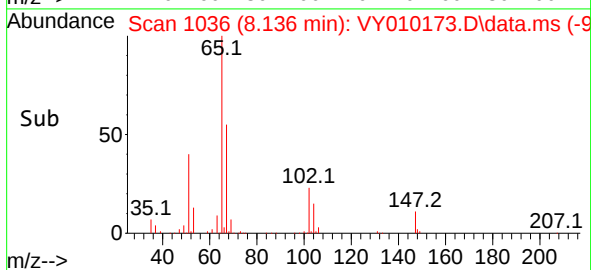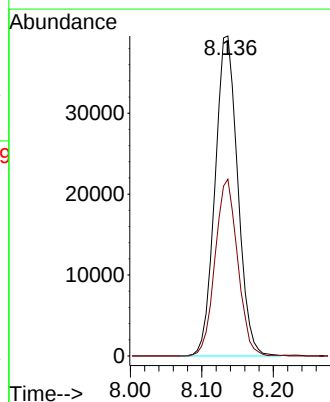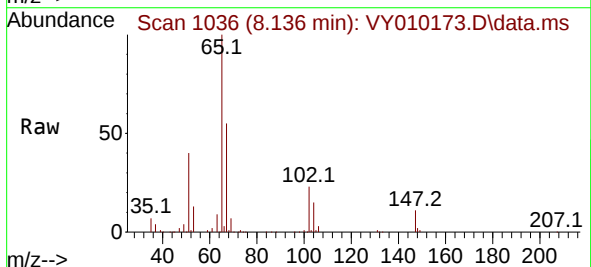

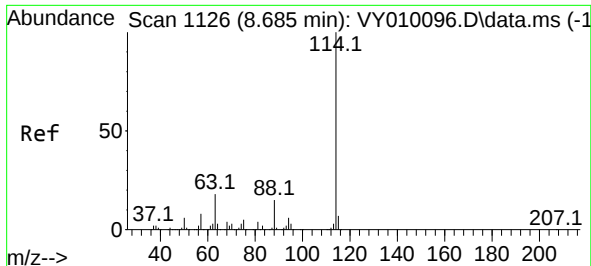

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.685 min Scan# 1126

Delta R.T. 0.000 min

Lab File: VY010173.D

Acq: 23 Aug 2022 18:21

Instrument :

MSVOA_Y

ClientSampleId :

PSC-164717





Tgt Ion:114 Resp: 281313

Ion Ratio Lower Upper

114 100

63 20.1 0.0 35.6

88 14.4 0.0 29.6

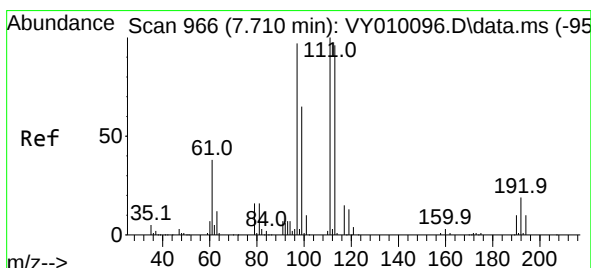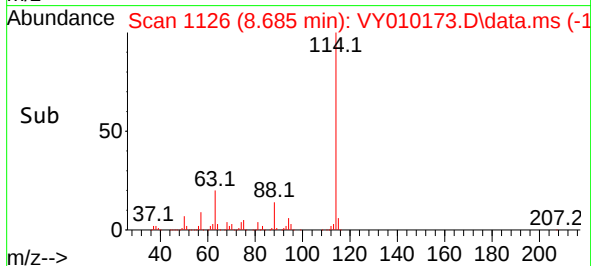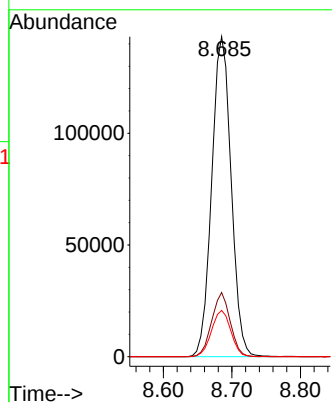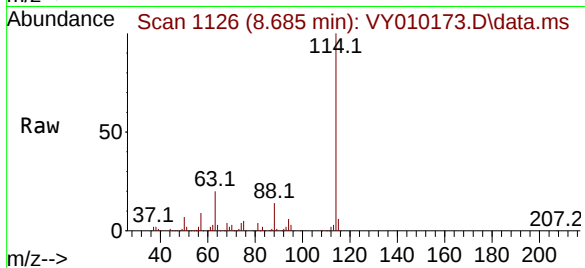

#35

Dibromofluoromethane

Concen: 50.106 ug/l

RT: 7.710 min Scan# 966

Delta R.T. -0.000 min

Lab File: VY010173.D

Acq: 23 Aug 2022 18:21




Tgt Ion:113 Resp: 79426


Ion Ratio Lower Upper

113 100

111 102.1 82.8 124.2

192 20.1 16.3 24.5


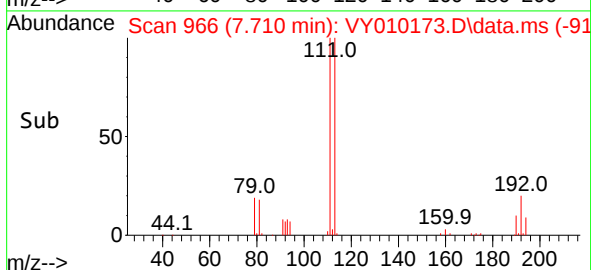
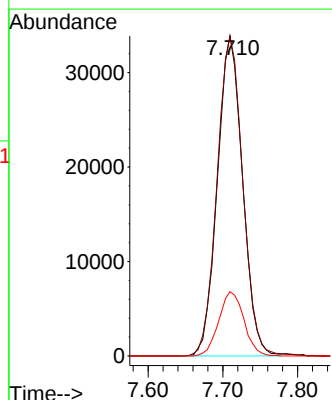
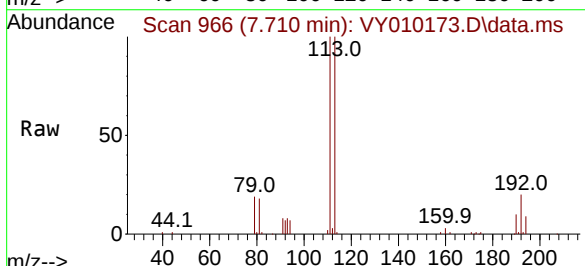


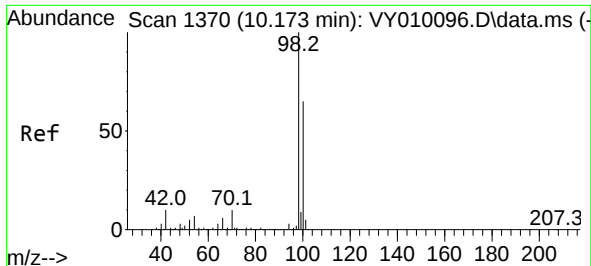

#50
Toluene-d8
Concen: 48.952 ug/l
RT: 10.179 min Scan# 1370
Delta R.T. 0.006 min
Lab File: VY010173.D
Acq: 23 Aug 2022 18:21




Instrument :
MSVOA_Y
ClientSampleId :
PSC-164717


Tgt Ion: 98 Resp: 290760
Ion Ratio Lower Upper
98 100
100 63.7 51.9 77.9

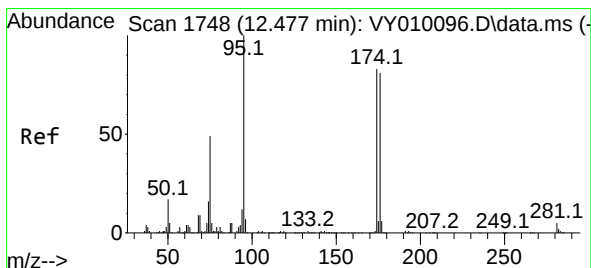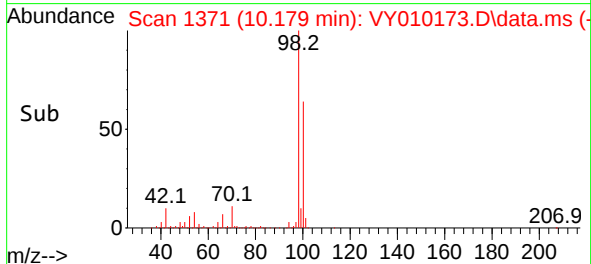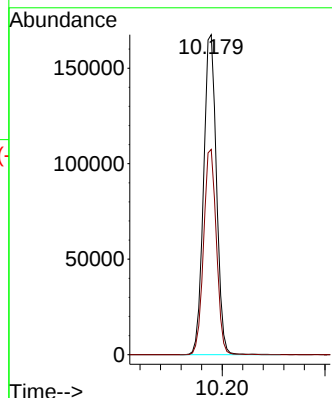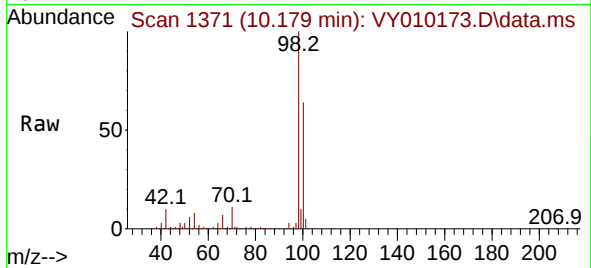

#62
4-Bromofluorobenzene
Concen: 43.091 ug/l
RT: 12.477 min Scan# 1748
Delta R.T. 0.000 min
Lab File: VY010173.D
Acq: 23 Aug 2022 18:21

Tgt Ion: 95 Resp: 91448
Ion Ratio Lower Upper
95 100
174 89.3 0.0 173.8
176 86.4 0.0 167.2


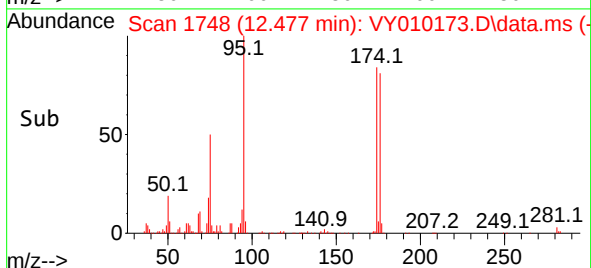
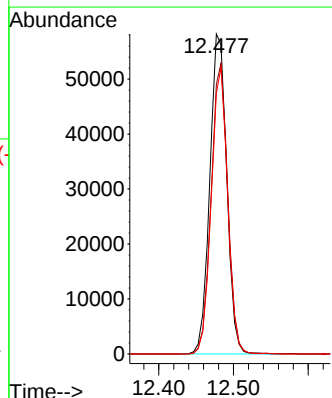
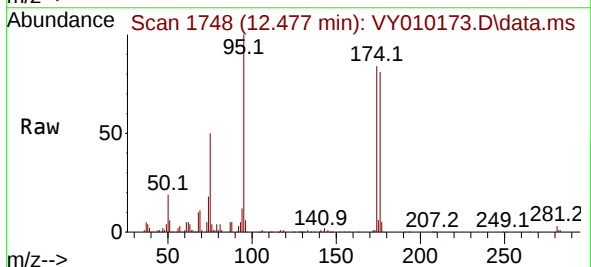


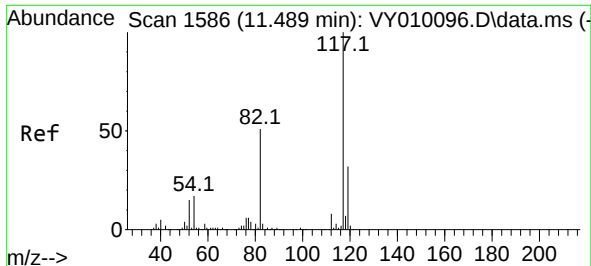

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.489 min Scan# 11
Delta R.T. 0.000 min
Lab File: VY010173.D
Acq: 23 Aug 2022 18:21

Instrument :
MSVOA_Y
ClientSampleId :
PSC-164717

Tgt Ion:117 Resp: 283993
Ion Ratio Lower Upper
117 100
82 50.5 40.6 61.0
119 31.3 25.8 38.8

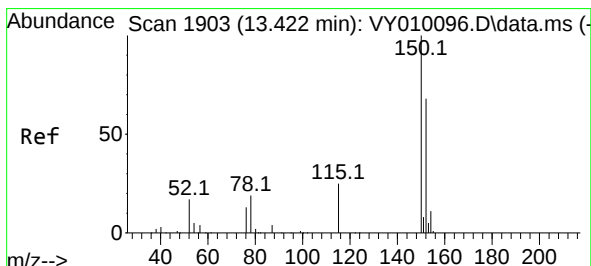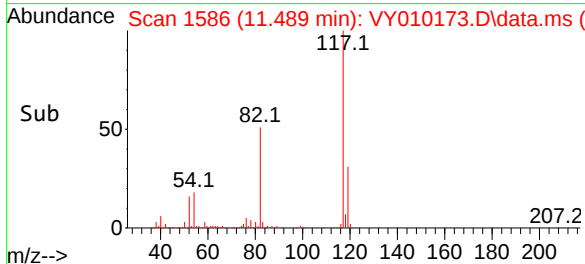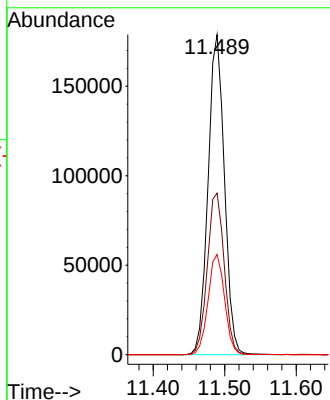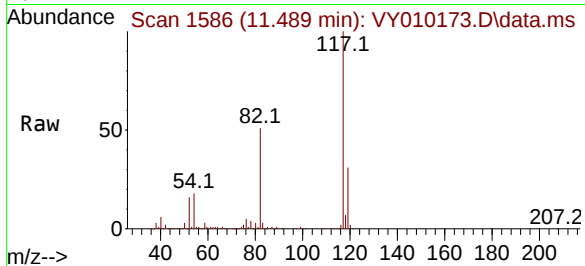

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.422 min Scan# 1903
Delta R.T. 0.000 min
Lab File: VY010173.D
Acq: 23 Aug 2022 18:21

Tgt Ion:152 Resp: 130373
Ion Ratio Lower Upper
152 100
115 55.6 28.1 84.2
150 155.4 0.0 346.2

